

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
 Data File : PL096089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 19:54
 Operator : AR\AJ
 Sample : Q2338-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-061625

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/18/2025
 Supervised By : mohammad ahmed 06/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 06:30:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.569	2.881	40234128	50419918	11.057m	10.630
28) SA Decachlor...	9.113	8.065	29629075	37308125	10.347	6.190 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061725\
Data File : PL096089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 19:54
Operator : AR\AJ
Sample : Q2338-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-061625


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/18/2025
Supervised By : mohammad ahmed 06/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 06:30:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

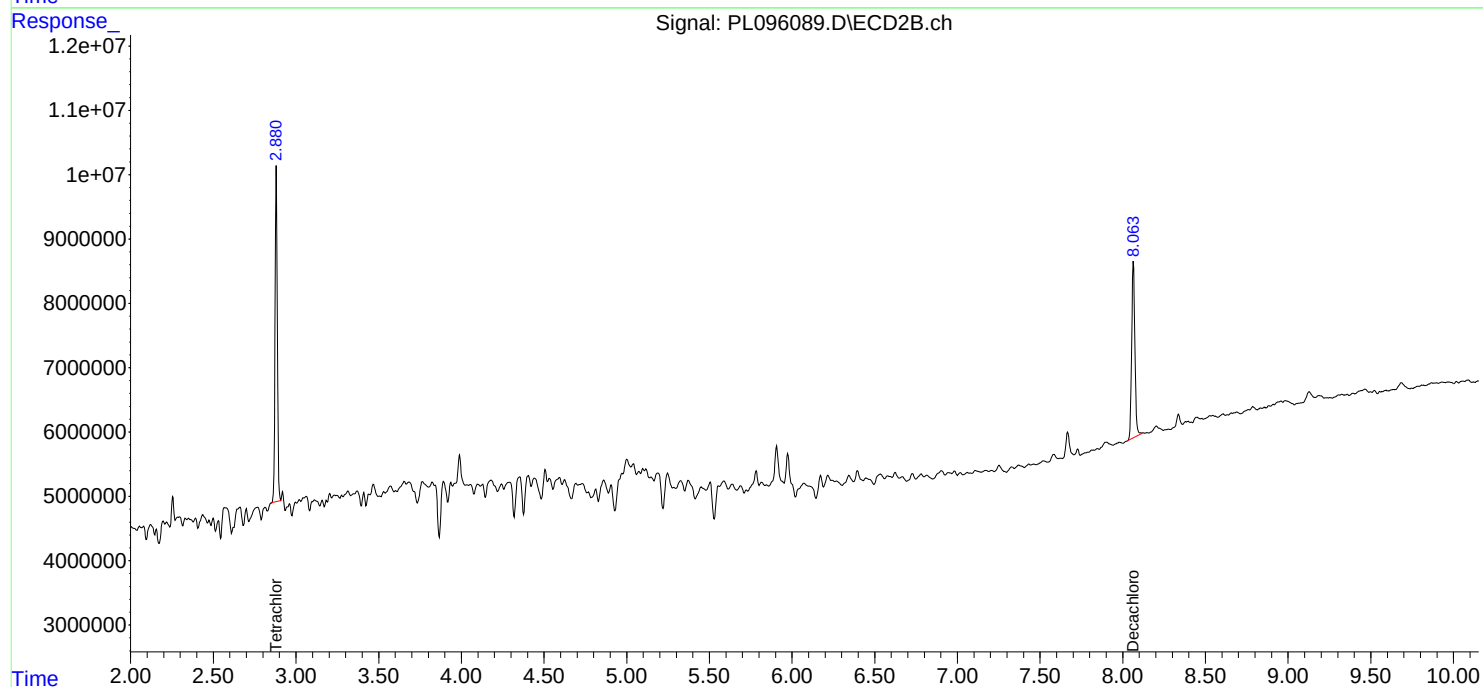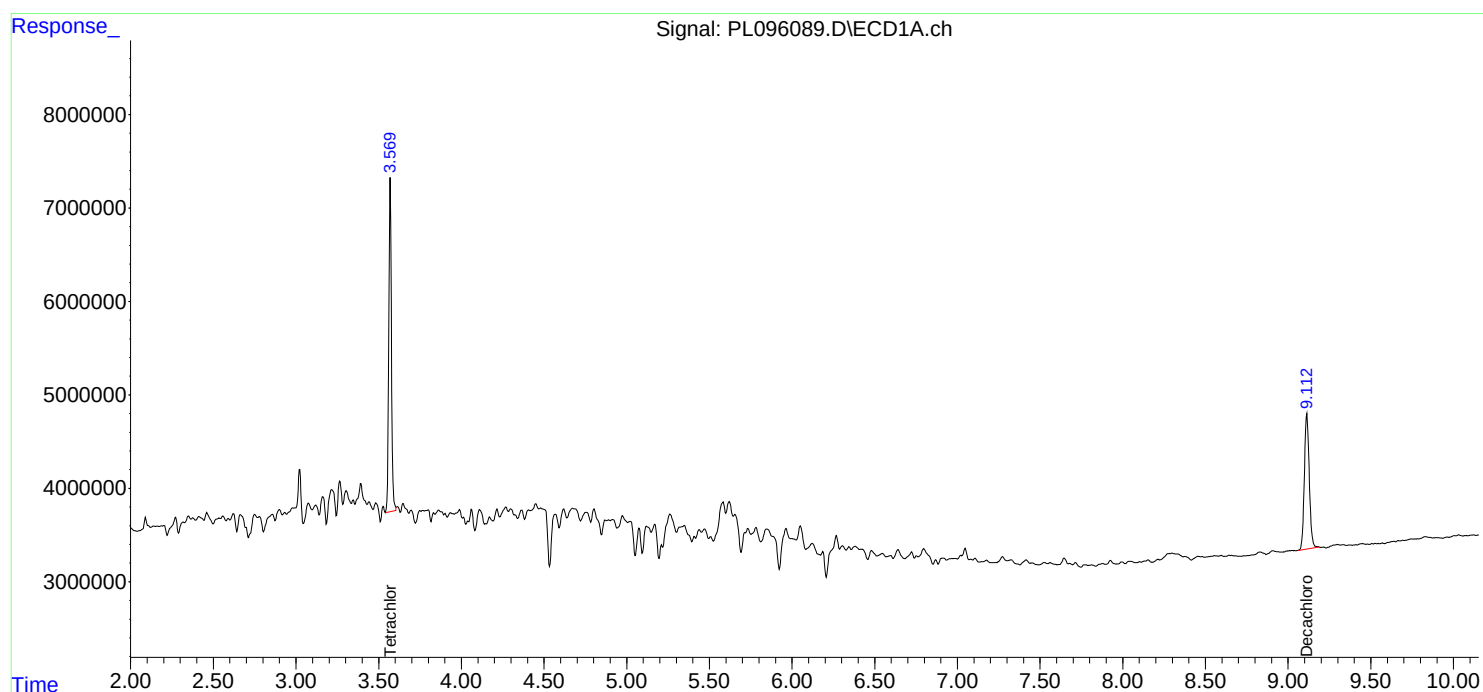

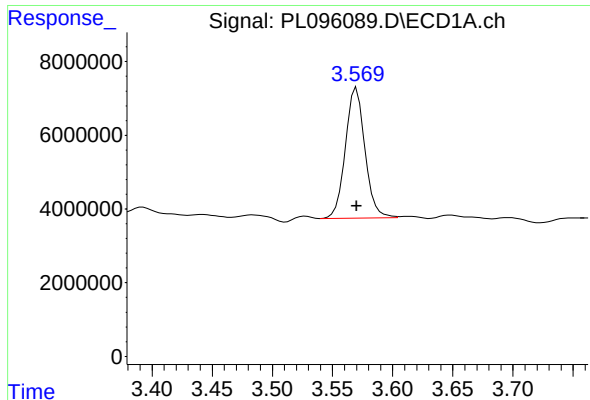


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: -0.001 min
Response: 40234128
Conc: 11.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061625


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/18/2025
Supervised By :mohammad ahmed 06/19/2025

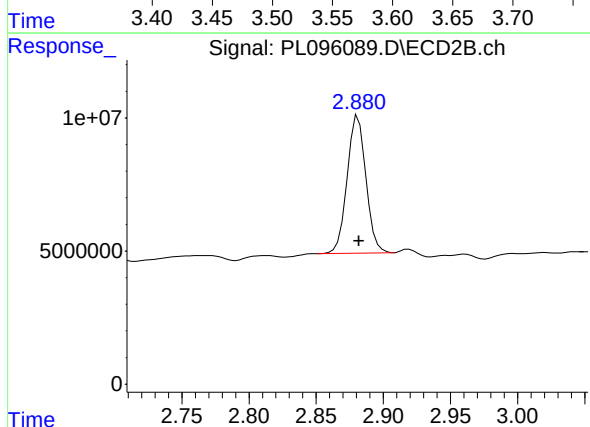


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 50419918
Conc: 10.63 ng/ml

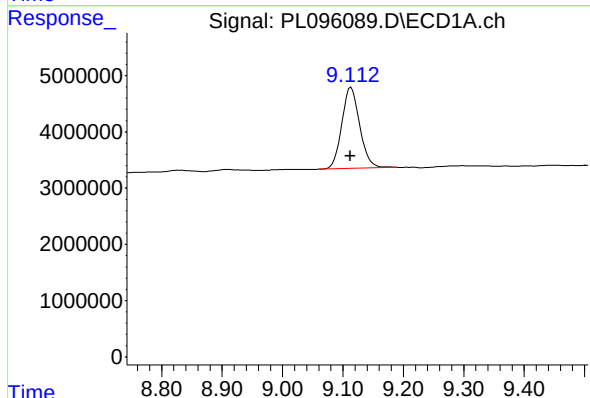

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 29629075
Conc: 10.35 ng/ml

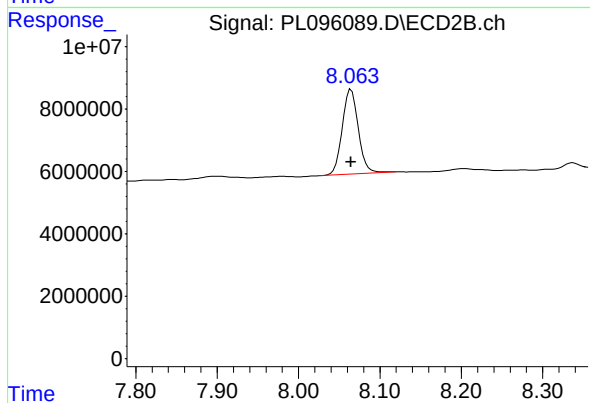

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 37308125
Conc: 6.19 ng/ml