

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061818\
 Data File : PL037079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2018 21:26
 Operator : UA\AJ
 Sample : J3512-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FADW4710L

Manual Integrations
 APPROVED

UGO
 6/19/2018 4:24:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 03:29:35 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 14 16:13:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.336	3.937	116.2E6	42770531	16.342m	16.730
28)	SA Decachlor...	8.021	8.949	73894624	27248208	11.358	10.681

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061818\
Data File : PL037079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2018 21:26
Operator : UA\AJ
Sample : J3512-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FADW4710L


Manual Integrations
APPROVED

UGO
6/19/2018 4:24:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 03:29:35 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL061418.M
Quant Title : GC Extractables
QLast Update : Thu Jun 14 16:13:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

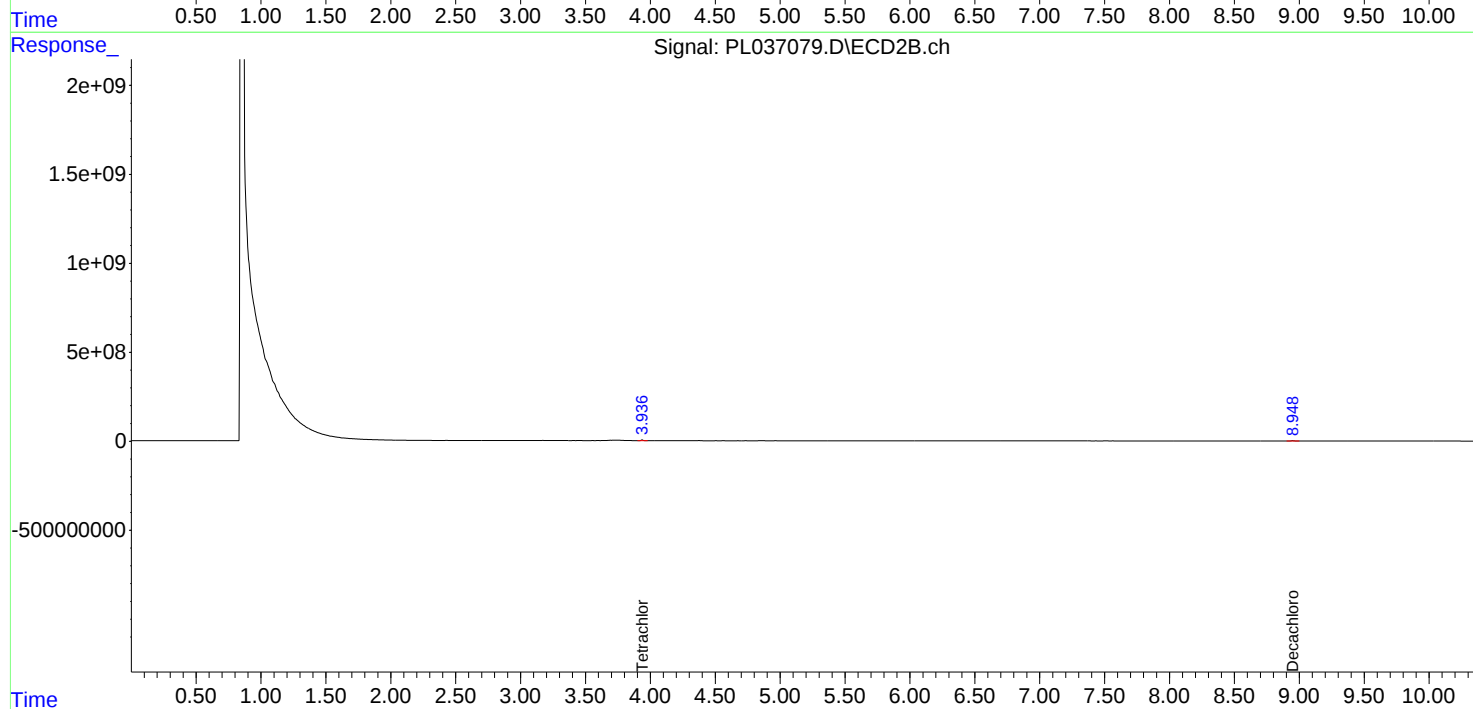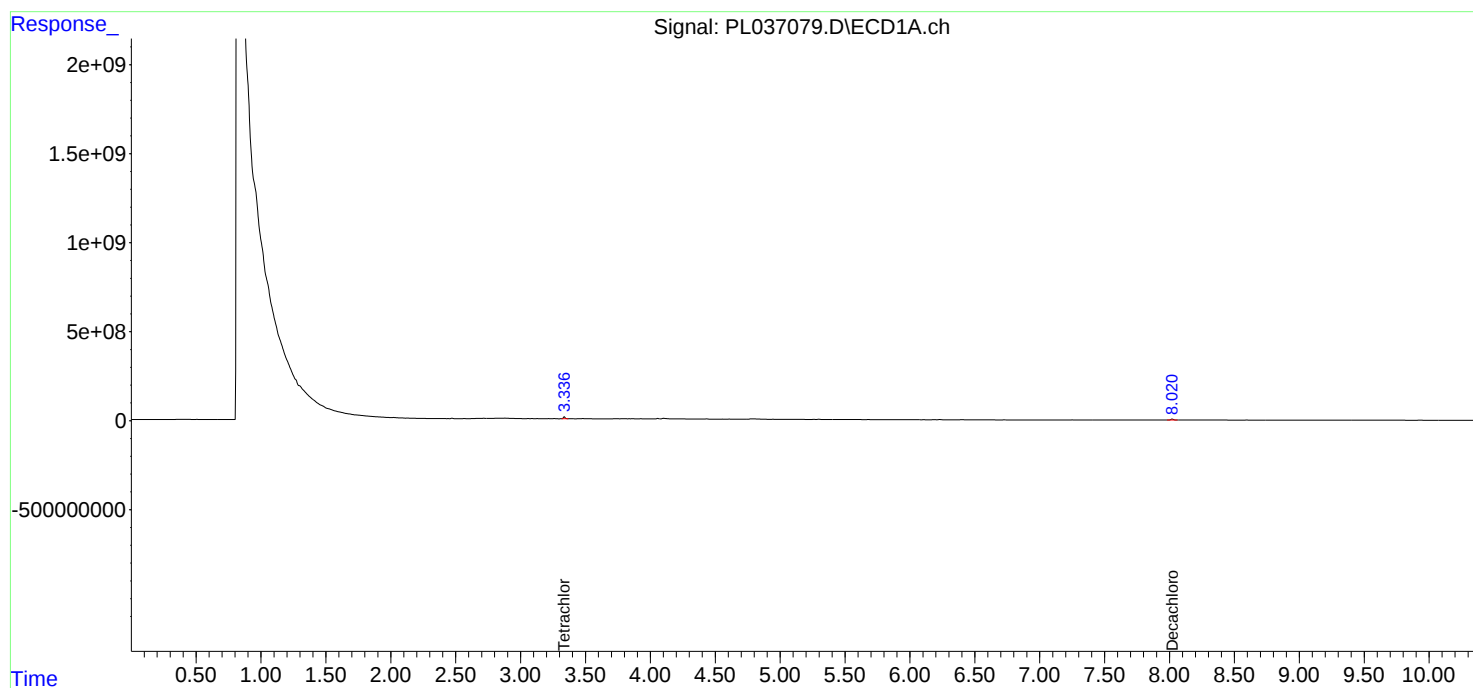

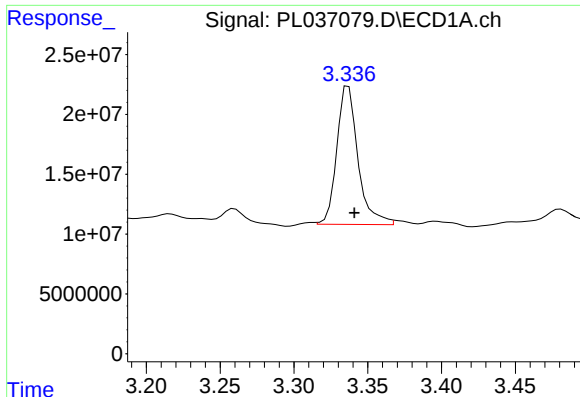


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: -0.005 min
Response: 116210829
Conc: 16.34 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FADW4710L


Manual Integrations
APPROVED

UGO
6/19/2018 4:24:10 PM

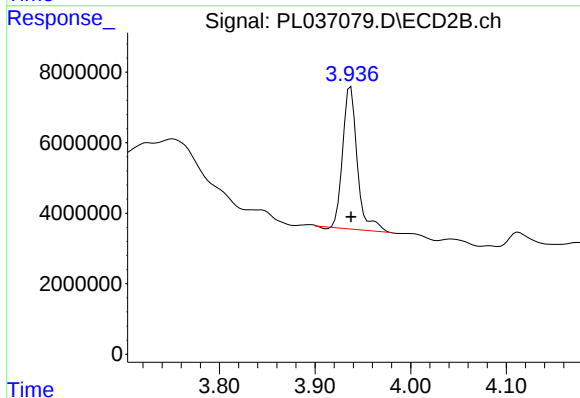


#1 Tetrachloro-m-xylene

R.T.: 3.937 min
Delta R.T.: 0.000 min
Response: 42770531
Conc: 16.73 ng/ml

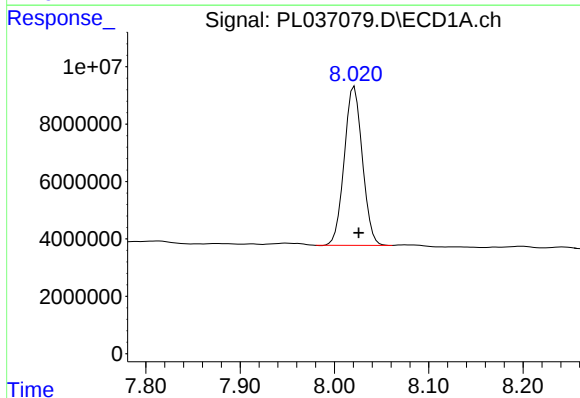

#28 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: -0.005 min
Response: 73894624
Conc: 11.36 ng/ml

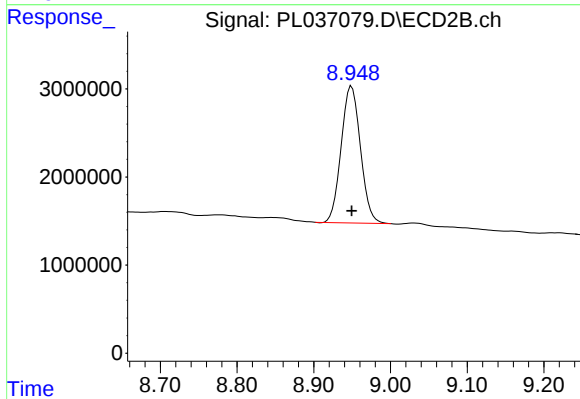

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: 0.000 min
Response: 27248208
Conc: 10.68 ng/ml