

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061819\
 Data File : PL049590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2019 14:58
 Operator : SM\AJ
 Sample : K3157-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-061719-D

Manual Integrations
 APPROVED

Ankita
 6/19/2019 11:51:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:04:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.935	50875568	14643237	4.617	5.069
28) SA Decachlor...	7.991	8.970	64455871	22592005	5.069	6.765m#
Target Compounds						
12) B 4,4'-DDE	5.432	6.264	10793319	2986960	0.690m	0.910 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061819\
Data File : PL049590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2019 14:58
Operator : SM\AJ
Sample : K3157-07
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-01-061719-D


Manual Integrations
APPROVED

Ankita
6/19/2019 11:51:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:04:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

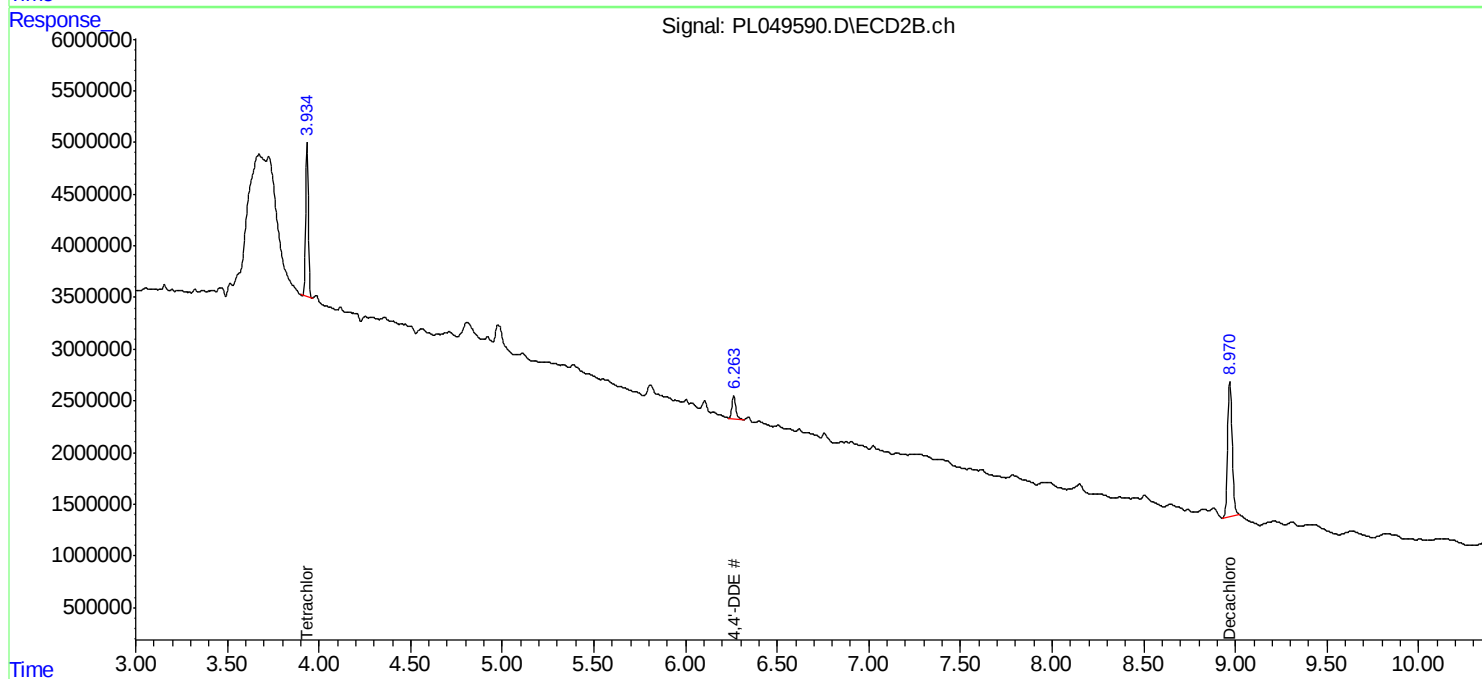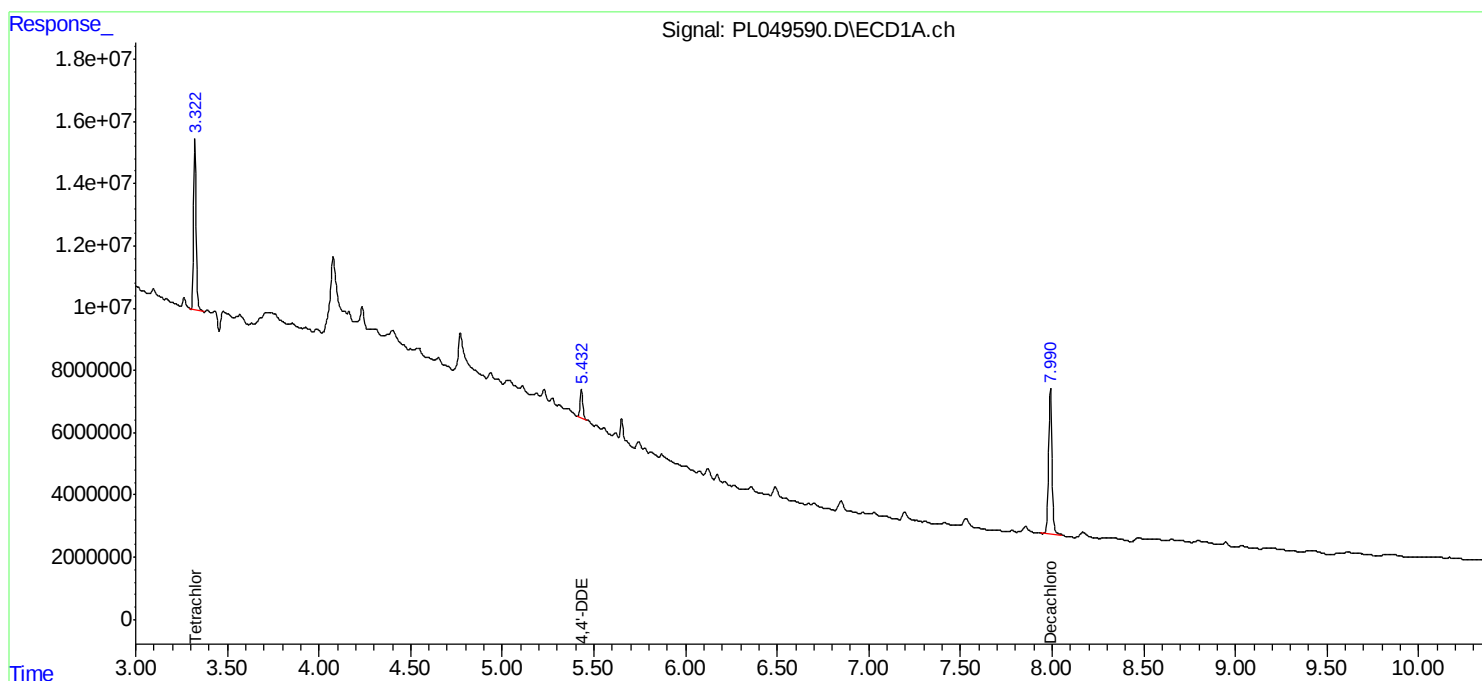

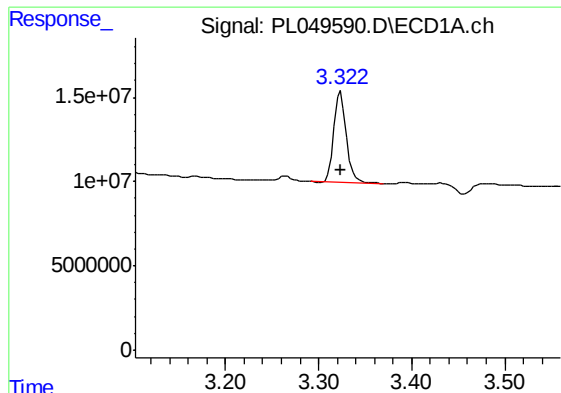


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 50875568
Conc: 4.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-061719-D


Manual Integrations
APPROVED

Ankita
6/19/2019 11:51:17 AM

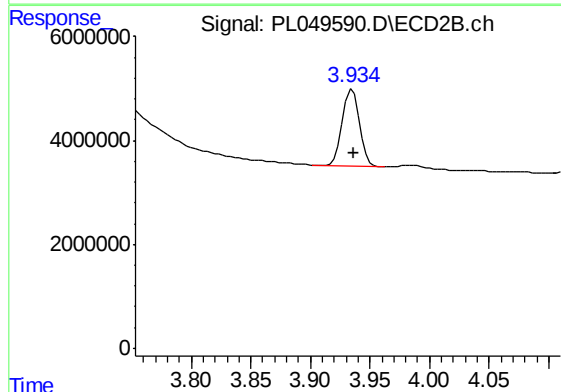


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 14643237
Conc: 5.07 ng/ml

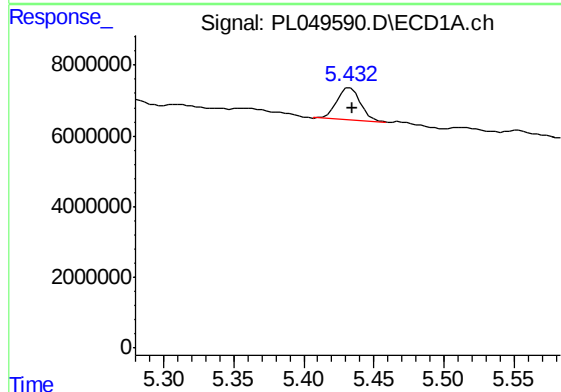


#12 4,4'-DDE

R.T.: 5.432 min
Delta R.T.: -0.003 min
Response: 10793319
Conc: 0.69 ng/ml m

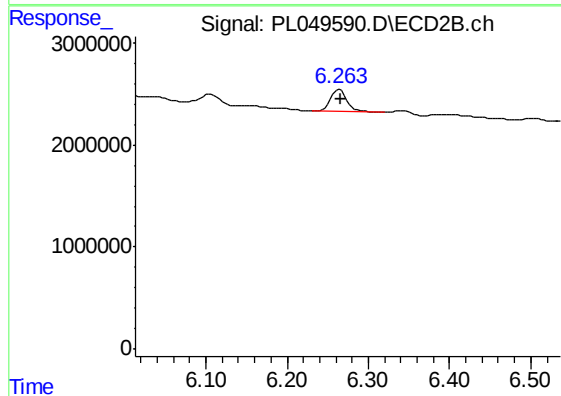

#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.002 min
Response: 2986960
Conc: 0.91 ng/ml

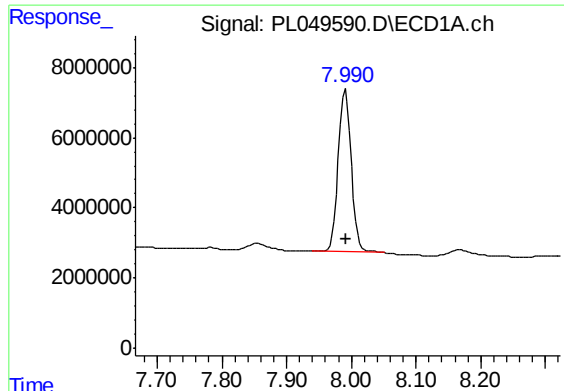


#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.002 min
Response: 64455871
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-061719-D

Manual Integrations
APPROVED

Ankita
6/19/2019 11:51:17 AM

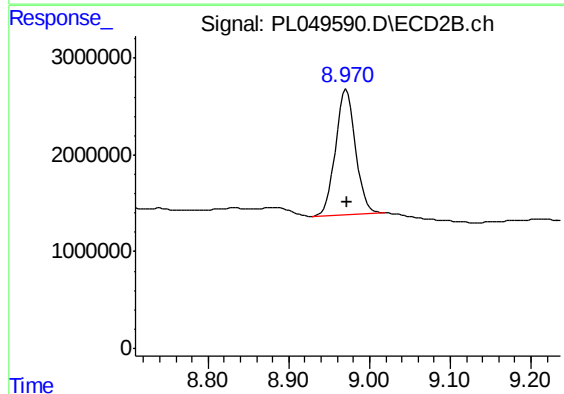

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.002 min
Response: 22592005
Conc: 6.76 ng/ml m