

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
 Data File : PL059362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 23:26
 Operator : AJ\MA
 Sample : L3024-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:44:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.519	4.072	36655168	57185726	21.227	21.978
28)	SA Decachlor...	8.290	9.181	29509098	42895213	17.945	18.095
Target Compounds							
4)	MA Heptachlor	0.000	5.261	0	1009921	N.D.	0.293 #
7)	B delta-BHC	0.000	5.166f	0	4308528	N.D.	1.536 #
8)	B Heptachlo...	0.000	5.984f	0	947297	N.D.	0.342 #
15)	B Endosulfa...	0.000	7.007	0	859933	N.D.	0.330 #
23)	Chlordane-1	4.426f	0.000	812813	0	16.159	N.D. #
24)	Chlordane-2	4.923f	0.000	595130	0	11.405	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
Data File : PL059362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 23:26
Operator : AJ\MA
Sample : L3024-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RO-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:44:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

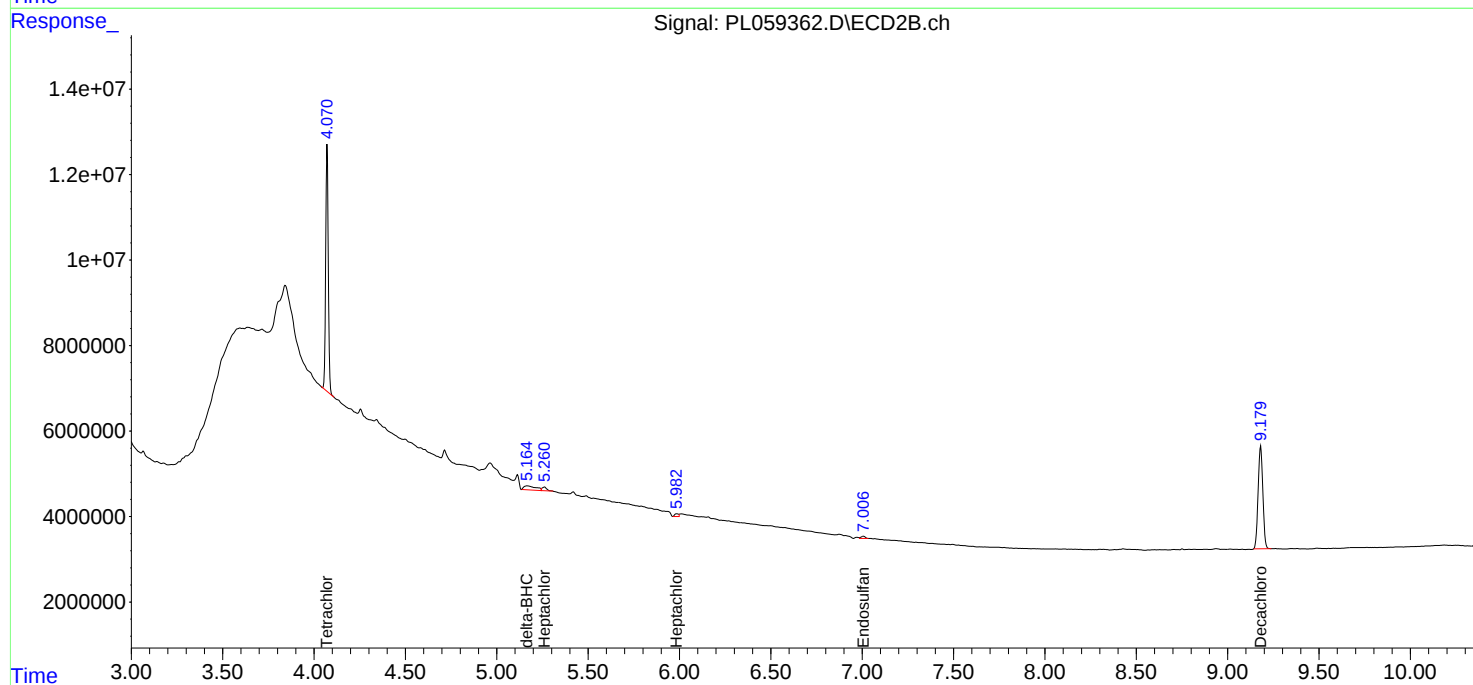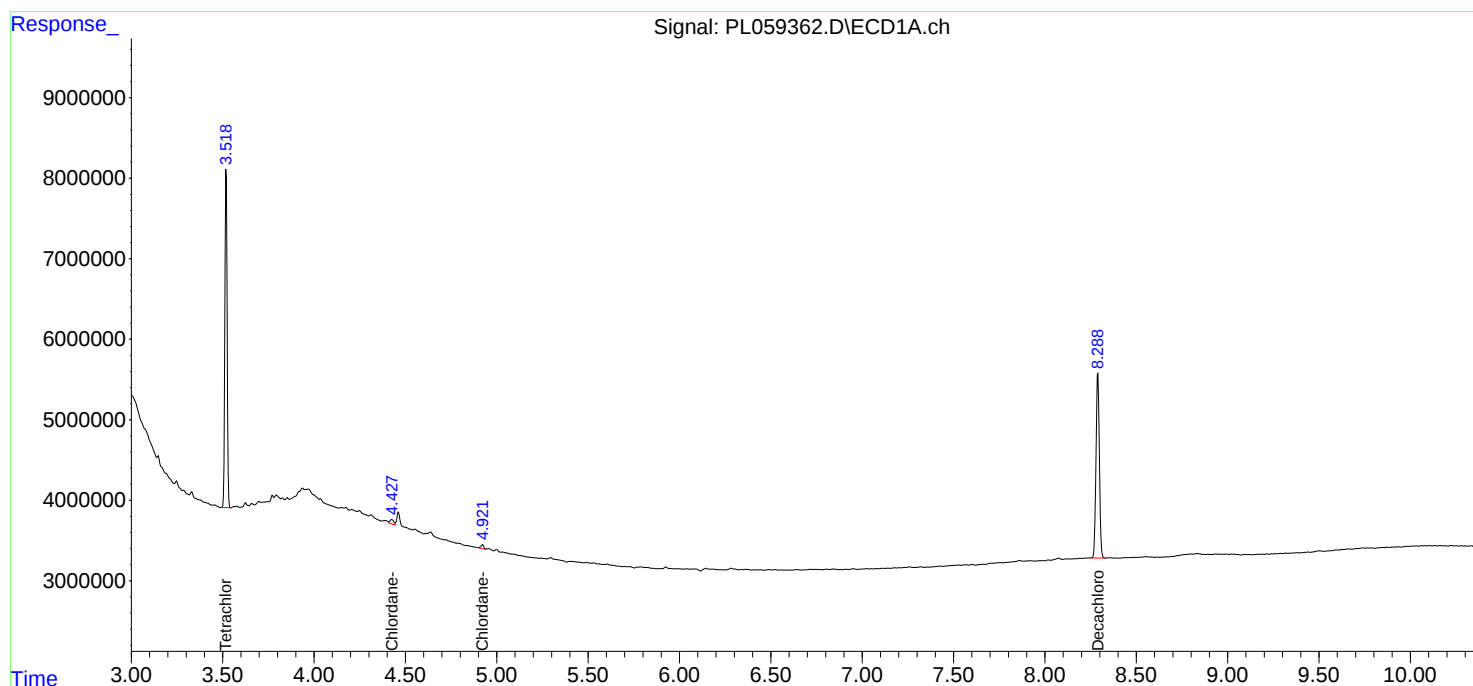


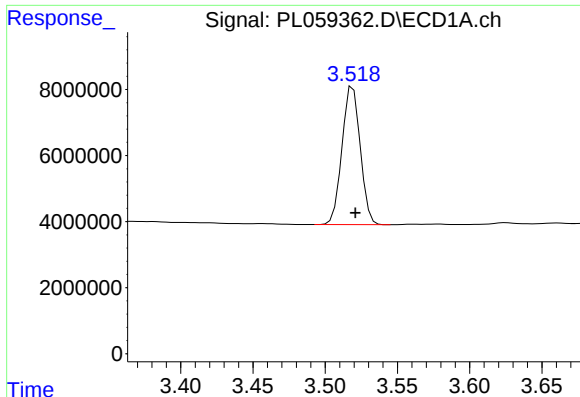

#1 Tetrachloro-m-xylene


R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 36655168
Conc: 21.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-6

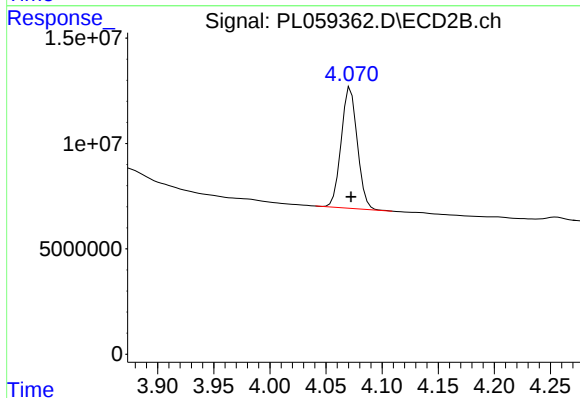


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 57185726
Conc: 21.98 ng/ml

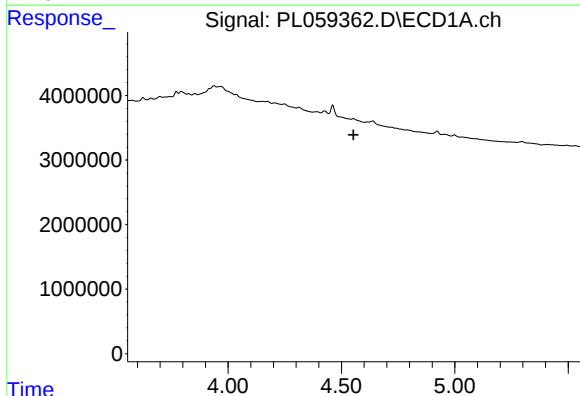


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

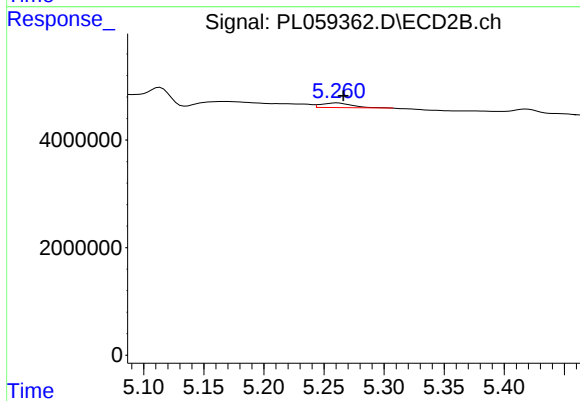

#4 Heptachlor


R.T.: 5.261 min
Delta R.T.: -0.005 min
Response: 1009921
Conc: 0.29 ng/ml

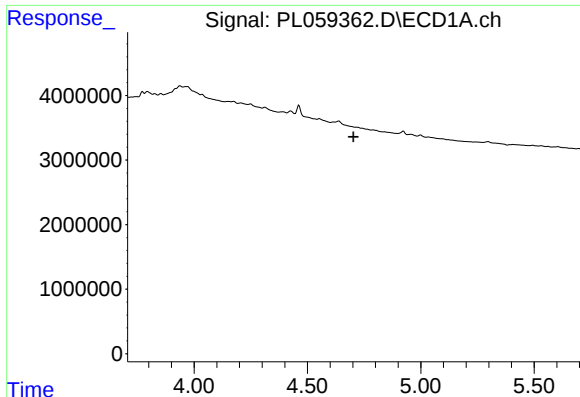

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-6

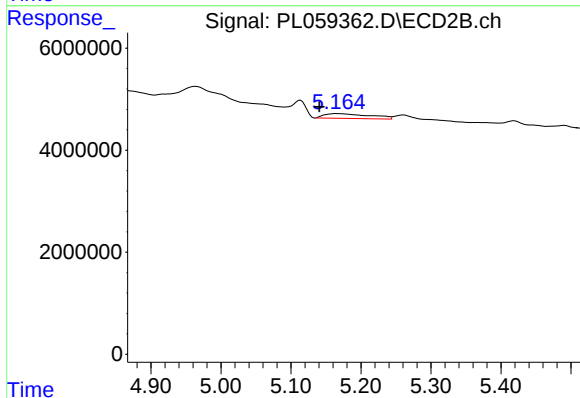


#7 delta-BHC

R.T.: 5.166 min
Delta R.T.: 0.026 min
Response: 4308528
Conc: 1.54 ng/ml

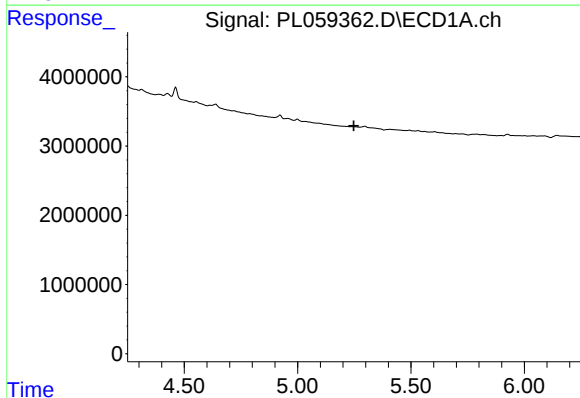


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.248 min
Response: 0
Conc: N.D.

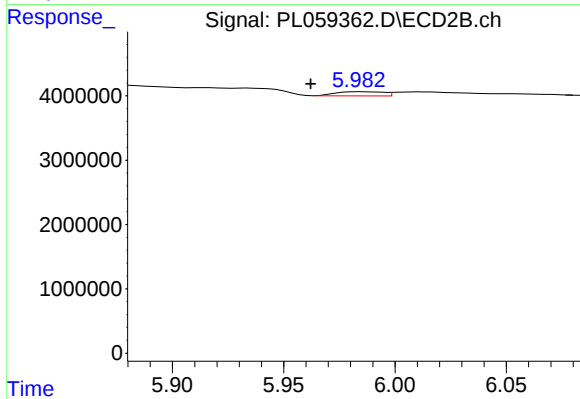

#8 Heptachlor epoxide


R.T.: 5.984 min
Delta R.T.: 0.022 min
Response: 947297
Conc: 0.34 ng/ml

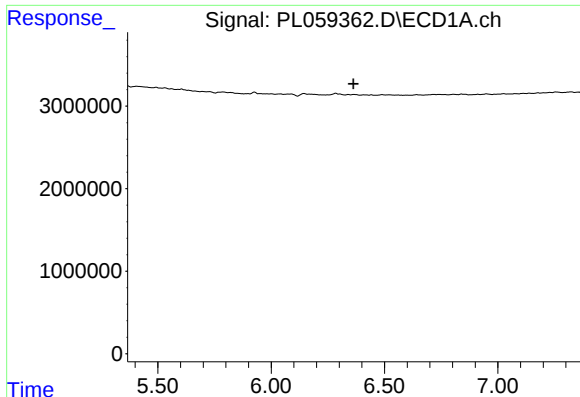

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-6

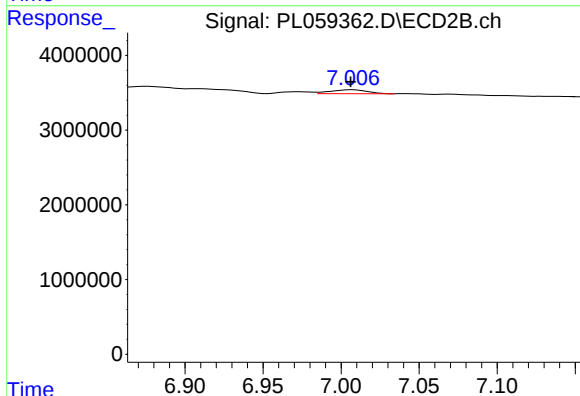


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.001 min
Response: 859933
Conc: 0.33 ng/ml

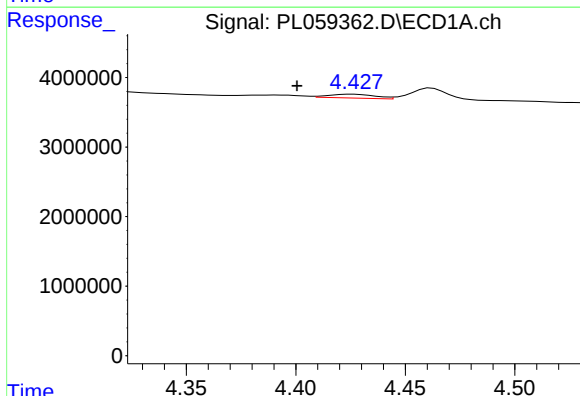


#23 Chlordane-1

R.T.: 4.426 min
Delta R.T.: 0.026 min
Response: 812813
Conc: 16.16 ng/ml

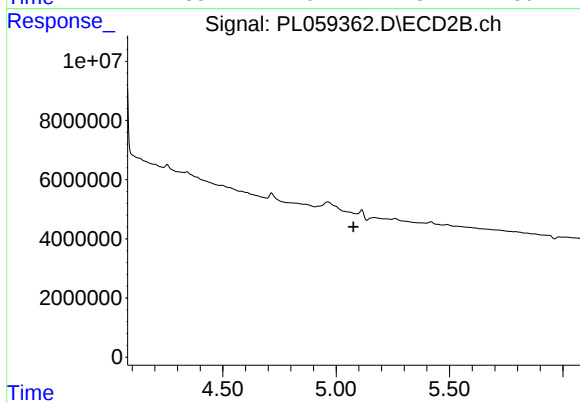

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

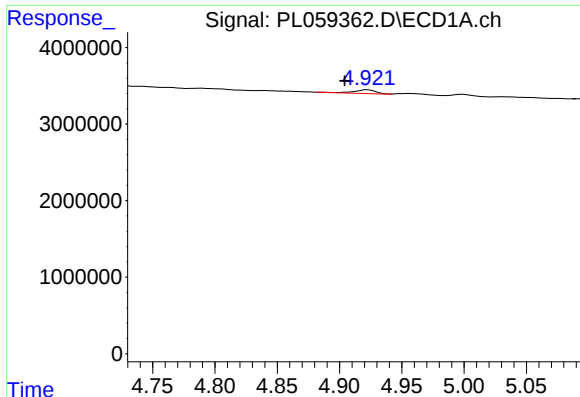

#24 Chlordane-2


R.T.: 4.923 min
Delta R.T.: 0.019 min
Response: 595130
Conc: 11.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-6

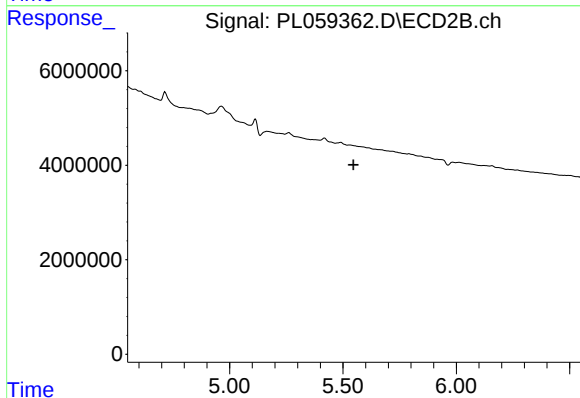


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

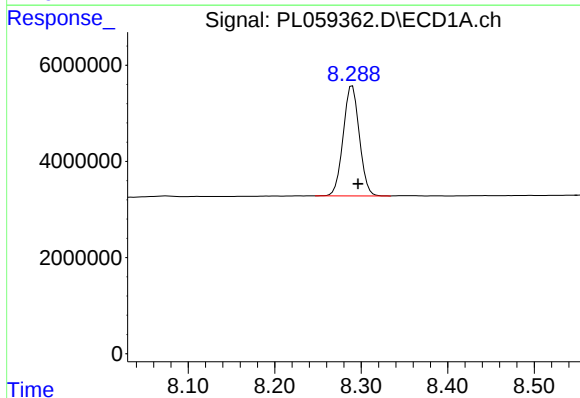

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 29509098
Conc: 17.95 ng/ml

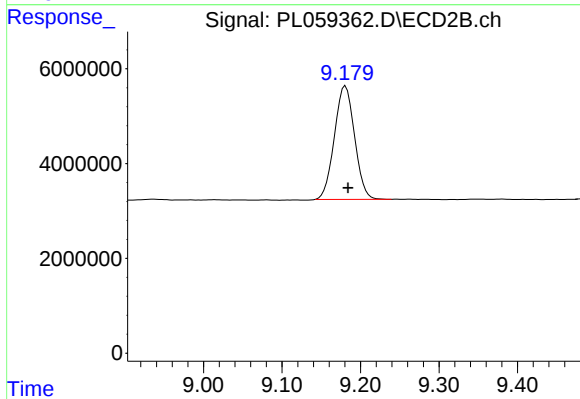

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 42895213
Conc: 18.10 ng/ml