

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
 Data File : PL059364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2020 23:54
 Operator : AJ\MA
 Sample : L3024-23
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:45:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.519	4.072	37348801	58226956	21.628	22.379
28)	SA Decachlor...	8.290	9.181	23856815	34669898	14.508	14.625
Target Compounds							
2)	A alpha-BHC	3.954	0.000	1487399	0	0.594	N.D. #
3)	MA gamma-BHC...	4.249	0.000	460387	0	0.210	N.D. #
4)	MA Heptachlor	4.554	5.258	3842271	972442	1.847	0.282 #
7)	B delta-BHC	0.000	5.115f	0	4688780	N.D.	1.671 #
8)	B Heptachlo...	0.000	5.946f	0	1072754	N.D.	0.387 #
15)	B Endosulfa...	0.000	7.008	0	671797	N.D.	0.258 #
23)	Chlordane-1	4.426f	0.000	754387	0	14.997	N.D. #
24)	Chlordane-2	4.920f	0.000	1673808	0	32.077	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
Data File : PL059364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2020 23:54
Operator : AJ\MA
Sample : L3024-23
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:45:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

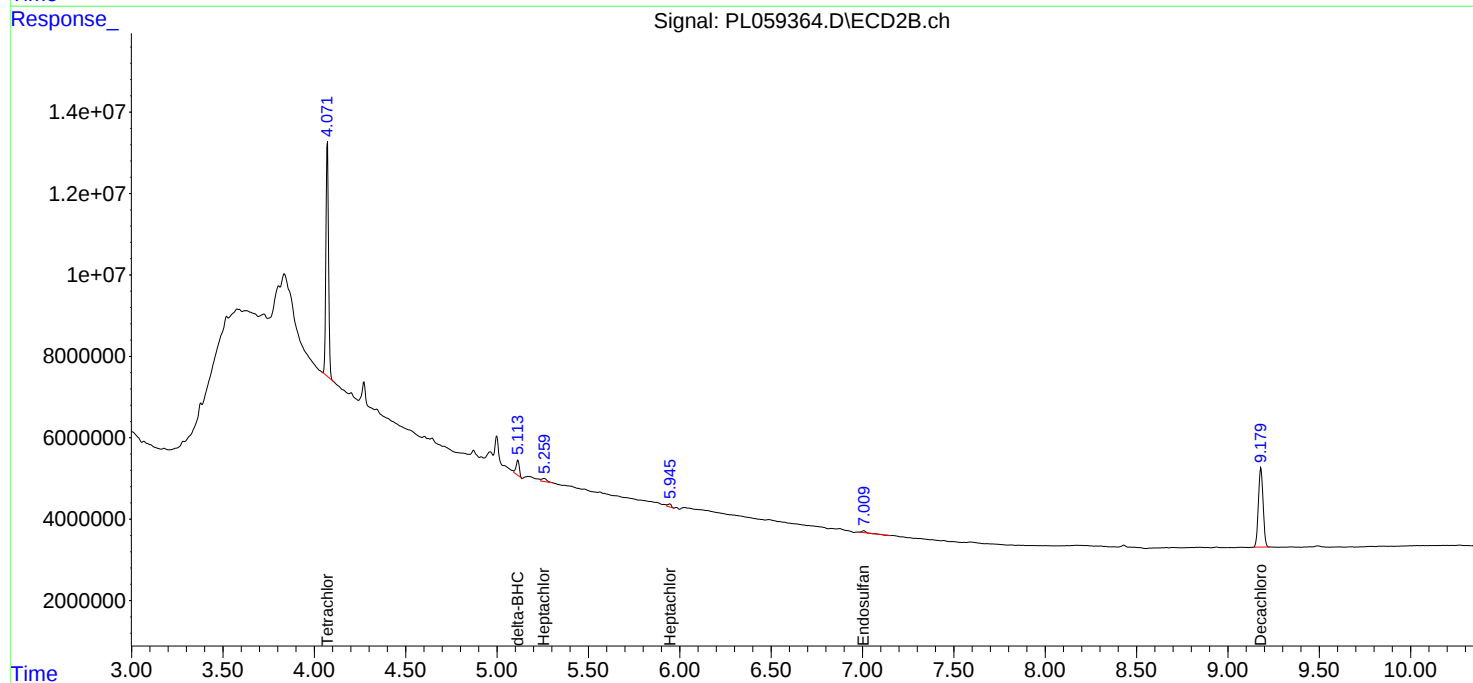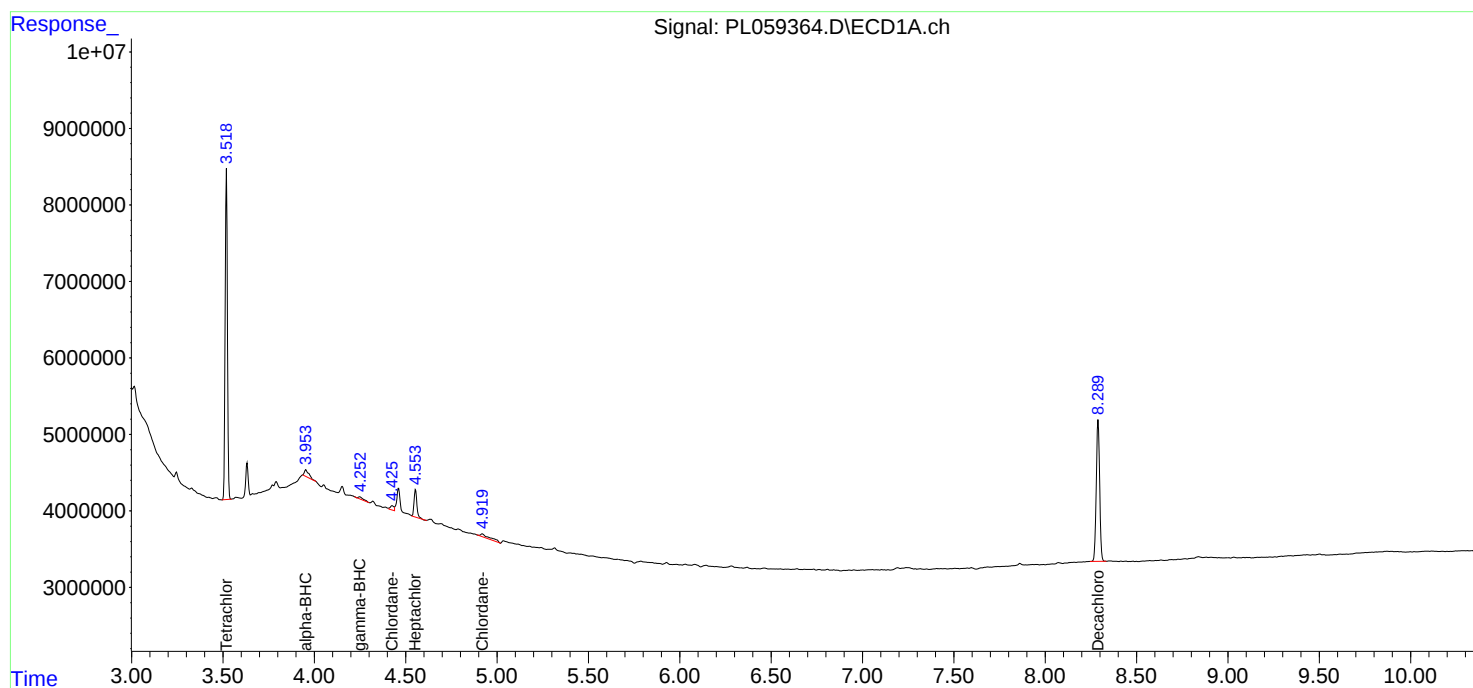


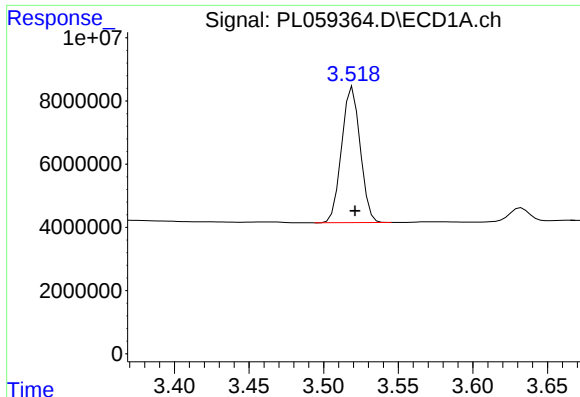

#1 Tetrachloro-m-xylene


R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 37348801
Conc: 21.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-11

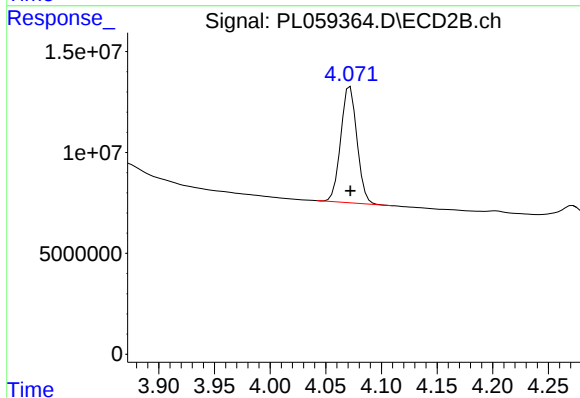


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 58226956
Conc: 22.38 ng/ml

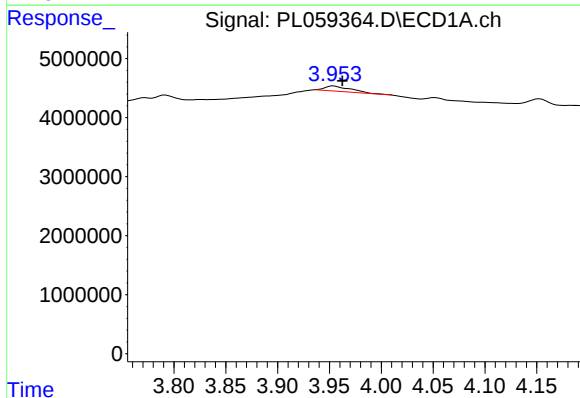


#2 alpha-BHC

R.T.: 3.954 min
Delta R.T.: -0.008 min
Response: 1487399
Conc: 0.59 ng/ml

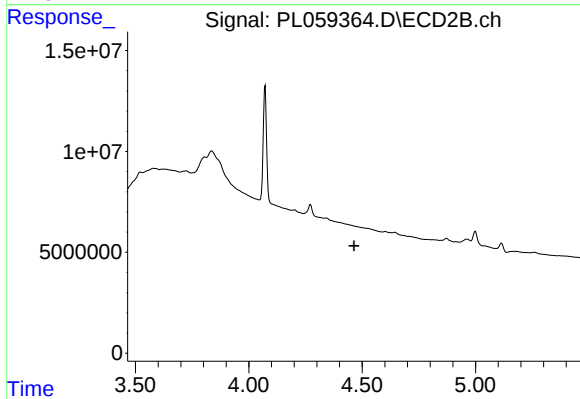

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

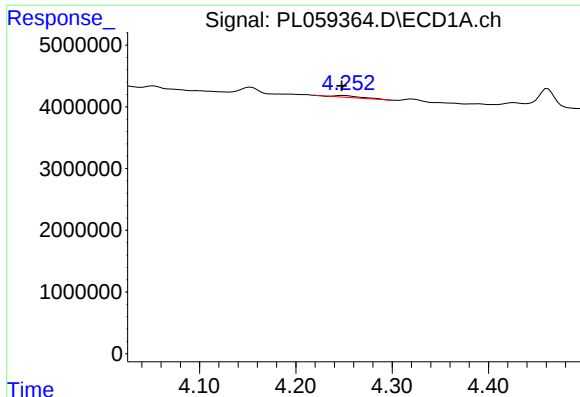

#3 gamma-BHC (Lindane)


R.T.: 4.249 min
Delta R.T.: 0.002 min
Response: 460387
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-11

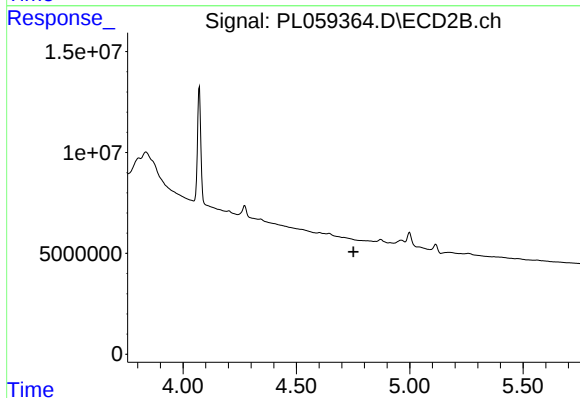


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.752 min
Response: 0
Conc: N.D.

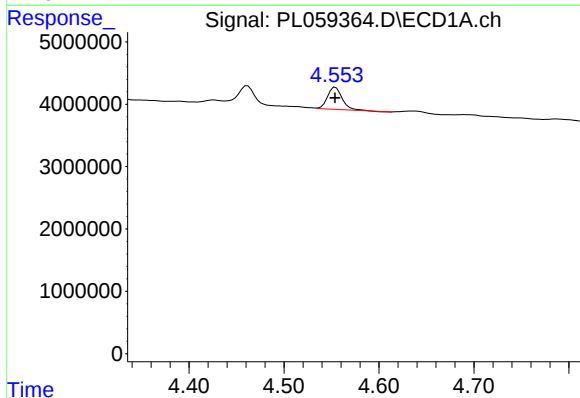


#4 Heptachlor

R.T.: 4.554 min
Delta R.T.: 0.000 min
Response: 3842271
Conc: 1.85 ng/ml

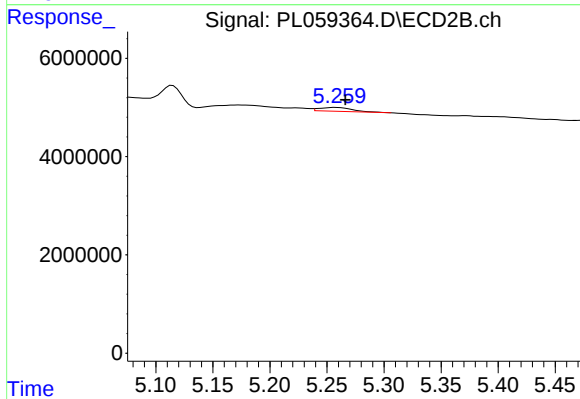

#4 Heptachlor


R.T.: 5.258 min
Delta R.T.: -0.008 min
Response: 972442
Conc: 0.28 ng/ml

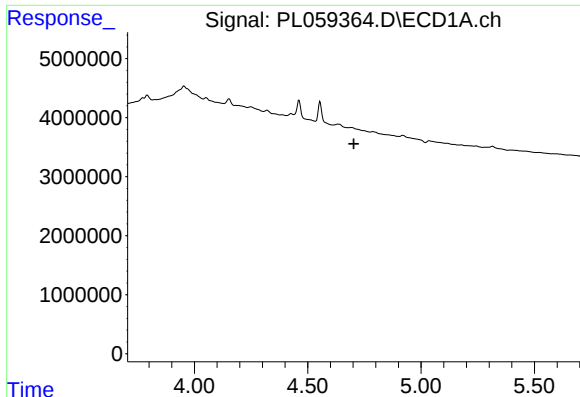

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-11

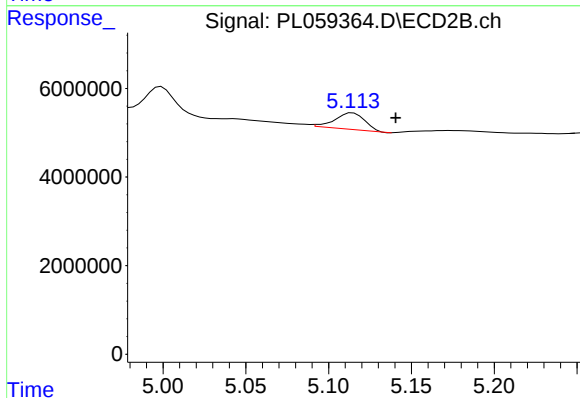


#7 delta-BHC

R.T.: 5.115 min
Delta R.T.: -0.026 min
Response: 4688780
Conc: 1.67 ng/ml

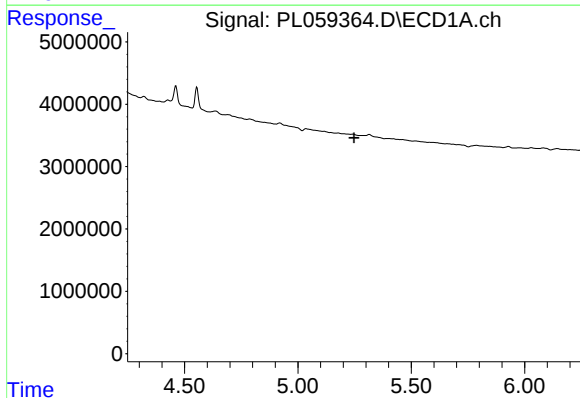


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.248 min
Response: 0
Conc: N.D.

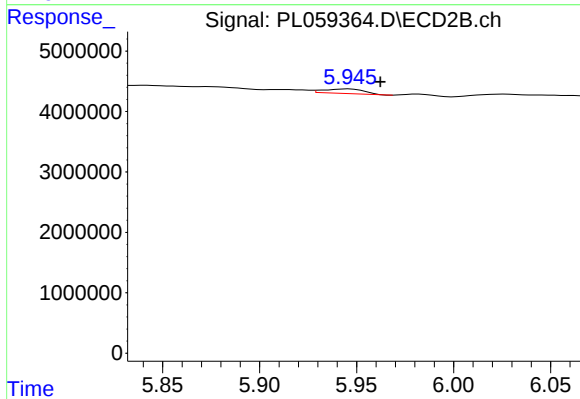

#8 Heptachlor epoxide


R.T.: 5.946 min
Delta R.T.: -0.016 min
Response: 1072754
Conc: 0.39 ng/ml

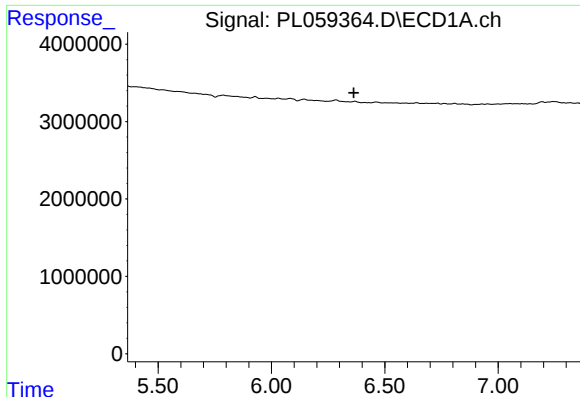

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-11

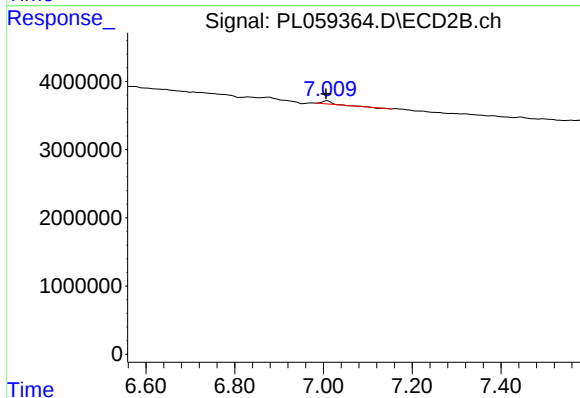


#15 Endosulfan II

R.T.: 7.008 min
Delta R.T.: 0.002 min
Response: 671797
Conc: 0.26 ng/ml

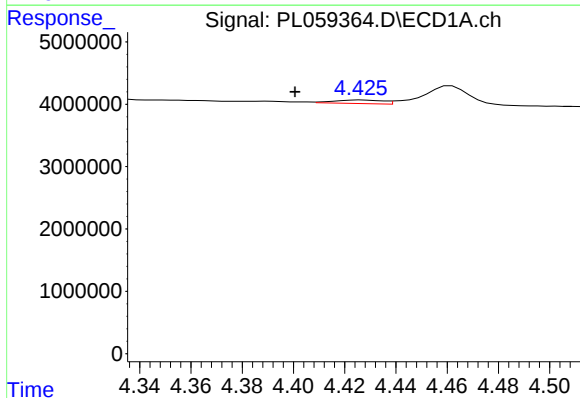


#23 Chlordane-1

R.T.: 4.426 min
Delta R.T.: 0.026 min
Response: 754387
Conc: 15.00 ng/ml

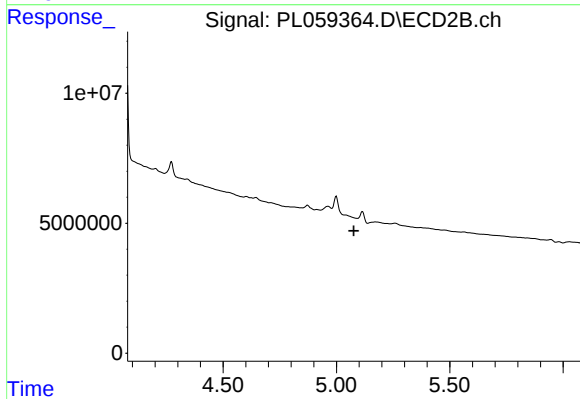

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

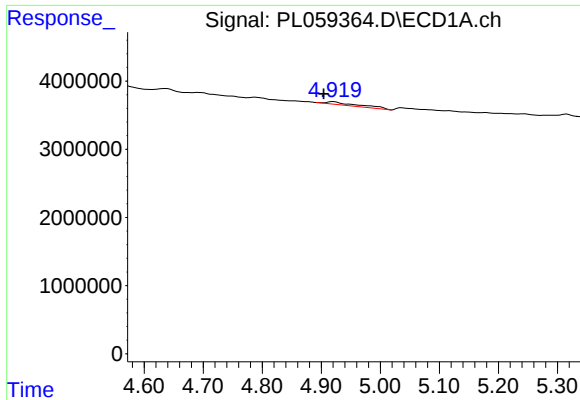

#24 Chlordane-2


R.T.: 4.920 min
Delta R.T.: 0.016 min
Response: 1673808
Conc: 32.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-11

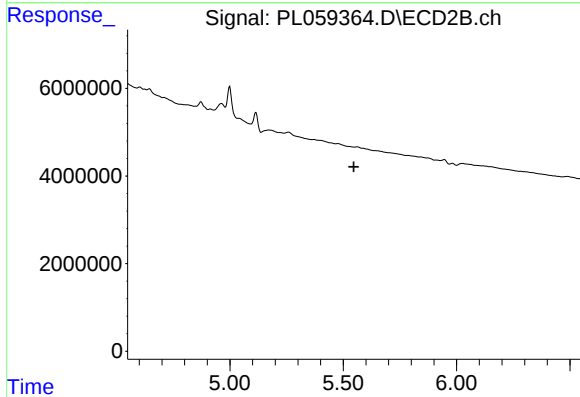


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

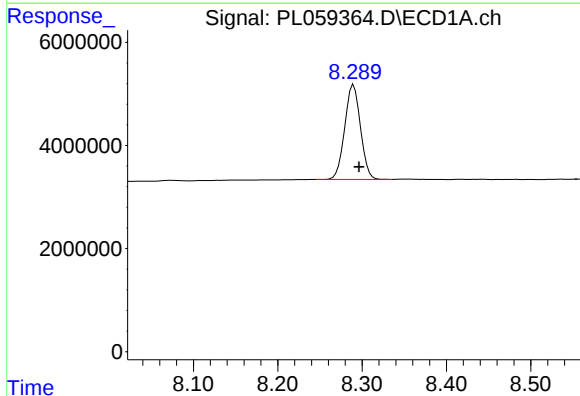

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 23856815
Conc: 14.51 ng/ml

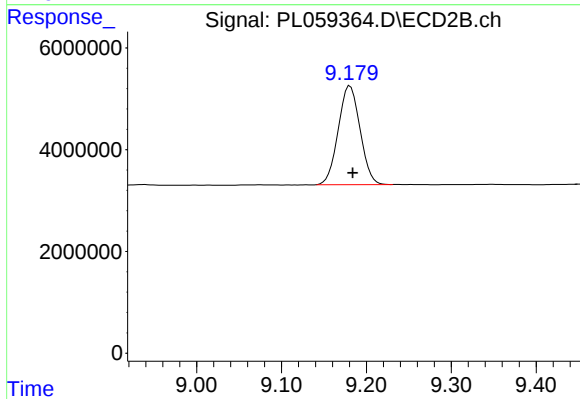

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 34669898
Conc: 14.63 ng/ml