

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
 Data File : PL059365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 00:08
 Operator : AJ\MA
 Sample : L3024-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RO-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 00:45:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.519	4.071	39522287	61454228	22.887	23.619
28)	SA Decachlor...	8.290	9.181	26366592	38778448	16.034	16.359
Target Compounds							
2)	A alpha-BHC	3.962	0.000	1071187	0	0.428	N.D. #
4)	MA Heptachlor	0.000	5.260	0	538735	N.D.	0.156 #
7)	B delta-BHC	0.000	5.161f	0	2299010	N.D.	0.820 #
15)	B Endosulfa...	6.368	7.009	247236	999438	0.160	0.384 #
20)	A Methoxychlor	0.000	7.694f	0	196477	N.D.	0.149 #
21)	B Endrin ke...	7.250	0.000	96360	0	0.055	N.D. #
23)	Chlordane-1	4.390	0.000	369676	0	7.349	N.D. #
27)	Chlordane-5	6.368	0.000	247236	0	4.968	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
Data File : PL059365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 00:08
Operator : AJ\MA
Sample : L3024-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RO-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 00:45:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

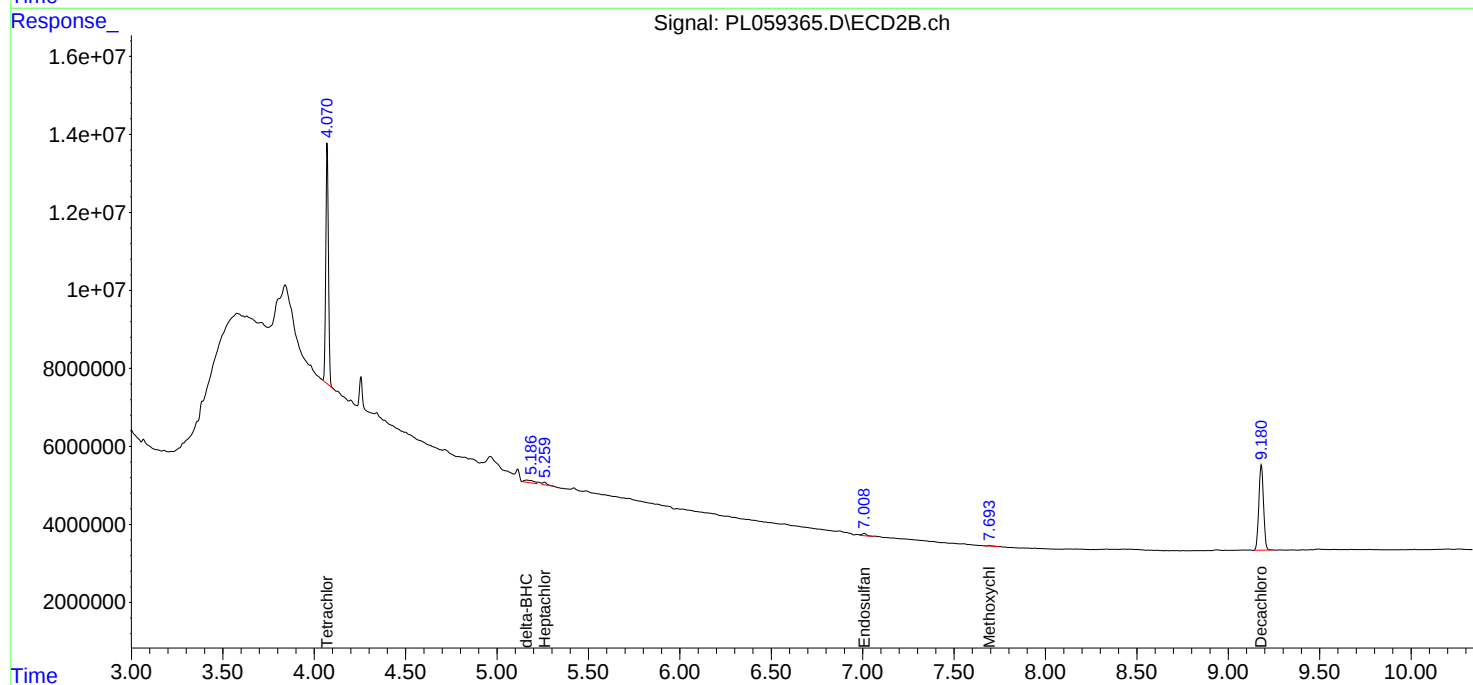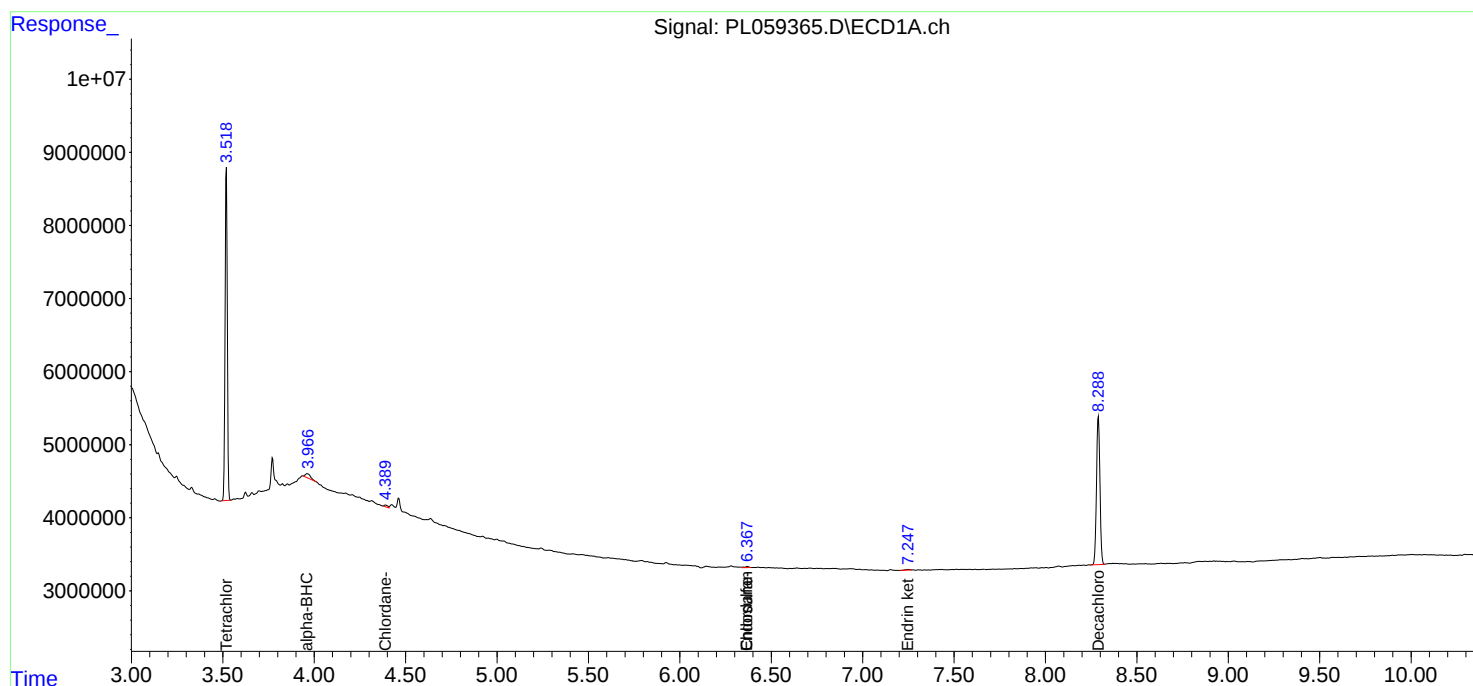


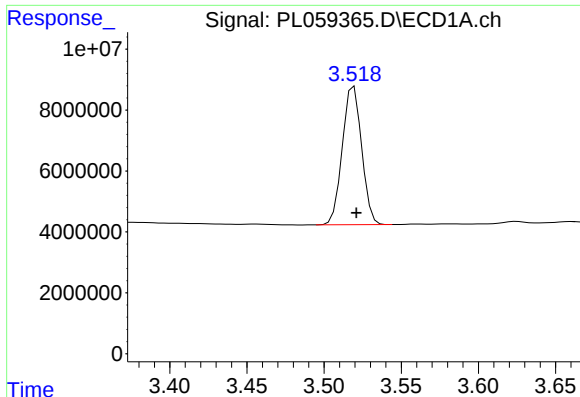

#1 Tetrachloro-m-xylene


R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 39522287
Conc: 22.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-25

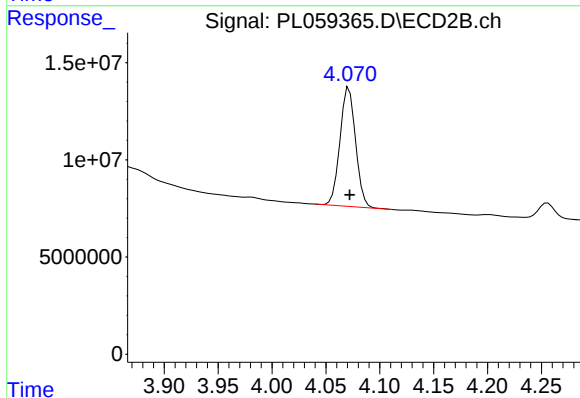


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 61454228
Conc: 23.62 ng/ml

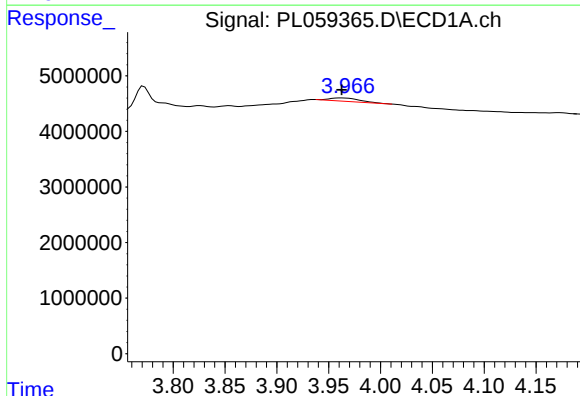


#2 alpha-BHC

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 1071187
Conc: 0.43 ng/ml

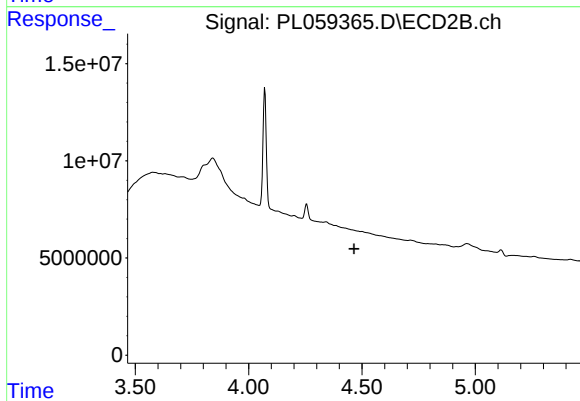

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

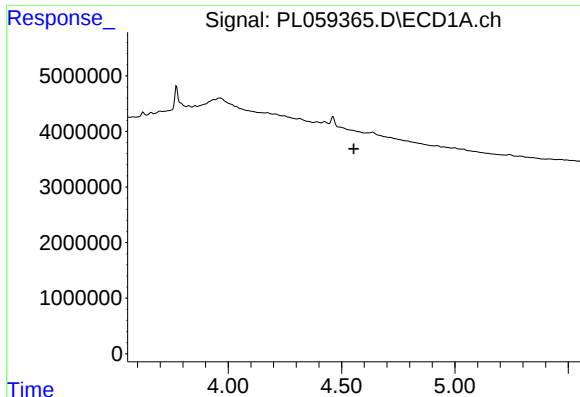

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RO-25

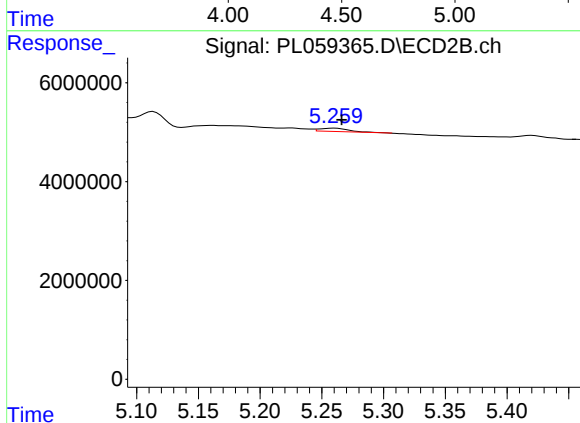


#4 Heptachlor

R.T.: 5.260 min
Delta R.T.: -0.006 min
Response: 538735
Conc: 0.16 ng/ml

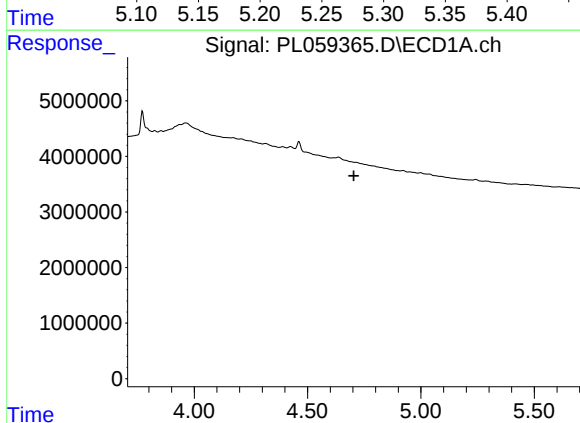


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

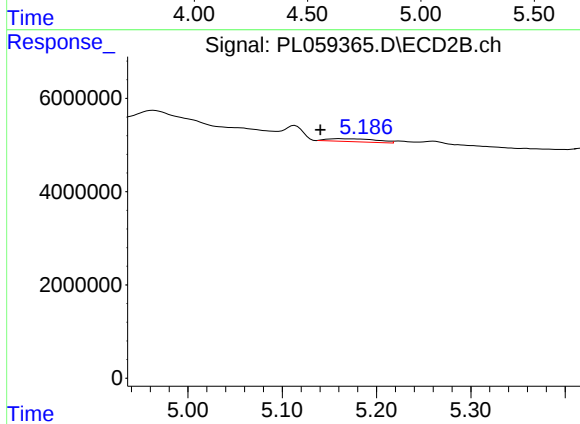

#7 delta-BHC


R.T.: 5.161 min
Delta R.T.: 0.021 min
Response: 2299010
Conc: 0.82 ng/ml

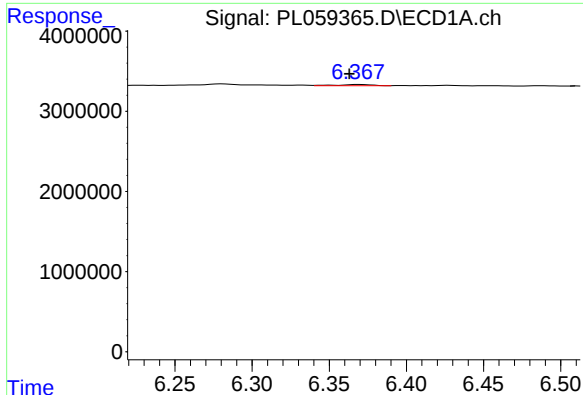

#15 Endosulfan II


R.T.: 6.368 min
Delta R.T.: 0.005 min
Response: 247236
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-25

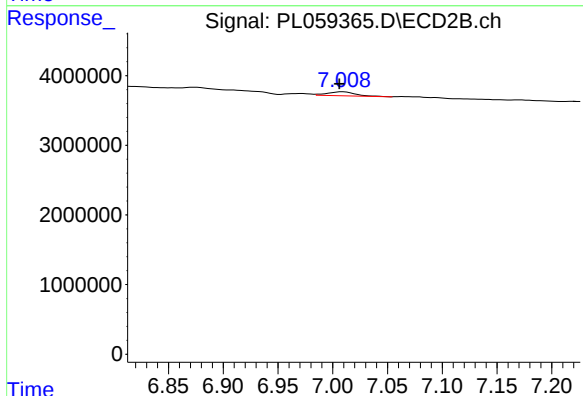


#15 Endosulfan II

R.T.: 7.009 min
Delta R.T.: 0.003 min
Response: 999438
Conc: 0.38 ng/ml

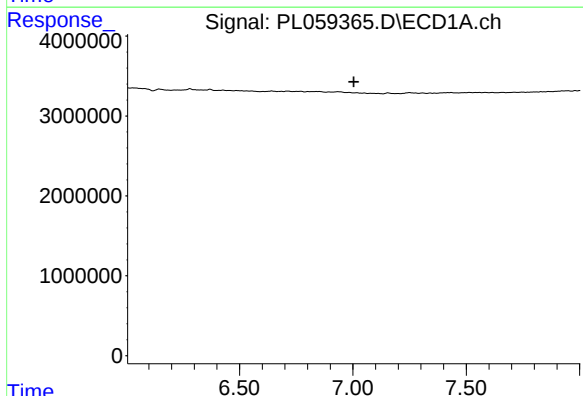


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.003 min
Response: 0
Conc: N.D.

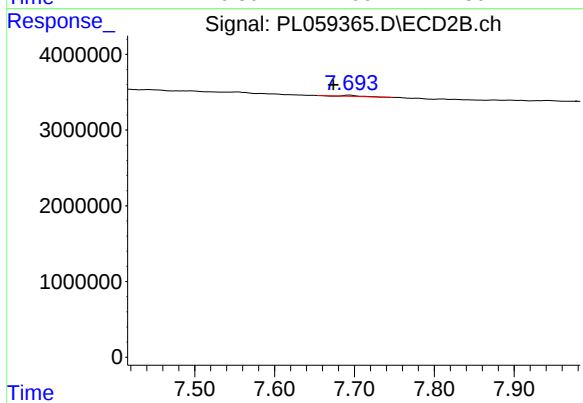

#20 Methoxychlor


R.T.: 7.694 min
Delta R.T.: 0.020 min
Response: 196477
Conc: 0.15 ng/ml

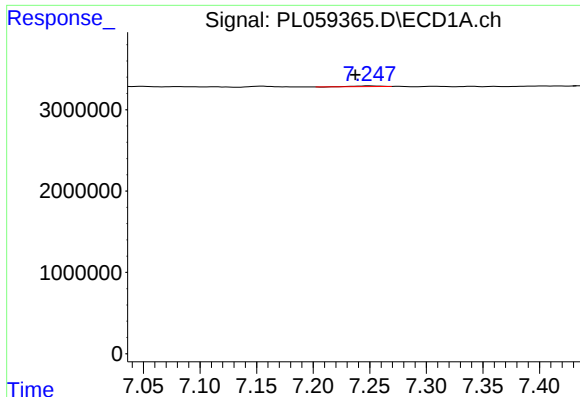

#21 Endrin ketone


R.T.: 7.250 min
Delta R.T.: 0.012 min
Response: 96360
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-25

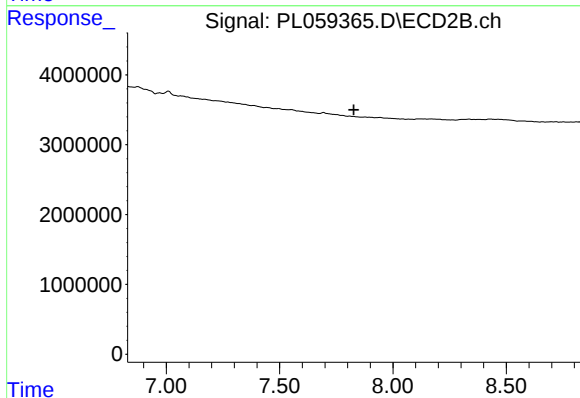


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.828 min
Response: 0
Conc: N.D.

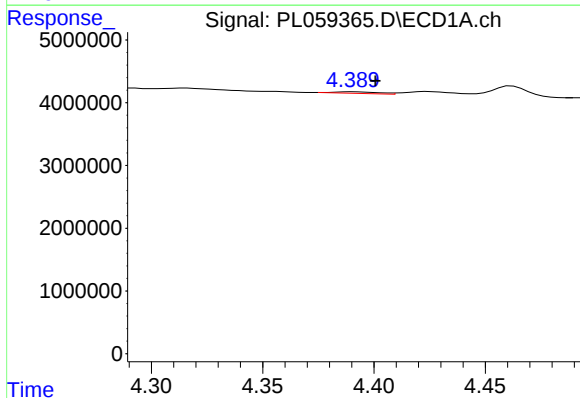


#23 Chlordane-1

R.T.: 4.390 min
Delta R.T.: -0.010 min
Response: 369676
Conc: 7.35 ng/ml

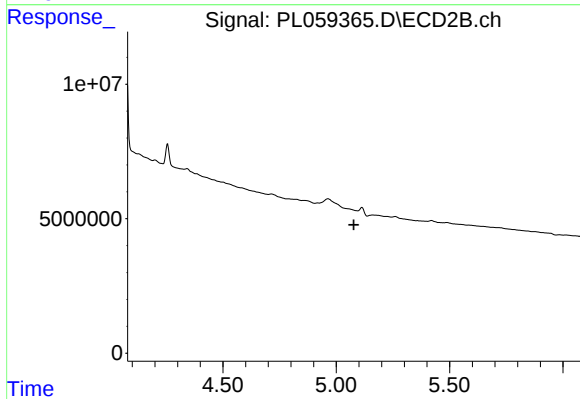

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.077 min
Response: 0
Conc: N.D.

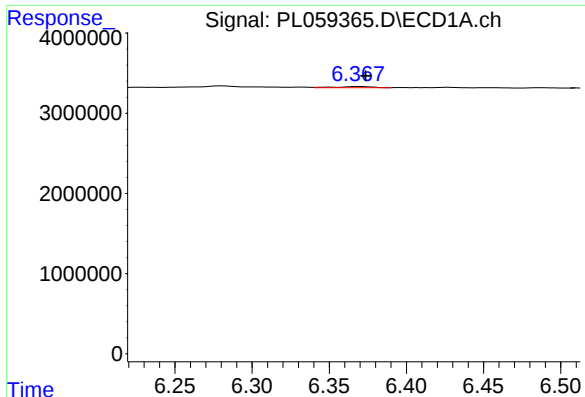

#27 Chlordane-5


R.T.: 6.368 min
Delta R.T.: -0.005 min
Response: 247236
Conc: 4.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
RO-25

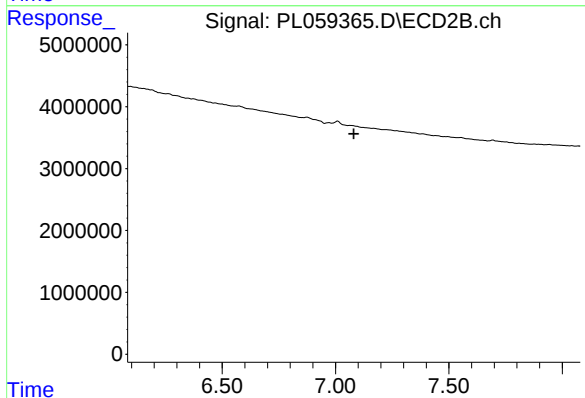


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

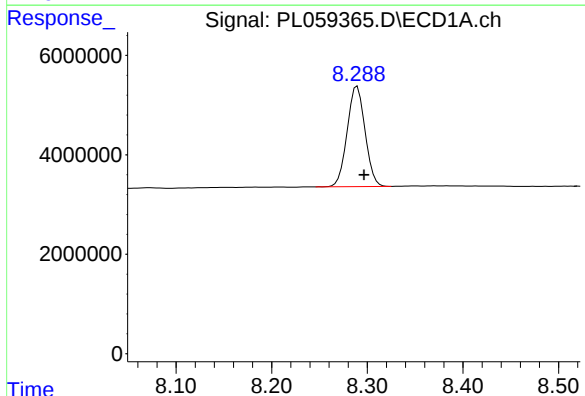

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 26366592
Conc: 16.03 ng/ml

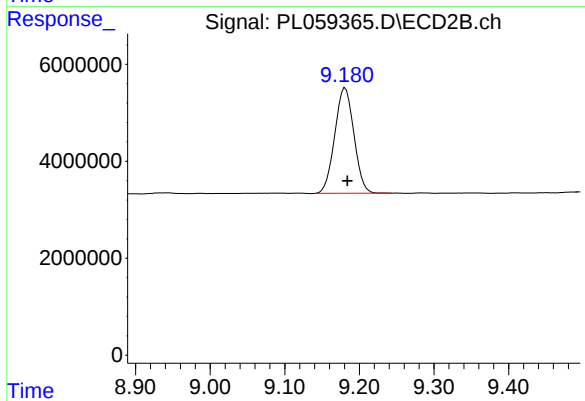

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 38778448
Conc: 16.36 ng/ml