

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
 Data File : PL059367.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 00:36
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:19:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.519	4.072	39445942	61308820	22.843	23.563
28)	SA Decachlor...	8.290	9.182	36662273	54114033	22.295	22.828
Target Compounds							
2)	A alpha-BHC	3.970	0.000	1102728	0	0.441	N.D. #
4)	MA Heptachlor	0.000	5.259	0	480271	N.D.	0.139 #
7)	B delta-BHC	0.000	5.111f	0	975351	N.D.	0.348 #
8)	B Heptachlo...	0.000	5.951	0	3194518	N.D.	1.153 #
15)	B Endosulfa...	0.000	7.007	0	594202	N.D.	0.228 #
23)	Chlordane-1	4.420f	0.000	937152	0	18.631	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061820\
Data File : PL059367.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 00:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:19:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

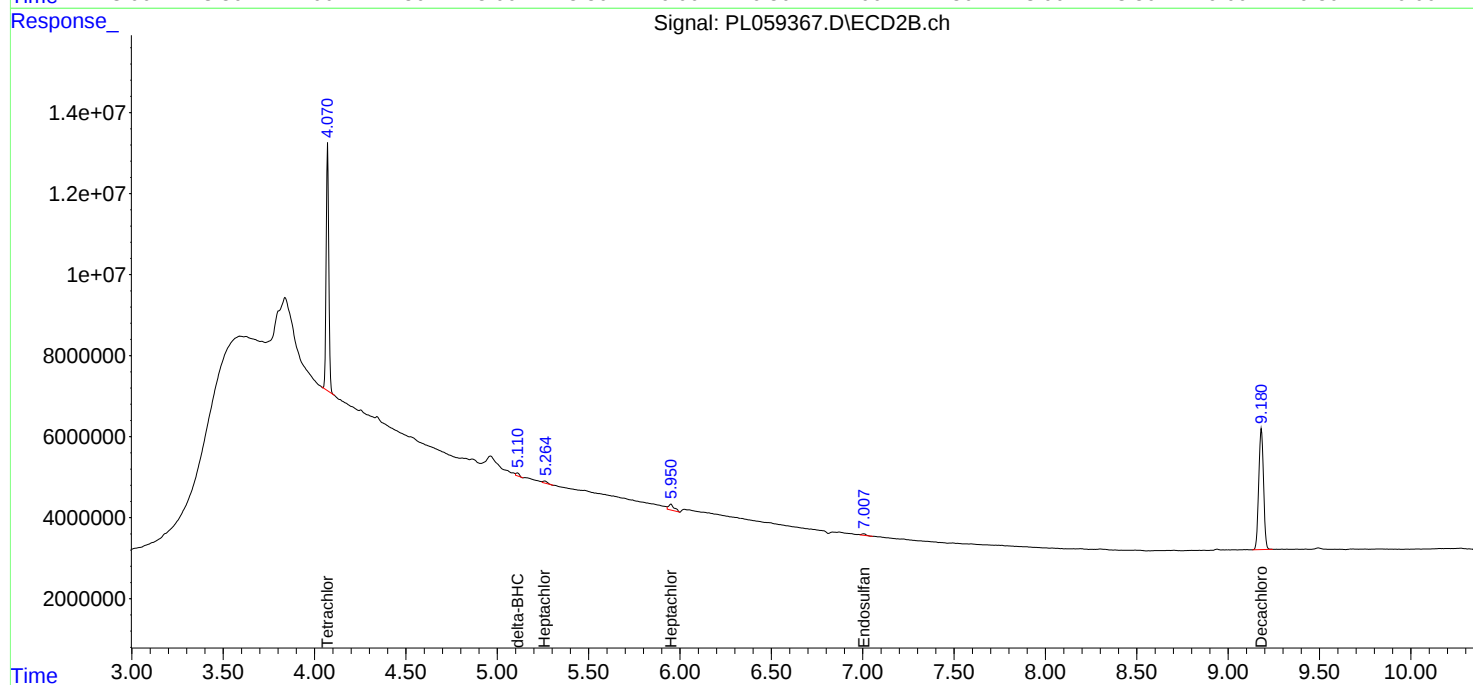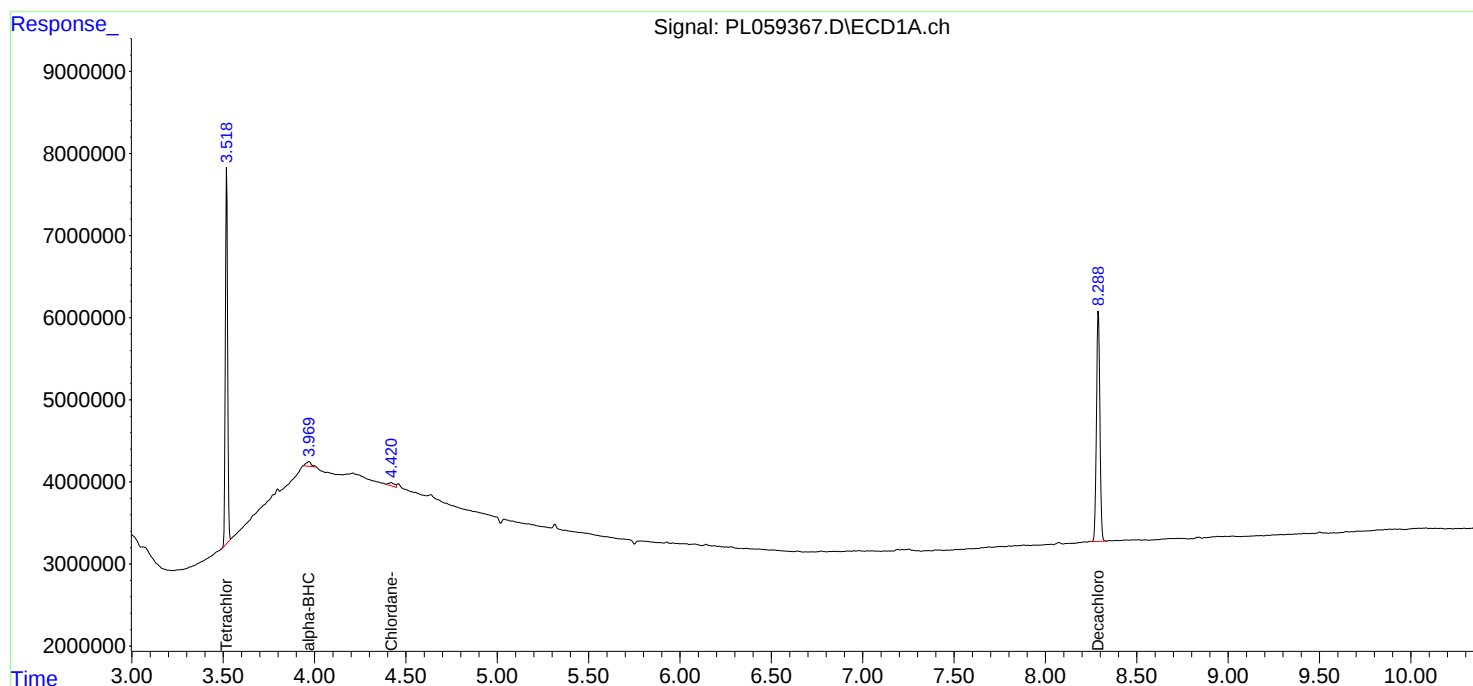


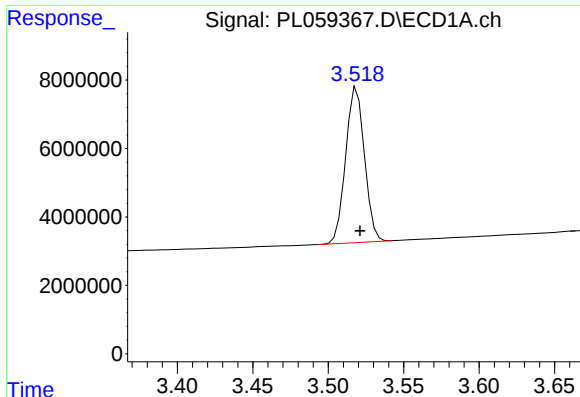

#1 Tetrachloro-m-xylene


R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 39445942
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

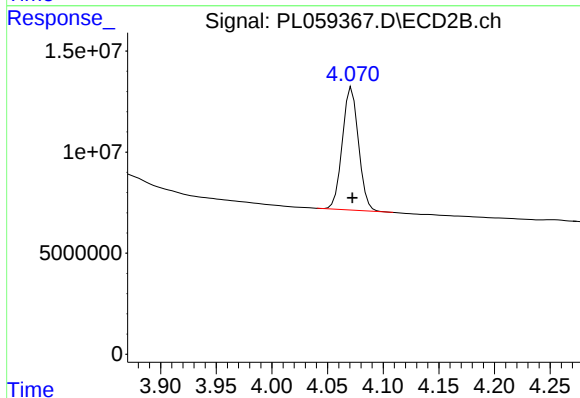


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 61308820
Conc: 23.56 ng/ml

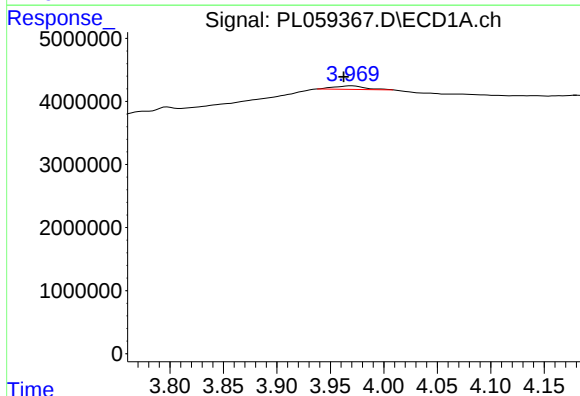


#2 alpha-BHC

R.T.: 3.970 min
Delta R.T.: 0.007 min
Response: 1102728
Conc: 0.44 ng/ml

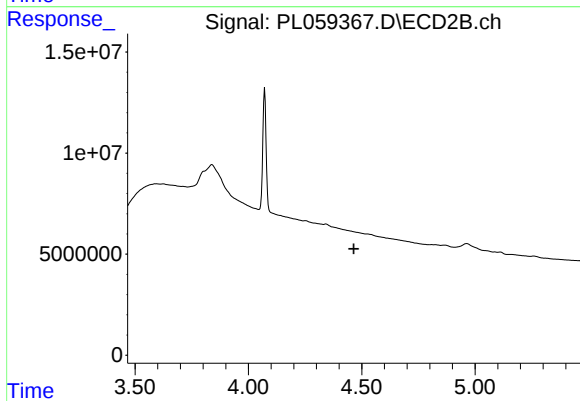

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

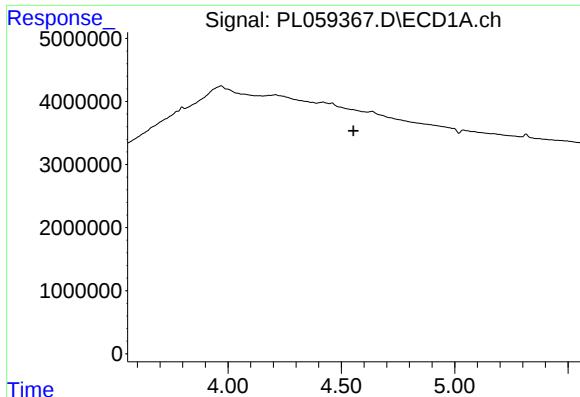

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.554 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

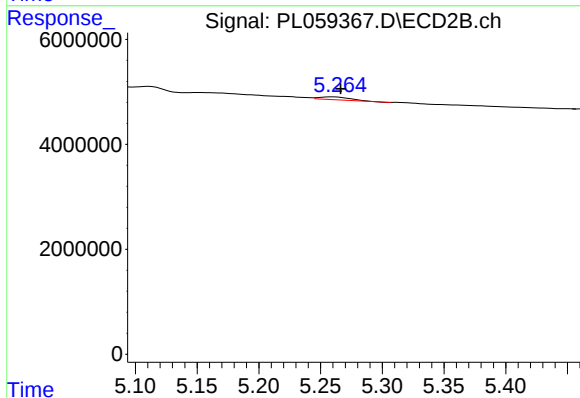


#4 Heptachlor

R.T.: 5.259 min
Delta R.T.: -0.007 min
Response: 480271
Conc: 0.14 ng/ml

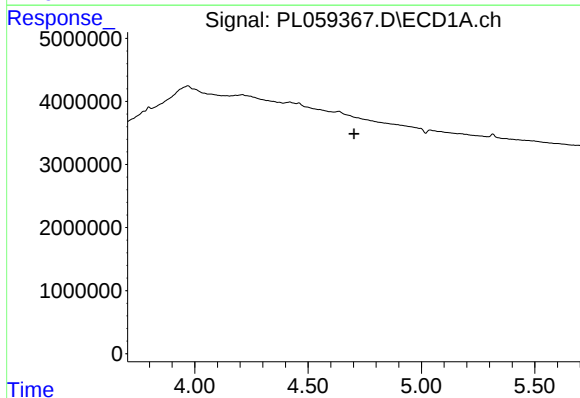


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

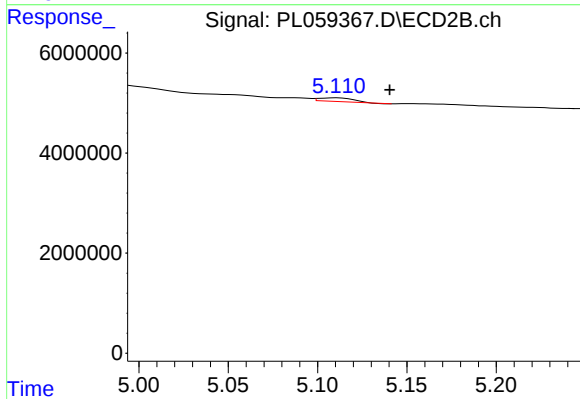

#7 delta-BHC


R.T.: 5.111 min
Delta R.T.: -0.029 min
Response: 975351
Conc: 0.35 ng/ml

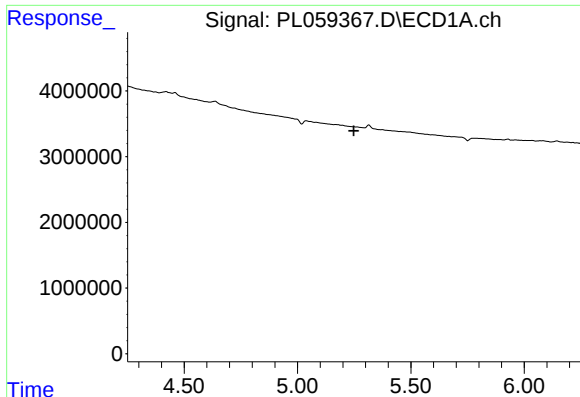

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

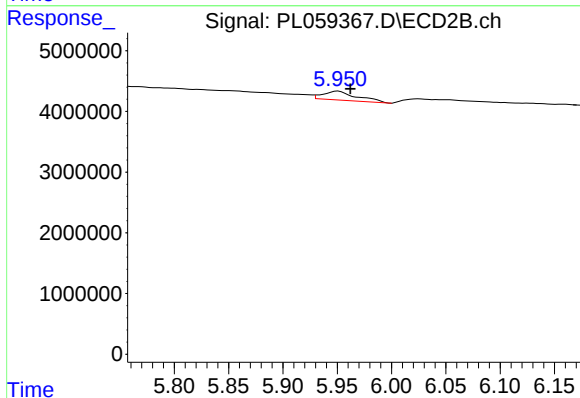


#8 Heptachlor epoxide

R.T.: 5.951 min
Delta R.T.: -0.011 min
Response: 3194518
Conc: 1.15 ng/ml

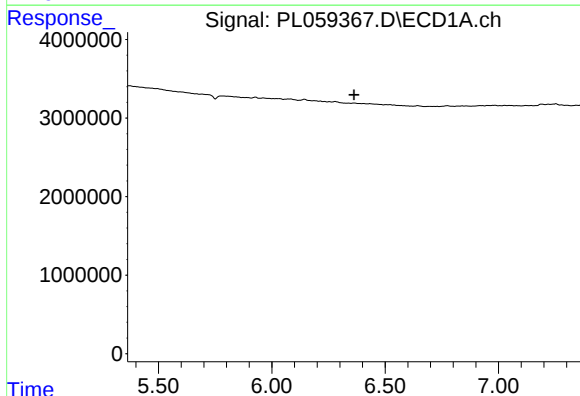


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.363 min
Response: 0
Conc: N.D.

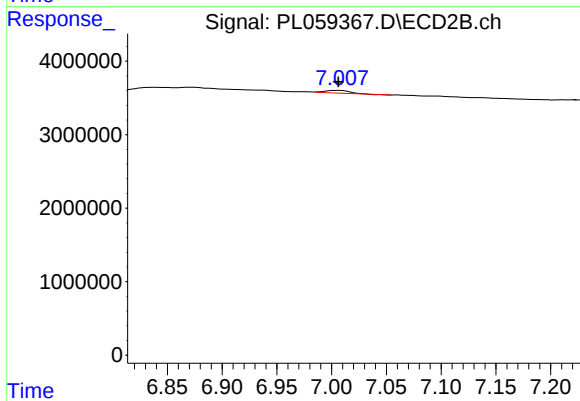

#15 Endosulfan II


R.T.: 7.007 min
Delta R.T.: 0.000 min
Response: 594202
Conc: 0.23 ng/ml

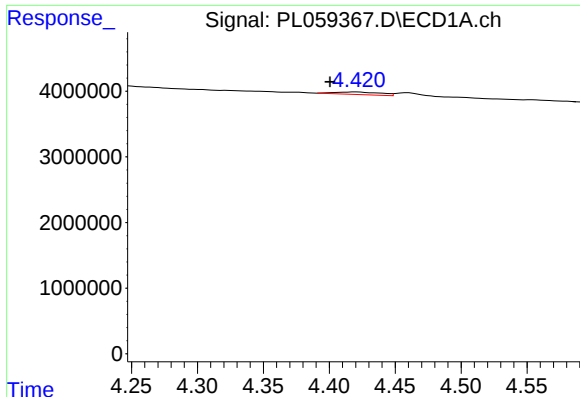

#23 Chlordane-1


R.T.: 4.420 min
Delta R.T.: 0.020 min
Response: 937152
Conc: 18.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

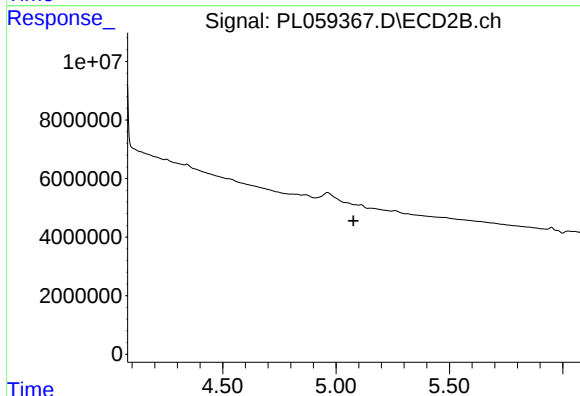


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.077 min
Response: 0
Conc: N.D.

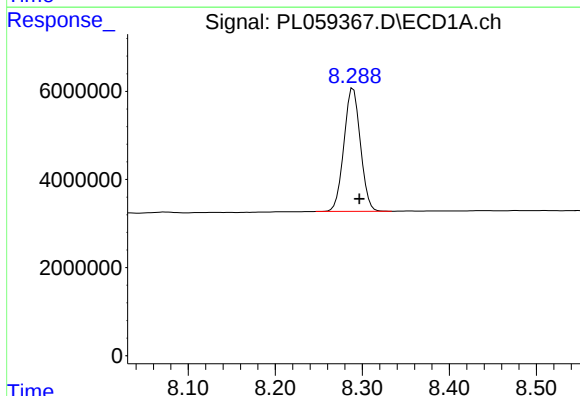

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 36662273
Conc: 22.30 ng/ml

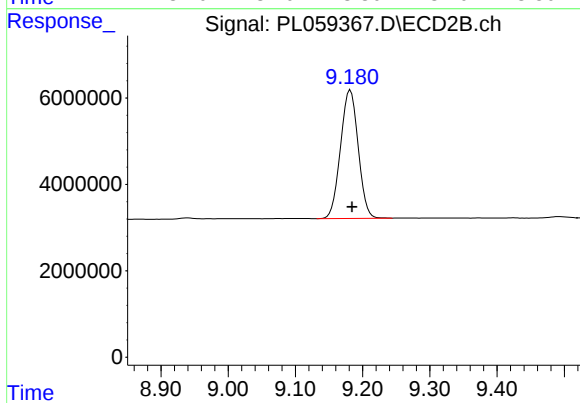

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: -0.002 min
Response: 54114033
Conc: 22.83 ng/ml