

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 09:25
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:30:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	28085820	49529728	51.085	52.538
28)	SA Decachlor...	10.219	11.426	33418649	49222206	47.156	49.417
Target Compounds							
2)	A alpha-BHC	5.177	6.109	40471558	67162564	55.026	54.318
3)	MA gamma-BHC...	5.596	6.505	38455127	63612737	51.313	53.956
4)	MA Heptachlor	6.007	7.152	38189082	59332694	50.628	53.202
5)	MB Aldrin	6.329	7.522	38016045	56624174	51.667	52.316
6)	B beta-BHC	5.980	6.759	18174371	29464299	50.794	54.261
7)	B delta-BHC	6.236	7.026	38686586	63456759	52.380	53.982
8)	B Heptachlo...	6.903	7.987	35994016	51734537	51.445	51.643
9)	A Endosulfan I	7.301	8.393	34510589	46782989	51.335	51.234
10)	B gamma-Chl...	7.181	8.257	37285240	51531395	51.427	51.038
11)	B alpha-Chl...	7.249	8.338	37469265	51096696	51.179	50.610
12)	B 4,4'-DDE	7.468	8.527	34630978	46888077	52.052	51.757
13)	MA Dieldrin	7.586	8.681	36358954	47221500	51.867	51.993
14)	MA Endrin	7.873	8.921	30170247	35441606	46.015	46.335
15)	B Endosulfa...	8.184	9.155	31257638	39689360	50.754	49.780
16)	A 4,4'-DDD	8.050	9.066	32088576	39167350	55.204	55.072
17)	MA 4,4'-DDT	8.308	9.383	25972799	33106474	44.636	45.156
18)	B Endrin al...	8.371	9.290	25632286	33073822	50.629	51.789
19)	B Endosulfa...	8.602	9.527	31798443	39962646	50.092	50.320
20)	A Methoxychlor	8.902	9.870	15844925	17599338	44.575	45.265
21)	B Endrin ke...	9.112	10.024	40432094	48784252	53.105	53.823
22)	Mirex	9.299	10.490	30900640	36935020	49.066	48.856
24)	Chlordane-2	6.485	7.522f	995895	56624174	37.190	1553.638 #
25)	Chlordane-3	7.181	8.257	37285240	51531395	554.917	385.028 #
26)	Chlordane-4	7.249	8.338	37469265	51096696	512.725	315.216 #
27)	Chlordane-5	8.184	0.000	31257638	0	1428.654	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 09:25
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:30:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

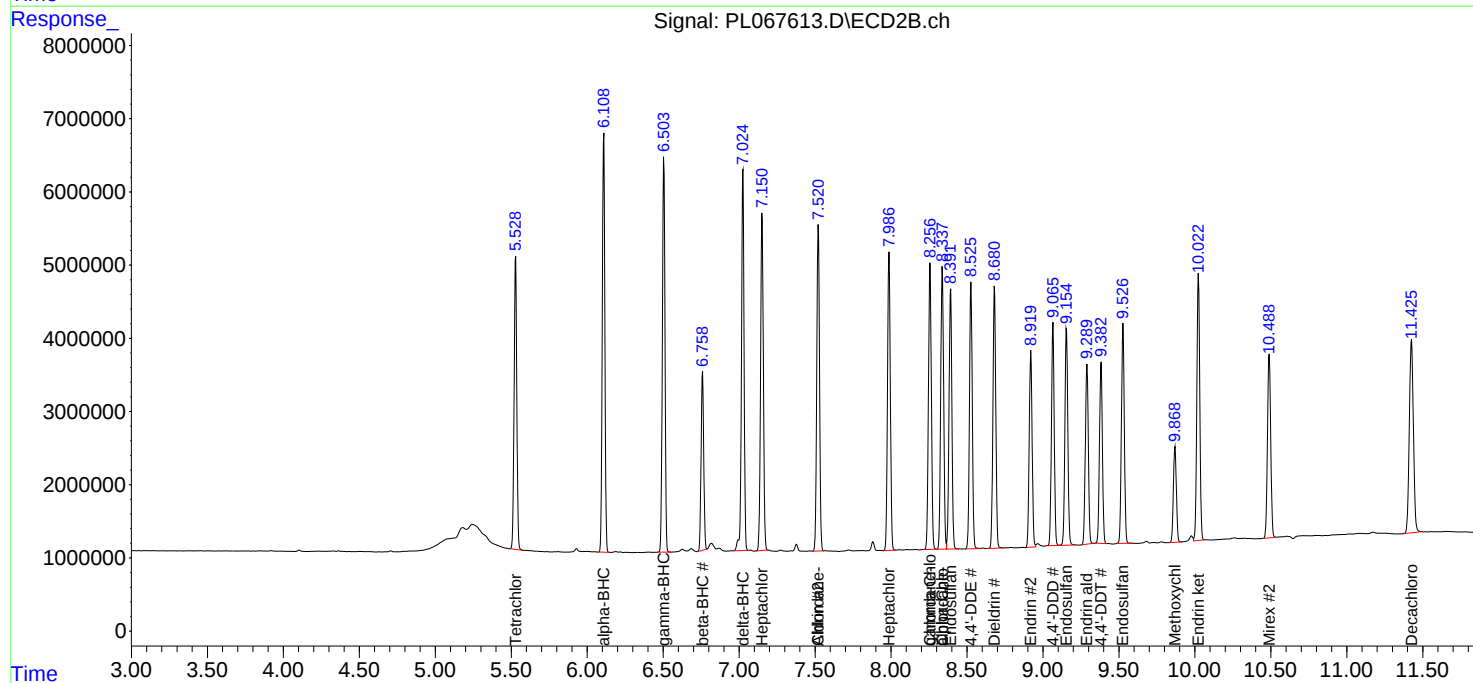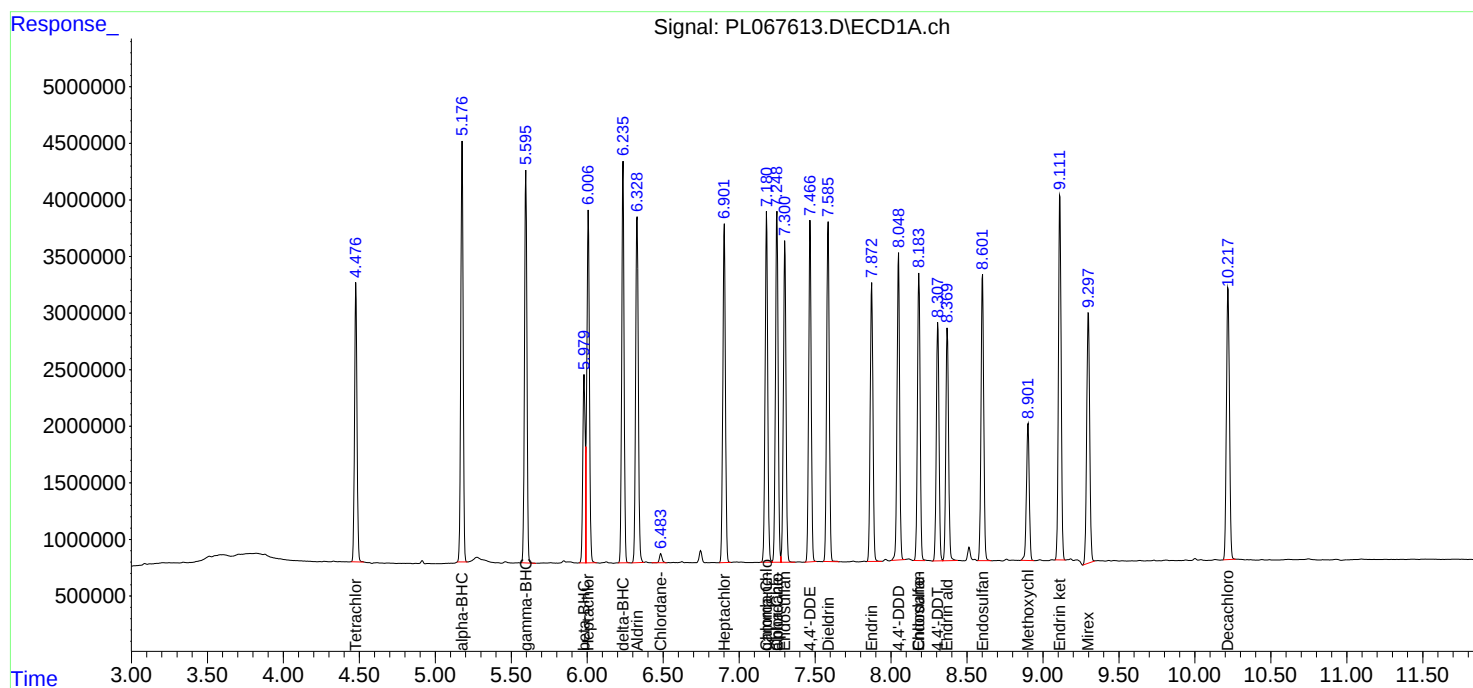


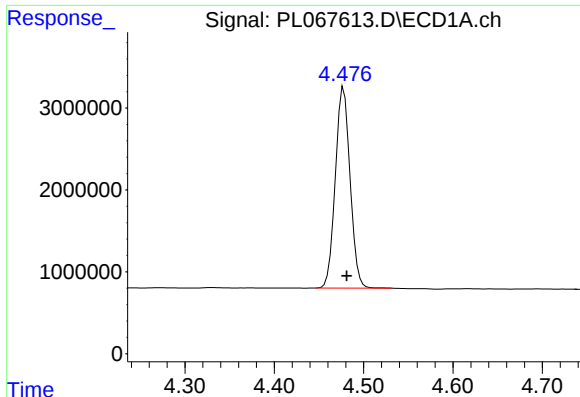

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 28085820
Conc: 51.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

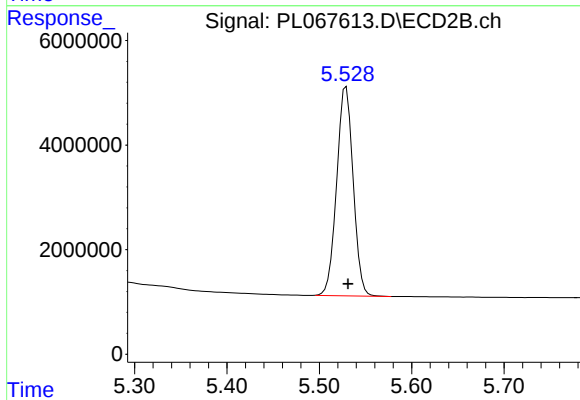


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 49529728
Conc: 52.54 ng/ml

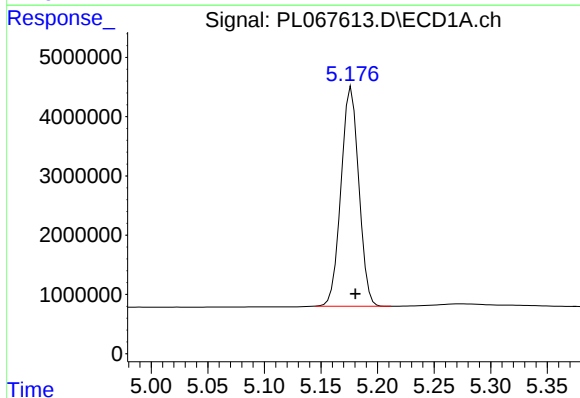


#2 alpha-BHC

R.T.: 5.177 min
Delta R.T.: -0.004 min
Response: 40471558
Conc: 55.03 ng/ml

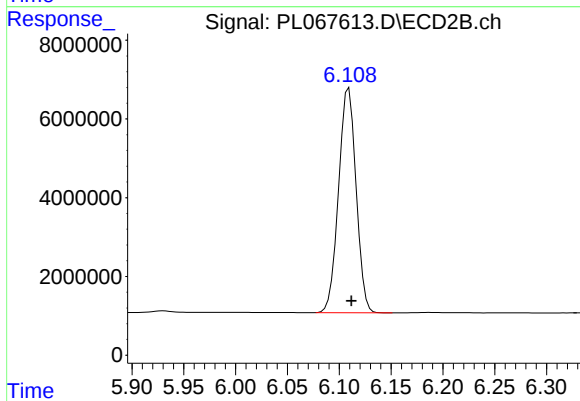

#2 alpha-BHC


R.T.: 6.109 min
Delta R.T.: -0.002 min
Response: 67162564
Conc: 54.32 ng/ml

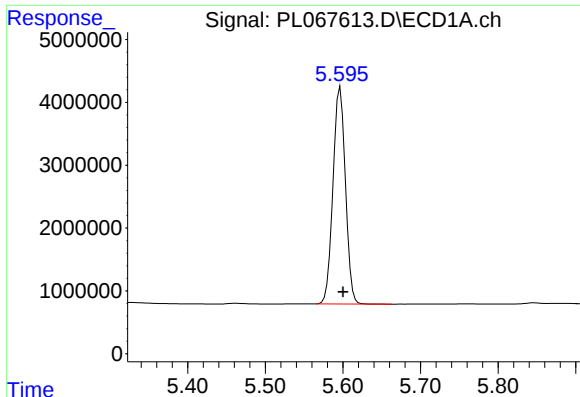

#3 gamma-BHC (Lindane)


R.T.: 5.596 min
Delta R.T.: -0.004 min
Response: 38455127
Conc: 51.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

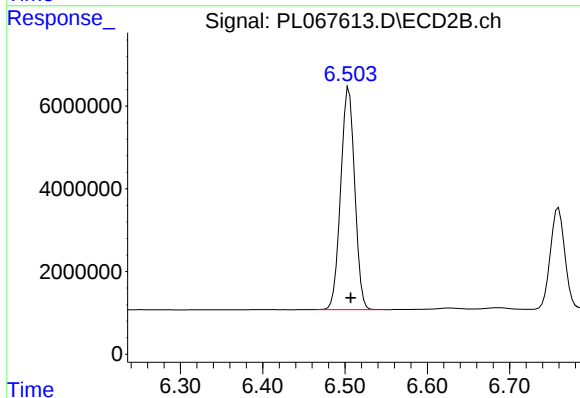


#3 gamma-BHC (Lindane)

R.T.: 6.505 min
Delta R.T.: -0.003 min
Response: 63612737
Conc: 53.96 ng/ml

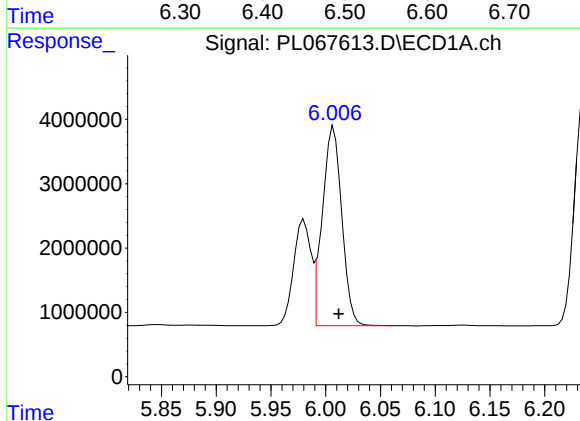


#4 Heptachlor

R.T.: 6.007 min
Delta R.T.: -0.005 min
Response: 38189082
Conc: 50.63 ng/ml

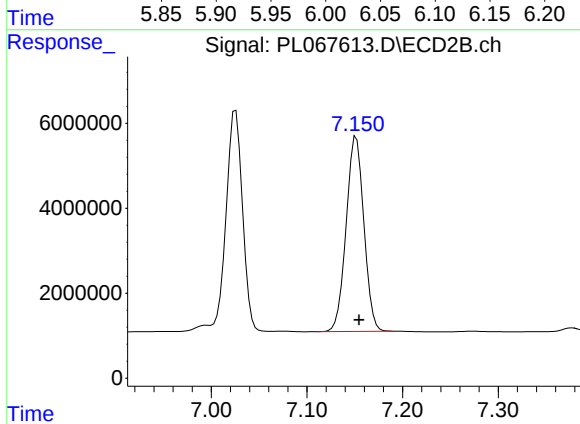

#4 Heptachlor


R.T.: 7.152 min
Delta R.T.: -0.003 min
Response: 59332694
Conc: 53.20 ng/ml

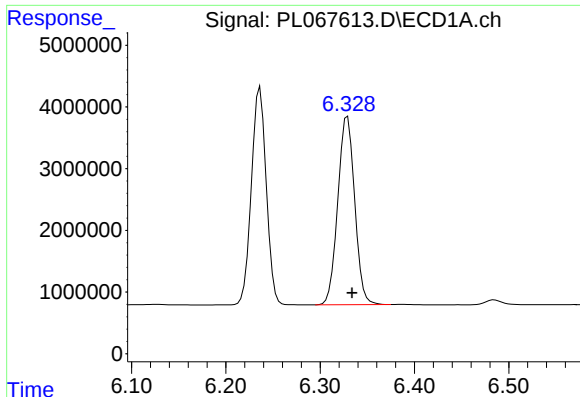

#5 Aldrin


R.T.: 6.329 min
Delta R.T.: -0.005 min
Response: 38016045
Conc: 51.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

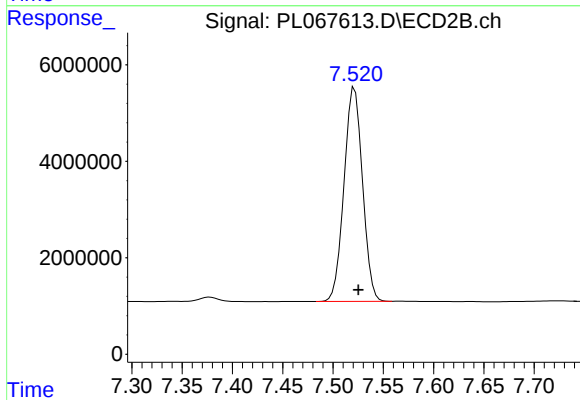


#5 Aldrin

R.T.: 7.522 min
Delta R.T.: -0.004 min
Response: 56624174
Conc: 52.32 ng/ml

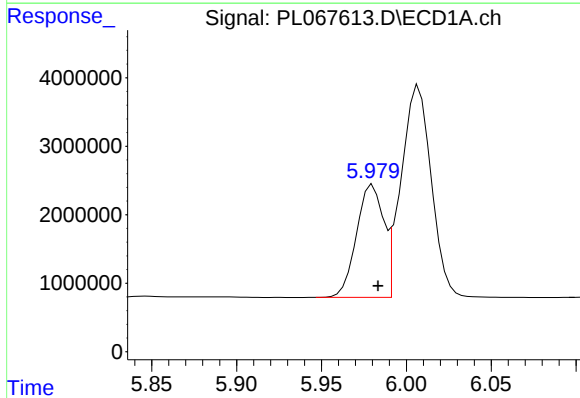


#6 beta-BHC

R.T.: 5.980 min
Delta R.T.: -0.003 min
Response: 18174371
Conc: 50.79 ng/ml

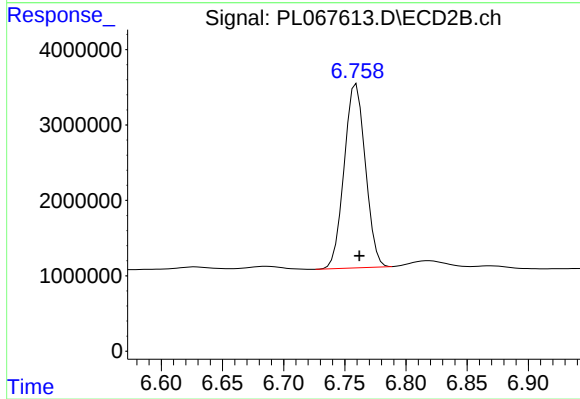

#6 beta-BHC


R.T.: 6.759 min
Delta R.T.: -0.003 min
Response: 29464299
Conc: 54.26 ng/ml

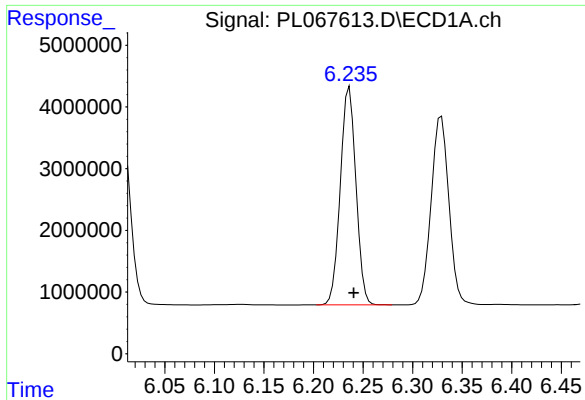

#7 delta-BHC


R.T.: 6.236 min
Delta R.T.: -0.004 min
Response: 38686586
Conc: 52.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

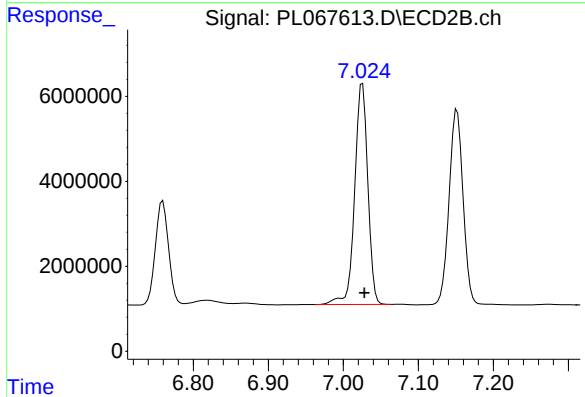


#7 delta-BHC

R.T.: 7.026 min
Delta R.T.: -0.003 min
Response: 63456759
Conc: 53.98 ng/ml

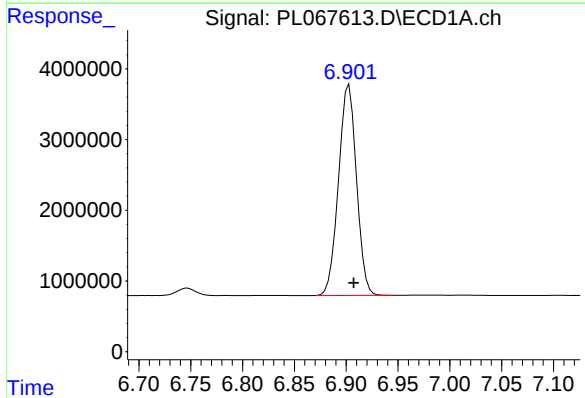


#8 Heptachlor epoxide

R.T.: 6.903 min
Delta R.T.: -0.004 min
Response: 35994016
Conc: 51.44 ng/ml

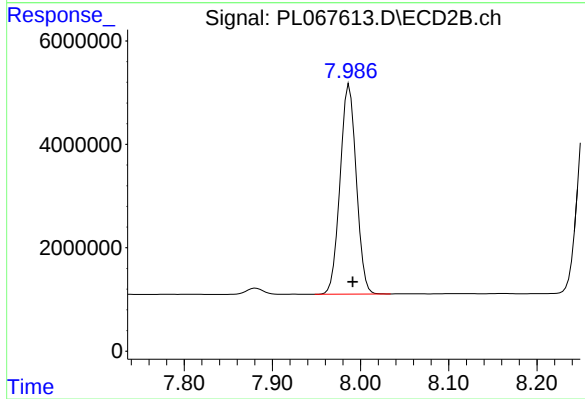

#8 Heptachlor epoxide


R.T.: 7.987 min
Delta R.T.: -0.004 min
Response: 51734537
Conc: 51.64 ng/ml

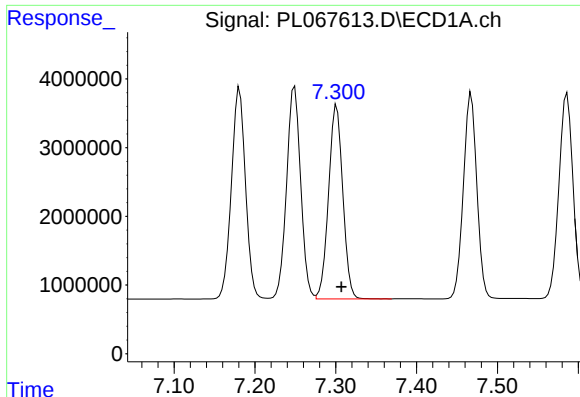

#9 Endosulfan I


R.T.: 7.301 min
Delta R.T.: -0.006 min
Response: 34510589
Conc: 51.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

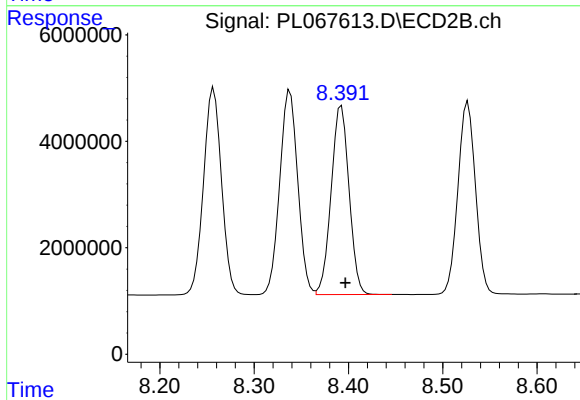


#9 Endosulfan I

R.T.: 8.393 min
Delta R.T.: -0.004 min
Response: 46782989
Conc: 51.23 ng/ml

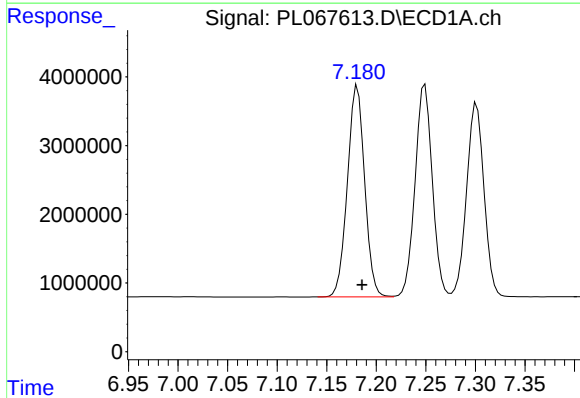


#10 gamma-Chlordane

R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 37285240
Conc: 51.43 ng/ml

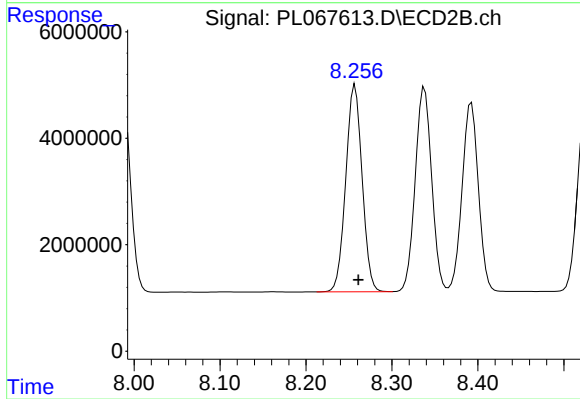

#10 gamma-Chlordane


R.T.: 8.257 min
Delta R.T.: -0.004 min
Response: 51531395
Conc: 51.04 ng/ml

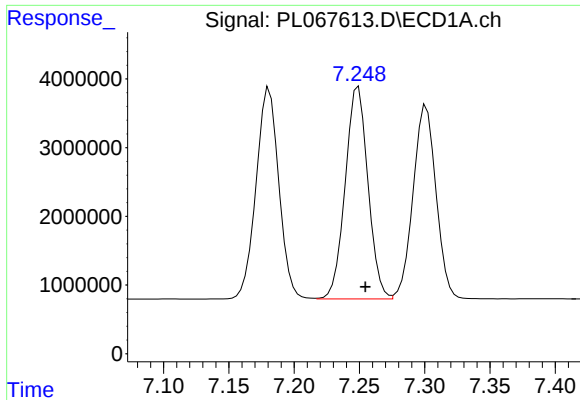

#11 alpha-Chlordane


R.T.: 7.249 min
Delta R.T.: -0.005 min
Response: 37469265
Conc: 51.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

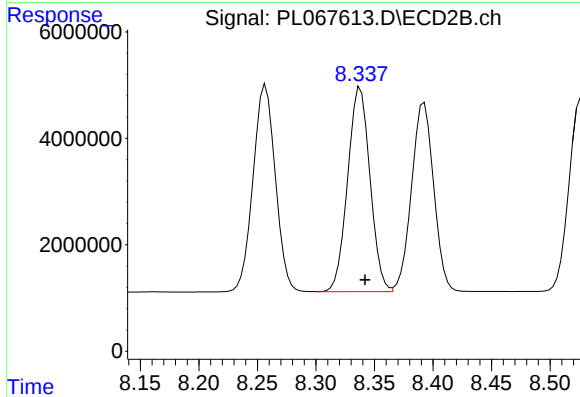


#11 alpha-Chlordane

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 51096696
Conc: 50.61 ng/ml

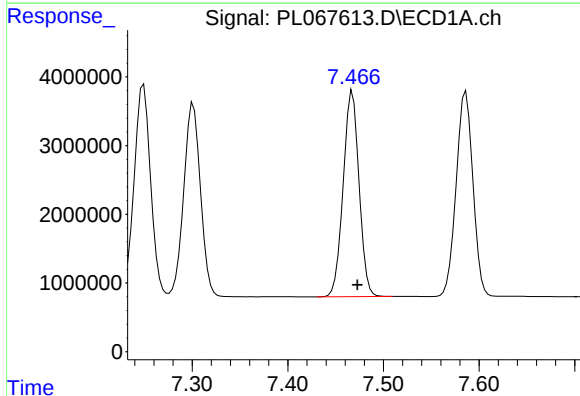


#12 4,4'-DDE

R.T.: 7.468 min
Delta R.T.: -0.005 min
Response: 34630978
Conc: 52.05 ng/ml

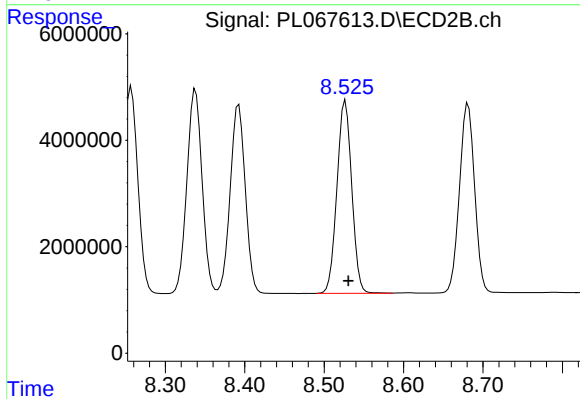

#12 4,4'-DDE


R.T.: 8.527 min
Delta R.T.: -0.004 min
Response: 46888077
Conc: 51.76 ng/ml

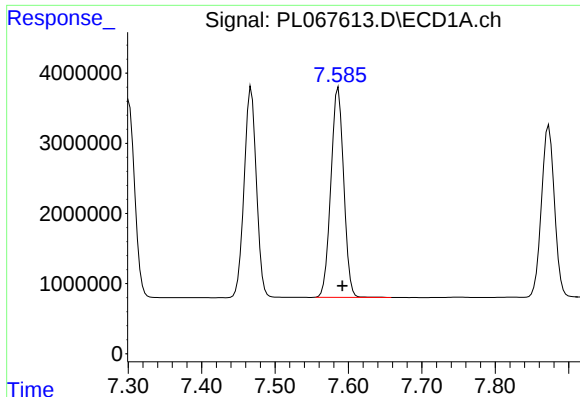

#13 Dieldrin


R.T.: 7.586 min
Delta R.T.: -0.005 min
Response: 36358954
Conc: 51.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

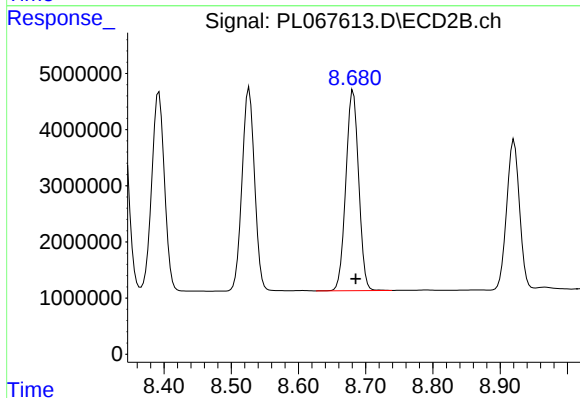


#13 Dieldrin

R.T.: 8.681 min
Delta R.T.: -0.004 min
Response: 47221500
Conc: 51.99 ng/ml

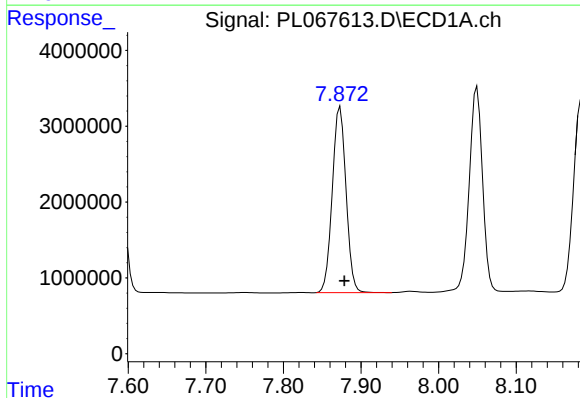


#14 Endrin

R.T.: 7.873 min
Delta R.T.: -0.005 min
Response: 30170247
Conc: 46.02 ng/ml

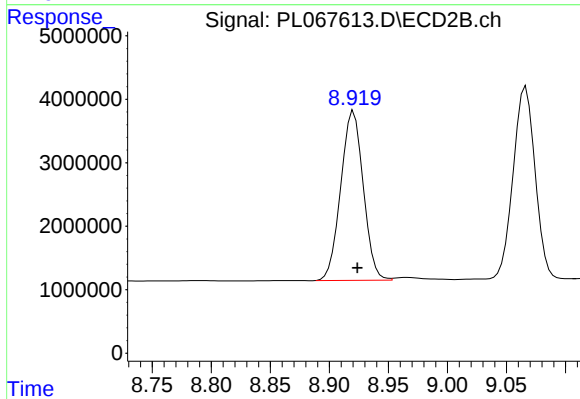

#14 Endrin


R.T.: 8.921 min
Delta R.T.: -0.003 min
Response: 35441606
Conc: 46.33 ng/ml

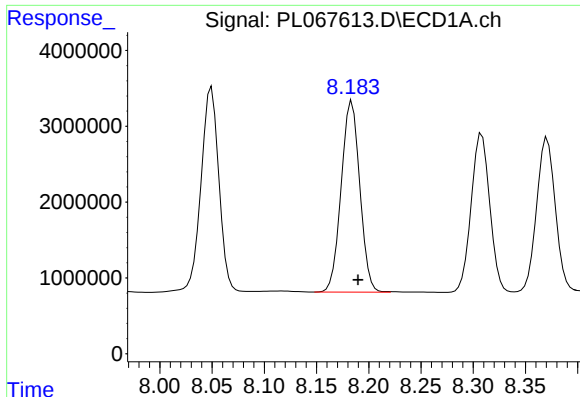

#15 Endosulfan II


R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 31257638
Conc: 50.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

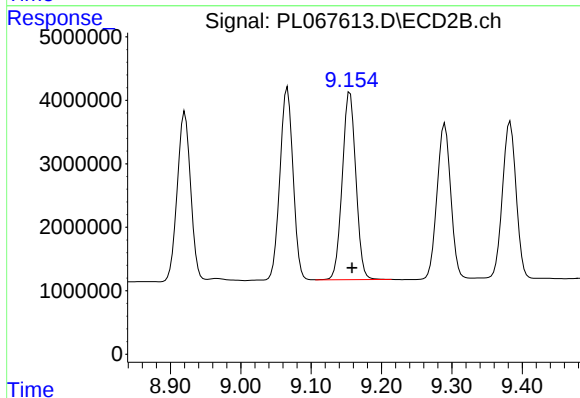


#15 Endosulfan II

R.T.: 9.155 min
Delta R.T.: -0.003 min
Response: 39689360
Conc: 49.78 ng/ml

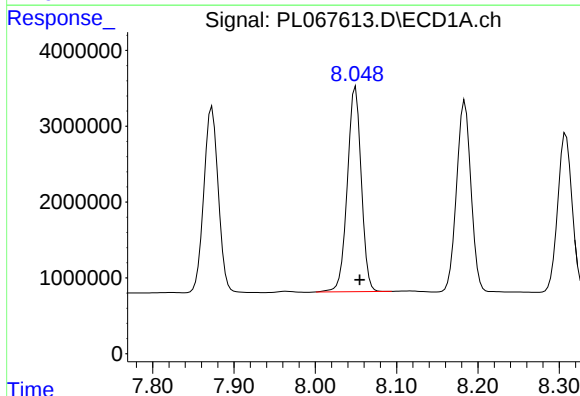


#16 4,4'-DDD

R.T.: 8.050 min
Delta R.T.: -0.005 min
Response: 32088576
Conc: 55.20 ng/ml

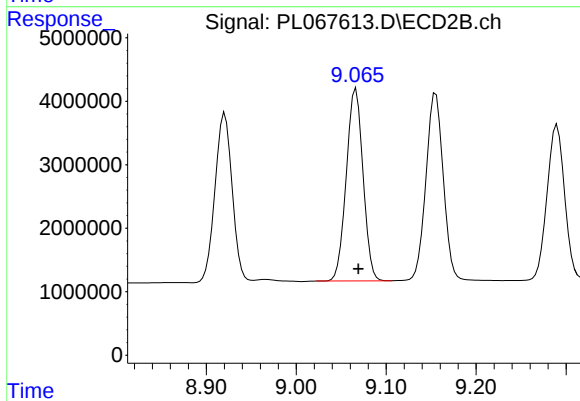

#16 4,4'-DDD


R.T.: 9.066 min
Delta R.T.: -0.003 min
Response: 39167350
Conc: 55.07 ng/ml

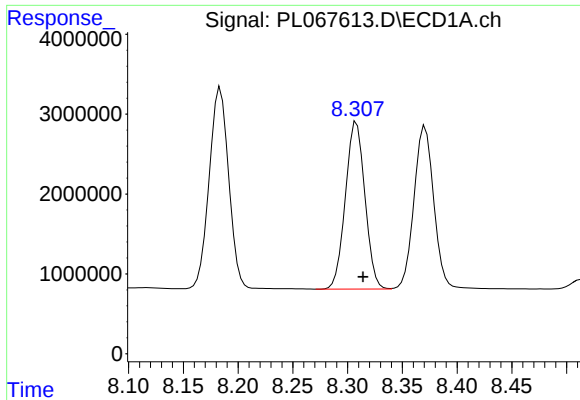

#17 4,4'-DDT


R.T.: 8.308 min
Delta R.T.: -0.006 min
Response: 25972799
Conc: 44.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

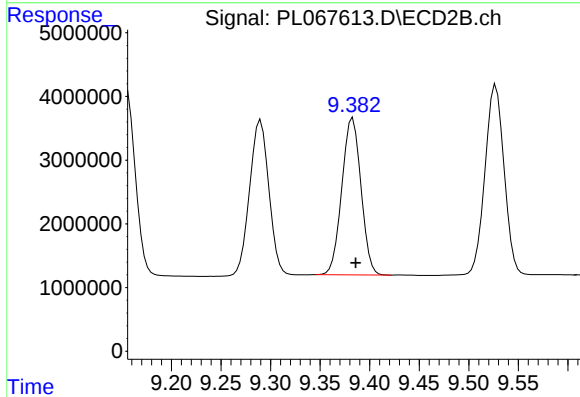


#17 4,4'-DDT

R.T.: 9.383 min
Delta R.T.: -0.003 min
Response: 33106474
Conc: 45.16 ng/ml

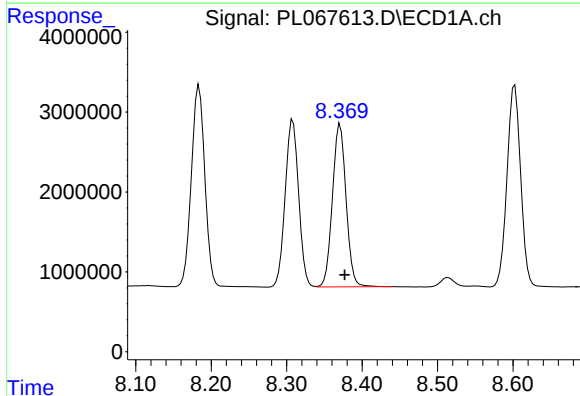


#18 Endrin aldehyde

R.T.: 8.371 min
Delta R.T.: -0.006 min
Response: 25632286
Conc: 50.63 ng/ml

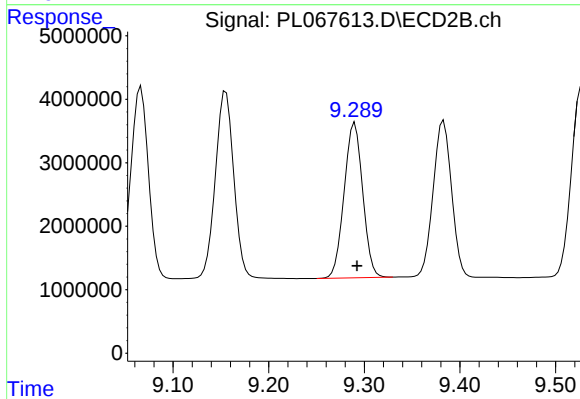

#18 Endrin aldehyde


R.T.: 9.290 min
Delta R.T.: -0.002 min
Response: 33073822
Conc: 51.79 ng/ml

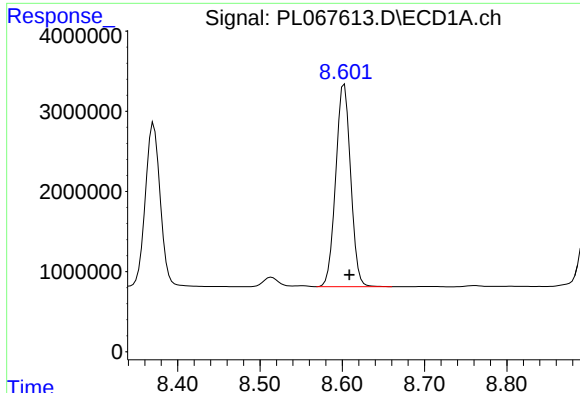

#19 Endosulfan Sulfate


R.T.: 8.602 min
Delta R.T.: -0.006 min
Response: 31798443
Conc: 50.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

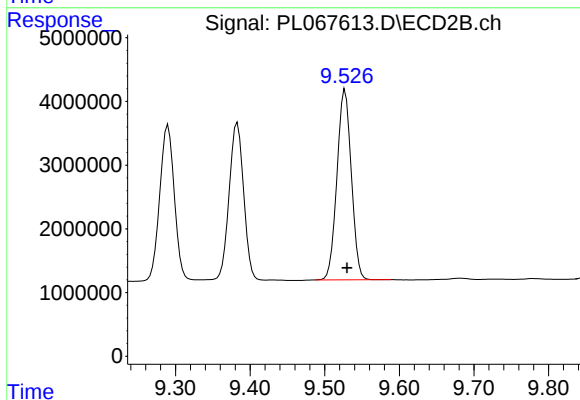


#19 Endosulfan Sulfate

R.T.: 9.527 min
Delta R.T.: -0.003 min
Response: 39962646
Conc: 50.32 ng/ml

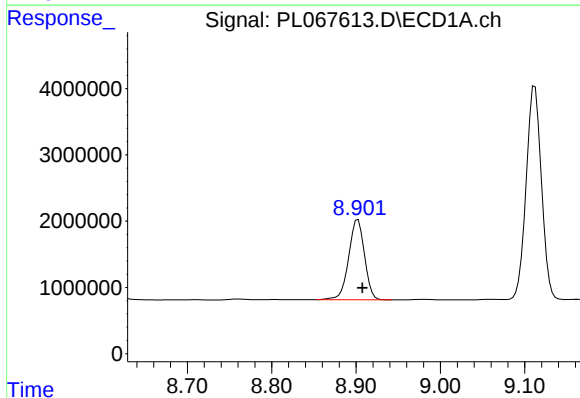


#20 Methoxychlor

R.T.: 8.902 min
Delta R.T.: -0.005 min
Response: 15844925
Conc: 44.57 ng/ml

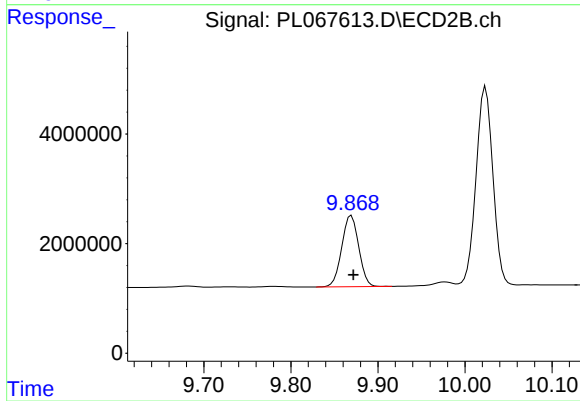

#20 Methoxychlor


R.T.: 9.870 min
Delta R.T.: -0.002 min
Response: 17599338
Conc: 45.27 ng/ml

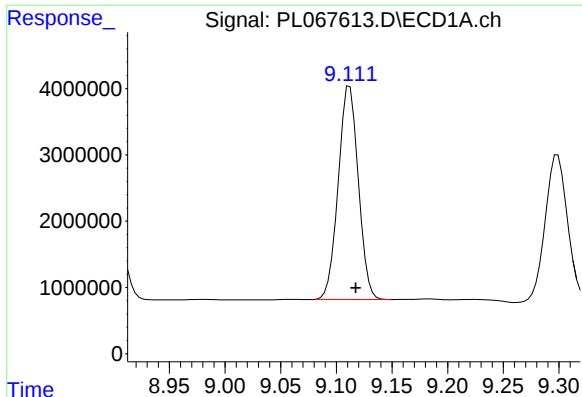

#21 Endrin ketone


R.T.: 9.112 min
Delta R.T.: -0.005 min
Response: 40432094
Conc: 53.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

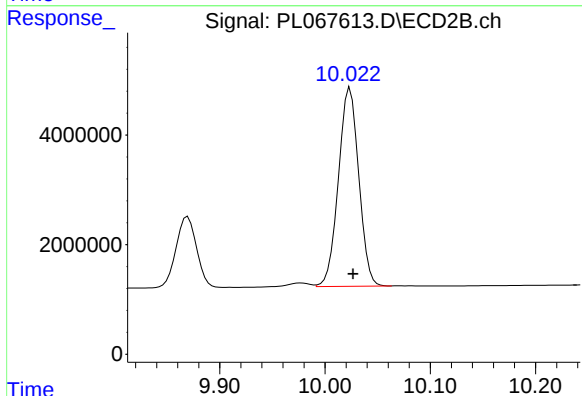


#21 Endrin ketone

R.T.: 10.024 min
Delta R.T.: -0.003 min
Response: 48784252
Conc: 53.82 ng/ml

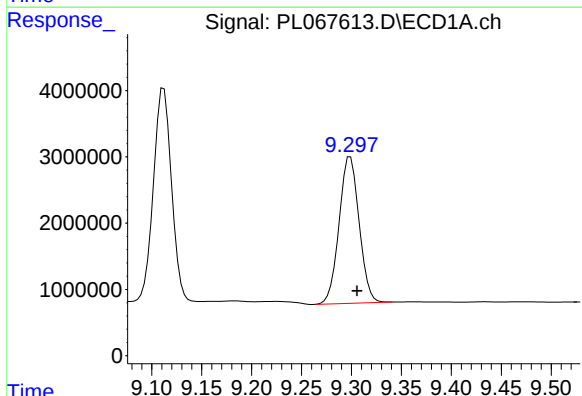


#22 Mirex

R.T.: 9.299 min
Delta R.T.: -0.007 min
Response: 30900640
Conc: 49.07 ng/ml

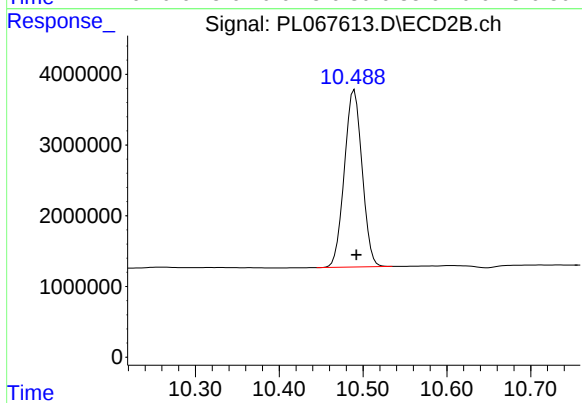

#22 Mirex


R.T.: 10.490 min
Delta R.T.: -0.003 min
Response: 36935020
Conc: 48.86 ng/ml

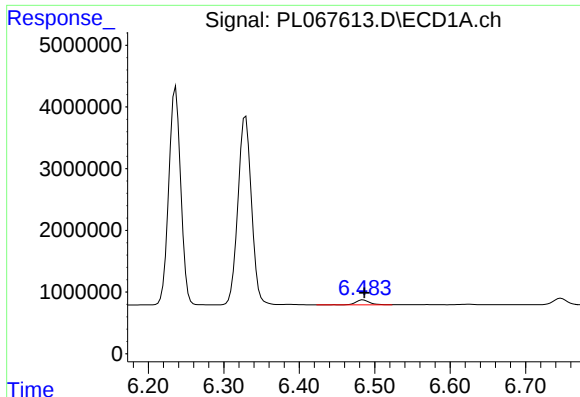

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 995895
Conc: 37.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

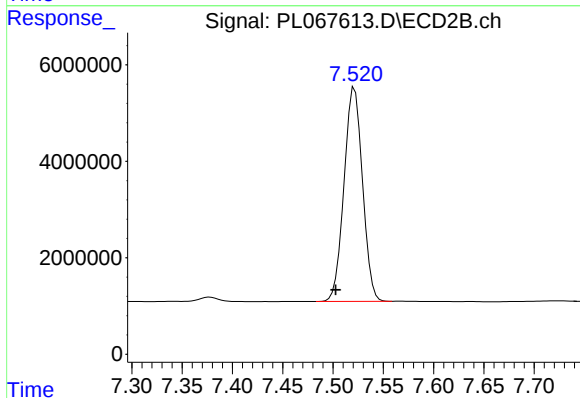


#24 Chlordane-2

R.T.: 7.522 min
Delta R.T.: 0.019 min
Response: 56624174
Conc: 1553.64 ng/ml

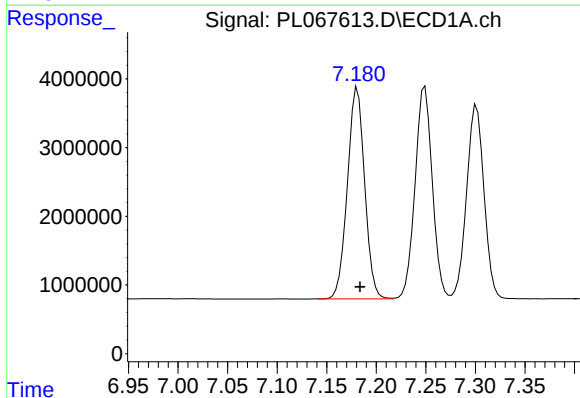


#25 Chlordane-3

R.T.: 7.181 min
Delta R.T.: -0.003 min
Response: 37285240
Conc: 554.92 ng/ml

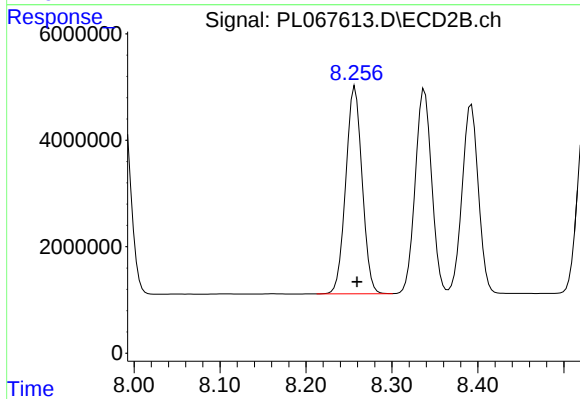

#25 Chlordane-3


R.T.: 8.257 min
Delta R.T.: -0.002 min
Response: 51531395
Conc: 385.03 ng/ml

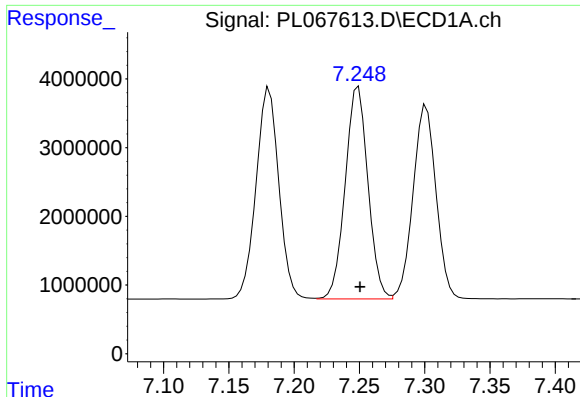

#26 Chlordane-4


R.T.: 7.249 min
Delta R.T.: -0.001 min
Response: 37469265
Conc: 512.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

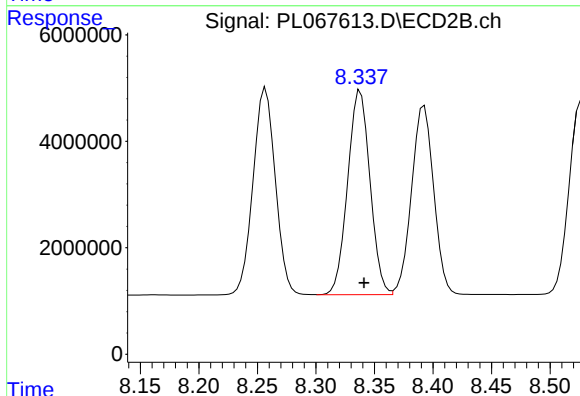


#26 Chlordane-4

R.T.: 8.338 min
Delta R.T.: -0.003 min
Response: 51096696
Conc: 315.22 ng/ml

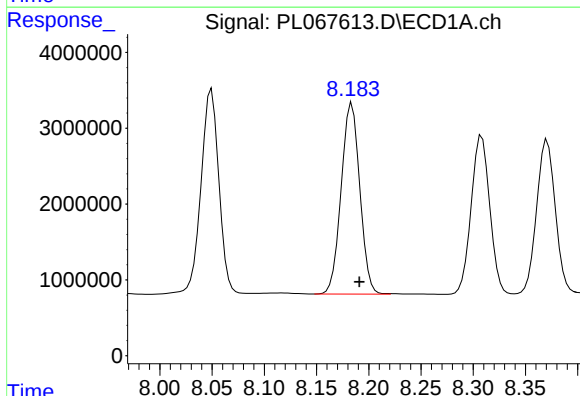


#27 Chlordane-5

R.T.: 8.184 min
Delta R.T.: -0.007 min
Response: 31257638
Conc: 1428.65 ng/ml

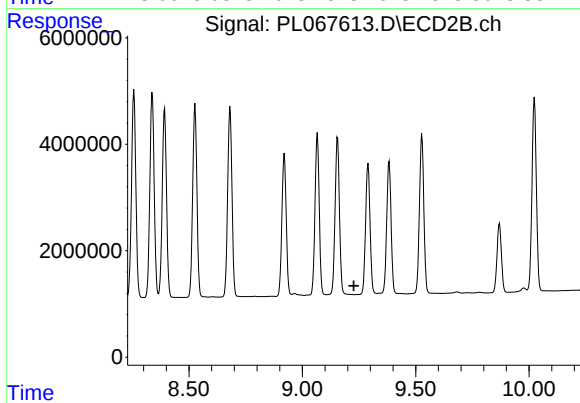

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

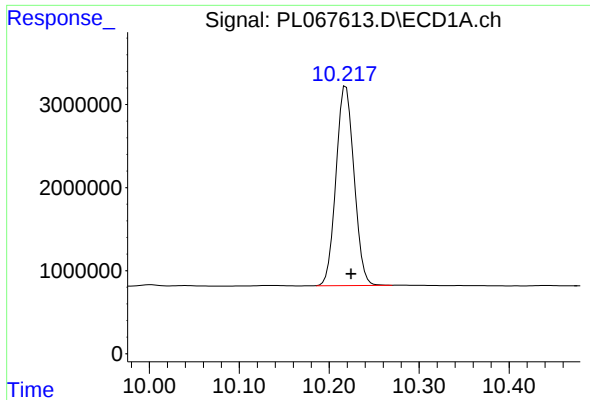

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.006 min
Response: 33418649
Conc: 47.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

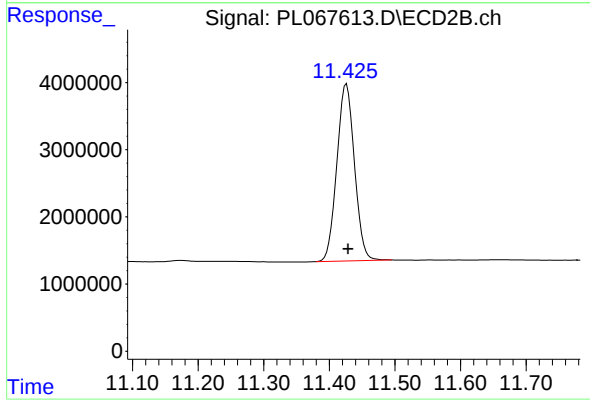

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 49222206
Conc: 49.42 ng/ml