

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 15:44
 Operator : AR\AJ
 Sample : M2709-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0224-COMP-O(DISCRETE-CL-24)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:31:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.528	10172389	18278572	18.502	19.389
28)	SA Decachlor...	10.219	11.426	11742140	16246915	16.569	16.311
Target Compounds							
6)	B beta-BHC	5.960f	0.000	147516	0	0.412	N.D. #
7)	B delta-BHC	0.000	7.000f	0	908457	N.D.	0.773 #
14)	MA Endrin	7.895f	0.000	228306	0	0.348	N.D. #
15)	B Endosulfa...	8.173f	9.177f	1383341	552929	2.246	0.694 #
19)	B Endosulfa...	8.587f	0.000	688089	0	1.084	N.D. #
21)	B Endrin ke...	0.000	10.003f	0	844226	N.D.	0.931 #
24)	Chlordane-2	6.482	0.000	346161	0	12.927	N.D. #
27)	Chlordane-5	8.173f	9.242	1383341	242913	63.227	8.354 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 15:44
Operator : AR\AJ
Sample : M2709-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:31:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

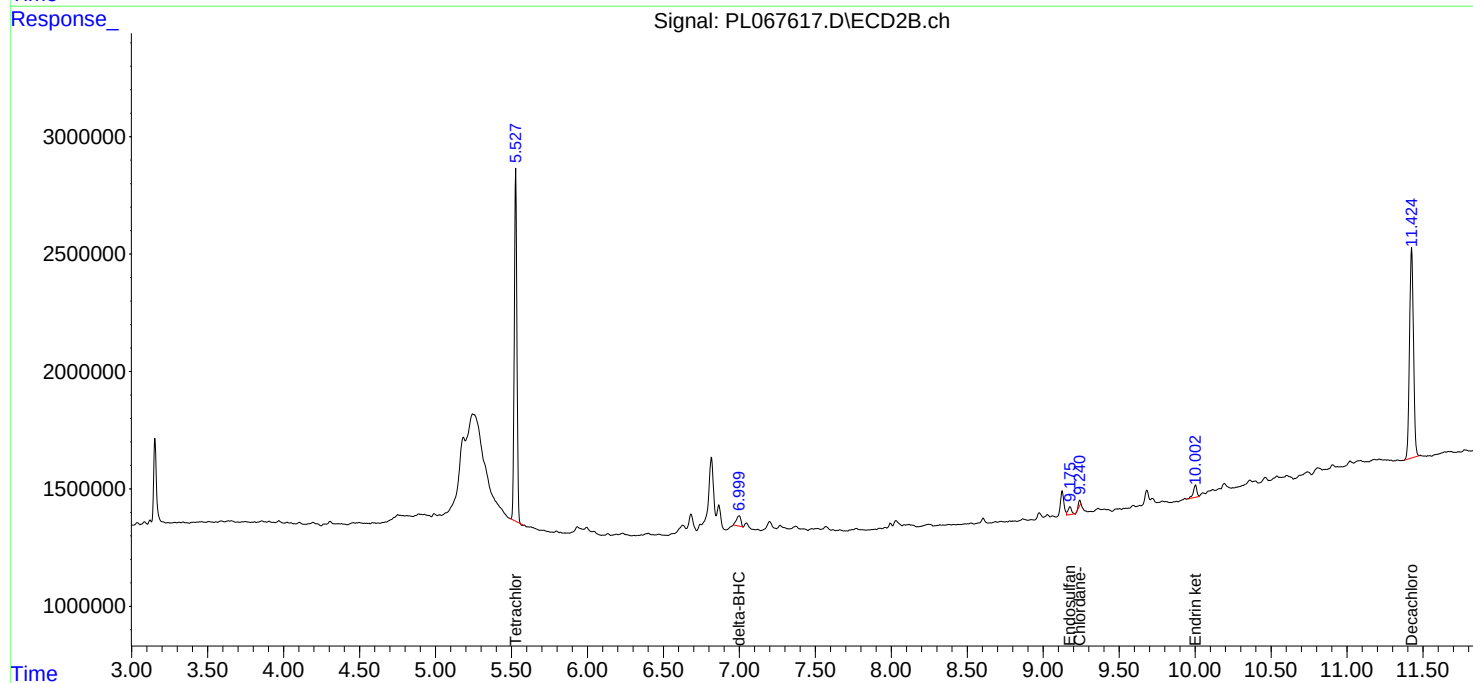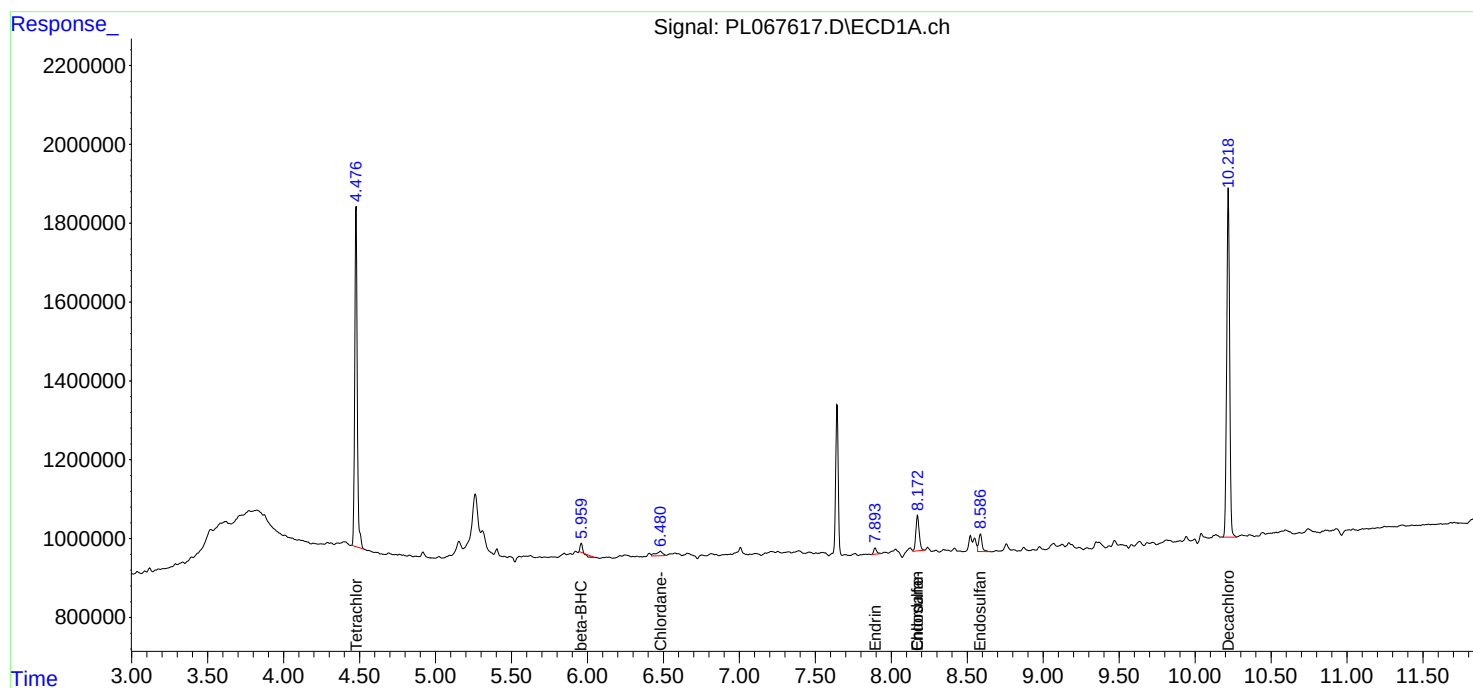


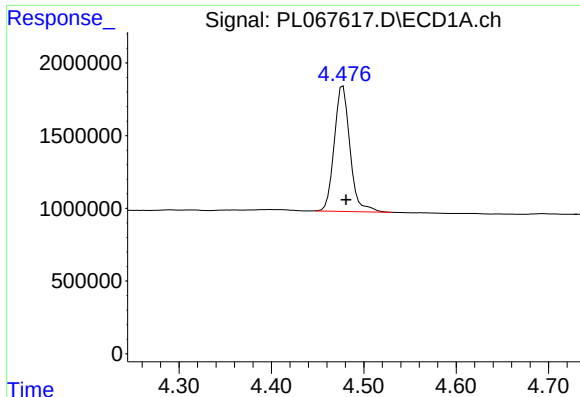

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10172389
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

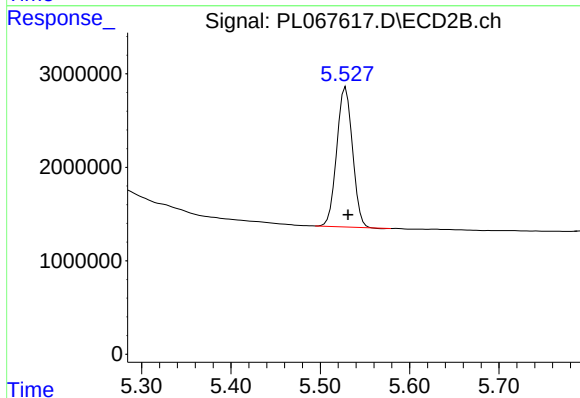


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 18278572
Conc: 19.39 ng/ml

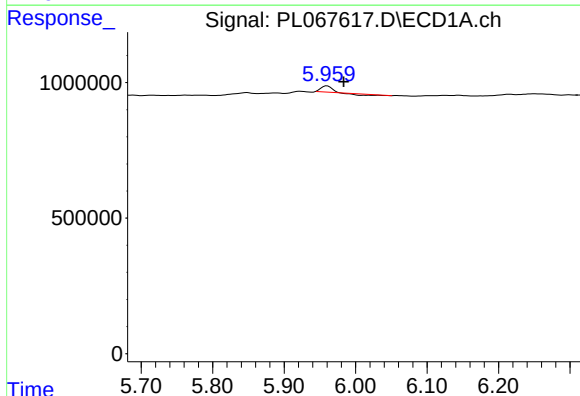


#6 beta-BHC

R.T.: 5.960 min
Delta R.T.: -0.023 min
Response: 147516
Conc: 0.41 ng/ml

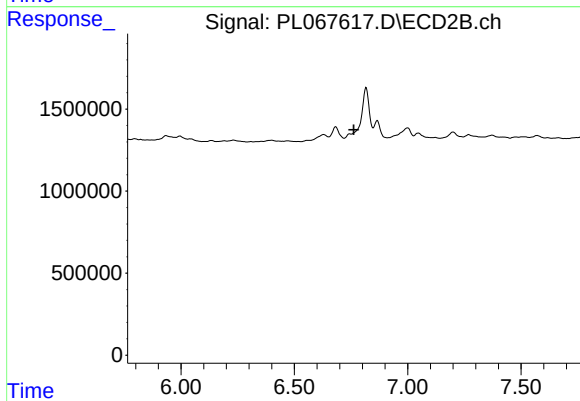

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

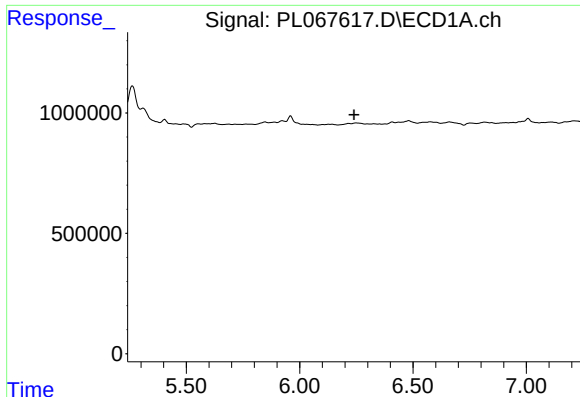

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.241 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

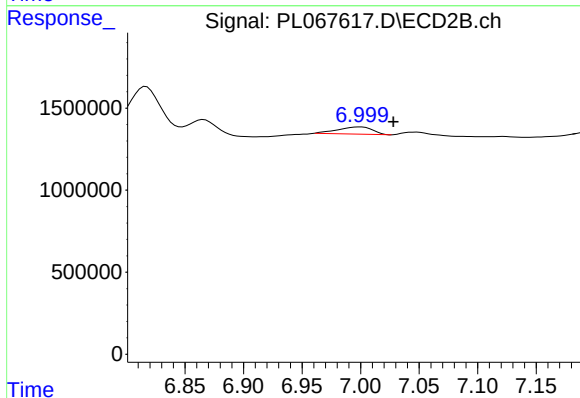


#7 delta-BHC

R.T.: 7.000 min
Delta R.T.: -0.028 min
Response: 908457
Conc: 0.77 ng/ml

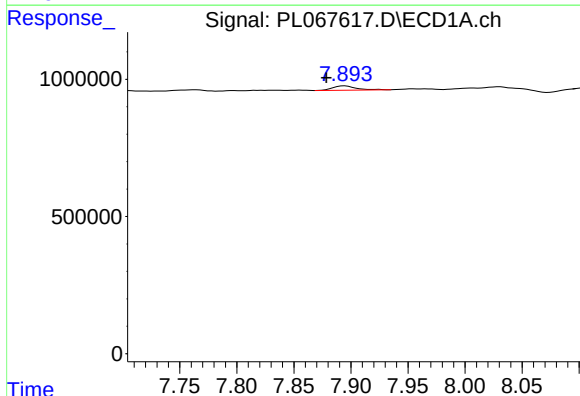


#14 Endrin

R.T.: 7.895 min
Delta R.T.: 0.016 min
Response: 228306
Conc: 0.35 ng/ml

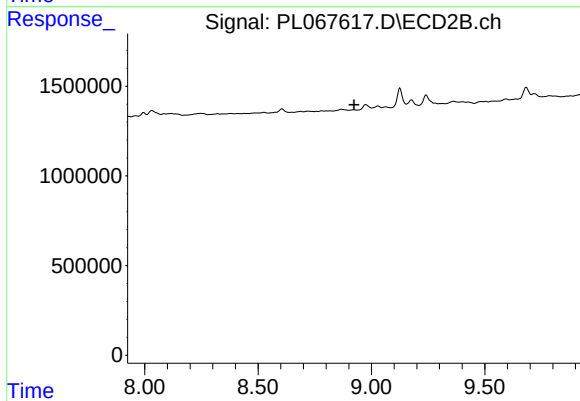

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.924 min
Response: 0
Conc: N.D.

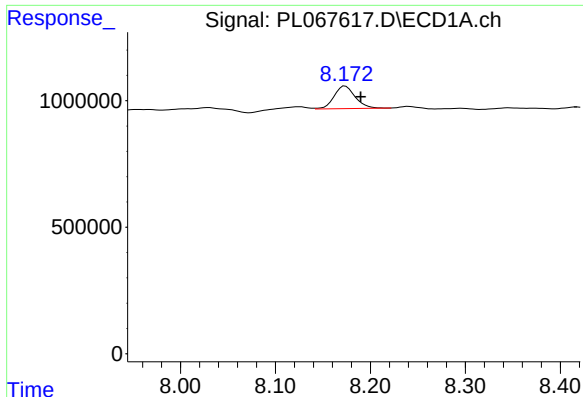

#15 Endosulfan II


R.T.: 8.173 min
Delta R.T.: -0.016 min
Response: 1383341
Conc: 2.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

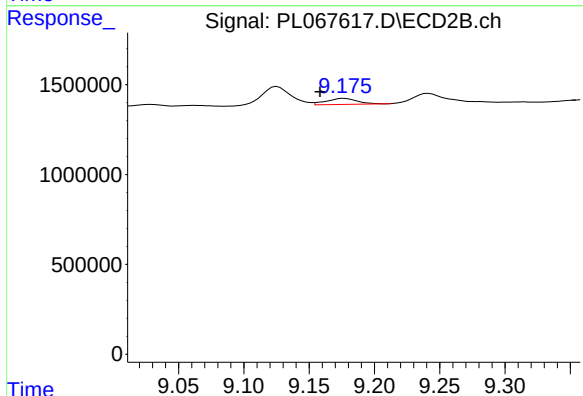


#15 Endosulfan II

R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 552929
Conc: 0.69 ng/ml

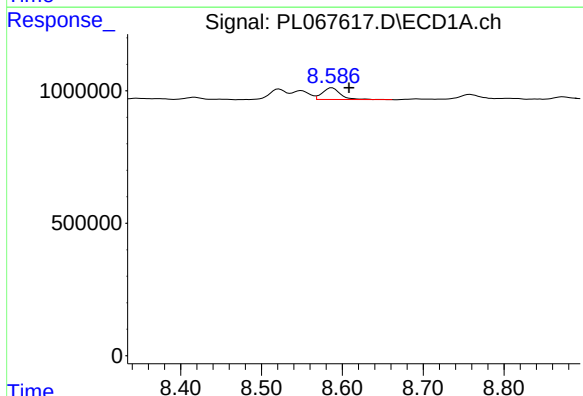


#19 Endosulfan Sulfate

R.T.: 8.587 min
Delta R.T.: -0.021 min
Response: 688089
Conc: 1.08 ng/ml

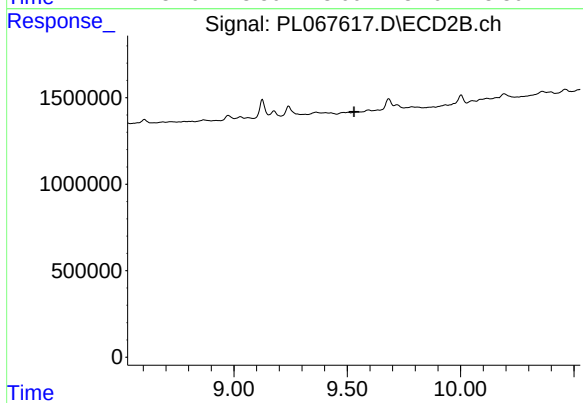

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.530 min
Response: 0
Conc: N.D.

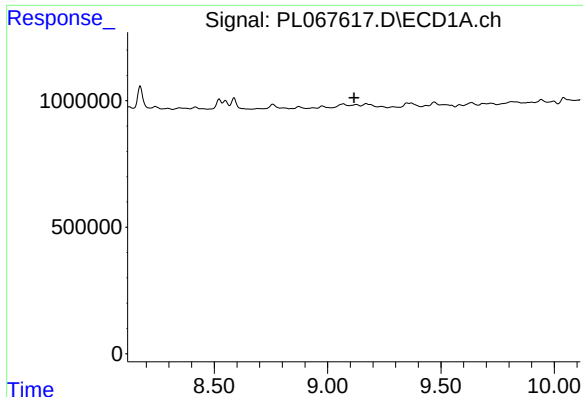

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

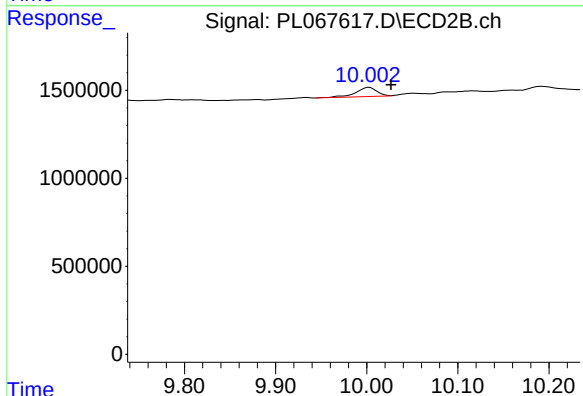


#21 Endrin ketone

R.T.: 10.003 min
Delta R.T.: -0.024 min
Response: 844226
Conc: 0.93 ng/ml

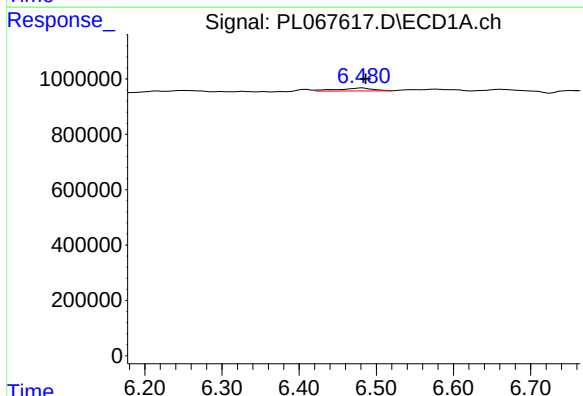


#24 Chlordane-2

R.T.: 6.482 min
Delta R.T.: -0.005 min
Response: 346161
Conc: 12.93 ng/ml

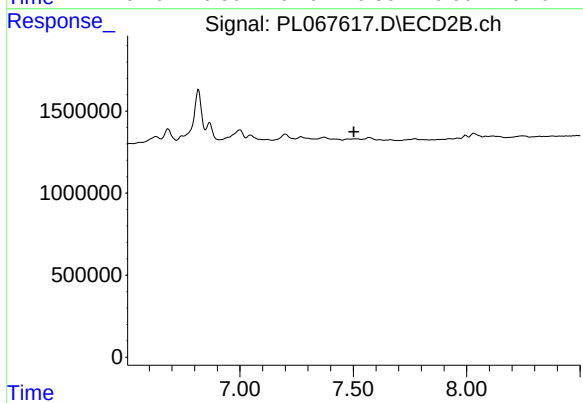

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

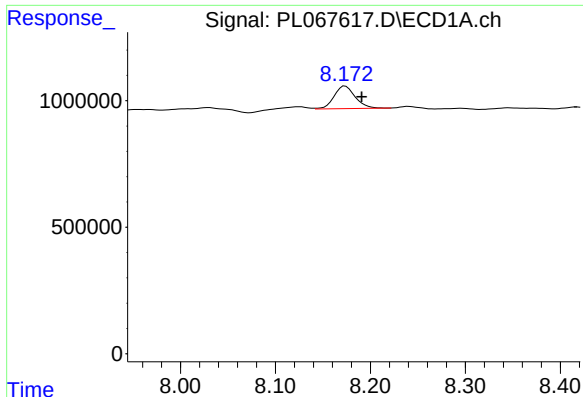

#27 Chlordane-5


R.T.: 8.173 min
Delta R.T.: -0.018 min
Response: 1383341
Conc: 63.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
0224-COMP-O(DISCRETE-CL-24)

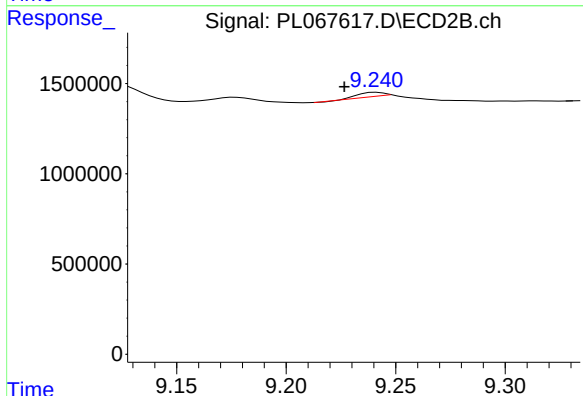


#27 Chlordane-5

R.T.: 9.242 min
Delta R.T.: 0.015 min
Response: 242913
Conc: 8.35 ng/ml

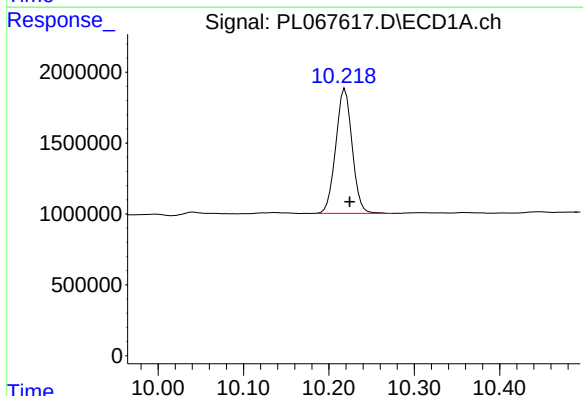

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 11742140
Conc: 16.57 ng/ml

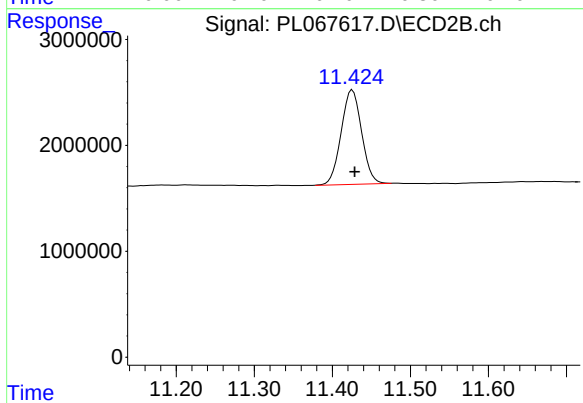

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.003 min
Response: 16246915
Conc: 16.31 ng/ml