

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 16:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:32:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	9627528	17919996	17.511	19.009
28)	SA Decachlor...	10.219	11.427	13573718	19957530	19.153	20.037
Target Compounds							
4)	MA Heptachlor	5.986f	0.000	378183	0	0.501	N.D. #
6)	B beta-BHC	5.986	0.000	378183	0	1.057	N.D. #
15)	B Endosulfa...	8.173f	9.178f	762684	446596	1.238	0.560 #
19)	B Endosulfa...	8.601	0.000	1046203	0	1.648	N.D. #
24)	Chlordane-2	6.484	0.000	443867	0	16.576	N.D. #
27)	Chlordane-5	8.173f	9.242f	762684	138085	34.859	4.749 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 16:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:32:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

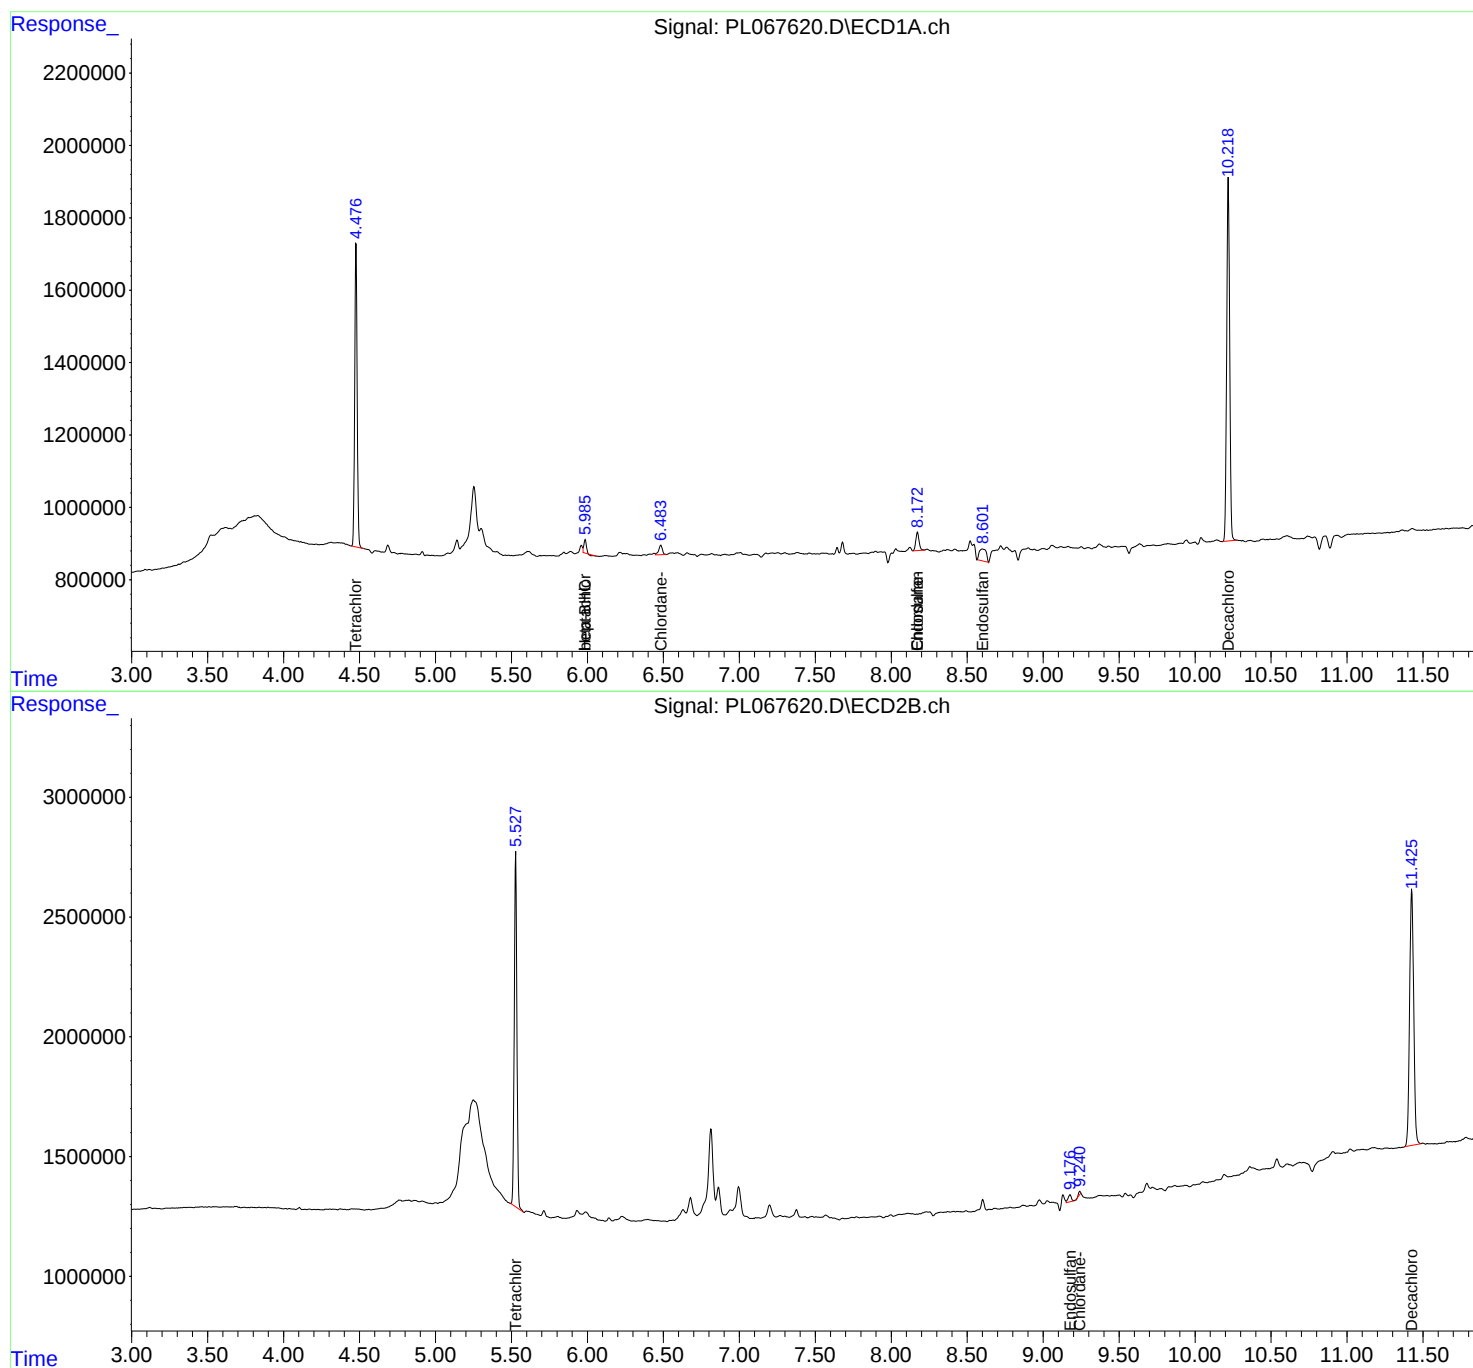


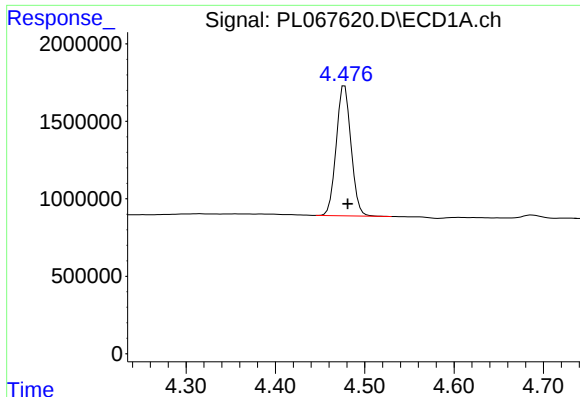

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 9627528
Conc: 17.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

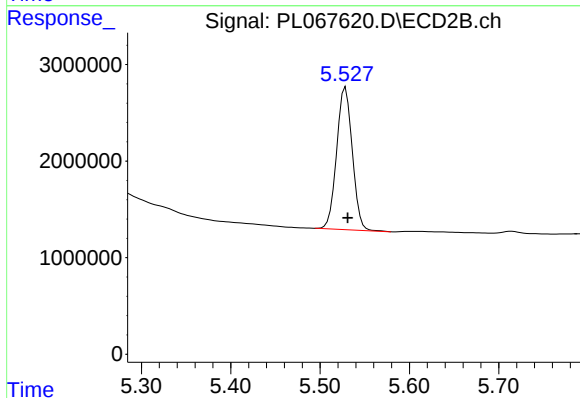


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.003 min
Response: 17919996
Conc: 19.01 ng/ml

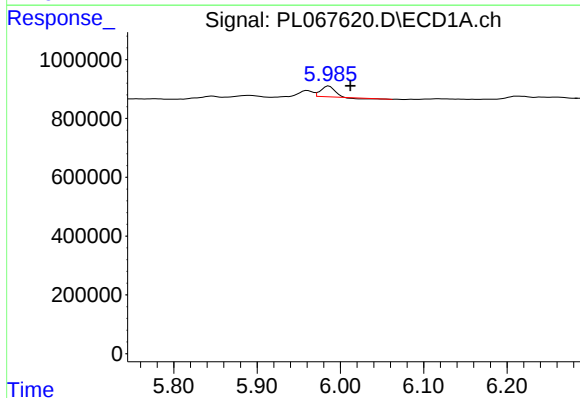


#4 Heptachlor

R.T.: 5.986 min
Delta R.T.: -0.026 min
Response: 378183
Conc: 0.50 ng/ml

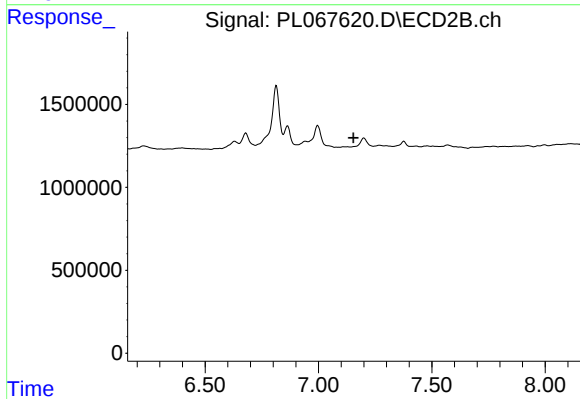

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

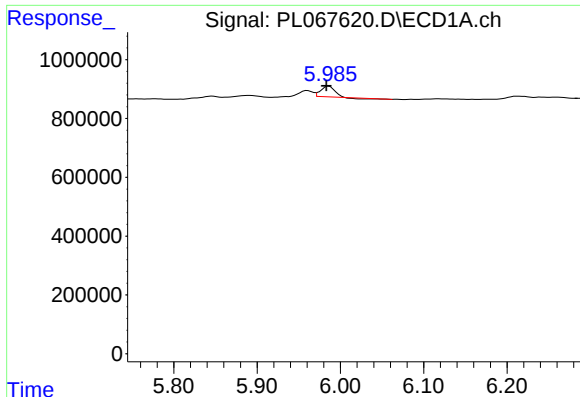

#6 beta-BHC


R.T.: 5.986 min
Delta R.T.: 0.003 min
Response: 378183
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

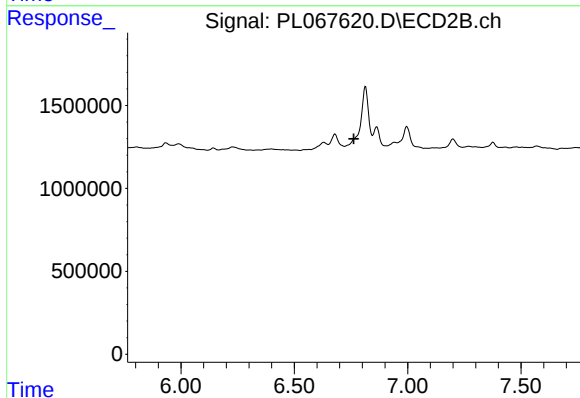


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

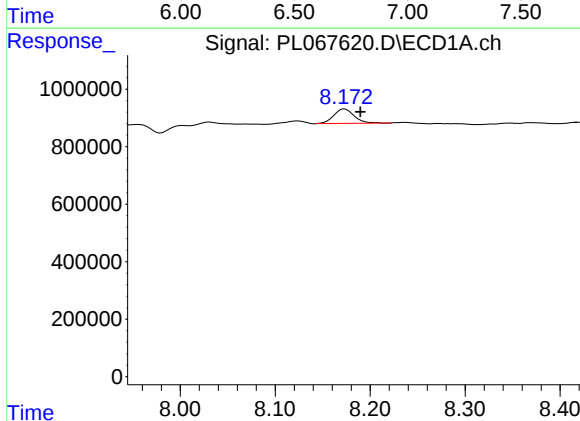


#15 Endosulfan II

R.T.: 8.173 min
Delta R.T.: -0.017 min
Response: 762684
Conc: 1.24 ng/ml

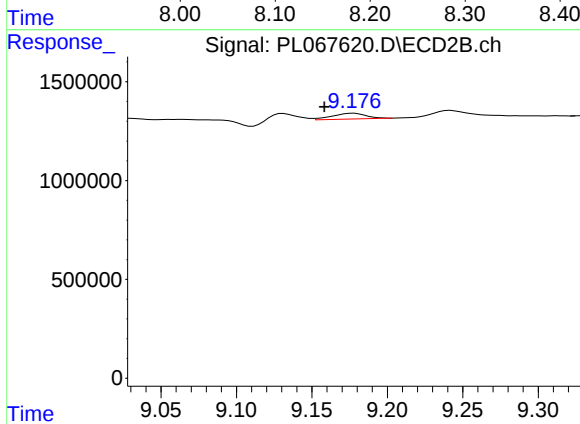

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 446596
Conc: 0.56 ng/ml

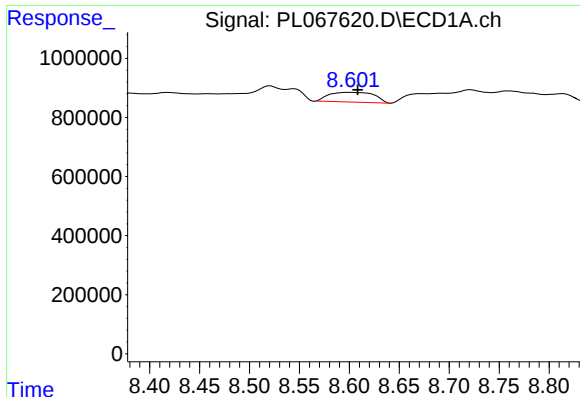

#19 Endosulfan Sulfate


R.T.: 8.601 min
Delta R.T.: -0.007 min
Response: 1046203
Conc: 1.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

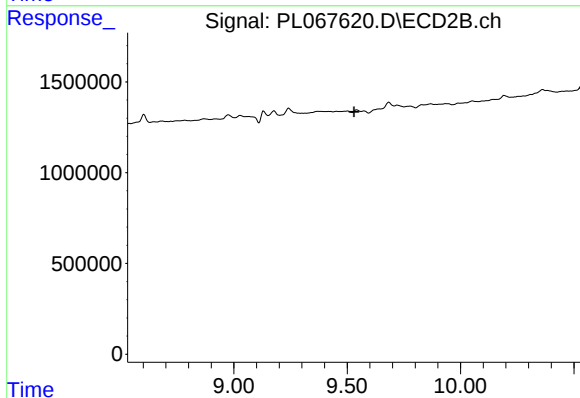


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

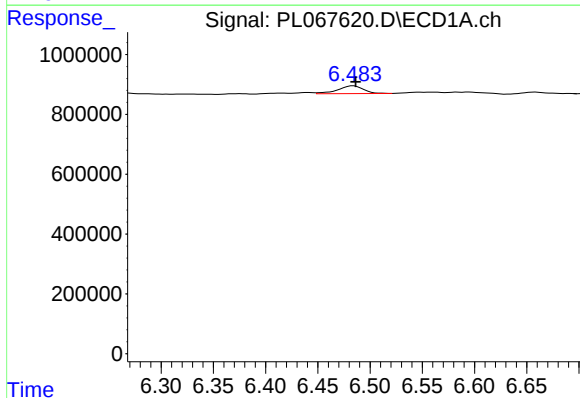


#24 Chlordane-2

R.T.: 6.484 min
Delta R.T.: -0.002 min
Response: 443867
Conc: 16.58 ng/ml

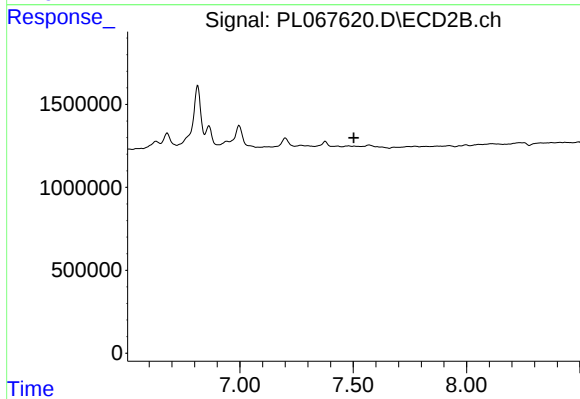

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.503 min
Response: 0
Conc: N.D.

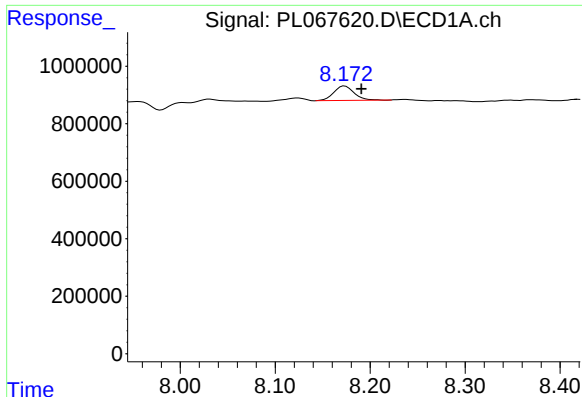

#27 Chlordane-5


R.T.: 8.173 min
Delta R.T.: -0.018 min
Response: 762684
Conc: 34.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

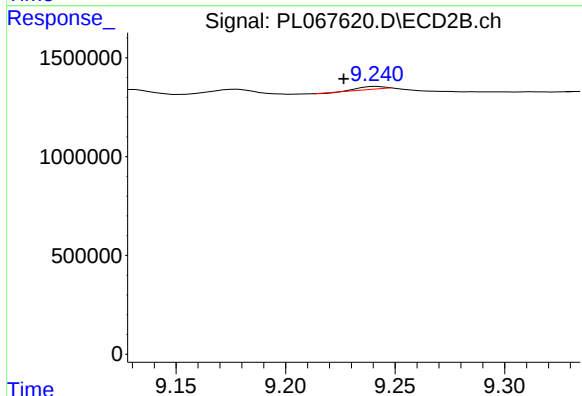


#27 Chlordane-5

R.T.: 9.242 min
Delta R.T.: 0.015 min
Response: 138085
Conc: 4.75 ng/ml

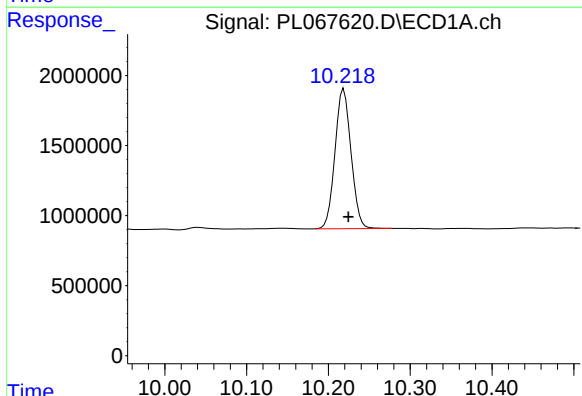

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 13573718
Conc: 19.15 ng/ml

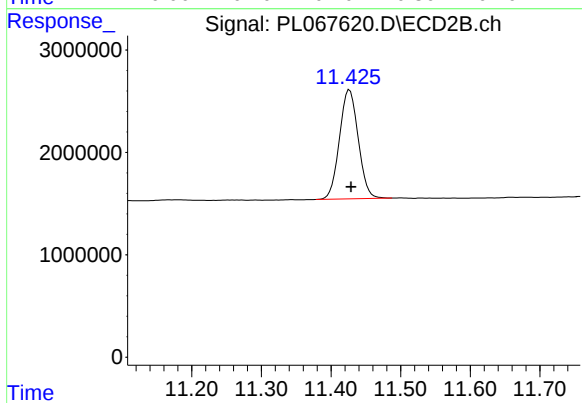

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 19957530
Conc: 20.04 ng/ml