

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 17:24
 Operator : AR\AJ
 Sample : M2709-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0236-COMPOSITE-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:33:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	10293057	18915996	18.722	20.065
28)	SA Decachlor...	10.219	11.426	13714548	20521620	19.352	20.603
Target Compounds							
10)	B gamma-Chl...	7.170f	0.000	93938	0	0.130	N.D. #
12)	B 4,4'-DDE	7.467	8.527	794689	1213025	1.194	1.339
15)	B Endosulfa...	8.176	9.177f	679241	528663	1.103	0.663 #
17)	MA 4,4'-DDT	8.301	0.000	183039	0	0.315	N.D. #
19)	B Endosulfa...	8.588f	0.000	949164	0	1.495	N.D. #
21)	B Endrin ke...	0.000	10.003f	0	1189920	N.D.	1.313 #
25)	Chlordane-3	7.170	0.000	93938	0	1.398	N.D. #
27)	Chlordane-5	8.176	0.000	679241	0	31.045	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 17:24
Operator : AR\AJ
Sample : M2709-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:33:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

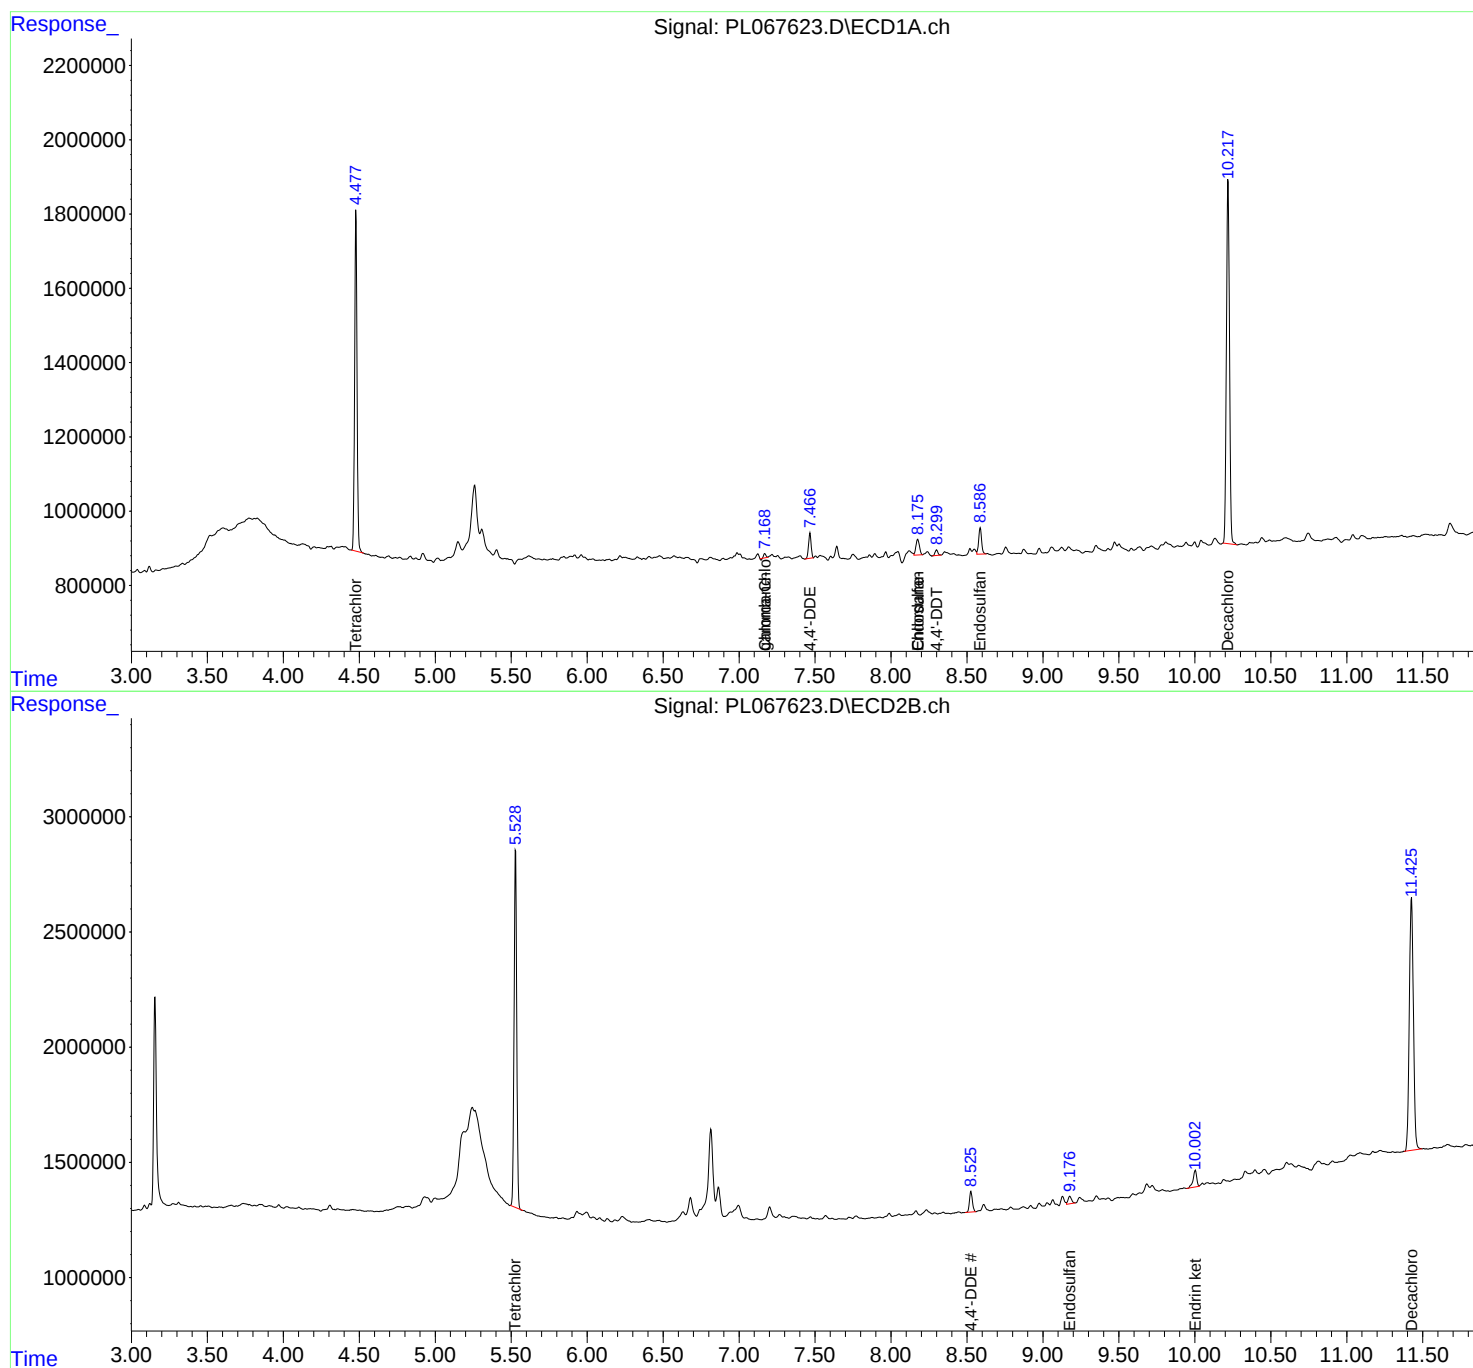


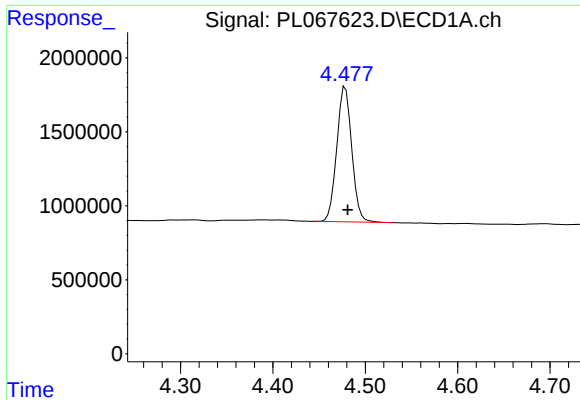

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10293057
Conc: 18.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

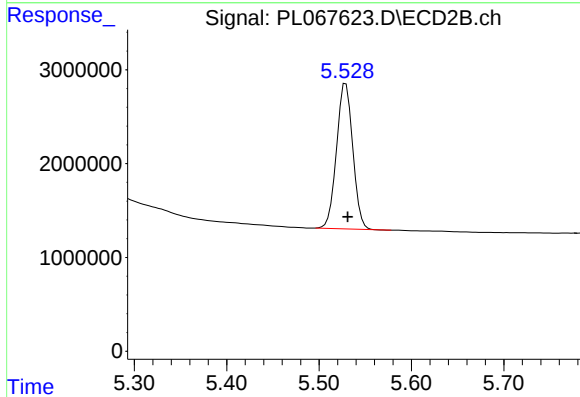


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 18915996
Conc: 20.07 ng/ml

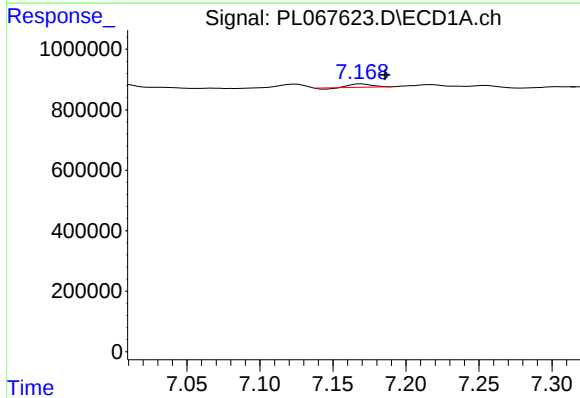


#10 gamma-Chlordane

R.T.: 7.170 min
Delta R.T.: -0.016 min
Response: 93938
Conc: 0.13 ng/ml

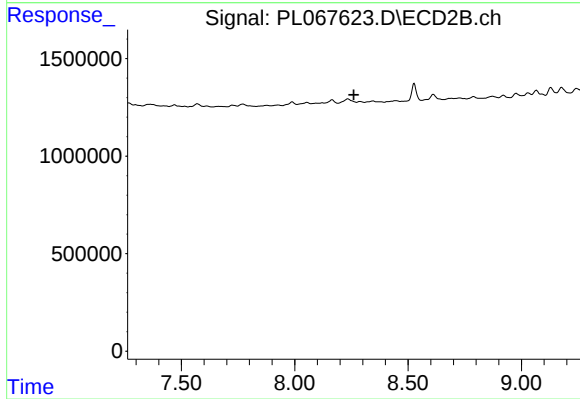

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.261 min
Response: 0
Conc: N.D.

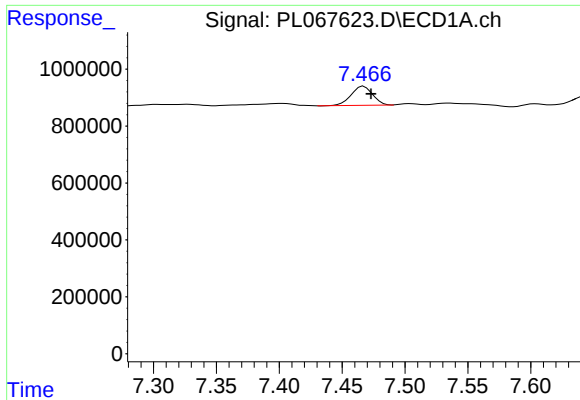

#12 4,4'-DDE


R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 794689
Conc: 1.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

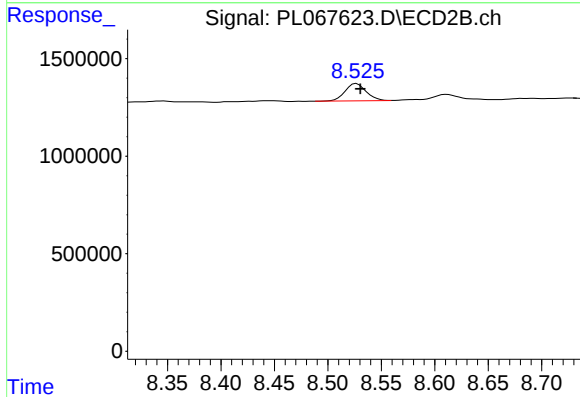


#12 4,4'-DDE

R.T.: 8.527 min
Delta R.T.: -0.004 min
Response: 1213025
Conc: 1.34 ng/ml

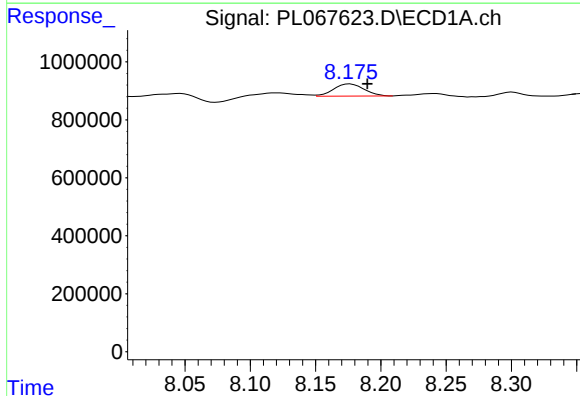


#15 Endosulfan II

R.T.: 8.176 min
Delta R.T.: -0.014 min
Response: 679241
Conc: 1.10 ng/ml

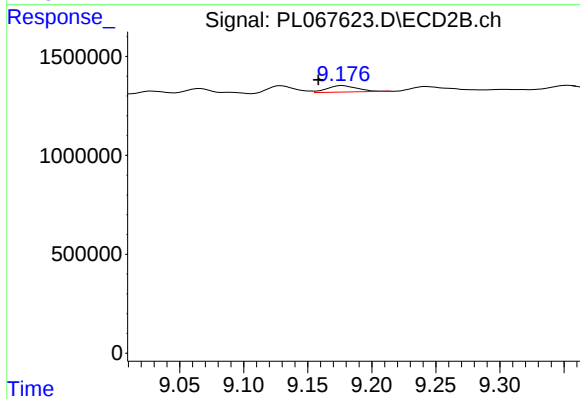

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.019 min
Response: 528663
Conc: 0.66 ng/ml

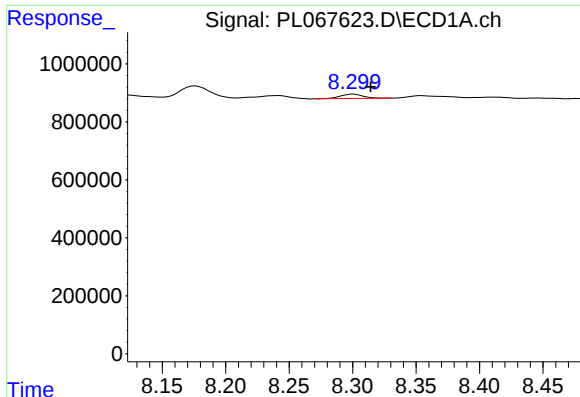

#17 4,4'-DDT


R.T.: 8.301 min
Delta R.T.: -0.013 min
Response: 183039
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

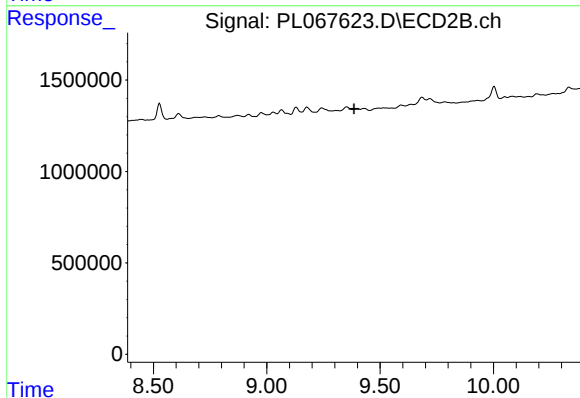


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.386 min
Response: 0
Conc: N.D.

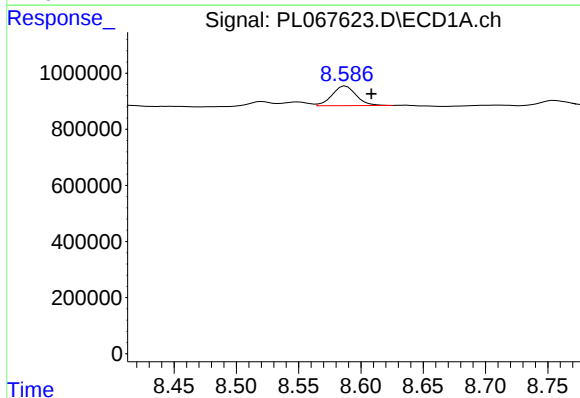


#19 Endosulfan Sulfate

R.T.: 8.588 min
Delta R.T.: -0.021 min
Response: 949164
Conc: 1.50 ng/ml

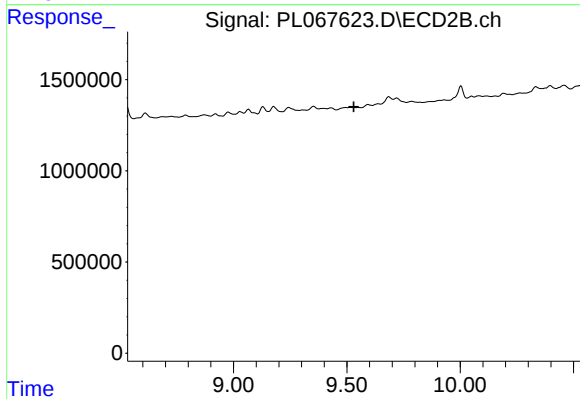

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

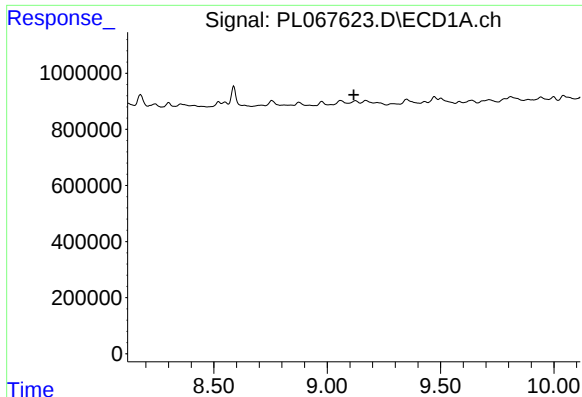

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

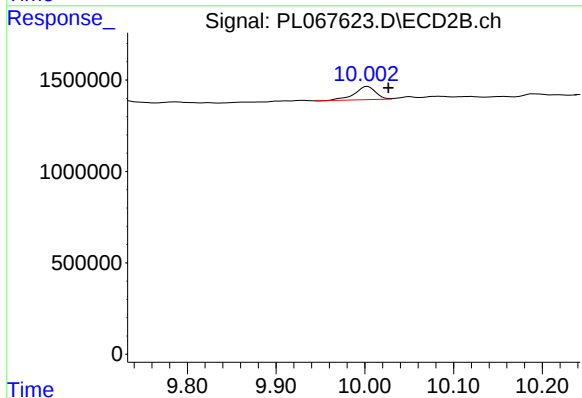


#21 Endrin ketone

R.T.: 10.003 min
Delta R.T.: -0.023 min
Response: 1189920
Conc: 1.31 ng/ml

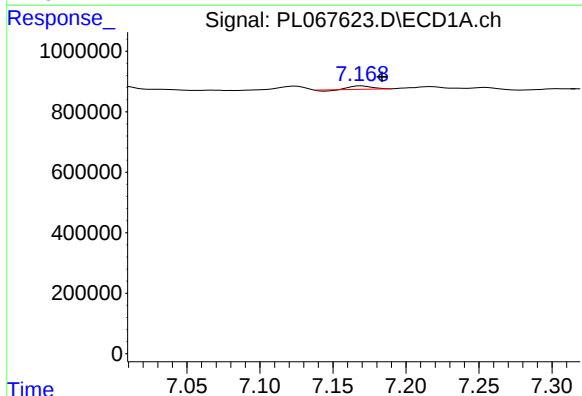


#25 Chlordane-3

R.T.: 7.170 min
Delta R.T.: -0.014 min
Response: 93938
Conc: 1.40 ng/ml

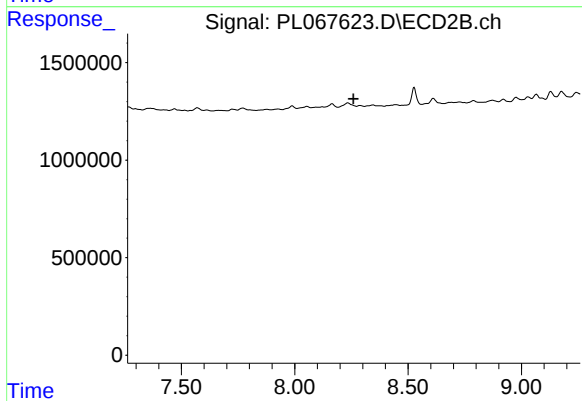

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.259 min
Response: 0
Conc: N.D.

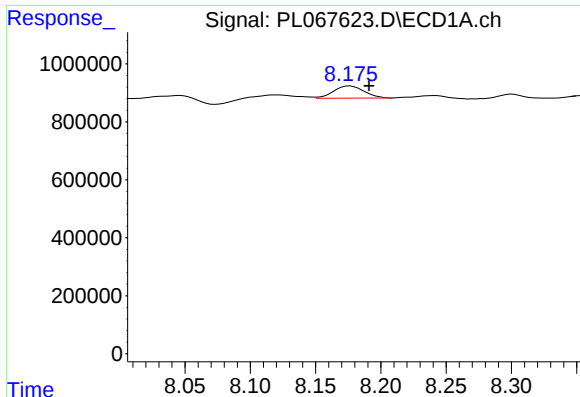

#27 Chlordane-5


R.T.: 8.176 min
Delta R.T.: -0.015 min
Response: 679241
Conc: 31.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
0236-COMPOSITE-M

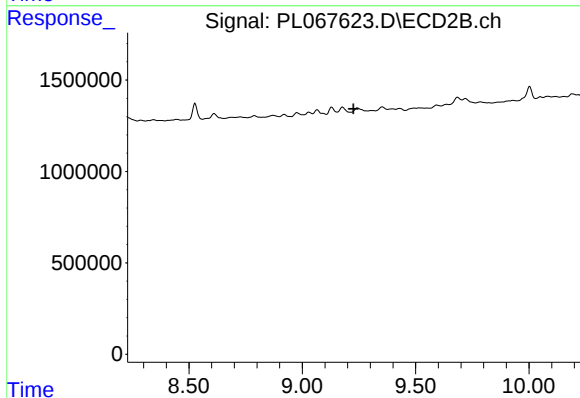


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

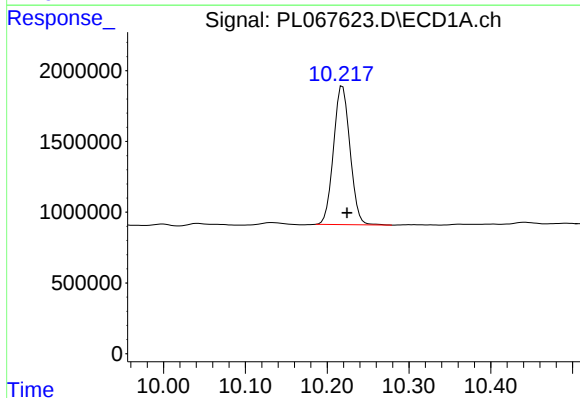

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 13714548
Conc: 19.35 ng/ml

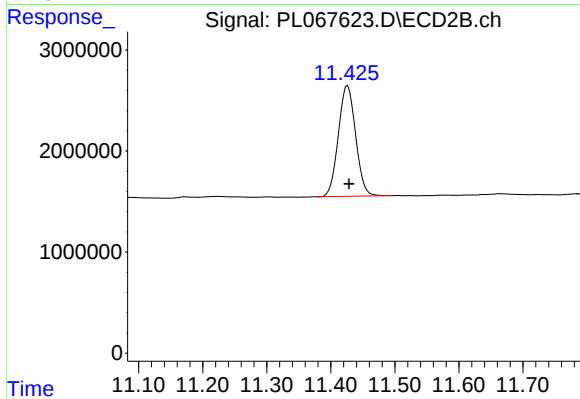

#28 Decachlorobiphenyl

R.T.: 11.426 min
Delta R.T.: -0.002 min
Response: 20521620
Conc: 20.60 ng/ml