

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067630.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 19:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:34:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	9821429	18238675	17.864	19.347
28)	SA Decachlor...	10.220	11.428	13319607	20870417	18.795	20.953
Target Compounds							
4)	MA Heptachlor	5.987f	0.000	550216	0	0.729	N.D. #
6)	B beta-BHC	5.987	0.000	550216	0	1.538	N.D. #
15)	B Endosulfa...	8.175f	9.177f	224196	321982	0.364	0.404
16)	A 4,4'-DDD	8.032f	0.000	168991	0	0.291	N.D. #
19)	B Endosulfa...	8.605	0.000	1144782	0	1.803	N.D. #
21)	B Endrin ke...	0.000	10.052f	0	367907	N.D.	0.406 #
24)	Chlordane-2	6.485	0.000	731334	0	27.311	N.D. #
27)	Chlordane-5	8.175f	0.000	224196	0	10.247	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067630.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 19:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:34:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

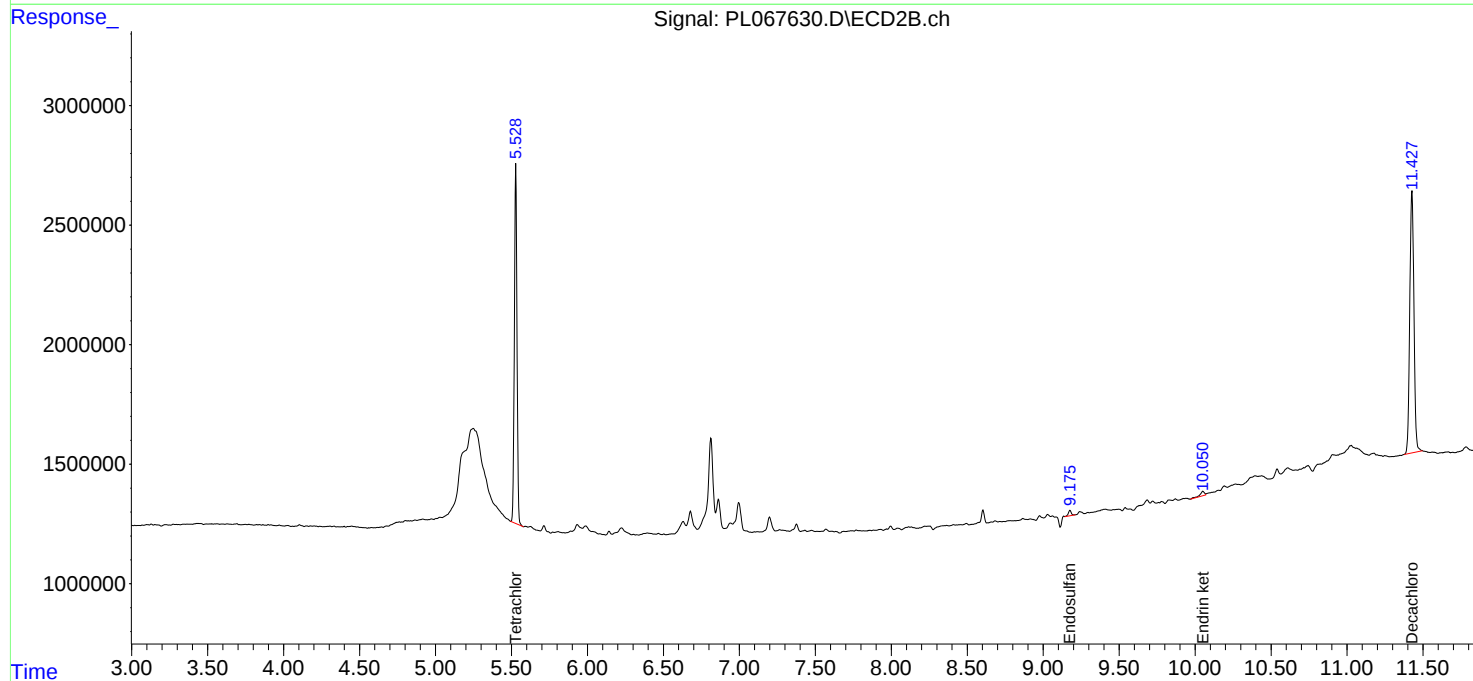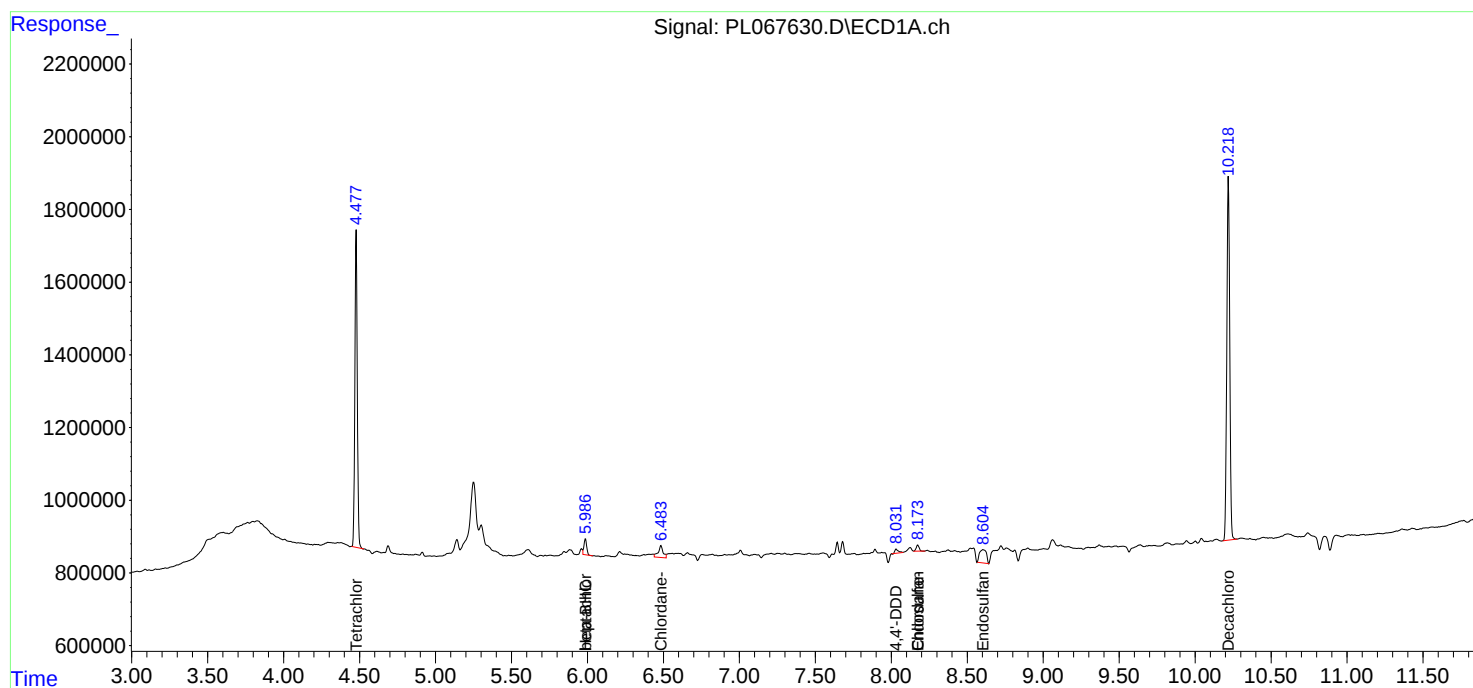


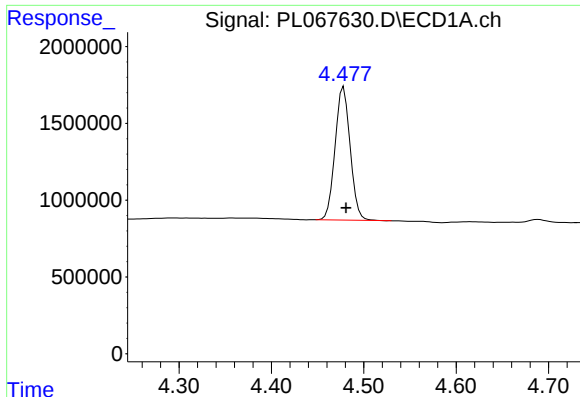

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 9821429
Conc: 17.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

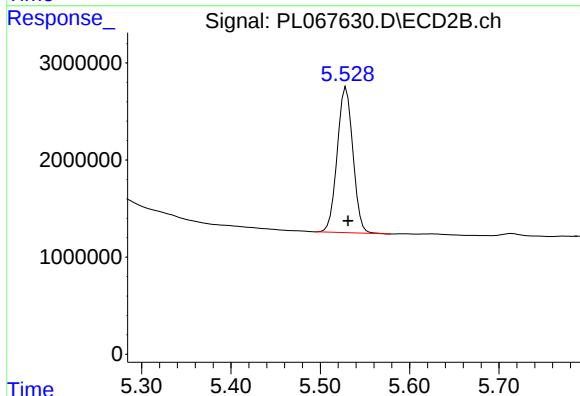


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 18238675
Conc: 19.35 ng/ml

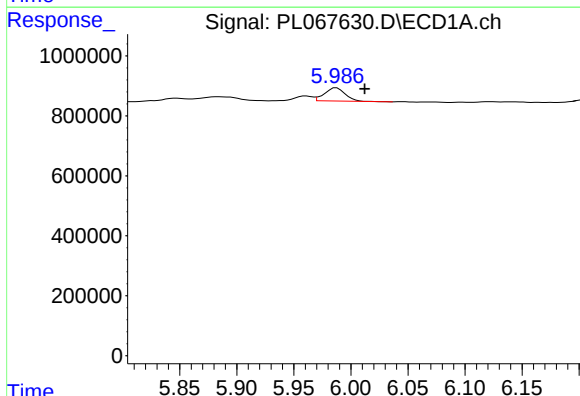


#4 Heptachlor

R.T.: 5.987 min
Delta R.T.: -0.025 min
Response: 550216
Conc: 0.73 ng/ml

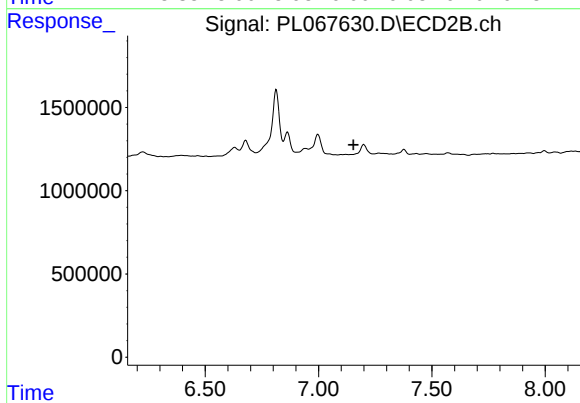

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

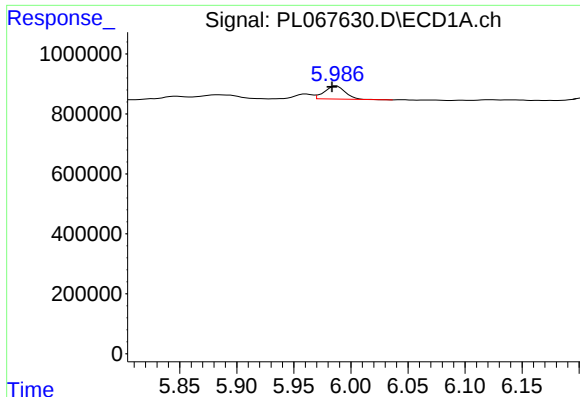

#6 beta-BHC


R.T.: 5.987 min
Delta R.T.: 0.004 min
Response: 550216
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

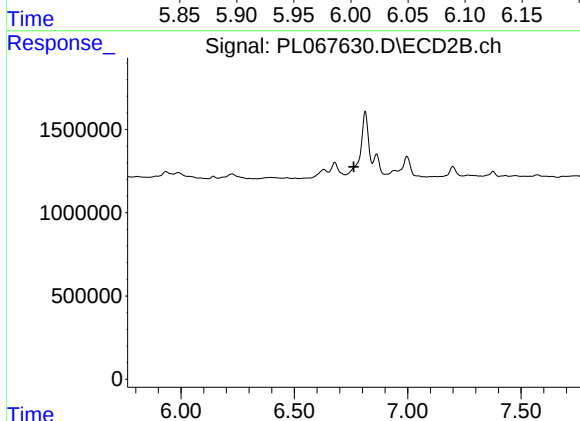


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

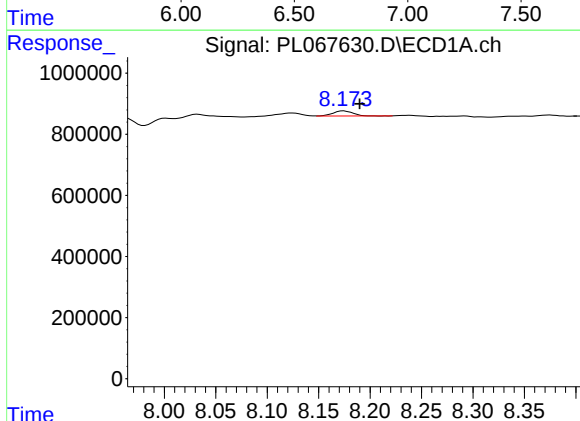


#15 Endosulfan II

R.T.: 8.175 min
Delta R.T.: -0.015 min
Response: 224196
Conc: 0.36 ng/ml

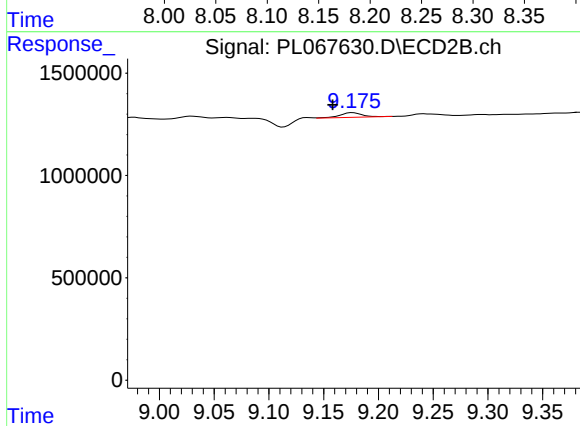

#15 Endosulfan II


R.T.: 9.177 min
Delta R.T.: 0.018 min
Response: 321982
Conc: 0.40 ng/ml

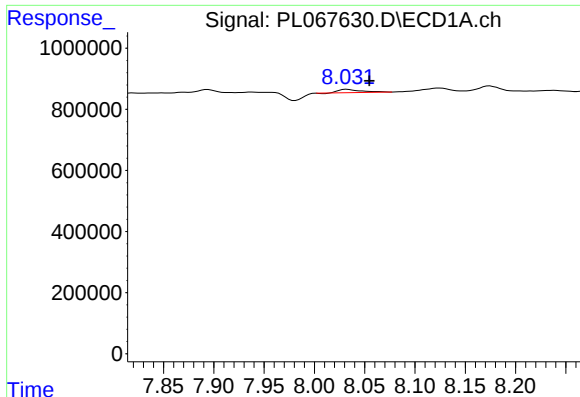

#16 4,4'-DDD


R.T.: 8.032 min
Delta R.T.: -0.022 min
Response: 168991
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

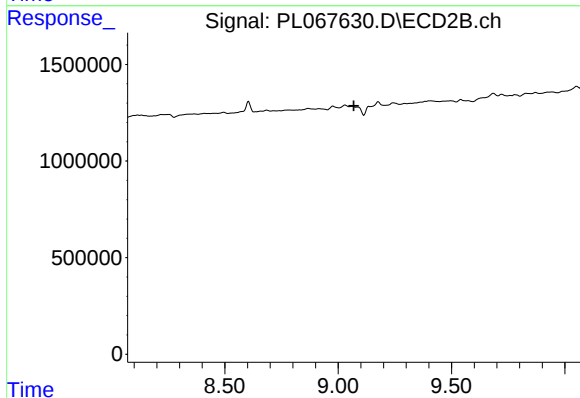


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

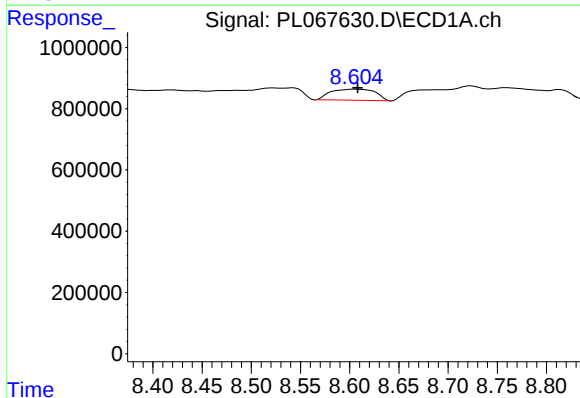


#19 Endosulfan Sulfate

R.T.: 8.605 min
Delta R.T.: -0.004 min
Response: 1144782
Conc: 1.80 ng/ml

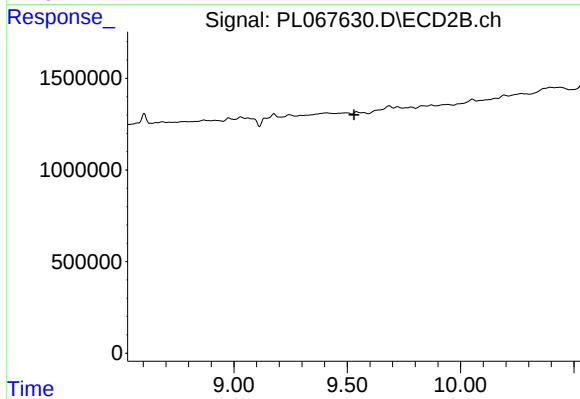

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

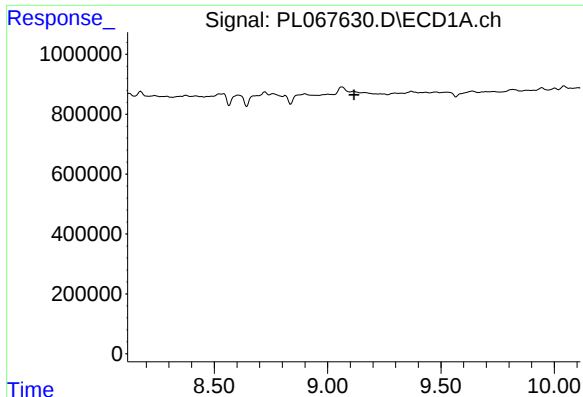

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

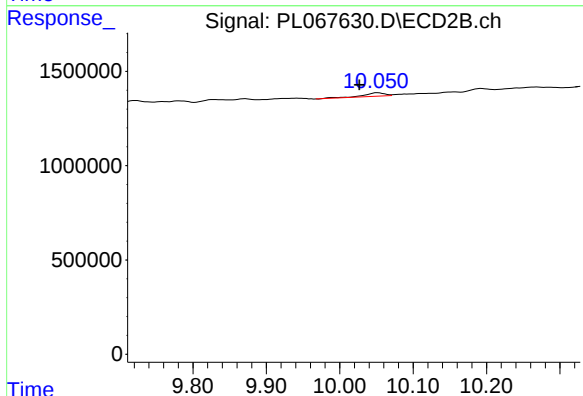


#21 Endrin ketone

R.T.: 10.052 min
Delta R.T.: 0.025 min
Response: 367907
Conc: 0.41 ng/ml

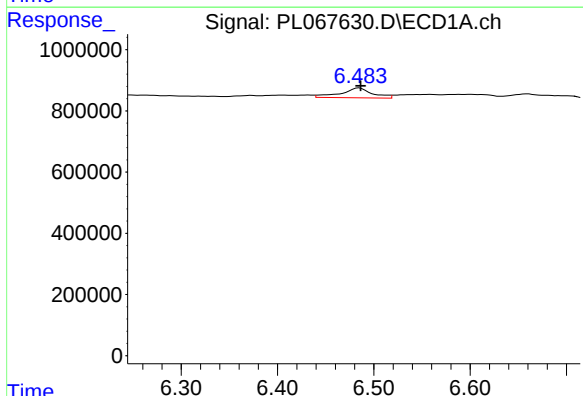


#24 Chlordane-2

R.T.: 6.485 min
Delta R.T.: -0.002 min
Response: 731334
Conc: 27.31 ng/ml

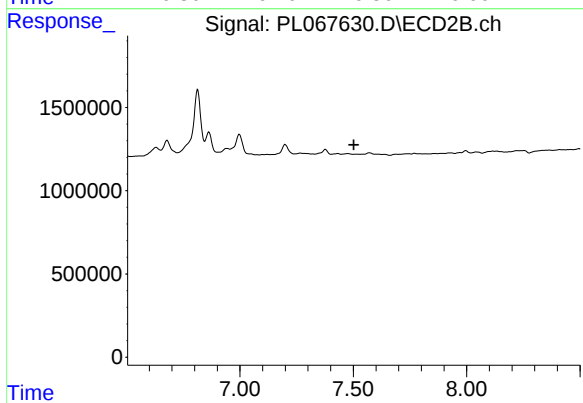

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.503 min
Response: 0
Conc: N.D.

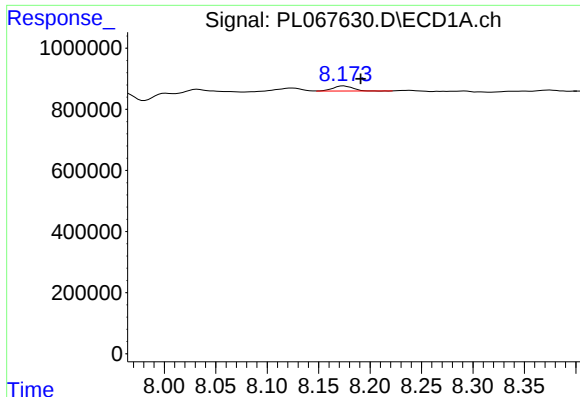

#27 Chlordane-5


R.T.: 8.175 min
Delta R.T.: -0.016 min
Response: 224196
Conc: 10.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

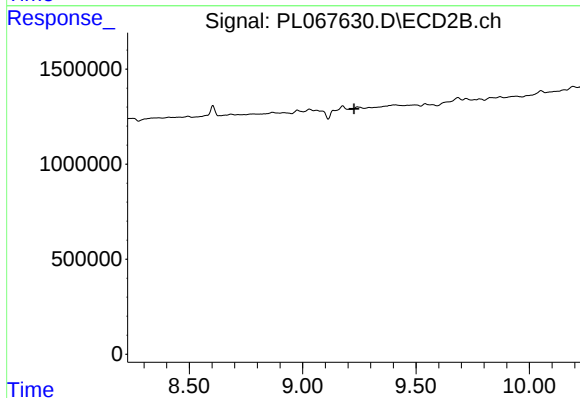


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

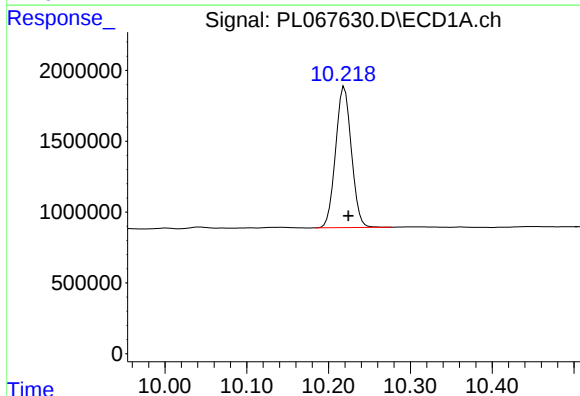

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 13319607
Conc: 18.79 ng/ml

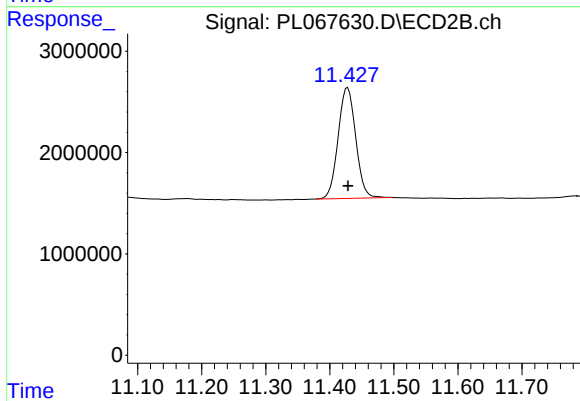

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 20870417
Conc: 20.95 ng/ml