

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 19:54
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:35:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	25298961	47166247	46.016	50.031
28)	SA Decachlor...	10.219	11.427	32281226	49902868	45.551	50.100
Target Compounds							
2)	A alpha-BHC	5.177	6.109	35906373	63978573	48.819	51.743
3)	MA gamma-BHC...	5.597	6.505	35218712	60998558	46.994	51.739
4)	MA Heptachlor	6.008	7.152	36543418	59285331	48.447	53.160
5)	MB Aldrin	6.329	7.522	34736769	54471110	47.210	50.327
6)	B beta-BHC	5.980	6.760	16884461	28350154	47.189	52.209
7)	B delta-BHC	6.237	7.026	35204303	59663925	47.665	50.756
8)	B Heptachlo...	6.903	7.988	33056574	50441368	47.246	50.352
9)	A Endosulfan I	7.302	8.393	31509076	46009227	46.870	50.386
10)	B gamma-Chl...	7.182	8.257	34022009	50375416	46.926	49.894
11)	B alpha-Chl...	7.249	8.339	34292785	50063799	46.841	49.587
12)	B 4,4'-DDE	7.468	8.527	31878433	46308430	47.915	51.117
13)	MA Dieldrin	7.587	8.682	32702130	46618339	46.650	51.329
14)	MA Endrin	7.873	8.921	30889494	39202868	47.112	51.252
15)	B Endosulfa...	8.184	9.155	28925584	40031421	46.967	50.209
16)	A 4,4'-DDD	8.049	9.066	27744290	37305761	47.730	52.455
17)	MA 4,4'-DDT	8.309	9.384	28423656	38352472	48.848	52.312
18)	B Endrin al...	8.372	9.290	23506933	32187226	46.431	50.401
19)	B Endosulfa...	8.603	9.528	29562969	39485460	46.570	49.719
20)	A Methoxychlor	8.903	9.871	17333574	21217610	48.762	54.572
21)	B Endrin ke...	9.112	10.024	35880840	45708768	47.127	50.430
22)	Mirex	9.299	10.490	29098156	36222693	46.204	47.914
24)	Chlordane-2	6.485	7.522f	1139918	54471110	42.569	1494.563 #
25)	Chlordane-3	7.182	8.257	34022009	50375416	506.351	376.391 #
26)	Chlordane-4	7.249	8.339	34292785	50063799	469.259	308.844 #
27)	Chlordane-5	8.184	0.000	28925584	0	1322.066	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 19:54
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:35:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

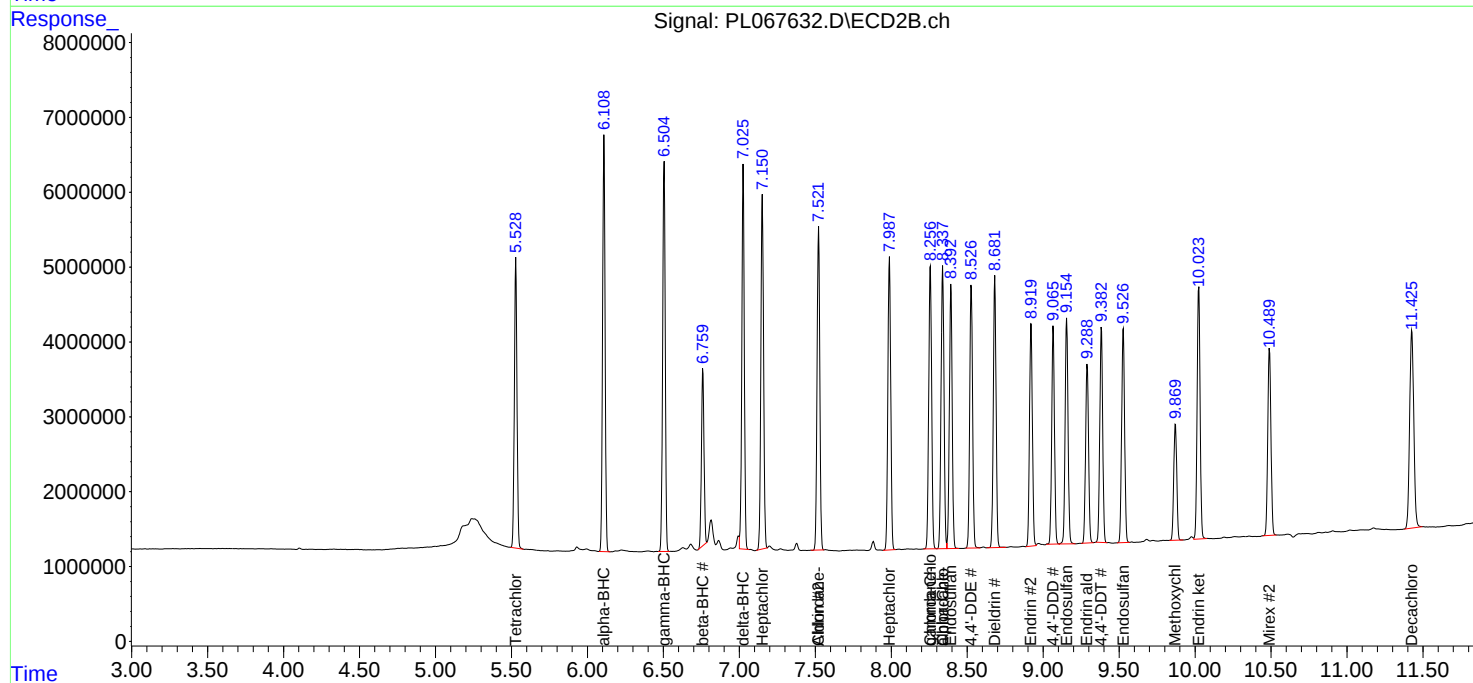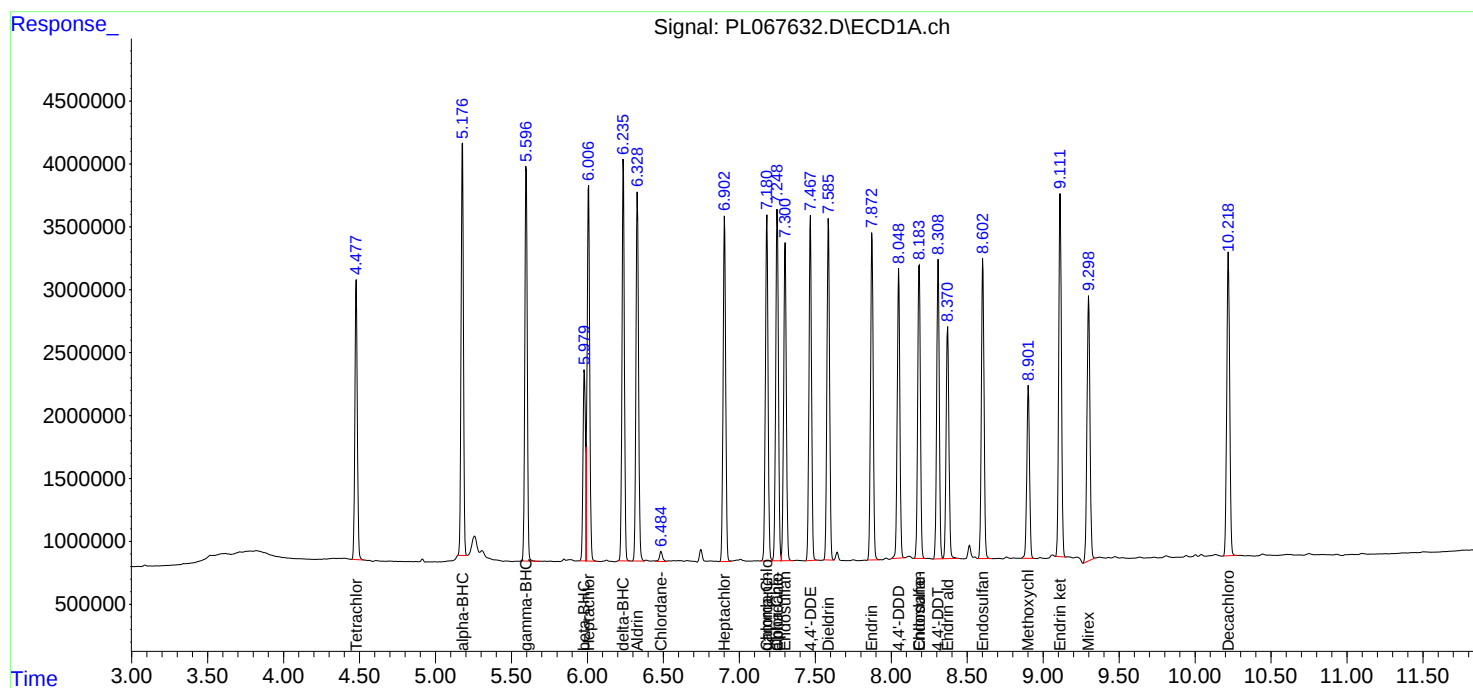


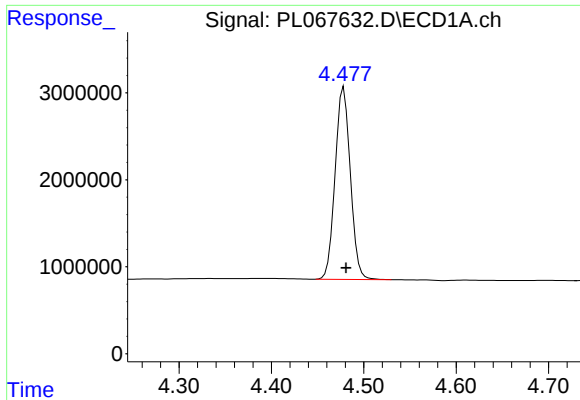

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 25298961
Conc: 46.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

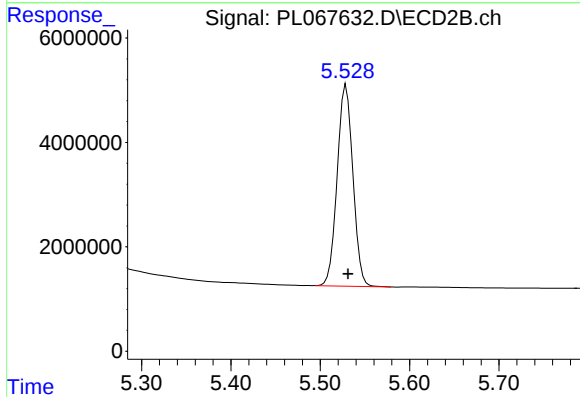


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 47166247
Conc: 50.03 ng/ml

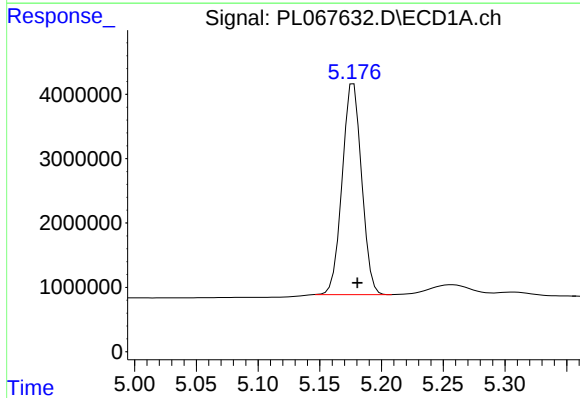


#2 alpha-BHC

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 35906373
Conc: 48.82 ng/ml

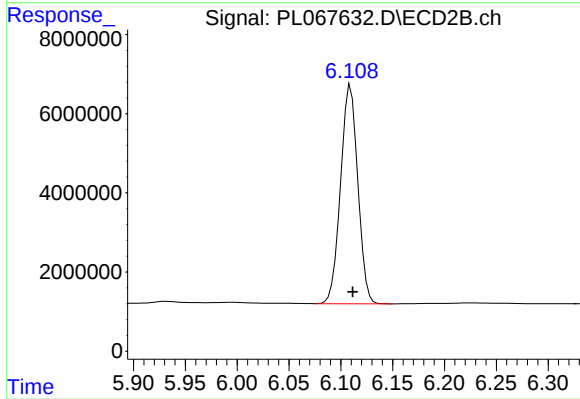

#2 alpha-BHC


R.T.: 6.109 min
Delta R.T.: -0.002 min
Response: 63978573
Conc: 51.74 ng/ml

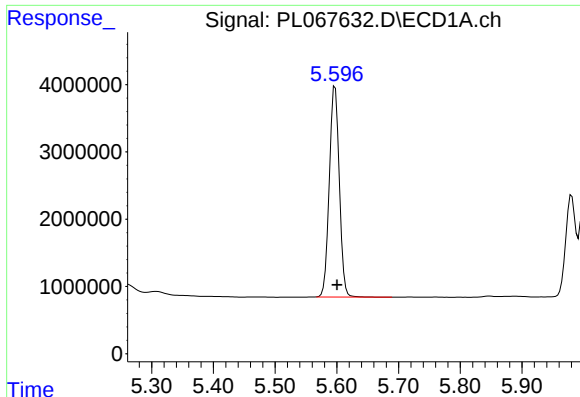

#3 gamma-BHC (Lindane)


R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 35218712
Conc: 46.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

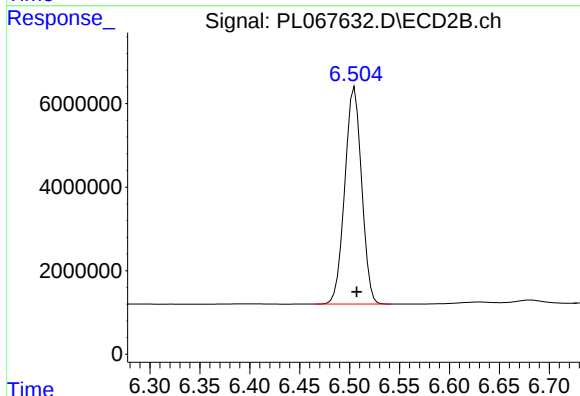


#3 gamma-BHC (Lindane)

R.T.: 6.505 min
Delta R.T.: -0.002 min
Response: 60998558
Conc: 51.74 ng/ml

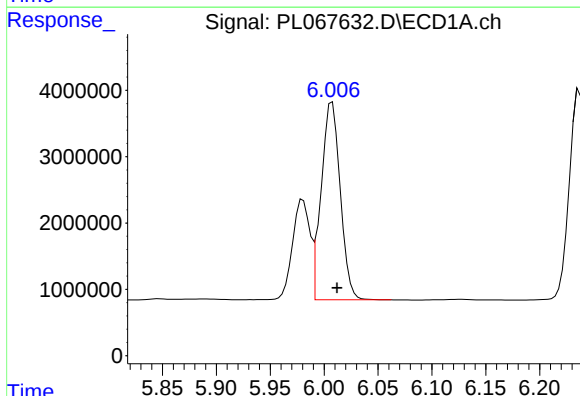


#4 Heptachlor

R.T.: 6.008 min
Delta R.T.: -0.004 min
Response: 36543418
Conc: 48.45 ng/ml

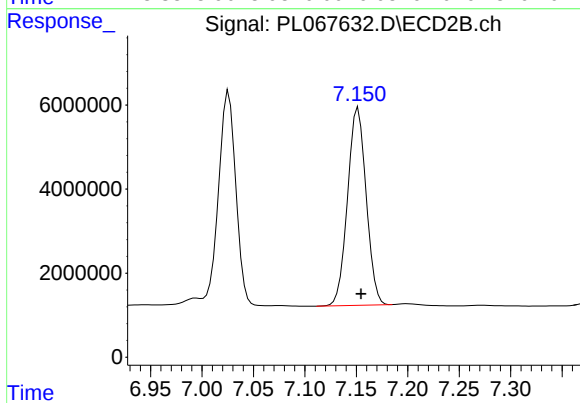

#4 Heptachlor


R.T.: 7.152 min
Delta R.T.: -0.003 min
Response: 59285331
Conc: 53.16 ng/ml

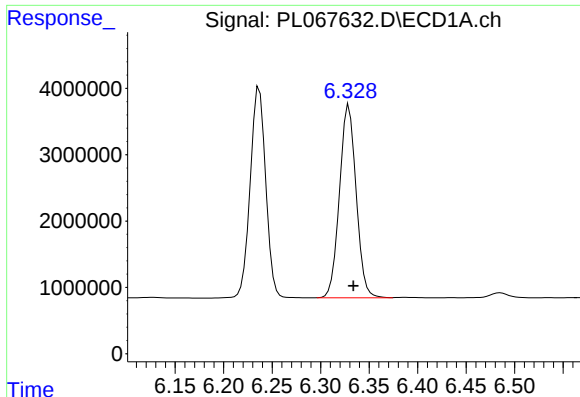

#5 Aldrin


R.T.: 6.329 min
Delta R.T.: -0.004 min
Response: 34736769
Conc: 47.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

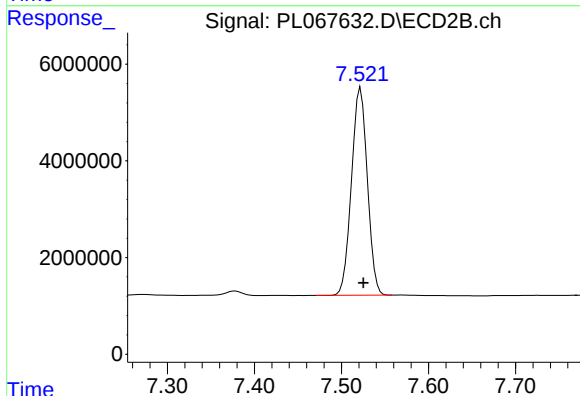


#5 Aldrin

R.T.: 7.522 min
Delta R.T.: -0.003 min
Response: 54471110
Conc: 50.33 ng/ml

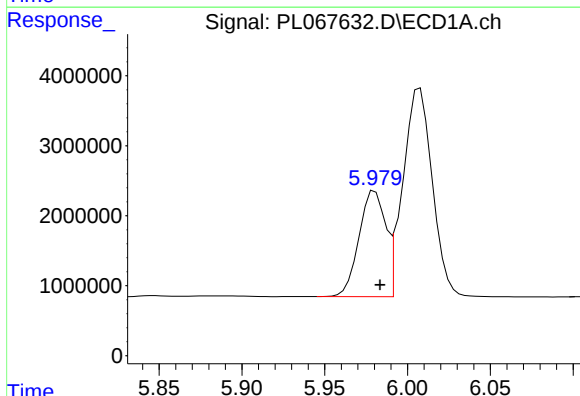


#6 beta-BHC

R.T.: 5.980 min
Delta R.T.: -0.003 min
Response: 16884461
Conc: 47.19 ng/ml

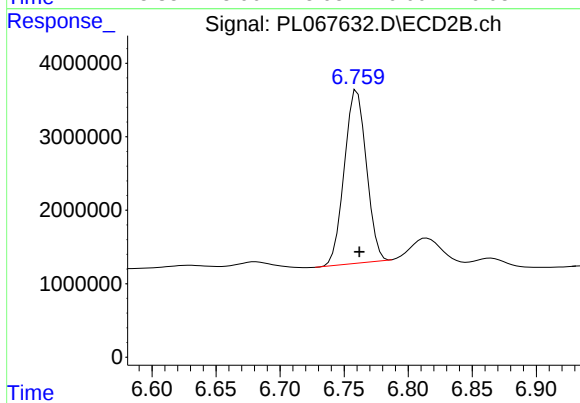

#6 beta-BHC


R.T.: 6.760 min
Delta R.T.: -0.002 min
Response: 28350154
Conc: 52.21 ng/ml

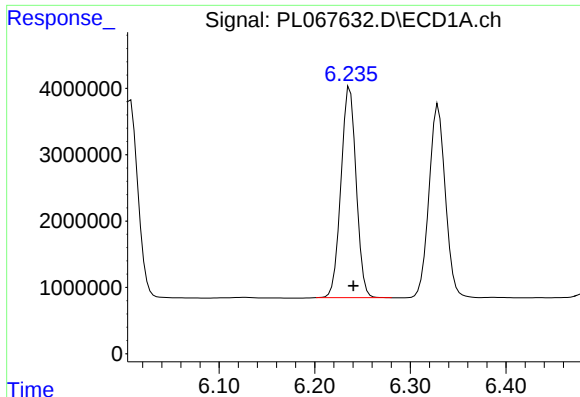

#7 delta-BHC


R.T.: 6.237 min
Delta R.T.: -0.004 min
Response: 35204303
Conc: 47.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

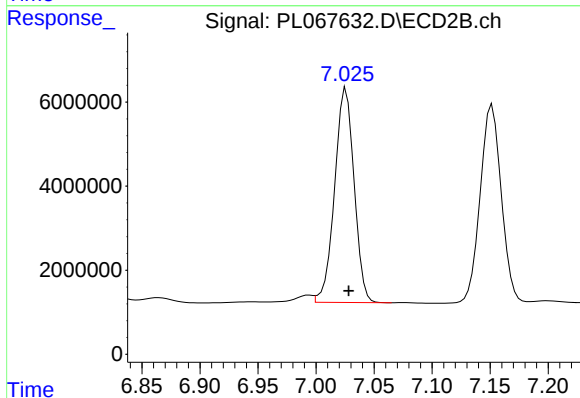


#7 delta-BHC

R.T.: 7.026 min
Delta R.T.: -0.002 min
Response: 59663925
Conc: 50.76 ng/ml

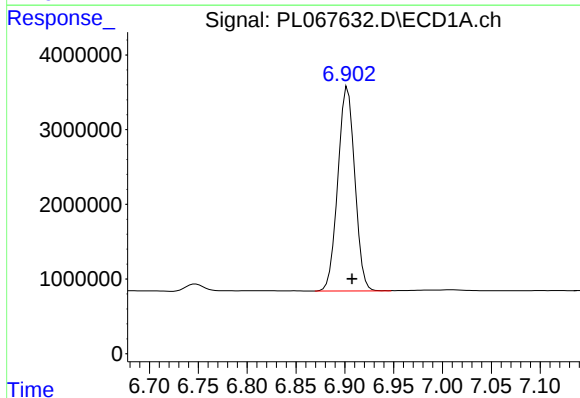


#8 Heptachlor epoxide

R.T.: 6.903 min
Delta R.T.: -0.004 min
Response: 33056574
Conc: 47.25 ng/ml

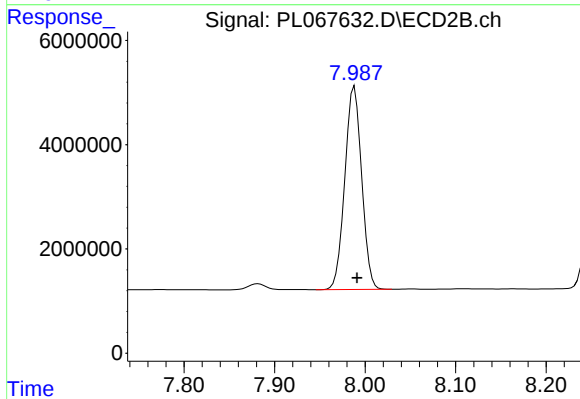

#8 Heptachlor epoxide


R.T.: 7.988 min
Delta R.T.: -0.003 min
Response: 50441368
Conc: 50.35 ng/ml

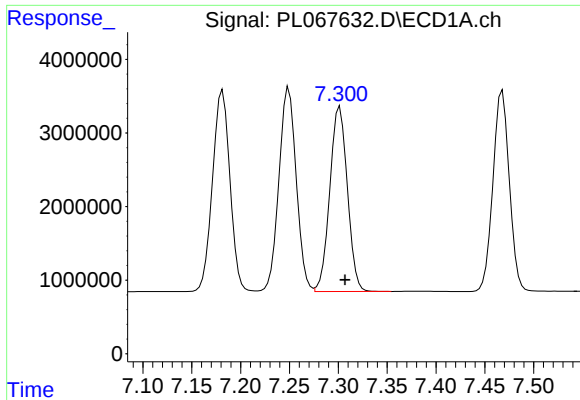

#9 Endosulfan I


R.T.: 7.302 min
Delta R.T.: -0.005 min
Response: 31509076
Conc: 46.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

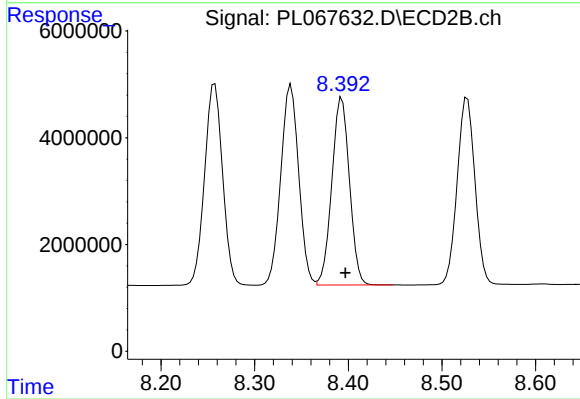


#9 Endosulfan I

R.T.: 8.393 min
Delta R.T.: -0.004 min
Response: 46009227
Conc: 50.39 ng/ml

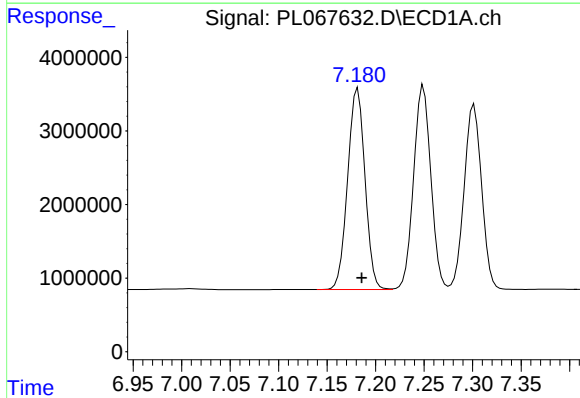


#10 gamma-Chlordane

R.T.: 7.182 min
Delta R.T.: -0.004 min
Response: 34022009
Conc: 46.93 ng/ml

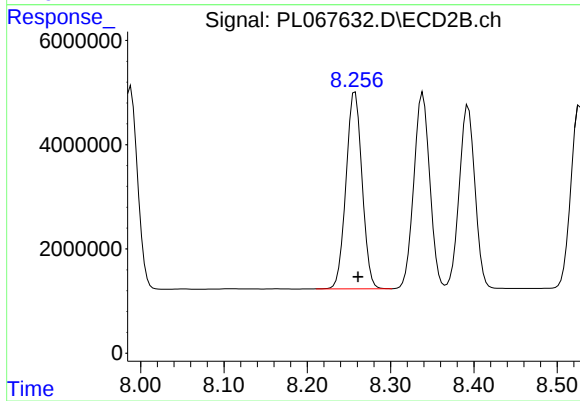

#10 gamma-Chlordane


R.T.: 8.257 min
Delta R.T.: -0.004 min
Response: 50375416
Conc: 49.89 ng/ml

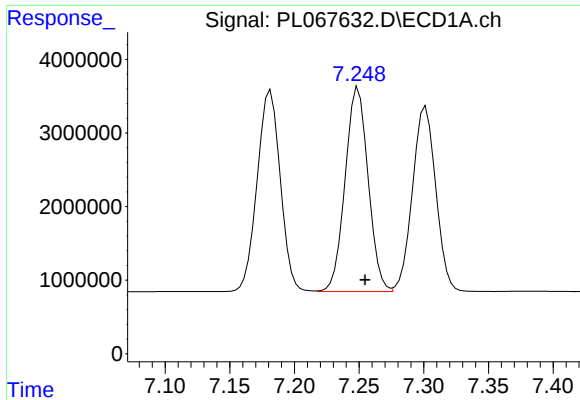

#11 alpha-Chlordane


R.T.: 7.249 min
Delta R.T.: -0.005 min
Response: 34292785
Conc: 46.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

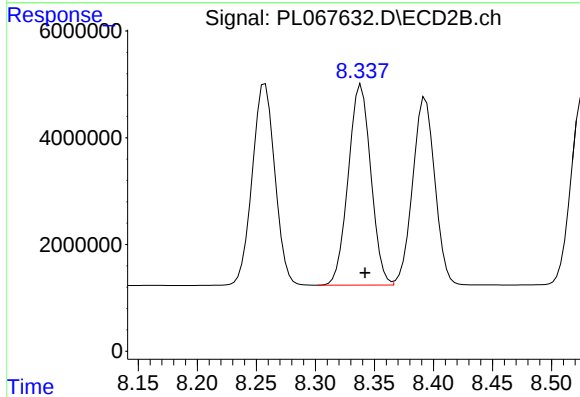


#11 alpha-Chlordane

R.T.: 8.339 min
Delta R.T.: -0.003 min
Response: 50063799
Conc: 49.59 ng/ml

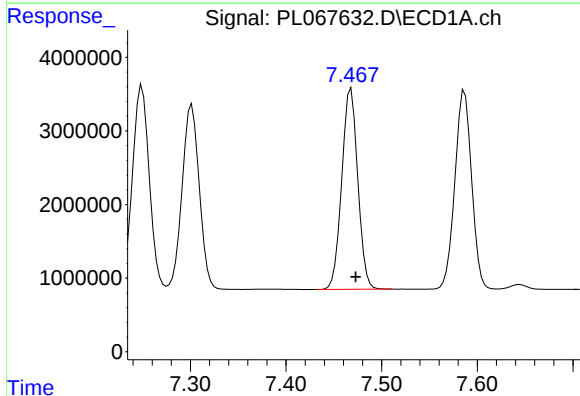


#12 4,4'-DDE

R.T.: 7.468 min
Delta R.T.: -0.005 min
Response: 31878433
Conc: 47.92 ng/ml

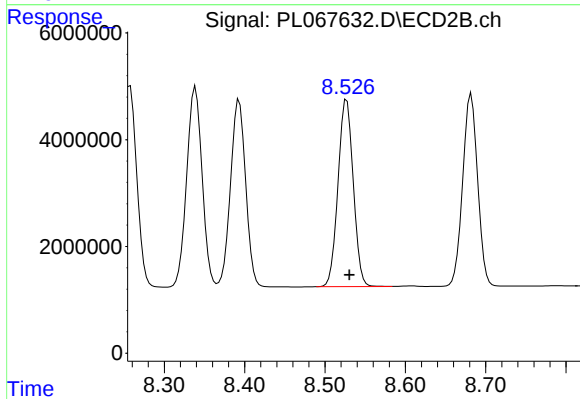

#12 4,4'-DDE


R.T.: 8.527 min
Delta R.T.: -0.003 min
Response: 46308430
Conc: 51.12 ng/ml

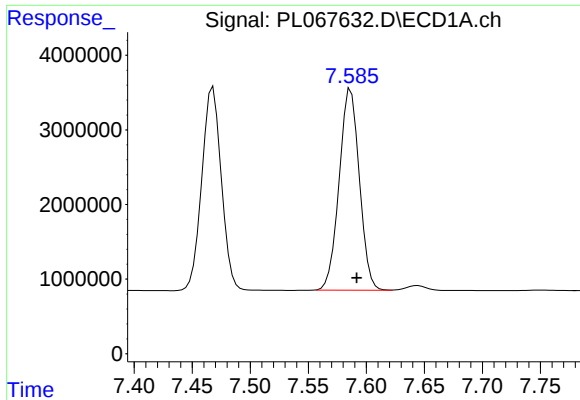

#13 Dieldrin


R.T.: 7.587 min
Delta R.T.: -0.005 min
Response: 32702130
Conc: 46.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

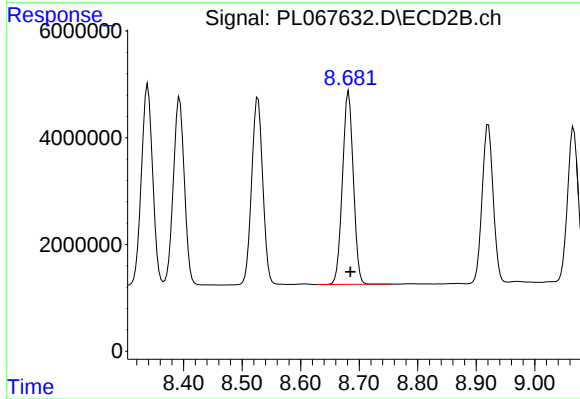


#13 Dieldrin

R.T.: 8.682 min
Delta R.T.: -0.003 min
Response: 46618339
Conc: 51.33 ng/ml

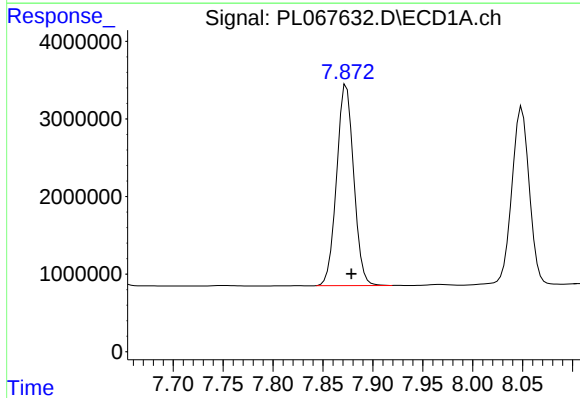


#14 Endrin

R.T.: 7.873 min
Delta R.T.: -0.005 min
Response: 30889494
Conc: 47.11 ng/ml

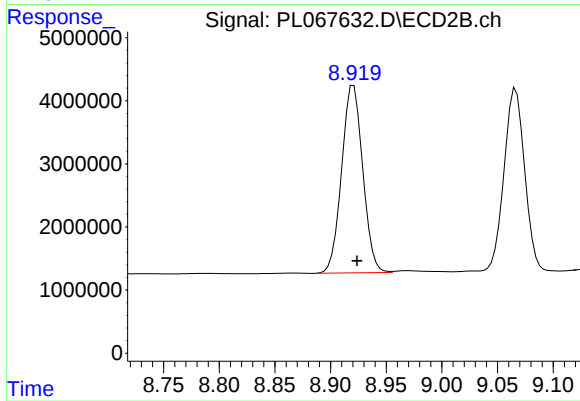

#14 Endrin


R.T.: 8.921 min
Delta R.T.: -0.003 min
Response: 39202868
Conc: 51.25 ng/ml

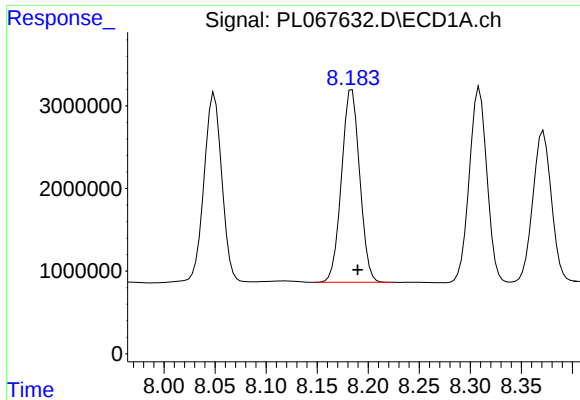

#15 Endosulfan II


R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 28925584
Conc: 46.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

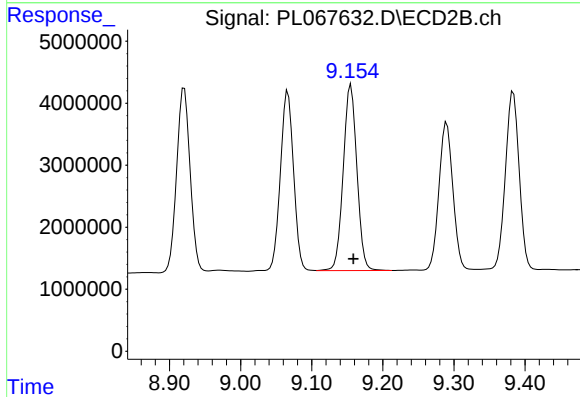


#15 Endosulfan II

R.T.: 9.155 min
Delta R.T.: -0.003 min
Response: 40031421
Conc: 50.21 ng/ml

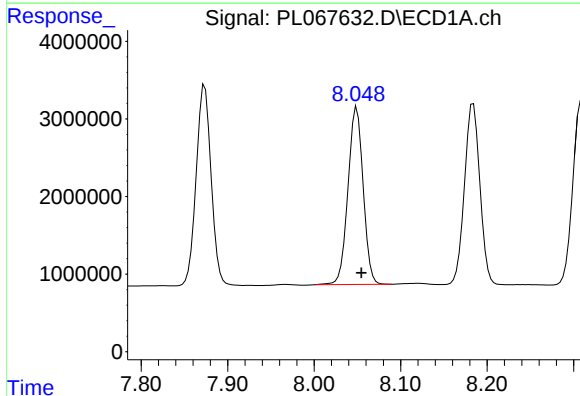


#16 4,4'-DDD

R.T.: 8.049 min
Delta R.T.: -0.005 min
Response: 27744290
Conc: 47.73 ng/ml

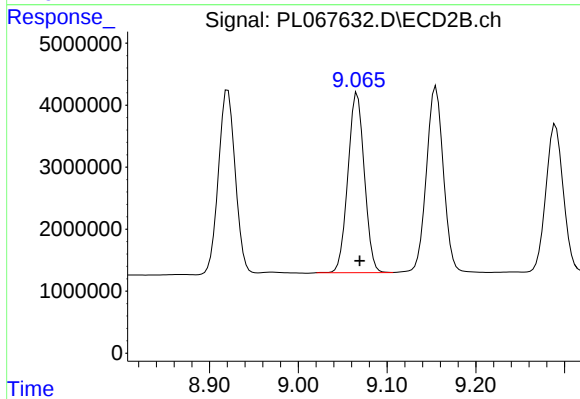

#16 4,4'-DDD


R.T.: 9.066 min
Delta R.T.: -0.003 min
Response: 37305761
Conc: 52.45 ng/ml

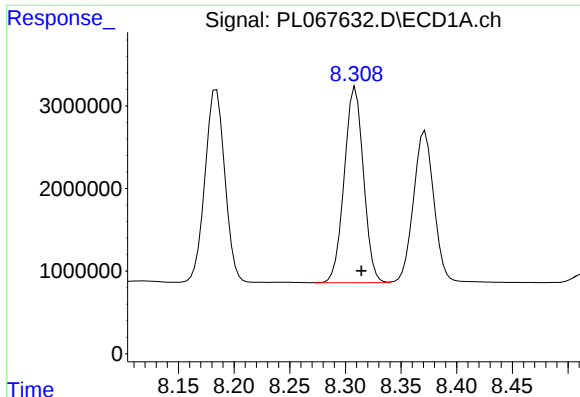

#17 4,4'-DDT


R.T.: 8.309 min
Delta R.T.: -0.005 min
Response: 28423656
Conc: 48.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

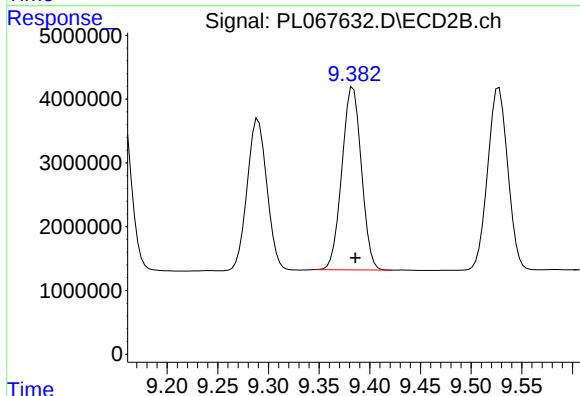


#17 4,4'-DDT

R.T.: 9.384 min
Delta R.T.: -0.002 min
Response: 38352472
Conc: 52.31 ng/ml

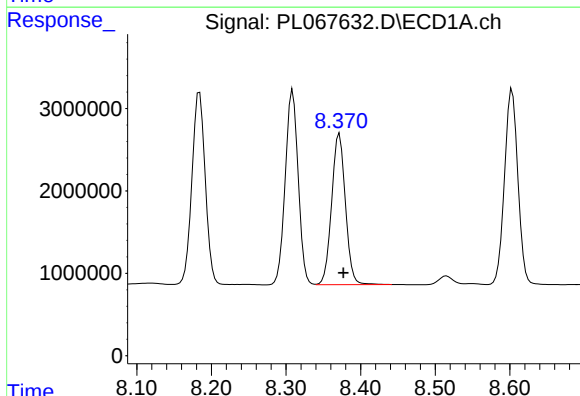


#18 Endrin aldehyde

R.T.: 8.372 min
Delta R.T.: -0.005 min
Response: 23506933
Conc: 46.43 ng/ml

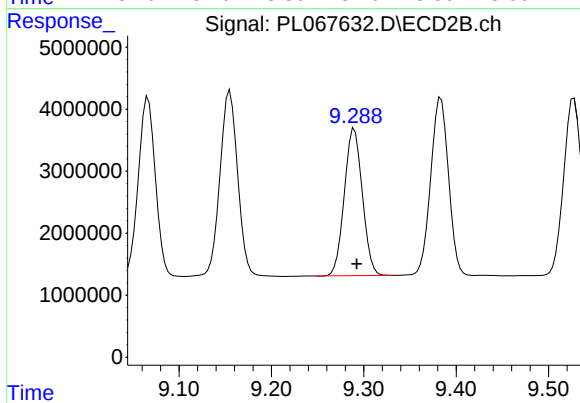

#18 Endrin aldehyde


R.T.: 9.290 min
Delta R.T.: -0.003 min
Response: 32187226
Conc: 50.40 ng/ml

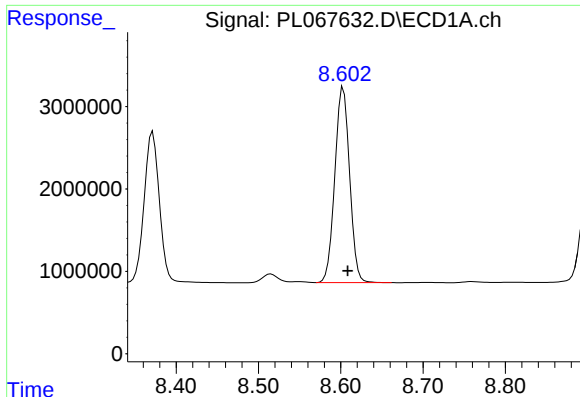

#19 Endosulfan Sulfate


R.T.: 8.603 min
Delta R.T.: -0.005 min
Response: 29562969
Conc: 46.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

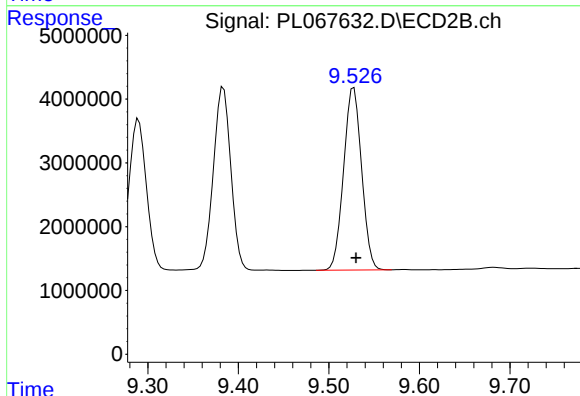


#19 Endosulfan Sulfate

R.T.: 9.528 min
Delta R.T.: -0.003 min
Response: 39485460
Conc: 49.72 ng/ml

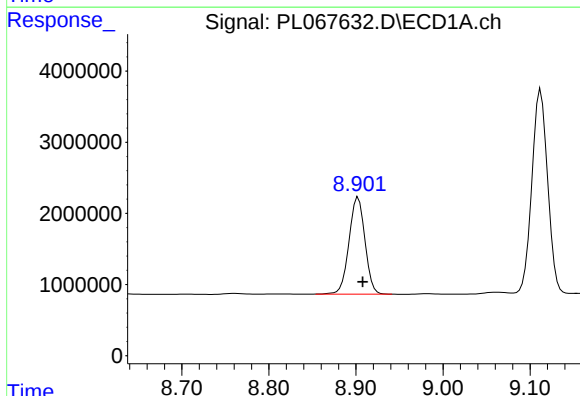


#20 Methoxychlor

R.T.: 8.903 min
Delta R.T.: -0.005 min
Response: 17333574
Conc: 48.76 ng/ml

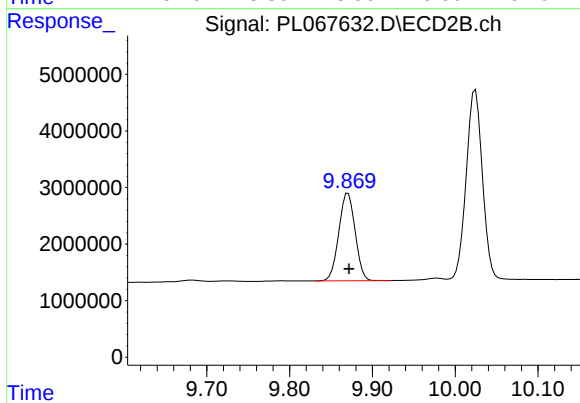

#20 Methoxychlor


R.T.: 9.871 min
Delta R.T.: -0.001 min
Response: 21217610
Conc: 54.57 ng/ml

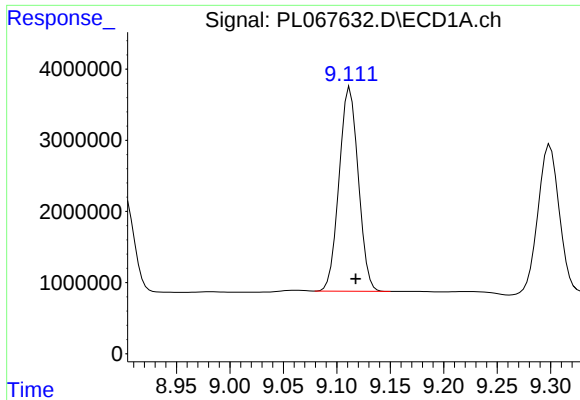

#21 Endrin ketone


R.T.: 9.112 min
Delta R.T.: -0.005 min
Response: 35880840
Conc: 47.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

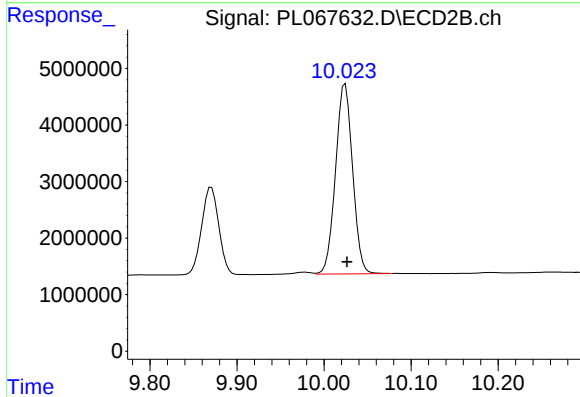


#21 Endrin ketone

R.T.: 10.024 min
Delta R.T.: -0.002 min
Response: 45708768
Conc: 50.43 ng/ml

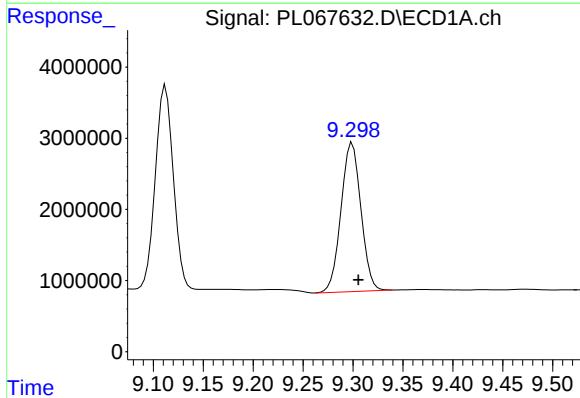


#22 Mirex

R.T.: 9.299 min
Delta R.T.: -0.006 min
Response: 29098156
Conc: 46.20 ng/ml

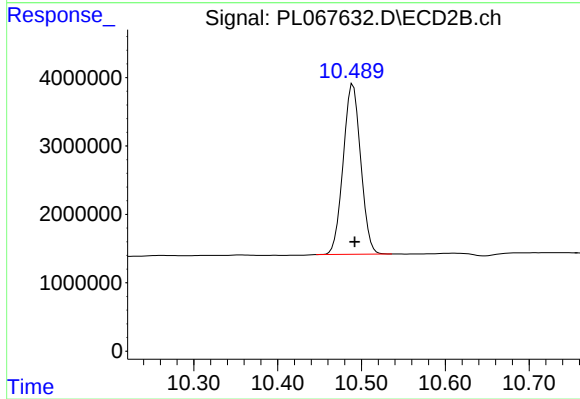

#22 Mirex


R.T.: 10.490 min
Delta R.T.: -0.002 min
Response: 36222693
Conc: 47.91 ng/ml

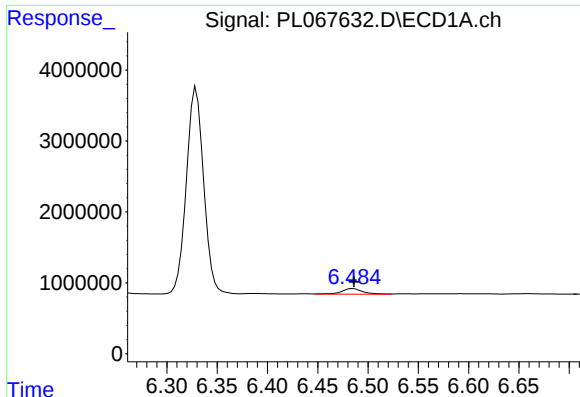

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 1139918
Conc: 42.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

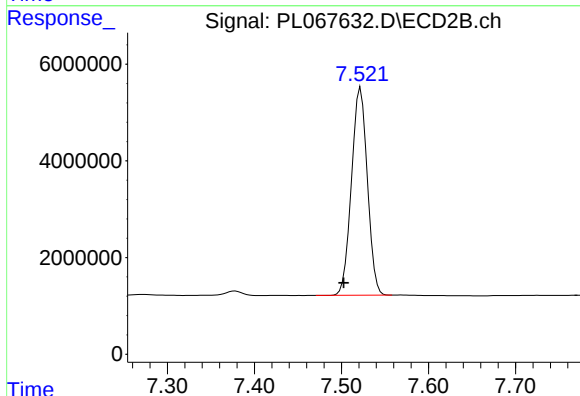


#24 Chlordane-2

R.T.: 7.522 min
Delta R.T.: 0.019 min
Response: 54471110
Conc: 1494.56 ng/ml

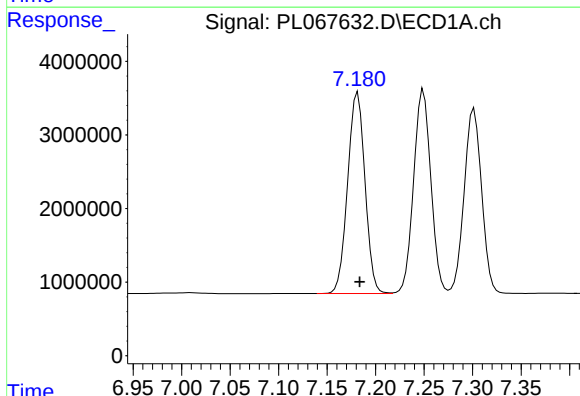


#25 Chlordane-3

R.T.: 7.182 min
Delta R.T.: -0.002 min
Response: 34022009
Conc: 506.35 ng/ml

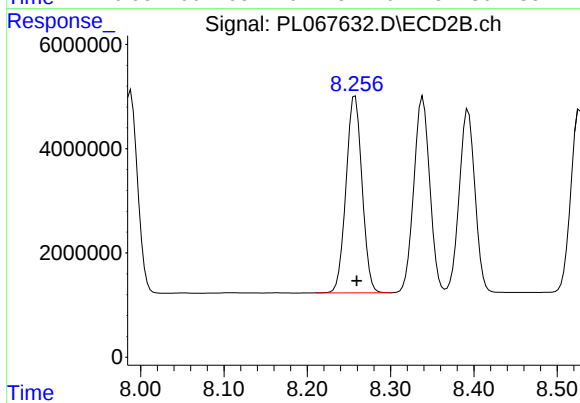

#25 Chlordane-3


R.T.: 8.257 min
Delta R.T.: -0.002 min
Response: 50375416
Conc: 376.39 ng/ml

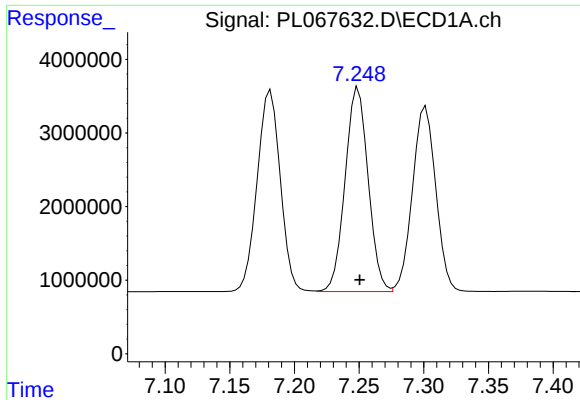

#26 Chlordane-4


R.T.: 7.249 min
Delta R.T.: -0.001 min
Response: 34292785
Conc: 469.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

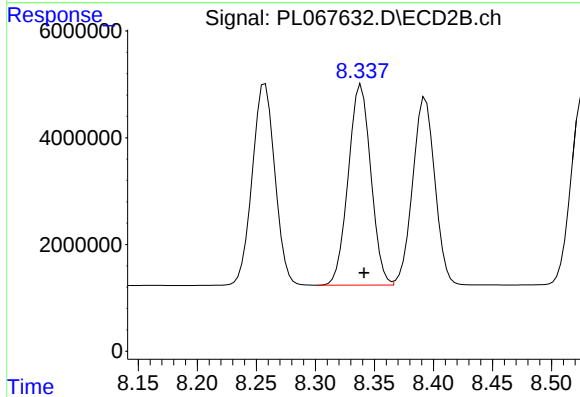


#26 Chlordane-4

R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 50063799
Conc: 308.84 ng/ml

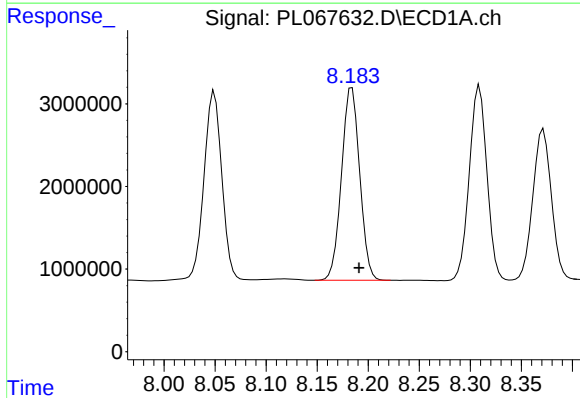


#27 Chlordane-5

R.T.: 8.184 min
Delta R.T.: -0.007 min
Response: 28925584
Conc: 1322.07 ng/ml

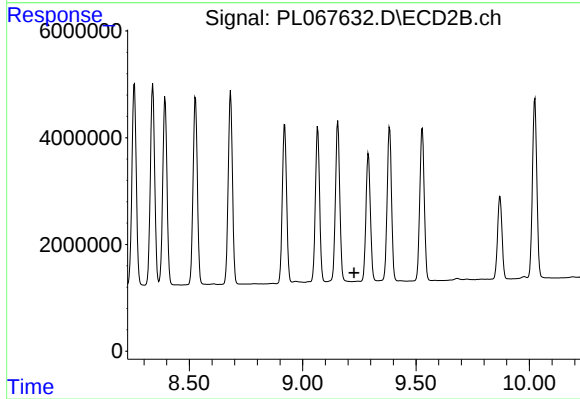

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

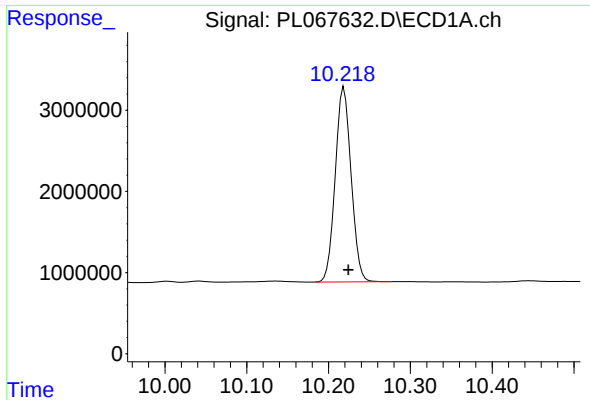

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 32281226
Conc: 45.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

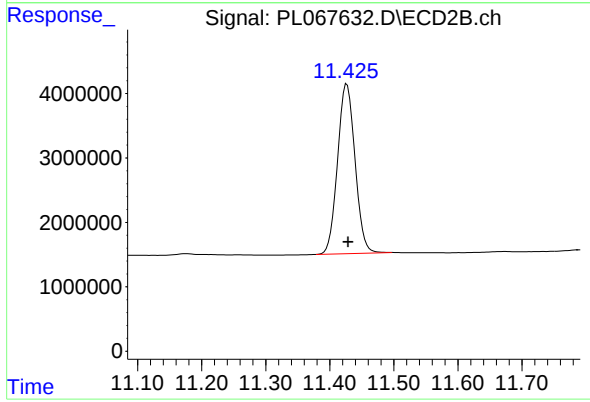

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 49902868
Conc: 50.10 ng/ml