

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 22:40
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:36:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	26913824	49532911	48.953	52.542
28)	SA Decachlor...	10.220	11.427	31921184	50452875	45.043	50.653
Target Compounds							
2)	A alpha-BHC	5.177	6.109	38342837	66890424	52.132	54.098
3)	MA gamma-BHC...	5.597	6.505	36794571	63100107	49.097	53.522
4)	MA Heptachlor	6.008	7.152	37875346	60826515	50.212	54.542
5)	MB Aldrin	6.329	7.522	36195320	56286666	49.192	52.004
6)	B beta-BHC	5.980	6.760	17600601	29254980	49.190	53.875
7)	B delta-BHC	6.236	7.026	36790961	61592423	49.813	52.396
8)	B Heptachlo...	6.902	7.988	33803063	52772987	48.313	52.680
9)	A Endosulfan I	7.302	8.393	32111640	46432998	47.766	50.850
10)	B gamma-Chl...	7.181	8.258	34791687	51159700	47.988	50.670
11)	B alpha-Chl...	7.250	8.338	34971797	50518557	47.768	50.037
12)	B 4,4'-DDE	7.467	8.527	32284901	46377117	48.526	51.193
13)	MA Dieldrin	7.586	8.682	31698843	46378946	45.219	51.065
14)	MA Endrin	7.873	8.921	31301784	38944028	47.741	50.914
15)	B Endosulfa...	8.184	9.155	29136637	40377147	47.310	50.642
16)	A 4,4'-DDD	8.050	9.066	28022972	37848220	48.210	53.217
17)	MA 4,4'-DDT	8.309	9.383	28175352	38019091	48.421	51.857
18)	B Endrin al...	8.371	9.290	23680176	32394913	46.773	50.726
19)	B Endosulfa...	8.603	9.528	29594820	39565352	46.621	49.820
20)	A Methoxychlor	8.902	9.870	17165463	21056654	48.290	54.158
21)	B Endrin ke...	9.113	10.024	35811544	45680997	47.036	50.400
22)	Mirex	9.299	10.490	29012781	36548730	46.068	48.345
24)	Chlordane-2	6.485	7.522f	1868909	56286666	69.792	1544.378 #
25)	Chlordane-3	7.181	8.258	34791687	51159700	517.806	382.251 #
26)	Chlordane-4	7.250	8.338	34971797	50518557	478.550	311.650 #
27)	Chlordane-5	8.184	0.000	29136637	0	1331.712	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 22:40
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:36:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

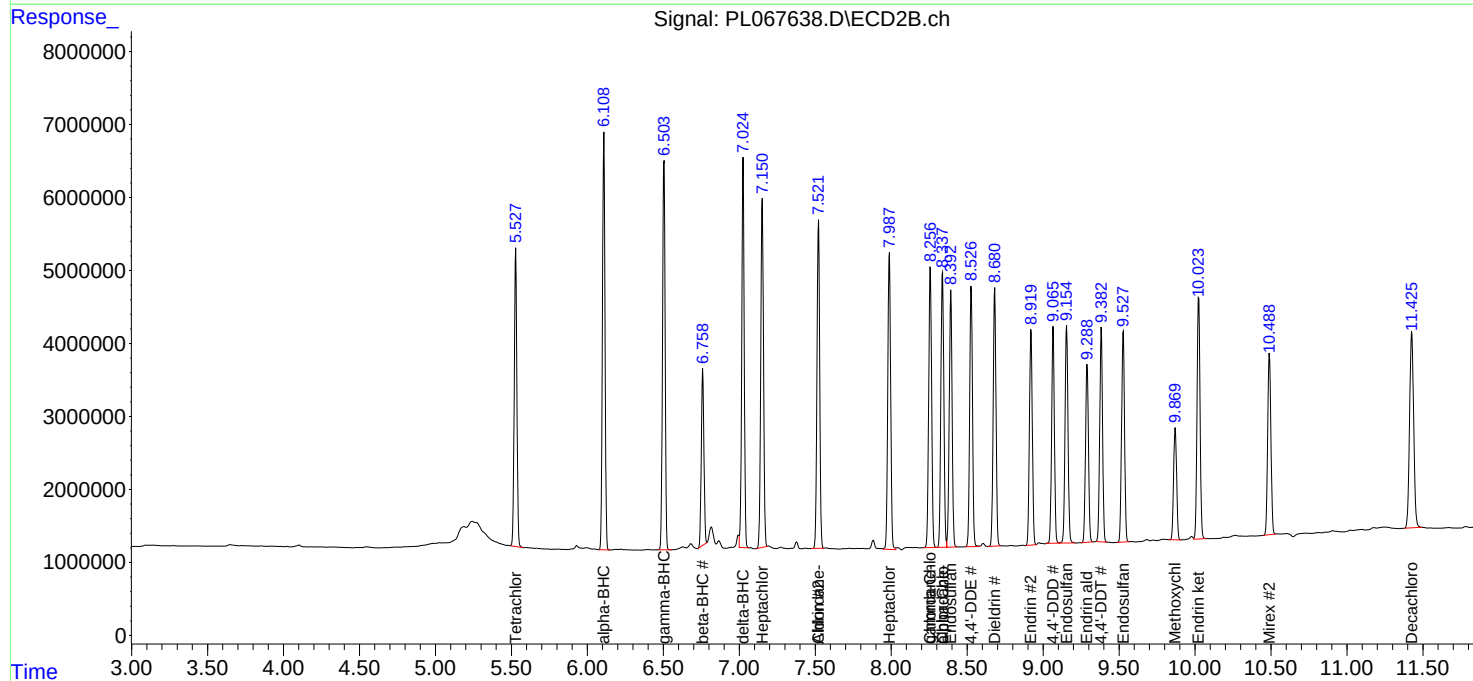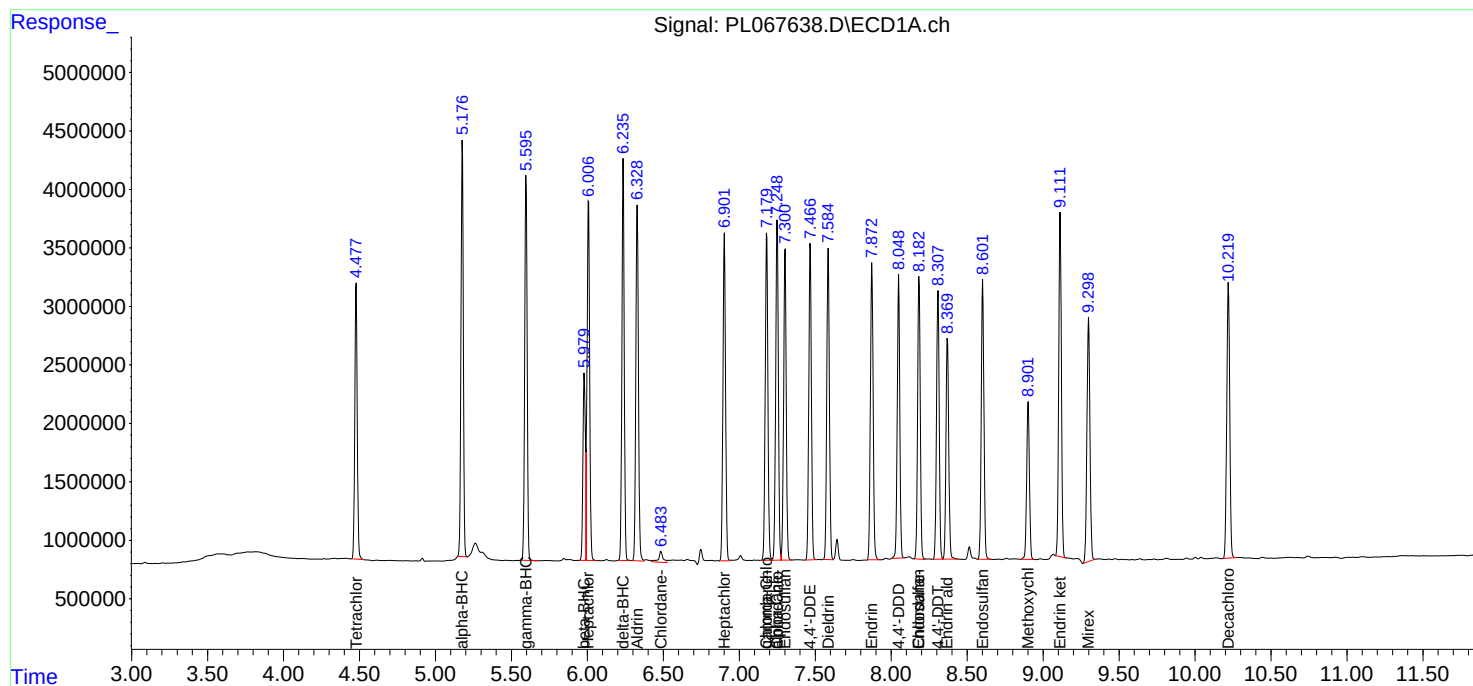


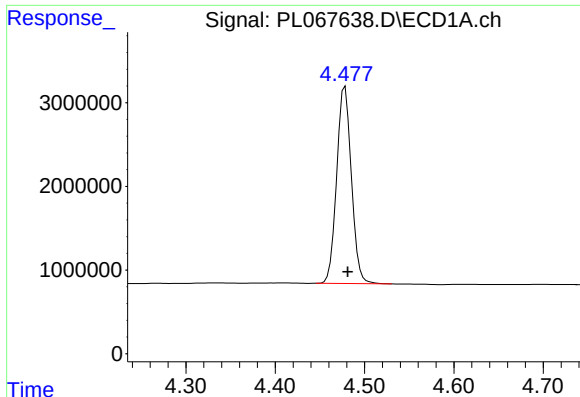

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 26913824
Conc: 48.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

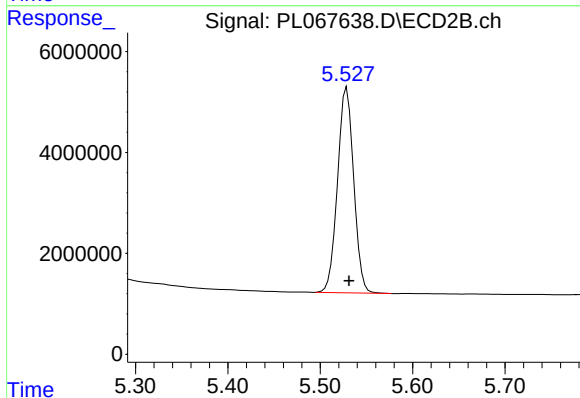


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 49532911
Conc: 52.54 ng/ml

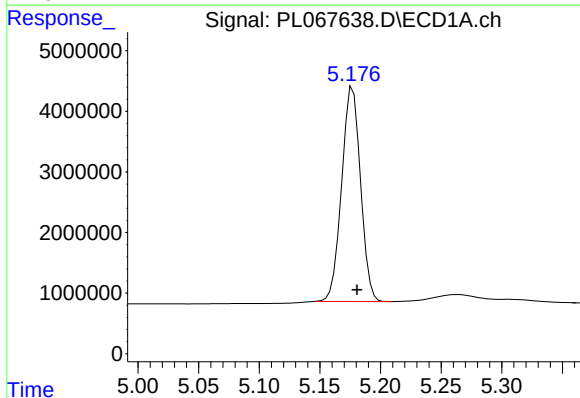


#2 alpha-BHC

R.T.: 5.177 min
Delta R.T.: -0.003 min
Response: 38342837
Conc: 52.13 ng/ml

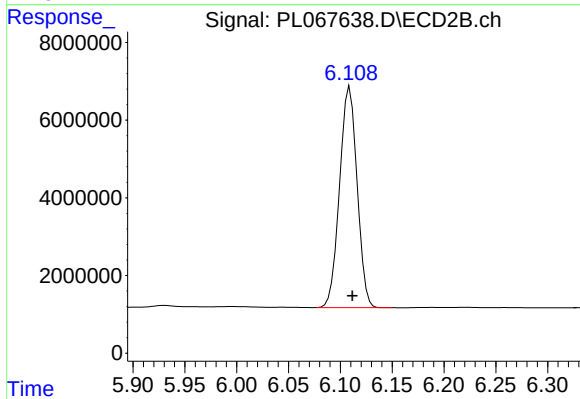

#2 alpha-BHC


R.T.: 6.109 min
Delta R.T.: -0.002 min
Response: 66890424
Conc: 54.10 ng/ml

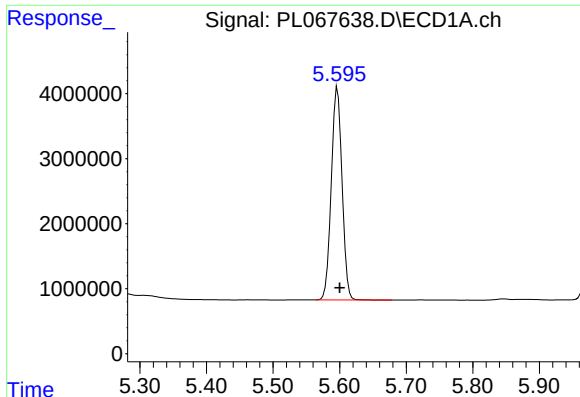

#3 gamma-BHC (Lindane)


R.T.: 5.597 min
Delta R.T.: -0.003 min
Response: 36794571
Conc: 49.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

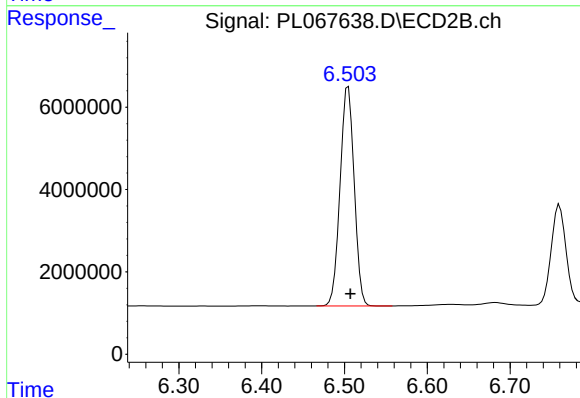


#3 gamma-BHC (Lindane)

R.T.: 6.505 min
Delta R.T.: -0.003 min
Response: 63100107
Conc: 53.52 ng/ml

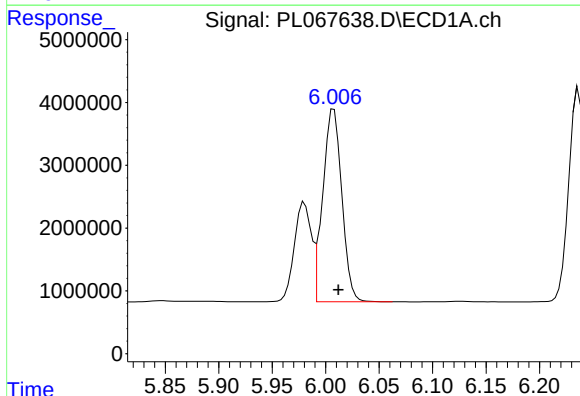


#4 Heptachlor

R.T.: 6.008 min
Delta R.T.: -0.004 min
Response: 37875346
Conc: 50.21 ng/ml

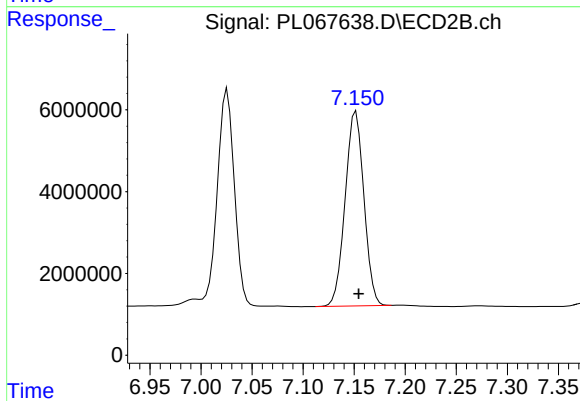

#4 Heptachlor


R.T.: 7.152 min
Delta R.T.: -0.003 min
Response: 60826515
Conc: 54.54 ng/ml

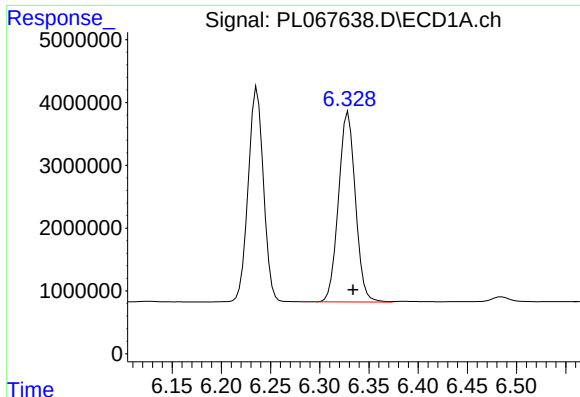

#5 Aldrin


R.T.: 6.329 min
Delta R.T.: -0.005 min
Response: 36195320
Conc: 49.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

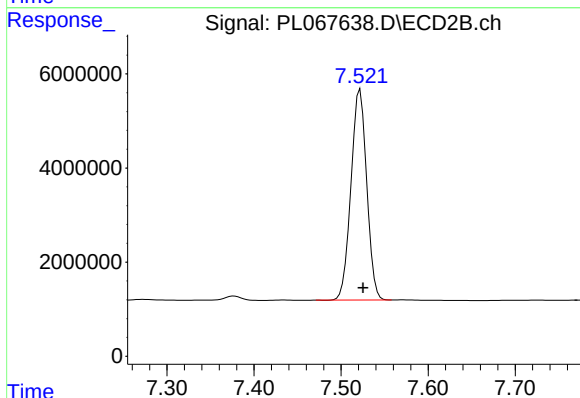


#5 Aldrin

R.T.: 7.522 min
Delta R.T.: -0.003 min
Response: 56286666
Conc: 52.00 ng/ml

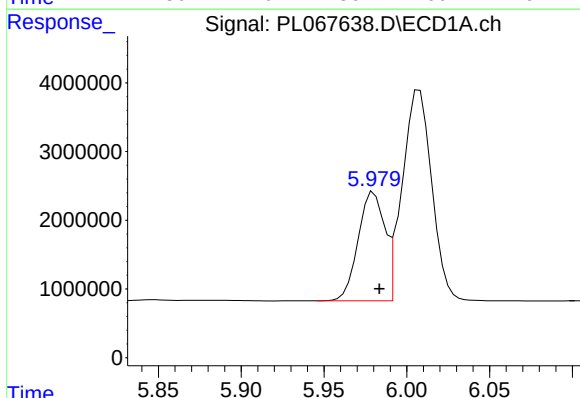


#6 beta-BHC

R.T.: 5.980 min
Delta R.T.: -0.003 min
Response: 17600601
Conc: 49.19 ng/ml

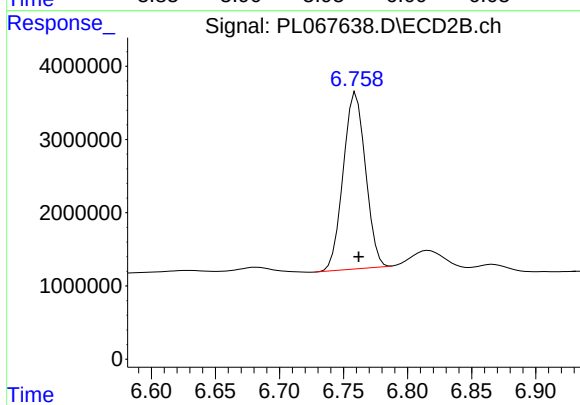

#6 beta-BHC


R.T.: 6.760 min
Delta R.T.: -0.002 min
Response: 29254980
Conc: 53.88 ng/ml

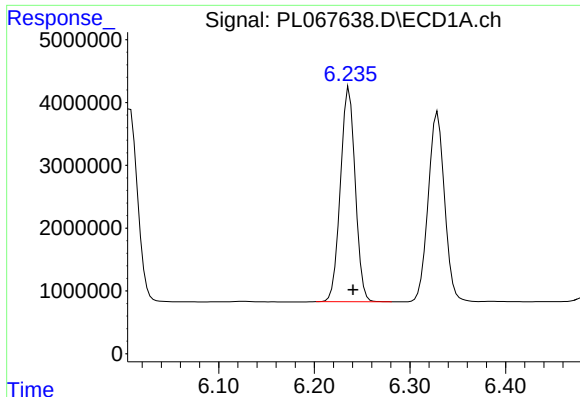

#7 delta-BHC


R.T.: 6.236 min
Delta R.T.: -0.004 min
Response: 36790961
Conc: 49.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

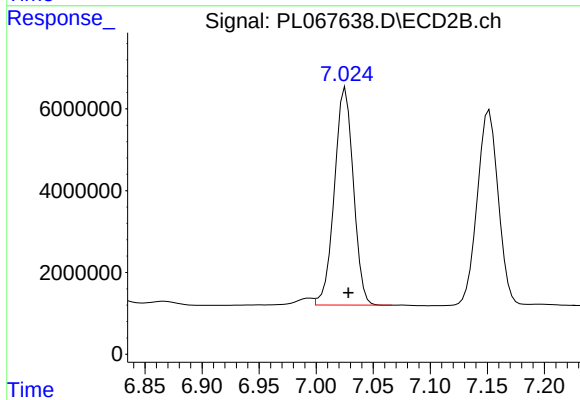


#7 delta-BHC

R.T.: 7.026 min
Delta R.T.: -0.002 min
Response: 61592423
Conc: 52.40 ng/ml

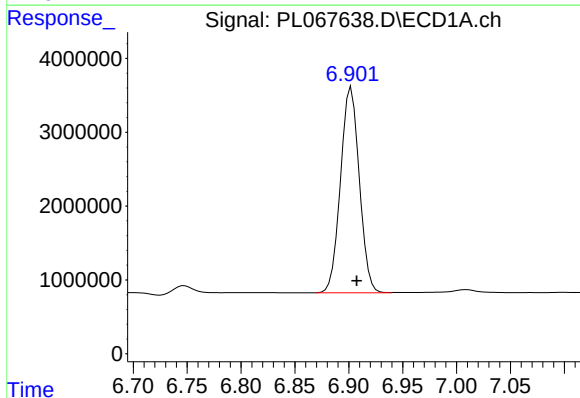


#8 Heptachlor epoxide

R.T.: 6.902 min
Delta R.T.: -0.005 min
Response: 33803063
Conc: 48.31 ng/ml

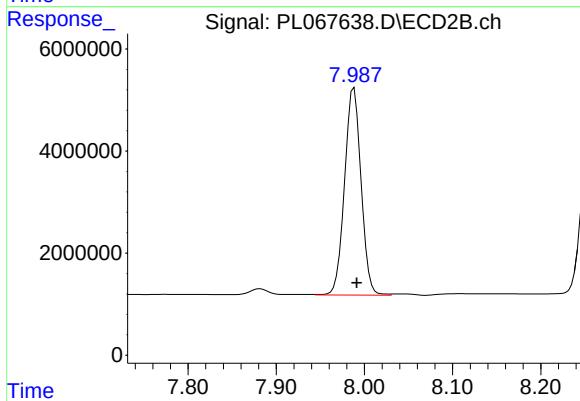

#8 Heptachlor epoxide


R.T.: 7.988 min
Delta R.T.: -0.003 min
Response: 52772987
Conc: 52.68 ng/ml

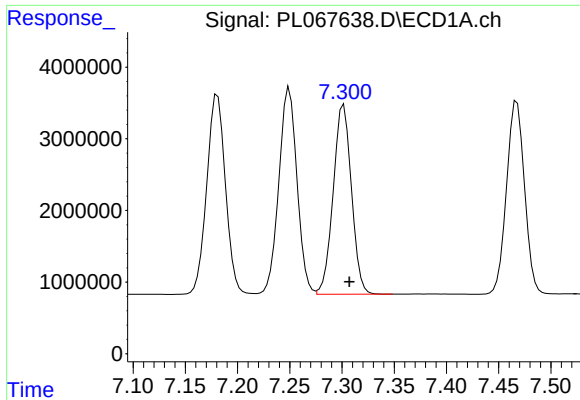

#9 Endosulfan I


R.T.: 7.302 min
Delta R.T.: -0.005 min
Response: 32111640
Conc: 47.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

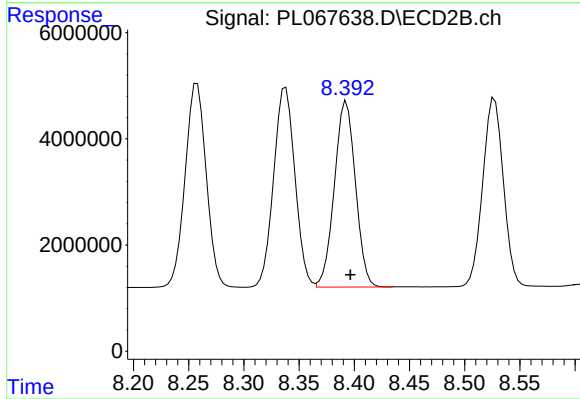


#9 Endosulfan I

R.T.: 8.393 min
Delta R.T.: -0.004 min
Response: 46432998
Conc: 50.85 ng/ml

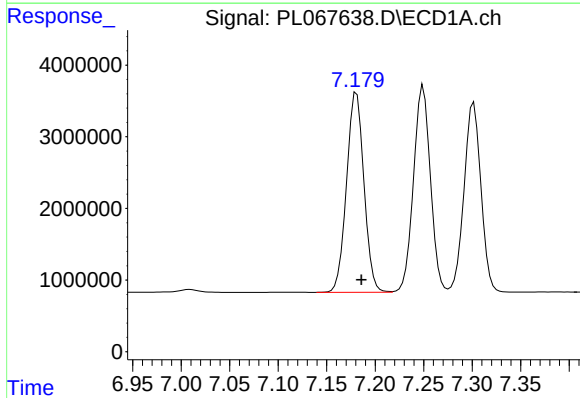


#10 gamma-Chlordane

R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 34791687
Conc: 47.99 ng/ml

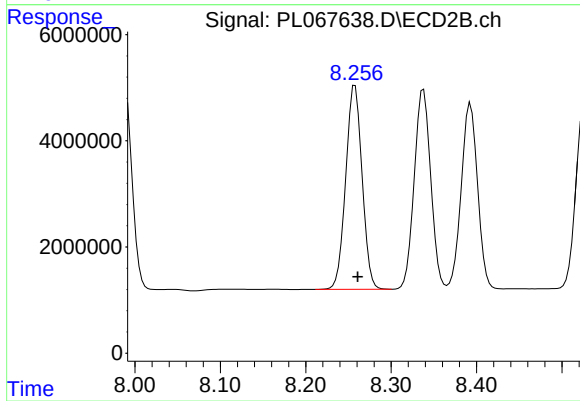

#10 gamma-Chlordane


R.T.: 8.258 min
Delta R.T.: -0.003 min
Response: 51159700
Conc: 50.67 ng/ml

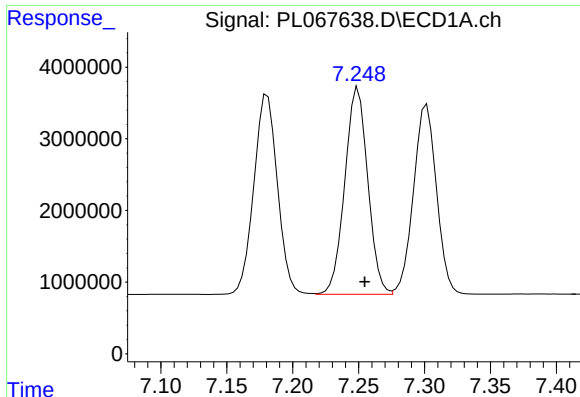

#11 alpha-Chlordane


R.T.: 7.250 min
Delta R.T.: -0.005 min
Response: 34971797
Conc: 47.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

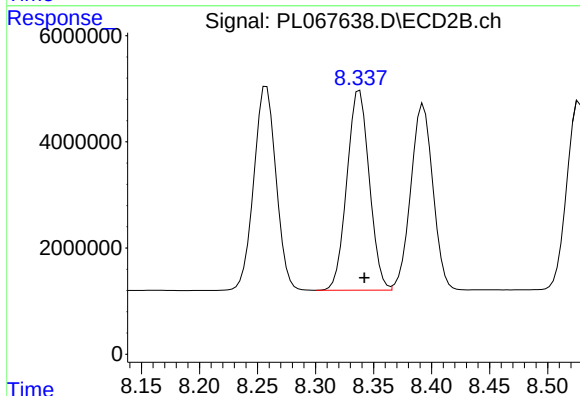


#11 alpha-Chlordane

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 50518557
Conc: 50.04 ng/ml

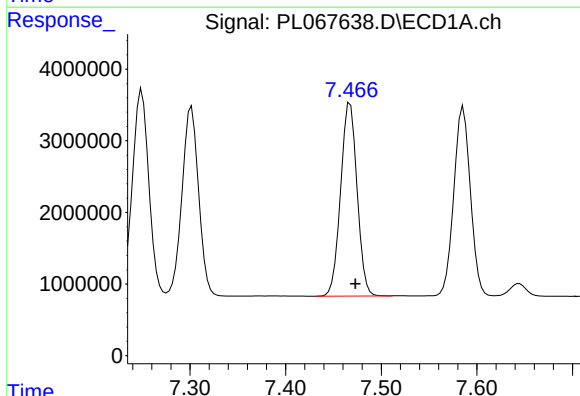


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 32284901
Conc: 48.53 ng/ml

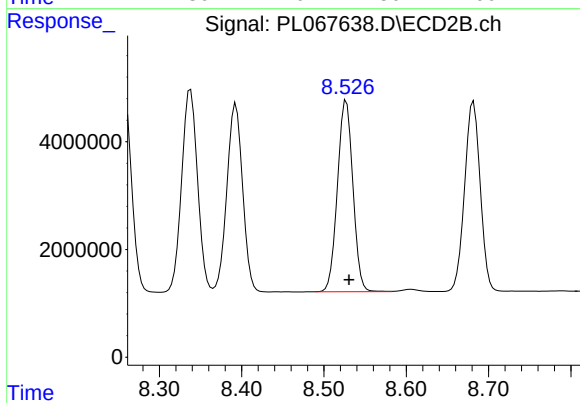

#12 4,4'-DDE


R.T.: 8.527 min
Delta R.T.: -0.003 min
Response: 46377117
Conc: 51.19 ng/ml

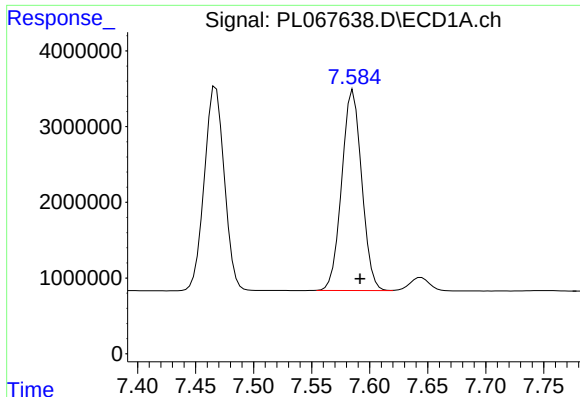

#13 Dieldrin


R.T.: 7.586 min
Delta R.T.: -0.006 min
Response: 31698843
Conc: 45.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

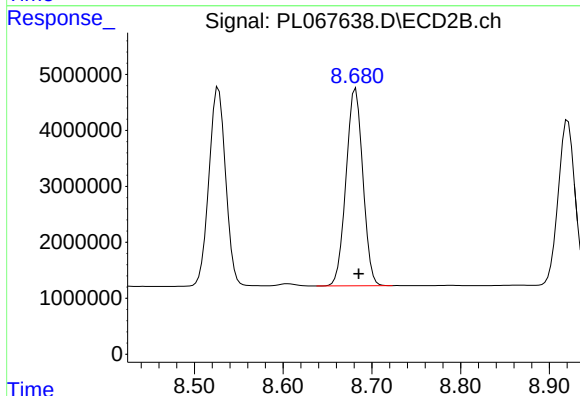


#13 Dieldrin

R.T.: 8.682 min
Delta R.T.: -0.003 min
Response: 46378946
Conc: 51.07 ng/ml

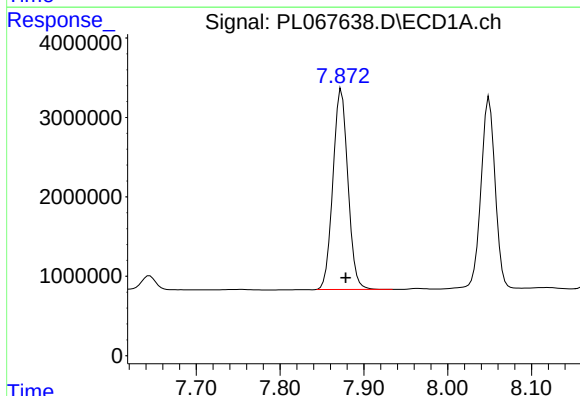


#14 Endrin

R.T.: 7.873 min
Delta R.T.: -0.005 min
Response: 31301784
Conc: 47.74 ng/ml

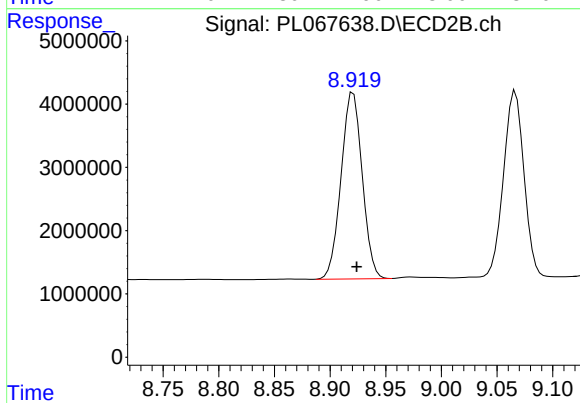

#14 Endrin


R.T.: 8.921 min
Delta R.T.: -0.003 min
Response: 38944028
Conc: 50.91 ng/ml

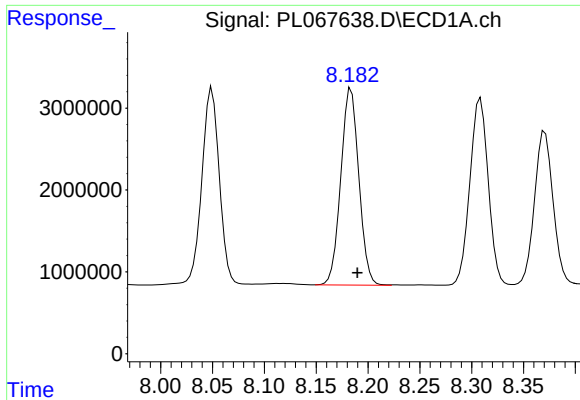

#15 Endosulfan II


R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 29136637
Conc: 47.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

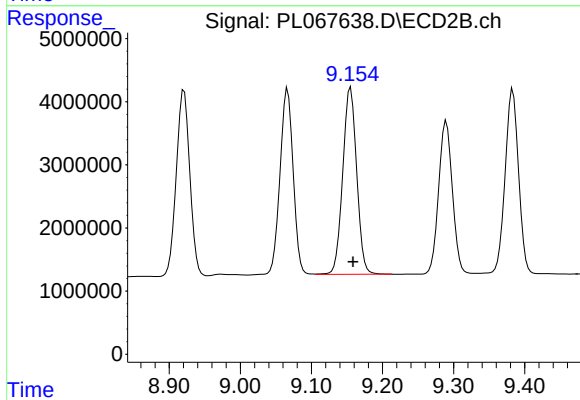


#15 Endosulfan II

R.T.: 9.155 min
Delta R.T.: -0.003 min
Response: 40377147
Conc: 50.64 ng/ml

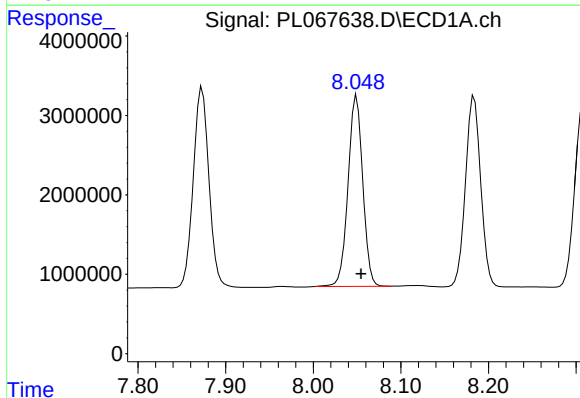


#16 4,4'-DDD

R.T.: 8.050 min
Delta R.T.: -0.005 min
Response: 28022972
Conc: 48.21 ng/ml

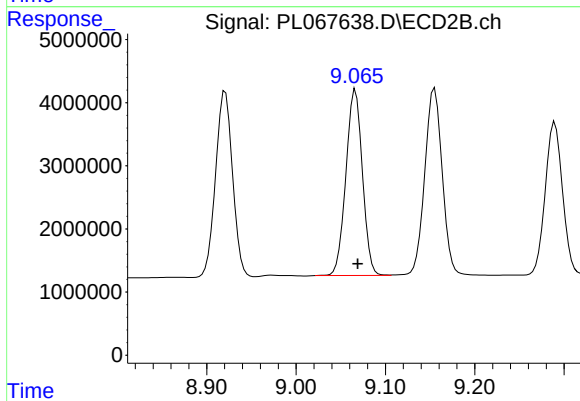

#16 4,4'-DDD


R.T.: 9.066 min
Delta R.T.: -0.003 min
Response: 37848220
Conc: 53.22 ng/ml

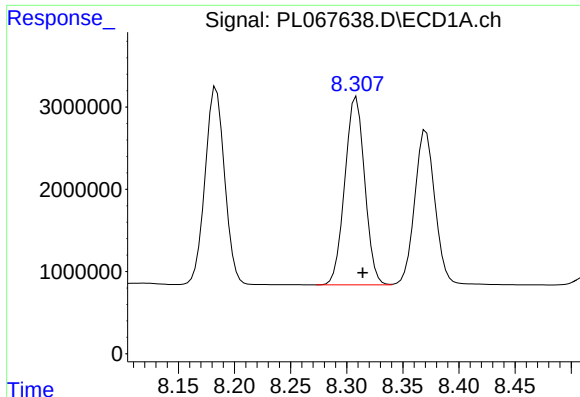

#17 4,4'-DDT


R.T.: 8.309 min
Delta R.T.: -0.006 min
Response: 28175352
Conc: 48.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

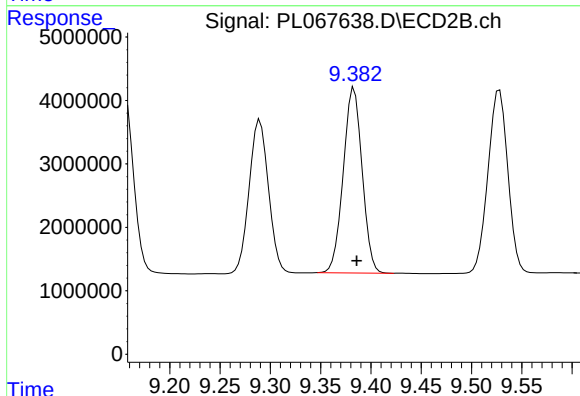


#17 4,4'-DDT

R.T.: 9.383 min
Delta R.T.: -0.003 min
Response: 38019091
Conc: 51.86 ng/ml

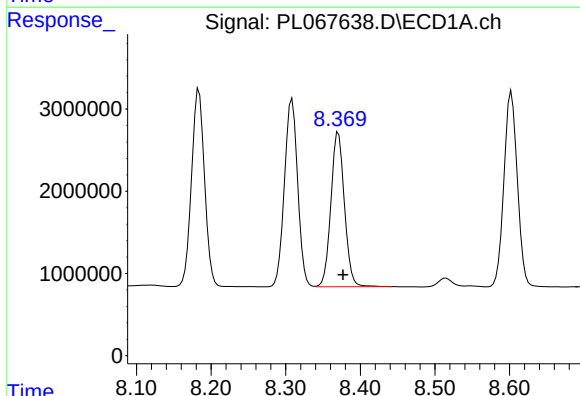


#18 Endrin aldehyde

R.T.: 8.371 min
Delta R.T.: -0.006 min
Response: 23680176
Conc: 46.77 ng/ml

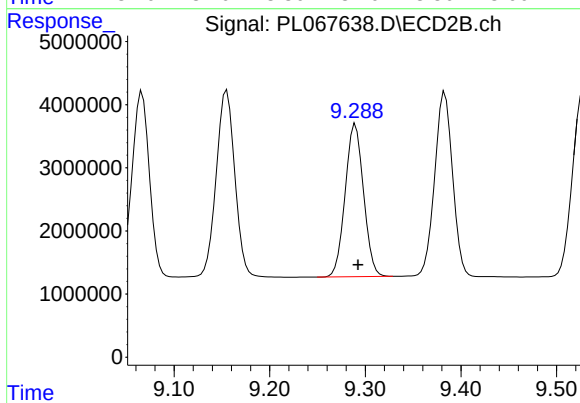

#18 Endrin aldehyde


R.T.: 9.290 min
Delta R.T.: -0.003 min
Response: 32394913
Conc: 50.73 ng/ml

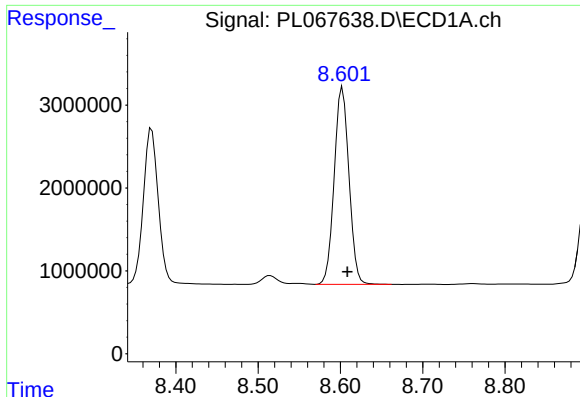

#19 Endosulfan Sulfate


R.T.: 8.603 min
Delta R.T.: -0.006 min
Response: 29594820
Conc: 46.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

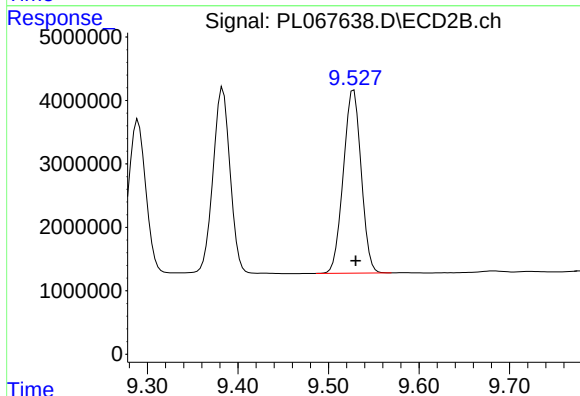


#19 Endosulfan Sulfate

R.T.: 9.528 min
Delta R.T.: -0.002 min
Response: 39565352
Conc: 49.82 ng/ml

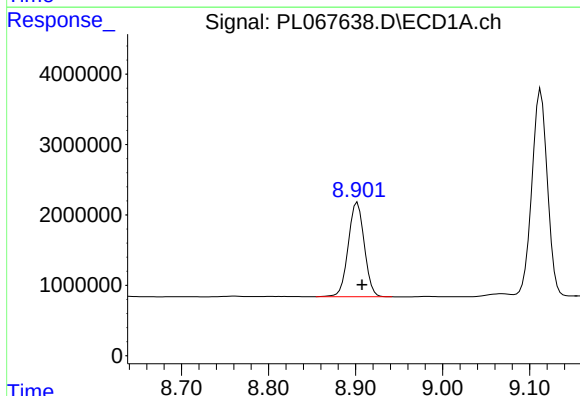


#20 Methoxychlor

R.T.: 8.902 min
Delta R.T.: -0.006 min
Response: 17165463
Conc: 48.29 ng/ml

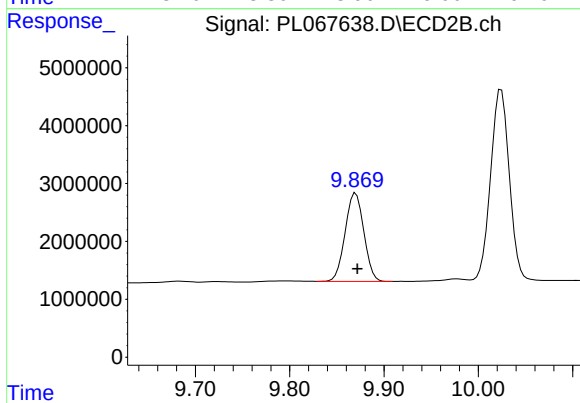

#20 Methoxychlor


R.T.: 9.870 min
Delta R.T.: -0.002 min
Response: 21056654
Conc: 54.16 ng/ml

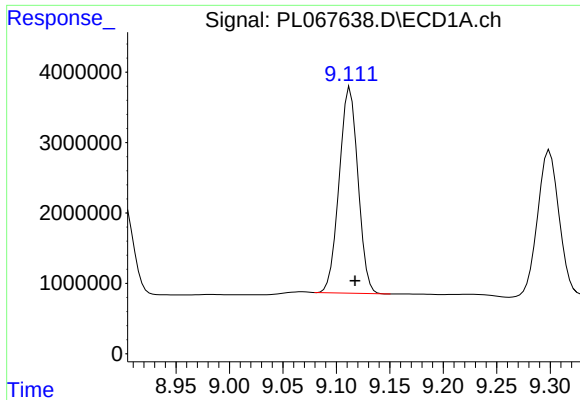

#21 Endrin ketone


R.T.: 9.113 min
Delta R.T.: -0.005 min
Response: 35811544
Conc: 47.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

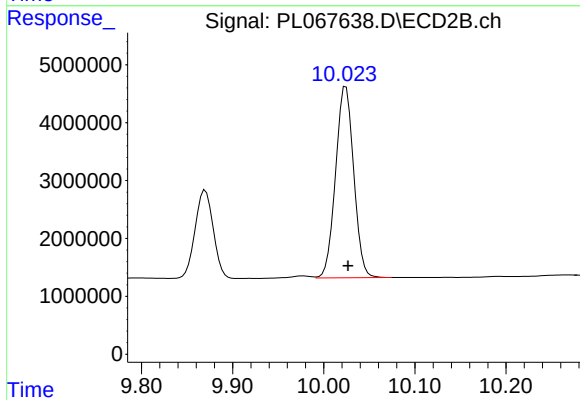


#21 Endrin ketone

R.T.: 10.024 min
Delta R.T.: -0.002 min
Response: 45680997
Conc: 50.40 ng/ml

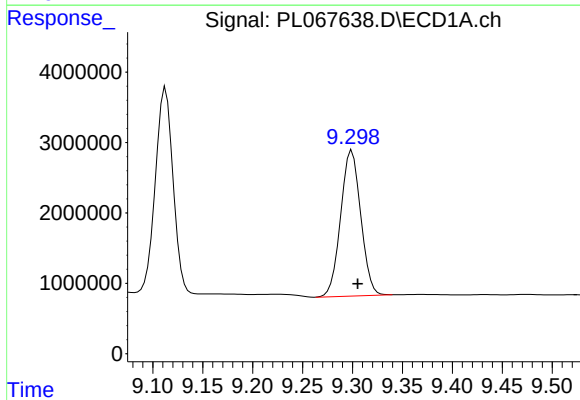


#22 Mirex

R.T.: 9.299 min
Delta R.T.: -0.006 min
Response: 29012781
Conc: 46.07 ng/ml

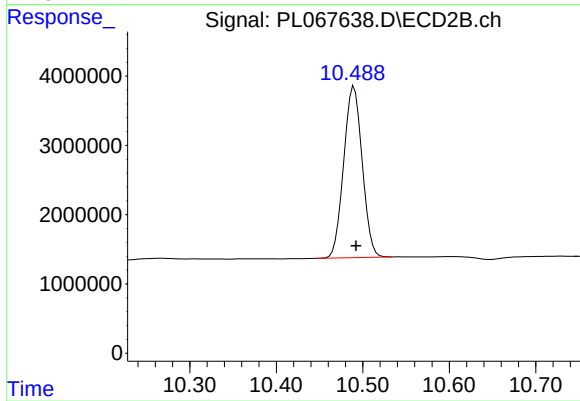

#22 Mirex


R.T.: 10.490 min
Delta R.T.: -0.002 min
Response: 36548730
Conc: 48.34 ng/ml

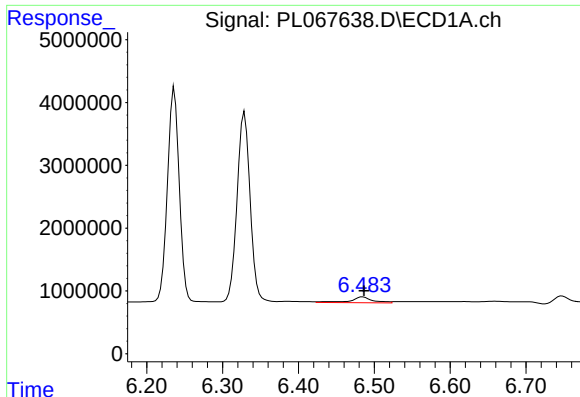

#24 Chlordane-2


R.T.: 6.485 min
Delta R.T.: -0.001 min
Response: 1868909
Conc: 69.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

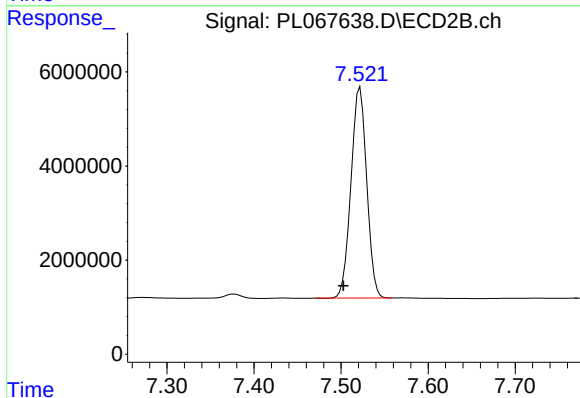


#24 Chlordane-2

R.T.: 7.522 min
Delta R.T.: 0.019 min
Response: 5628666
Conc: 1544.38 ng/ml

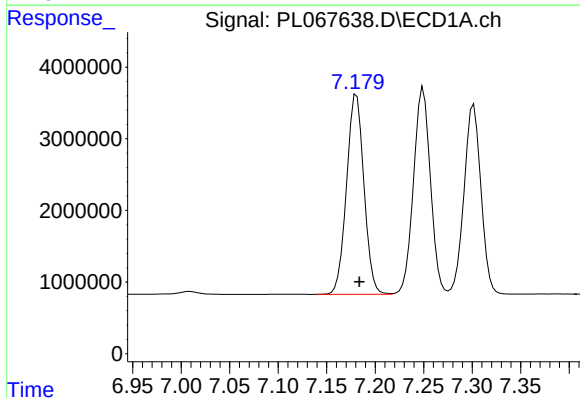


#25 Chlordane-3

R.T.: 7.181 min
Delta R.T.: -0.003 min
Response: 34791687
Conc: 517.81 ng/ml

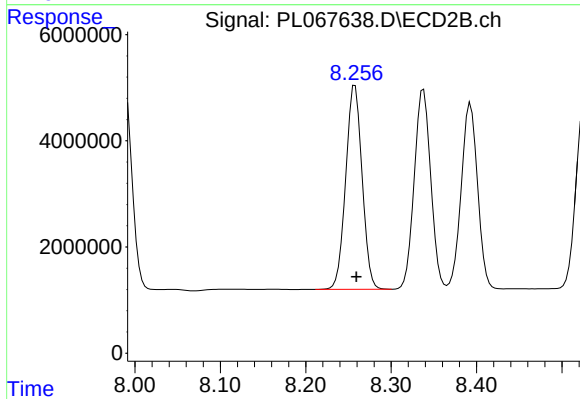

#25 Chlordane-3


R.T.: 8.258 min
Delta R.T.: -0.002 min
Response: 51159700
Conc: 382.25 ng/ml

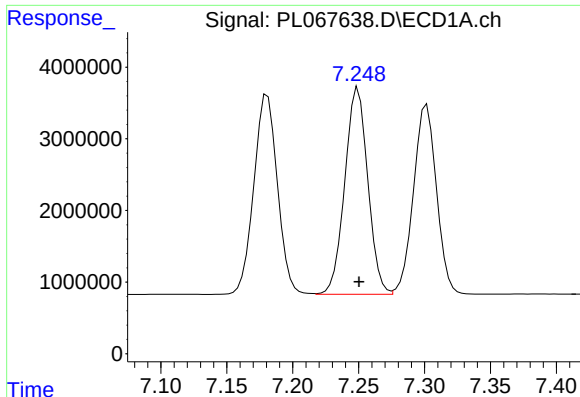

#26 Chlordane-4


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 34971797
Conc: 478.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

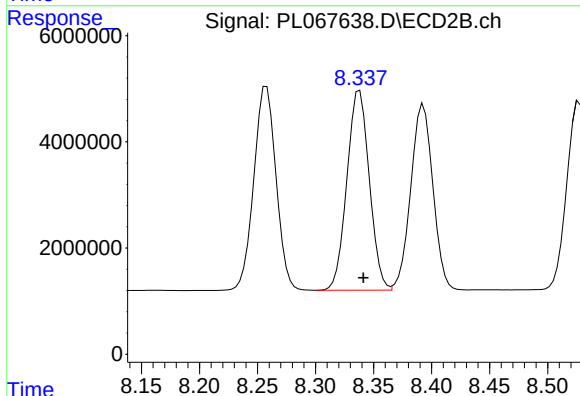


#26 Chlordane-4

R.T.: 8.338 min
Delta R.T.: -0.003 min
Response: 50518557
Conc: 311.65 ng/ml

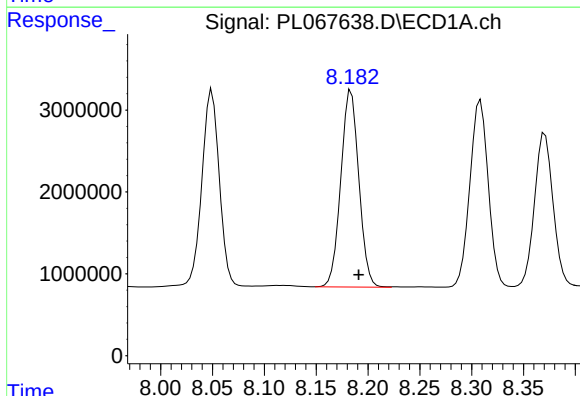


#27 Chlordane-5

R.T.: 8.184 min
Delta R.T.: -0.007 min
Response: 29136637
Conc: 1331.71 ng/ml

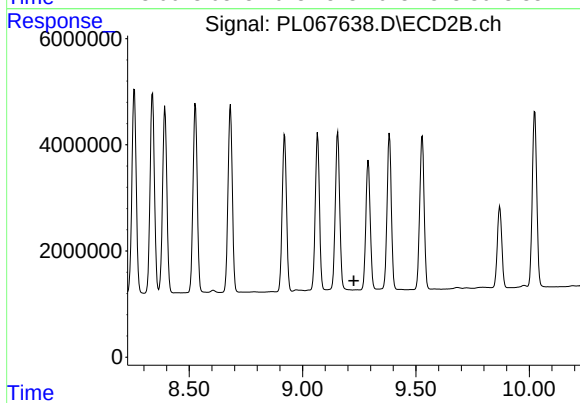

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

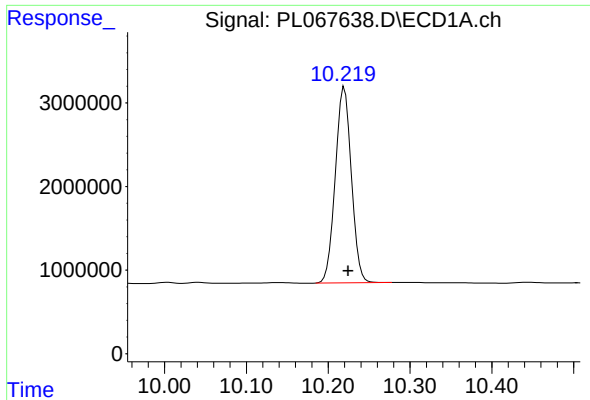

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 31921184
Conc: 45.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

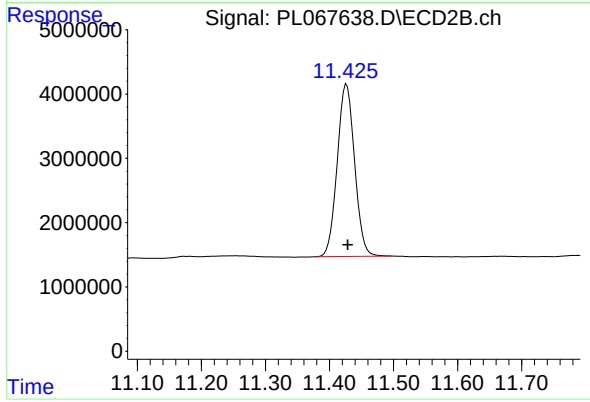

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 50452875
Conc: 50.65 ng/ml