

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 17:57
 Operator : AR\AJ
 Sample : M2709-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:33:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.529	8152621	15171586	14.829	16.093
28) SA Decachlor...	10.219	11.427	8803410	14891587	12.422	14.951
Target Compounds						
12) B 4,4'-DDE	7.466	8.528	795222	2237486	1.195m	2.470 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :

ECD_L

ClientSampleId :

0223-COMP-O(DISCRETE-CL-23

Manual Integrations

APPROVED

Ankita

6/21/2021 12:10:03 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 17:57
Operator : AR\AJ
Sample : M2709-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:33:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Instrument :


ECD_L


ClientSampleId :

0223-COMP-O(DISCRETE-CL-23

Manual Integrations
APPROVEDAnkita
6/21/2021 12:10:03 PM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

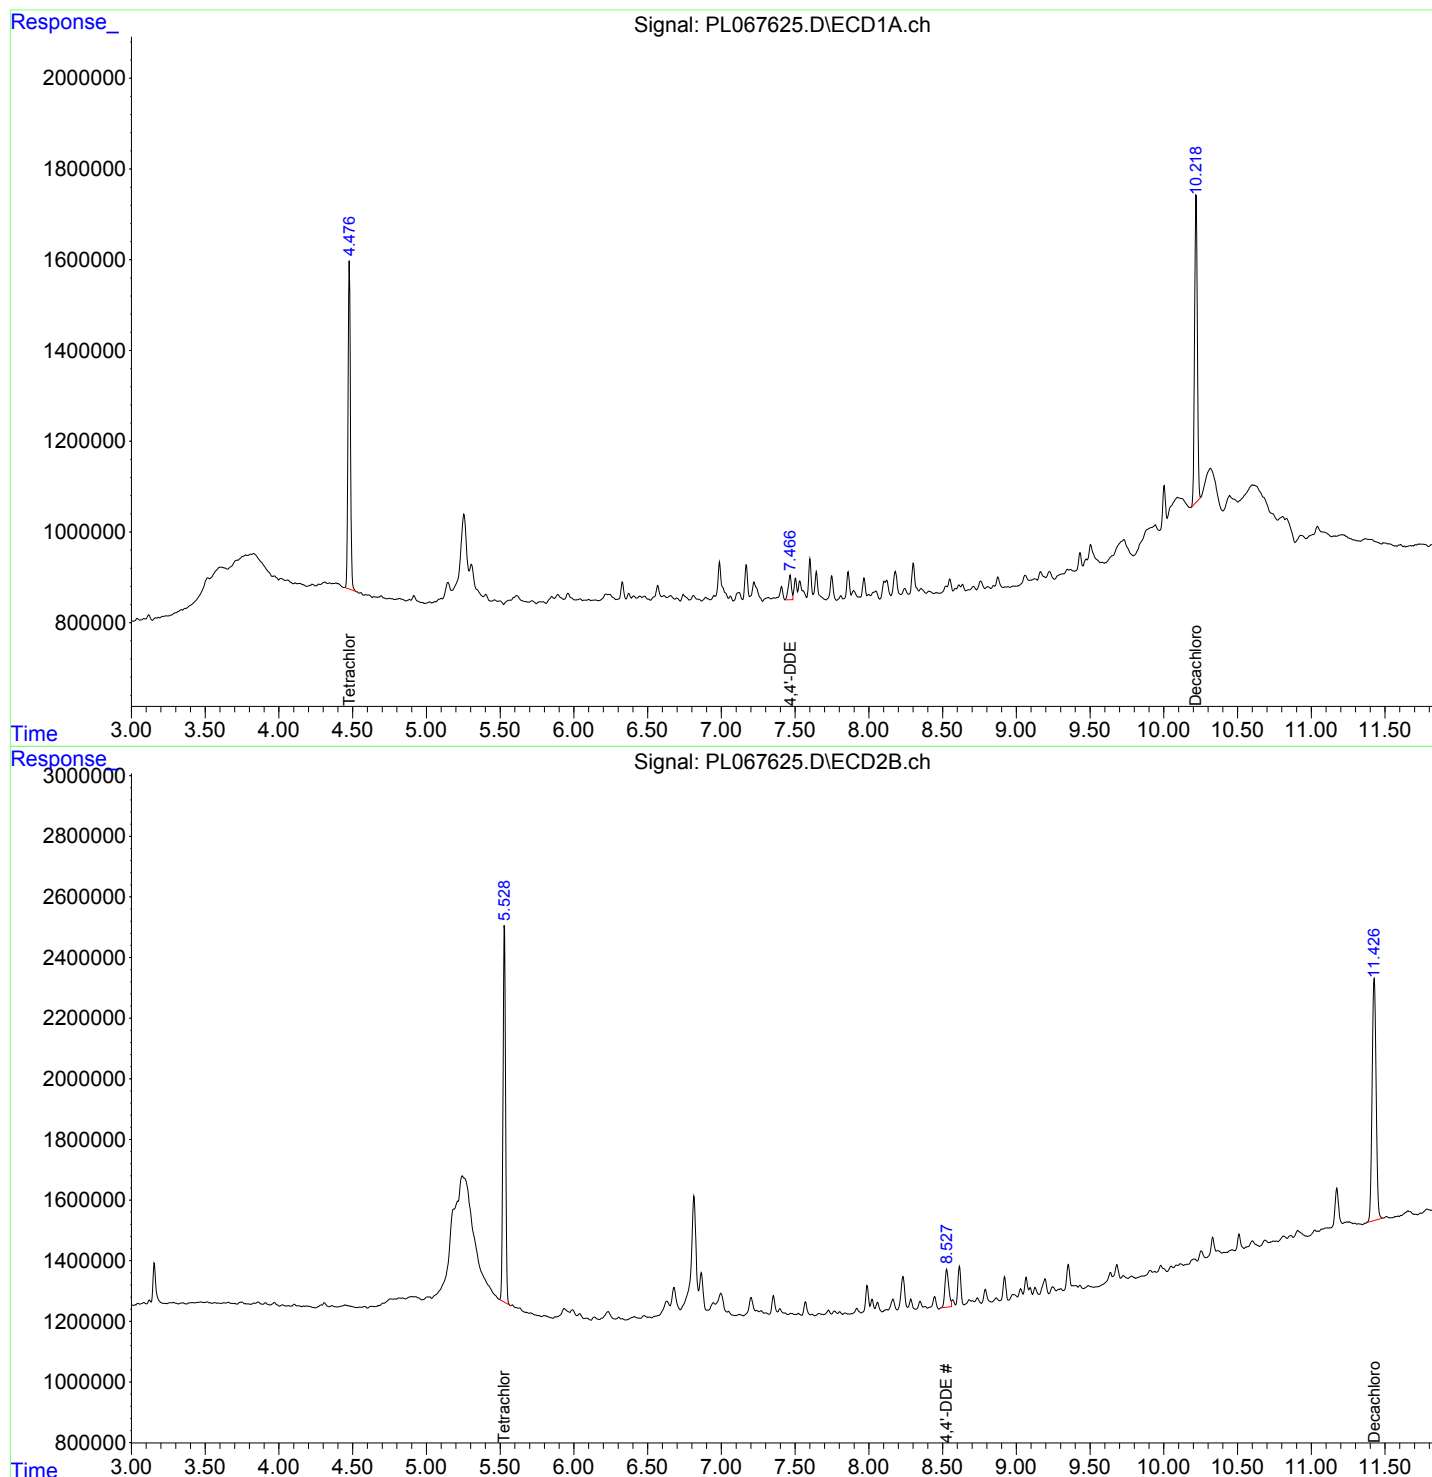

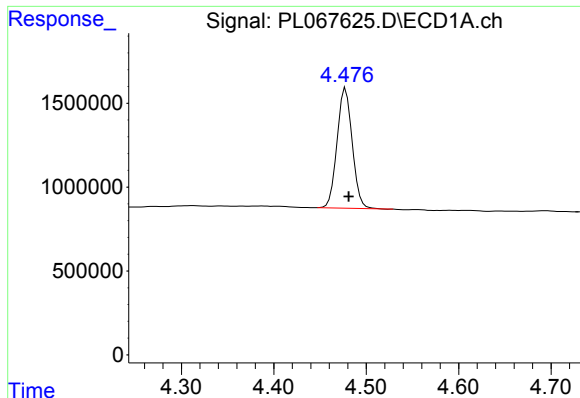


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 8152621
Conc: 14.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:03 PM

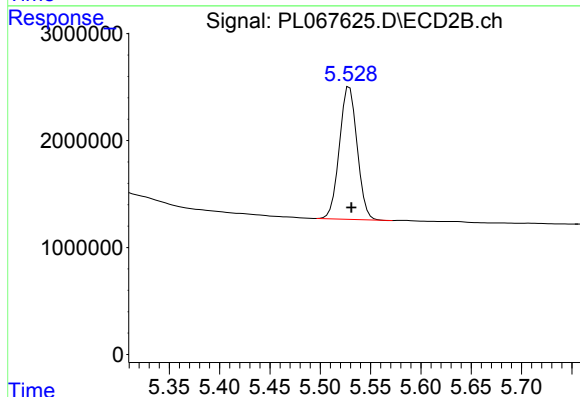


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 15171586
Conc: 16.09 ng/ml

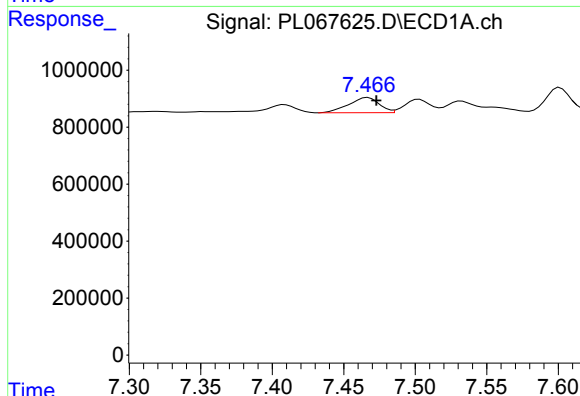


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 795222
Conc: 1.20 ng/ml m

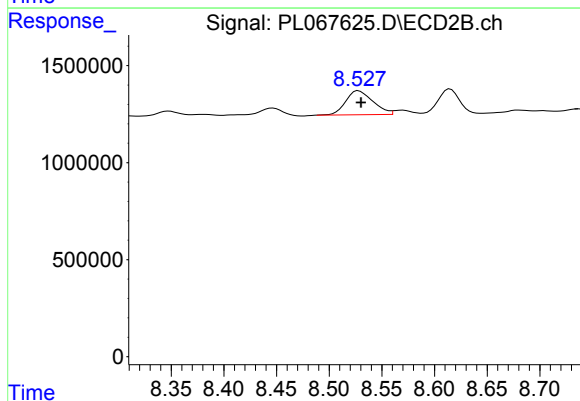

#12 4,4'-DDE


R.T.: 8.528 min
Delta R.T.: -0.002 min
Response: 2237486
Conc: 2.47 ng/ml

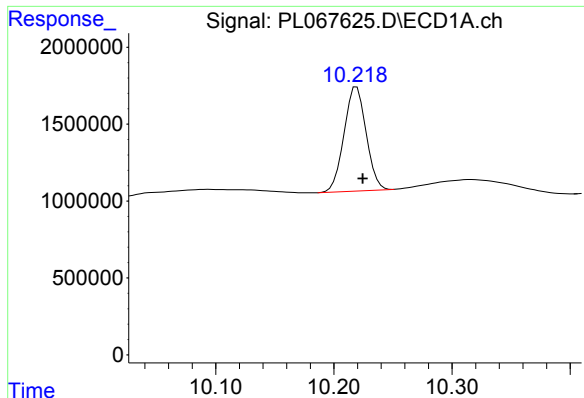

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 8803410
Conc: 12.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
0223-COMP-O(DISCRETE-CL-23

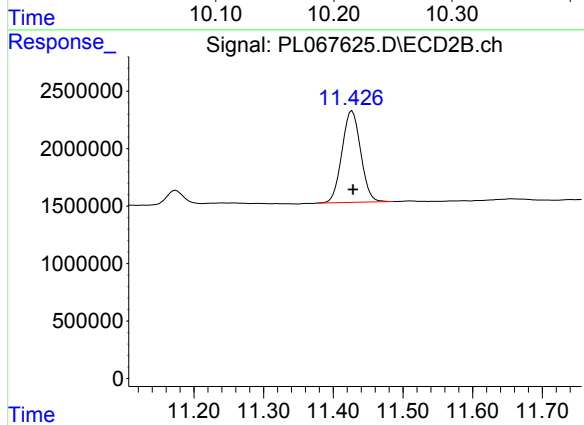

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 14891587
Conc: 14.95 ng/ml

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:03 PM