

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 18:14
 Operator : AR\AJ
 Sample : M2709-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:33:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	8694230	15906850	15.814	16.873
28)	SA Decachlor...	10.219	11.427	8560573	13355012	12.080	13.408
Target Compounds							
12)	B 4,4'-DDE	7.466	8.528	1091538	3454743	1.641m	3.813 #
16)	A 4,4'-DDD	8.047	9.065	510359	1051845	0.878m	1.479m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 0240-AMND-COMP-E

Manual Integrations
 APPROVED

Ankita
 6/21/2021 12:10:05 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 18:14
Operator : AR\AJ
Sample : M2709-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:33:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampled :
0240-AMND-COMP-E

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:05 PM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

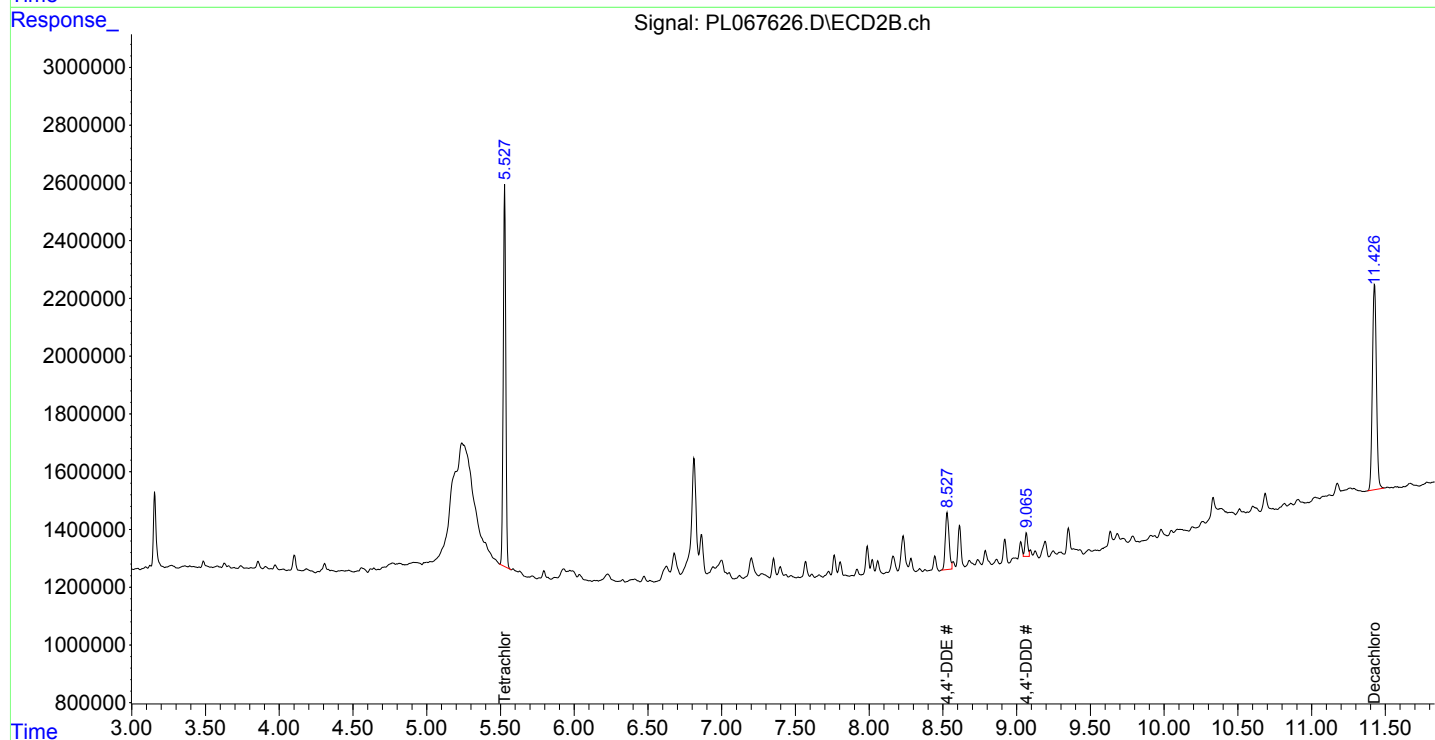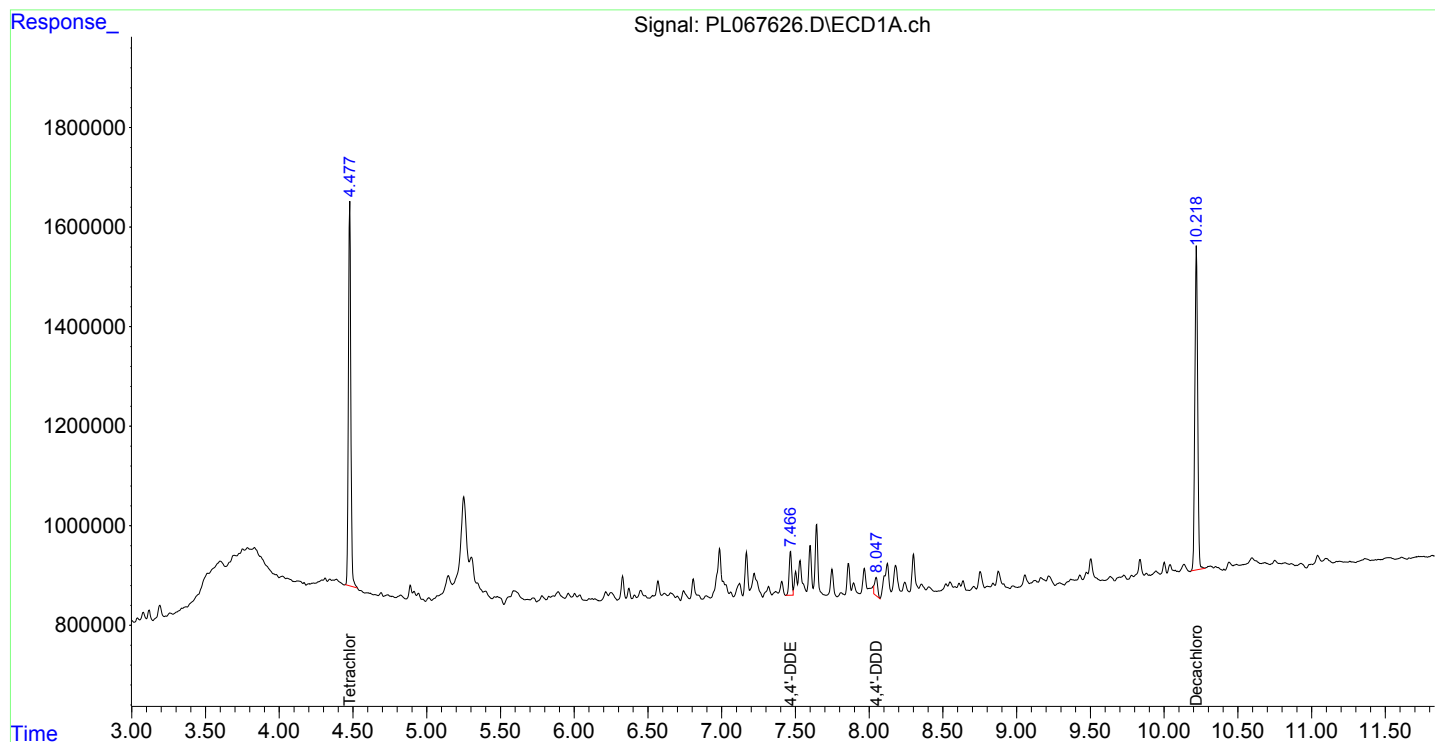

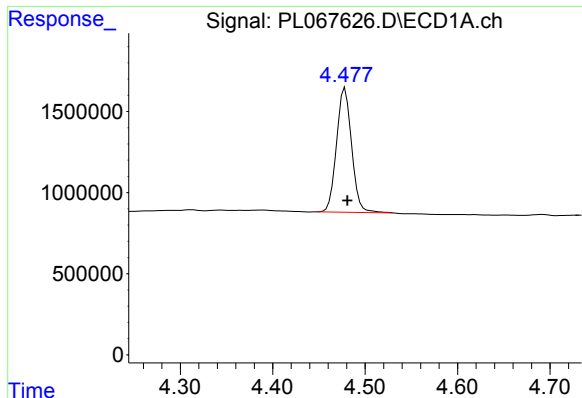


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 8694230
Conc: 15.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
0240-AMND-COMP-E


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:05 PM

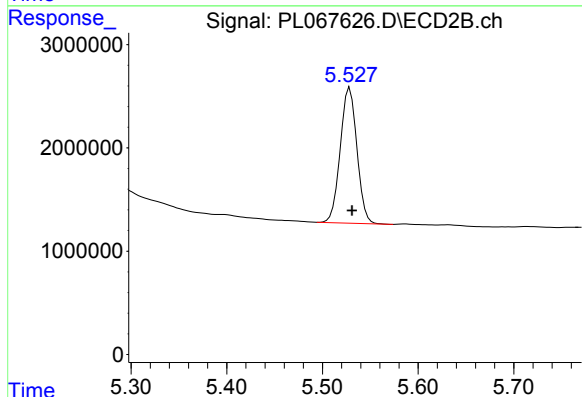


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 15906850
Conc: 16.87 ng/ml

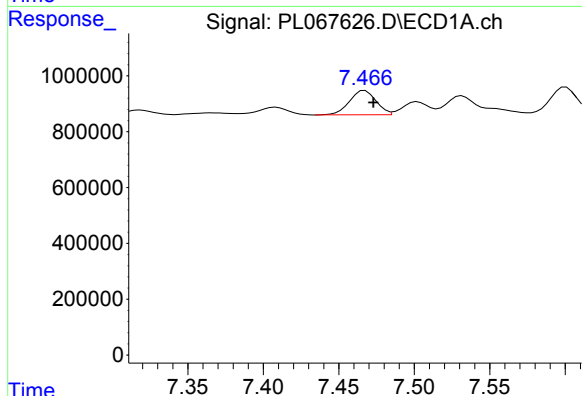


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 1091538
Conc: 1.64 ng/ml m

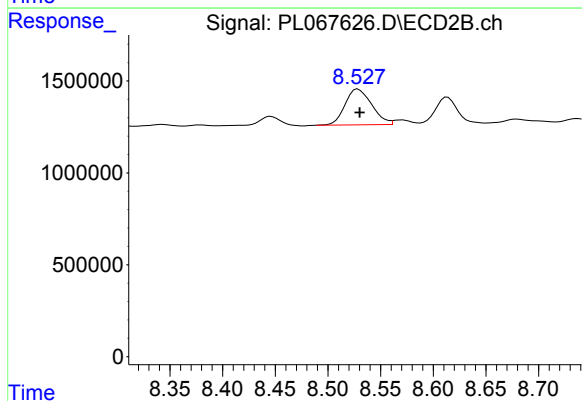

#12 4,4'-DDE

R.T.: 8.528 min
Delta R.T.: -0.002 min
Response: 3454743
Conc: 3.81 ng/ml

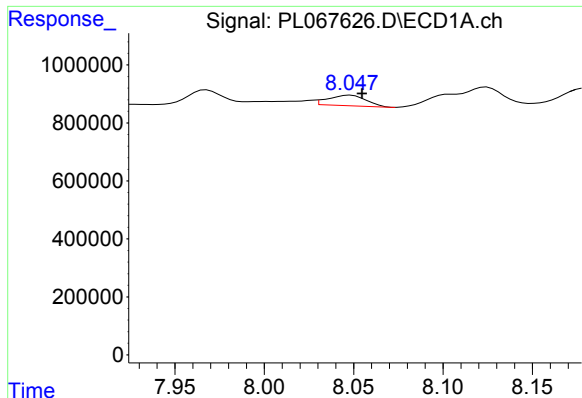


#16 4,4'-DDD

R.T.: 8.047 min
Delta R.T.: -0.007 min
Response: 510359
Conc: 0.88 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0240-AMND-COMP-E


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:05 PM

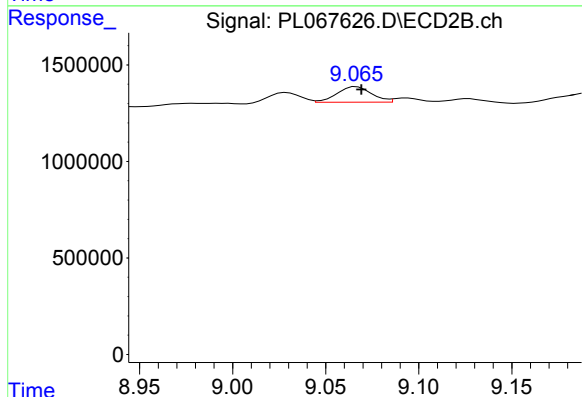


#16 4,4'-DDD

R.T.: 9.065 min
Delta R.T.: -0.004 min
Response: 1051845
Conc: 1.48 ng/ml m

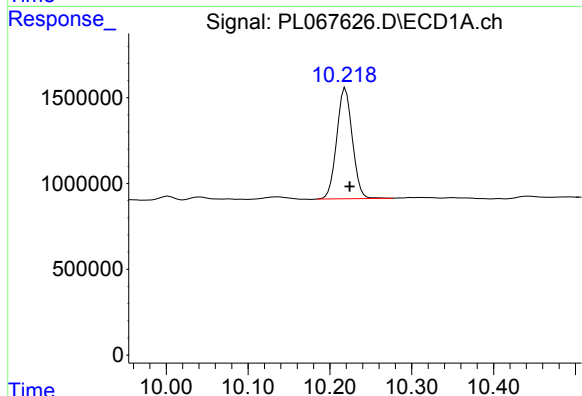

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 8560573
Conc: 12.08 ng/ml

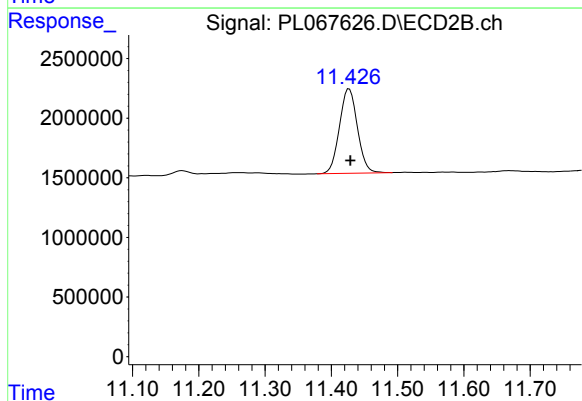

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 13355012
Conc: 13.41 ng/ml