

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 18:30
 Operator : AR\AJ
 Sample : M2709-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:34:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.529	4649191	8384890	8.456	8.894
28) SA Decachlor...	10.220	11.427	7293593	11297796	10.292	11.343
Target Compounds						
12) B 4,4'-DDE	7.466	8.525	764731	2280581	1.149m	2.517 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 0247-AMND-COMP-L

Manual Integrations
 APPROVED

Ankita
 6/21/2021 12:10:07 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 18:30
Operator : AR\AJ
Sample : M2709-08
Misc :
ALS Vial : 16 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:34:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampleID :
0247-AMND-COMP-L

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:07 PM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

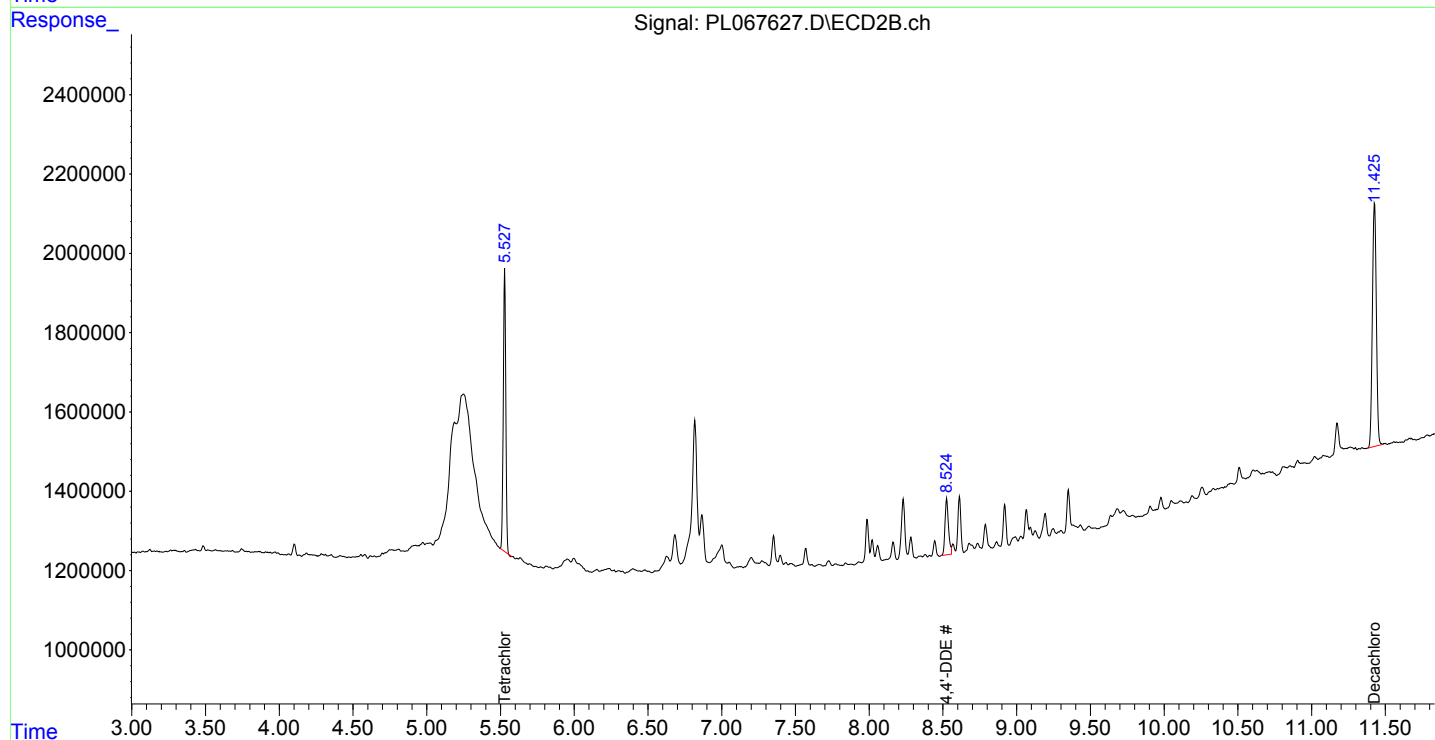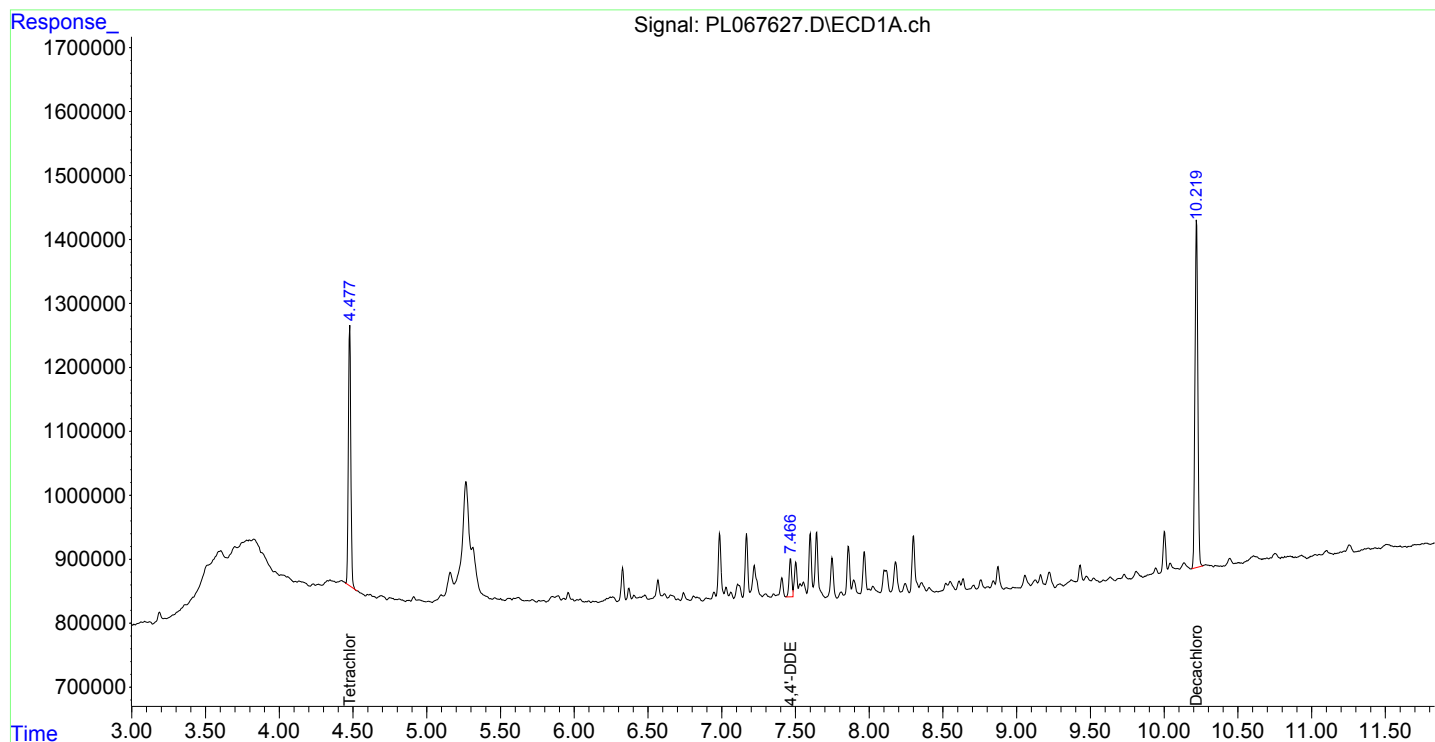

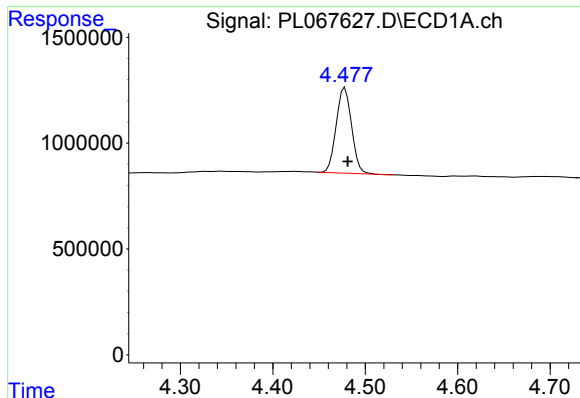


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 4649191
Conc: 8.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
0247-AMND-COMP-L


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:07 PM

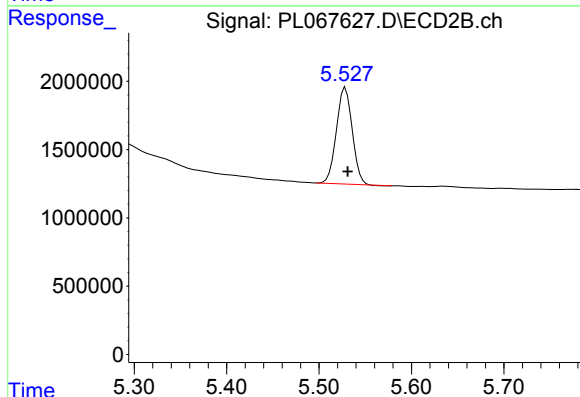


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 8384890
Conc: 8.89 ng/ml

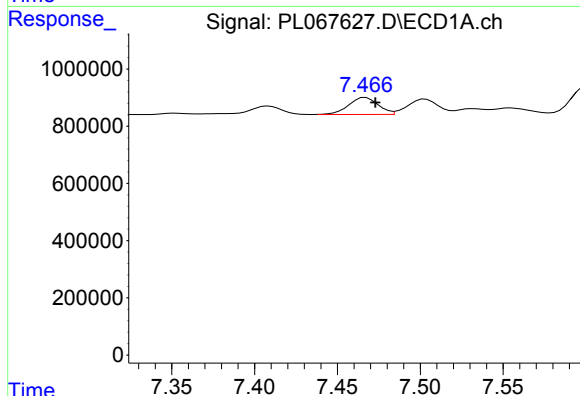


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 764731
Conc: 1.15 ng/ml m

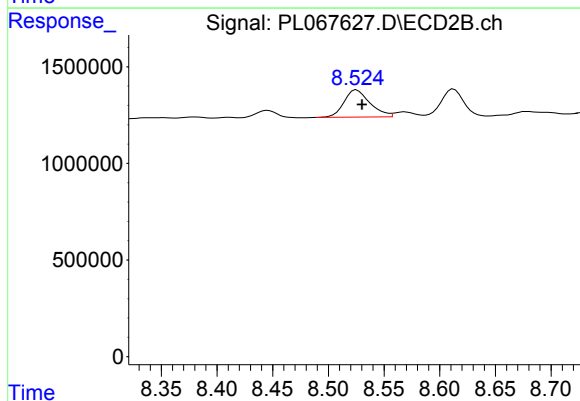

#12 4,4'-DDE


R.T.: 8.525 min
Delta R.T.: -0.005 min
Response: 2280581
Conc: 2.52 ng/ml

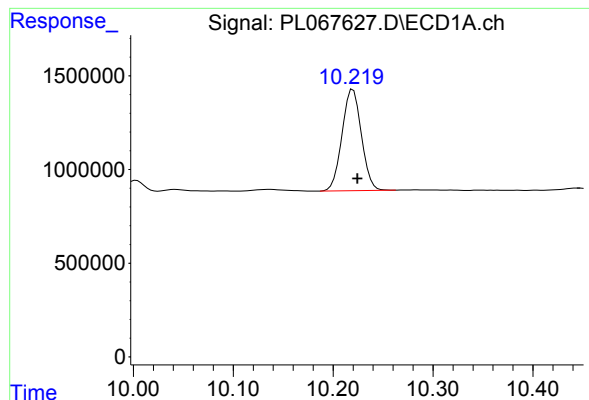

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 7293593
Conc: 10.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
0247-AMND-COMP-L

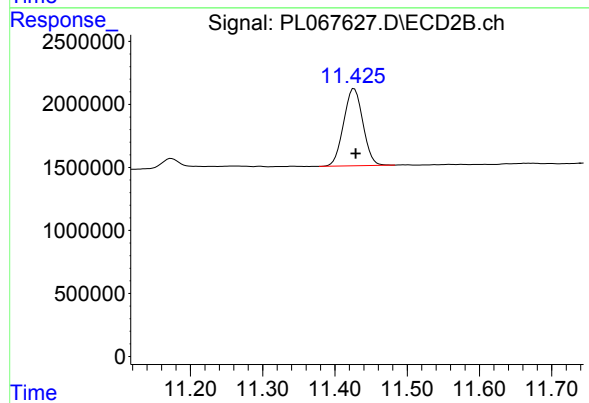

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 11297796
Conc: 11.34 ng/ml

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:07 PM