

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 18:47
 Operator : AR\AJ
 Sample : M2709-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:34:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.529	10020105	18549046	18.225	19.676
28) SA Decachlor...	10.220	11.427	12503694	19579114	17.644	19.657
Target Compounds						
12) B 4,4'-DDE	7.467	8.527	2374870	3838845	3.570	4.237
16) A 4,4'-DDD	8.048	9.065	599010	1052327	1.031	1.480m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 0248-AMND-COMP-M

Manual Integrations
 APPROVED

Ankita
 6/21/2021 12:10:09 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 18:47
Operator : AR\AJ
Sample : M2709-09
Misc :
ALS Vial : 17 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:34:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampleId :
0248-AMND-COMP-M

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:09 PM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

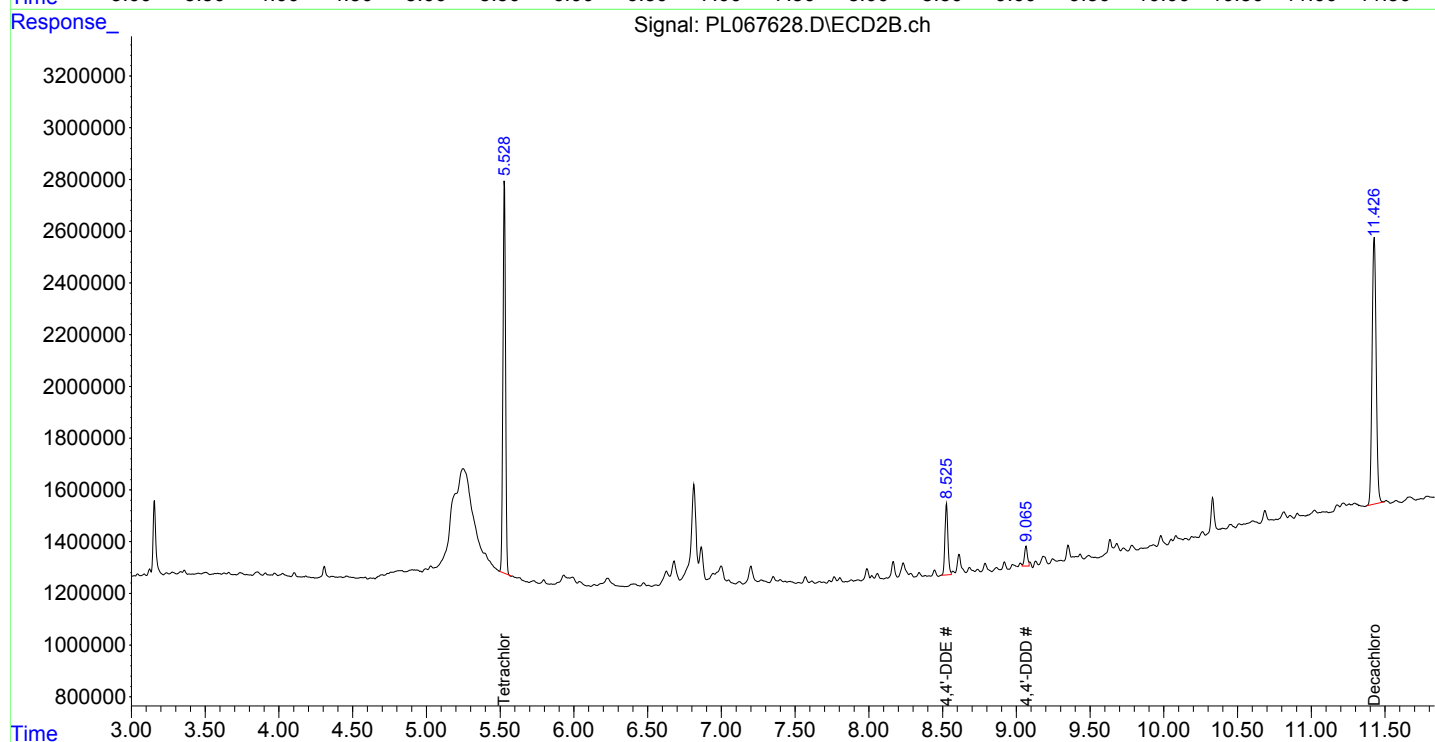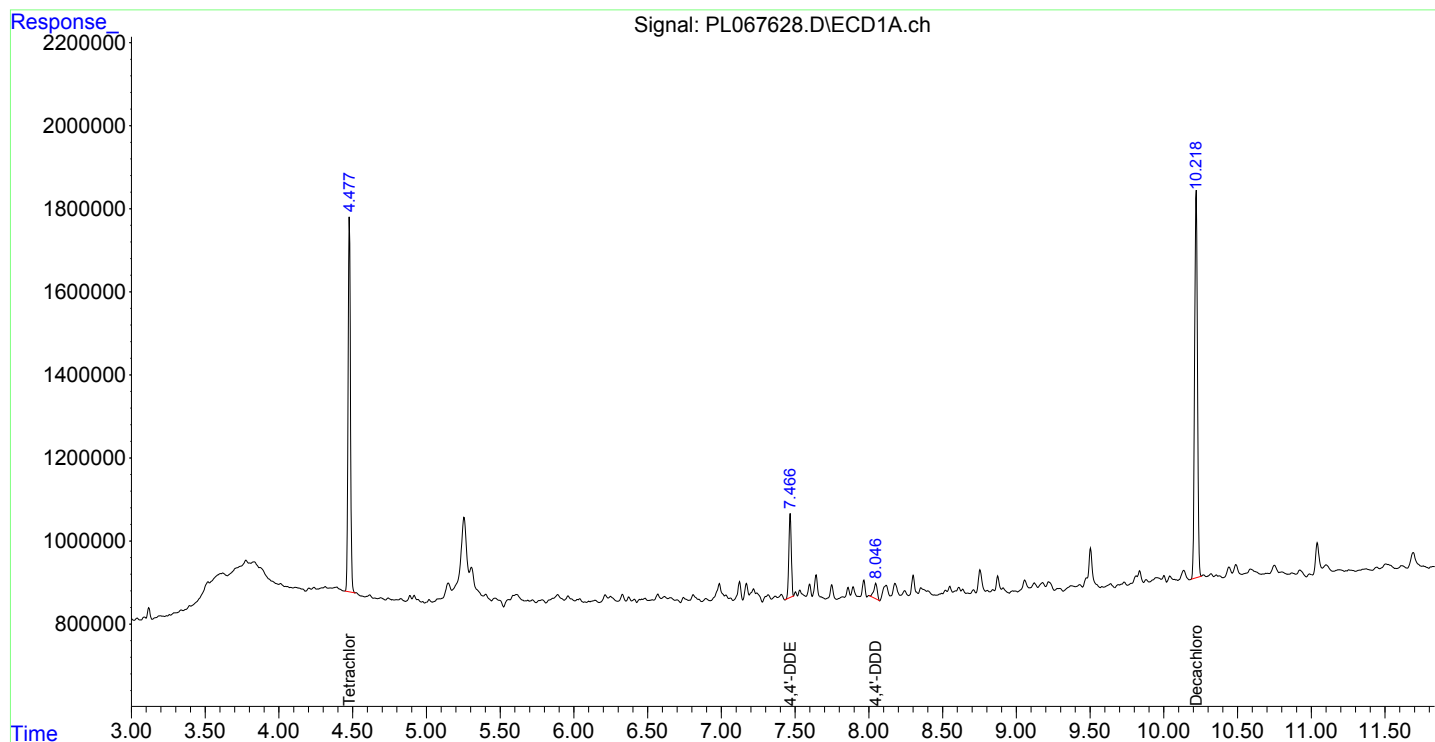

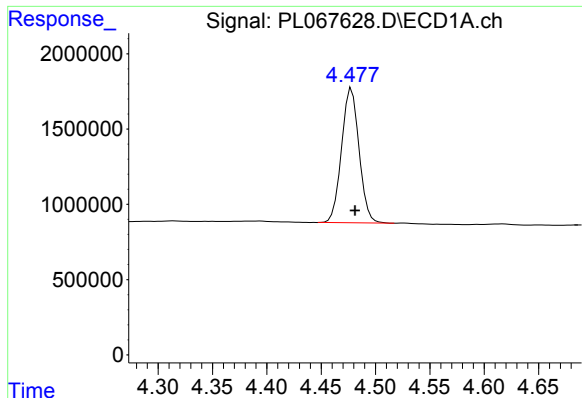


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10020105
Conc: 18.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
0248-AMND-COMP-M


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:09 PM

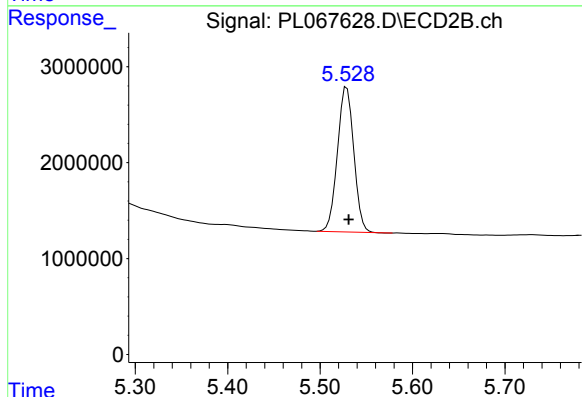


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 18549046
Conc: 19.68 ng/ml

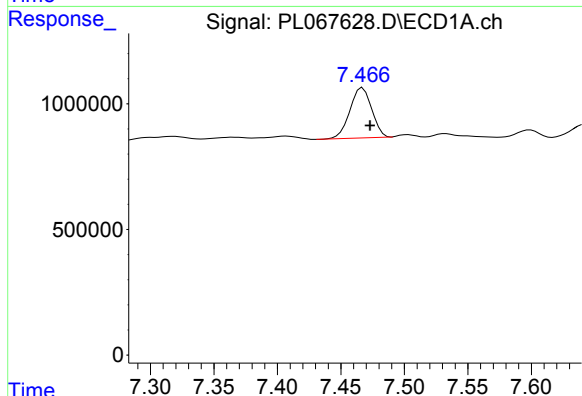


#12 4,4'-DDE

R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 2374870
Conc: 3.57 ng/ml

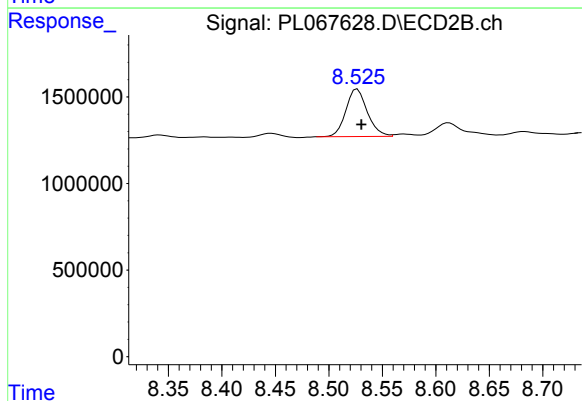

#12 4,4'-DDE

R.T.: 8.527 min
Delta R.T.: -0.004 min
Response: 3838845
Conc: 4.24 ng/ml

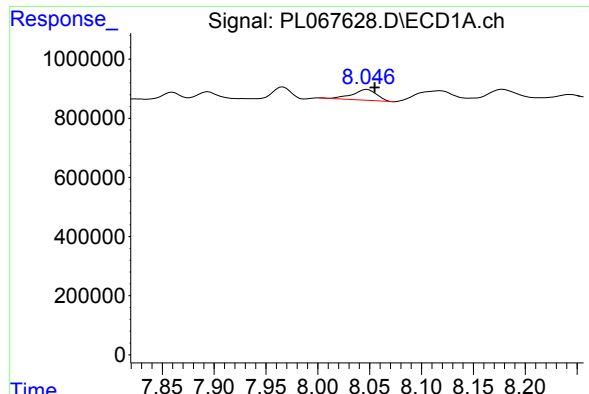


#16 4,4'-DDD

R.T.: 8.048 min
Delta R.T.: -0.007 min
Response: 599010
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
0248-AMND-COMP-M


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:09 PM

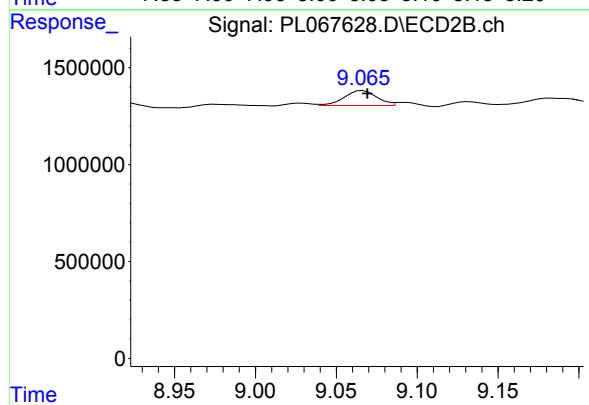


#16 4,4'-DDD

R.T.: 9.065 min
Delta R.T.: -0.004 min
Response: 1052327
Conc: 1.48 ng/ml m

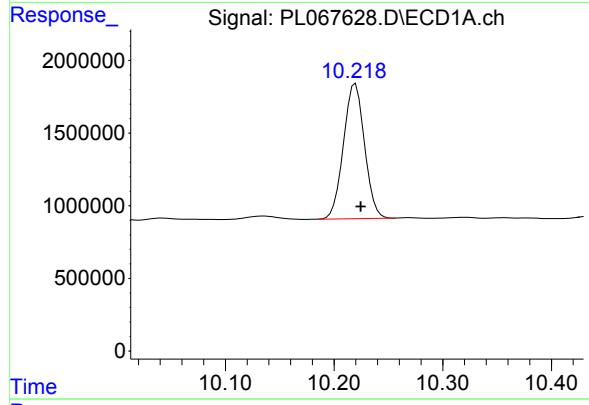

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 12503694
Conc: 17.64 ng/ml

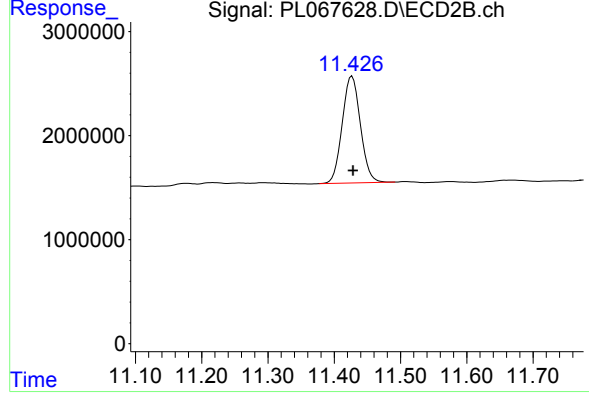

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 19579114
Conc: 19.66 ng/ml