

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
 Data File : PL067629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 19:04
 Operator : AR\AJ
 Sample : M2709-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 02:34:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.478	5.529	4974520	8933351	9.048	9.476
28) SA Decachlor...	10.220	11.427	9928352	15953344	14.010	16.016
Target Compounds						
12) B 4,4'-DDE	7.466	8.527	8362445	17159570	12.569m	18.941 #
17) MA 4,4'-DDT	8.305	9.382	9134674	6007459	15.698	8.194m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_L
 ClientSampleId :
 0249-AMND-COMP-N(CL-22)

Manual Integrations
 APPROVED

Ankita
 6/21/2021 12:10:11 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061821\
Data File : PL067629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 19:04
Operator : AR\AJ
Sample : M2709-10
Misc :
ALS Vial : 18 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 02:34:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation


Instrument :
ECD_L
ClientSampleId :
0249-AMND-COMP-N(CL-22)

Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:11 PM

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

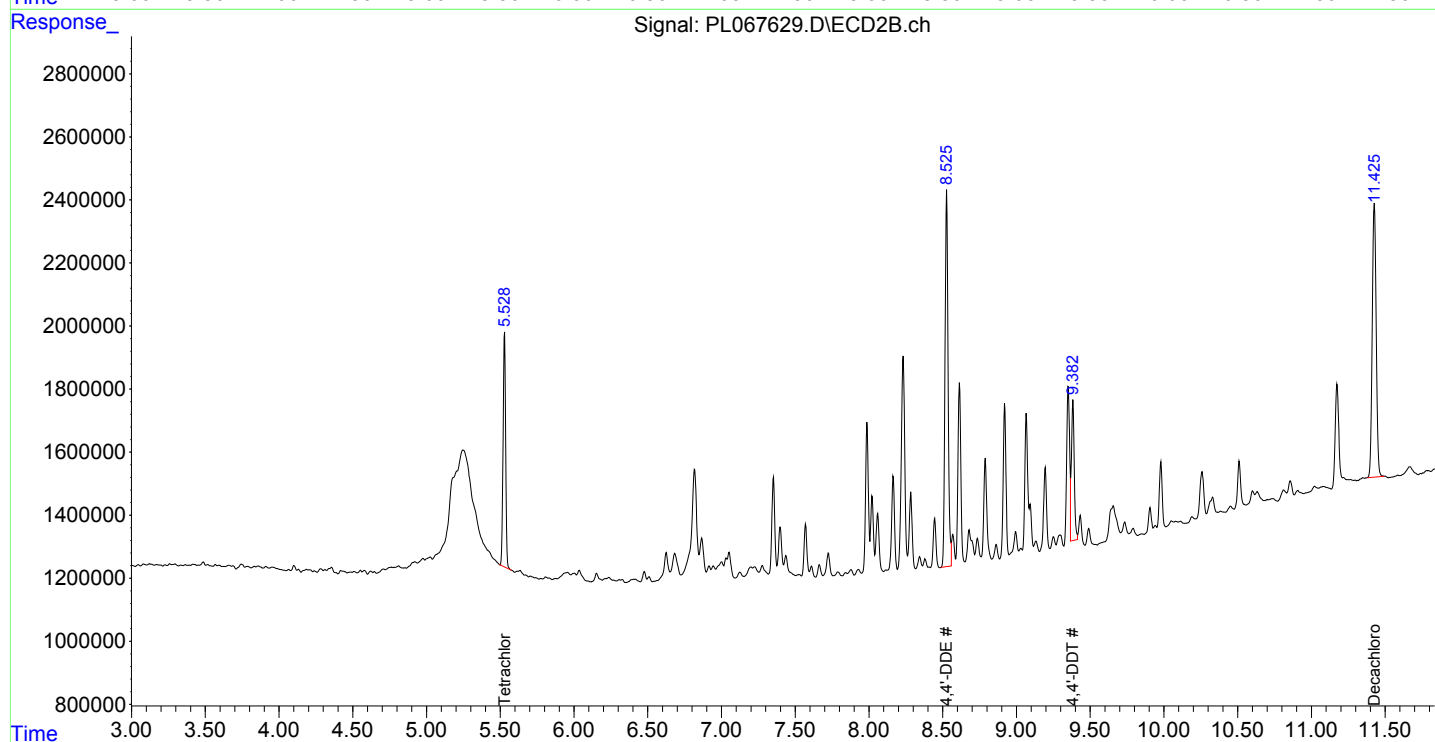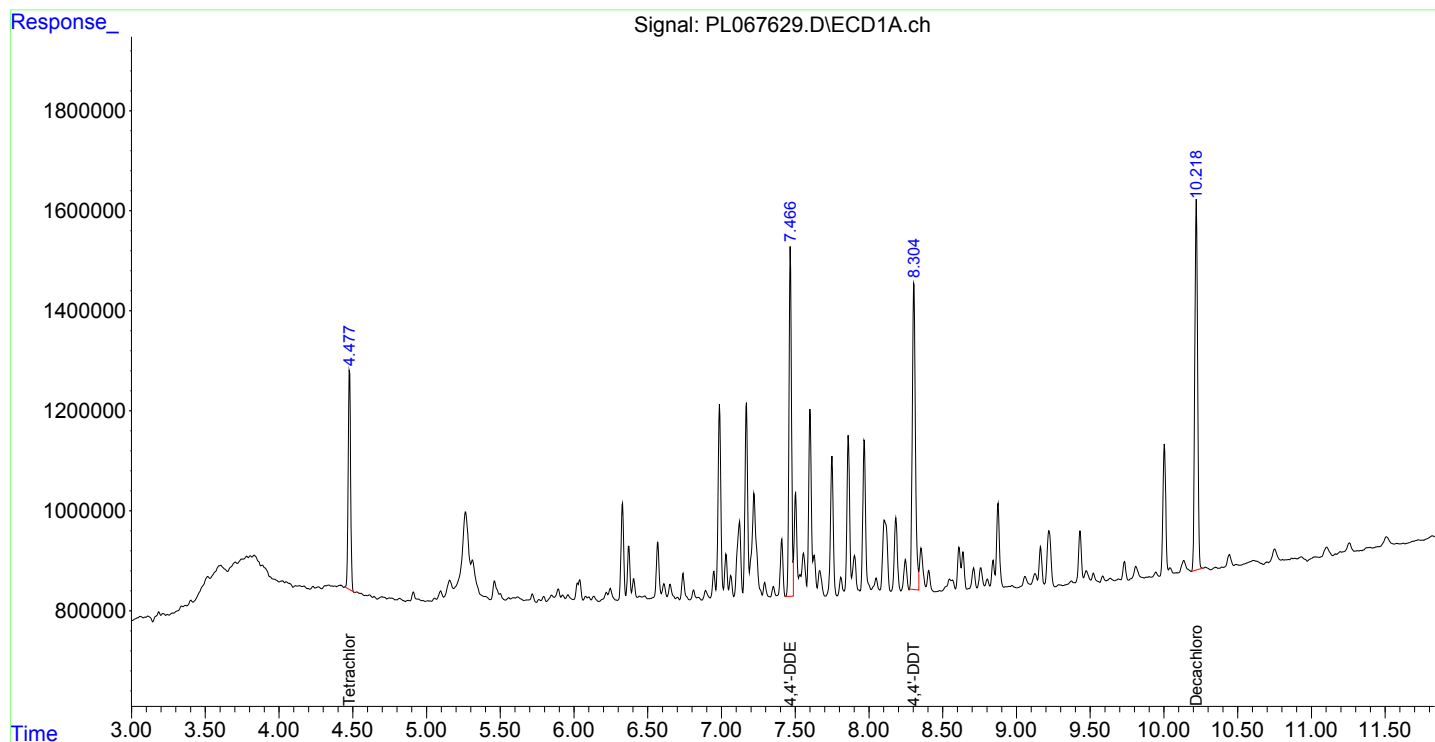

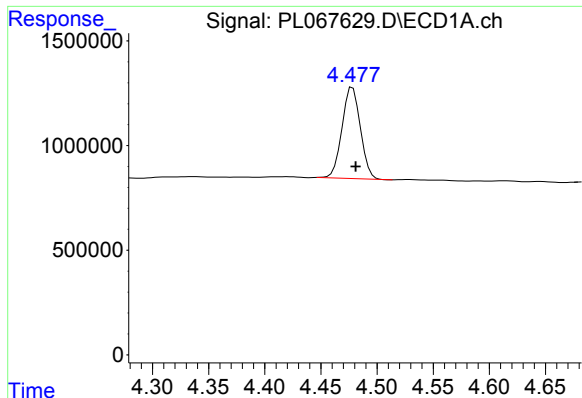


#1 Tetrachloro-m-xylene

R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 4974520
Conc: 9.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
0249-AMND-COMP-N(CL-22)


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:11 PM

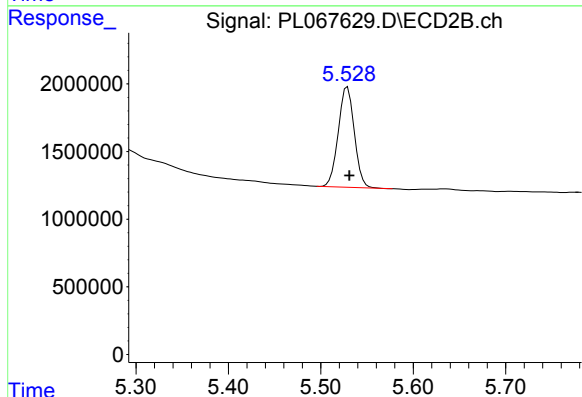


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 8933351
Conc: 9.48 ng/ml

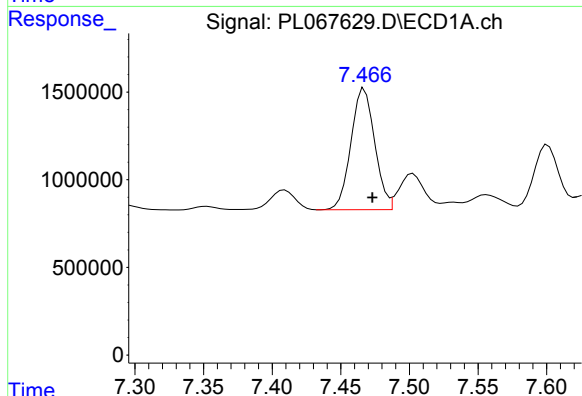


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 8362445
Conc: 12.57 ng/ml m

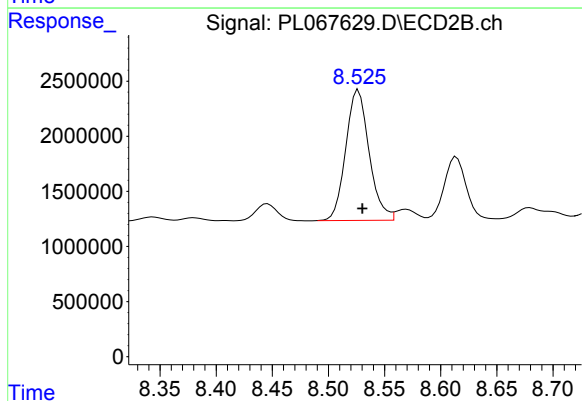

#12 4,4'-DDE

R.T.: 8.527 min
Delta R.T.: -0.004 min
Response: 17159570
Conc: 18.94 ng/ml

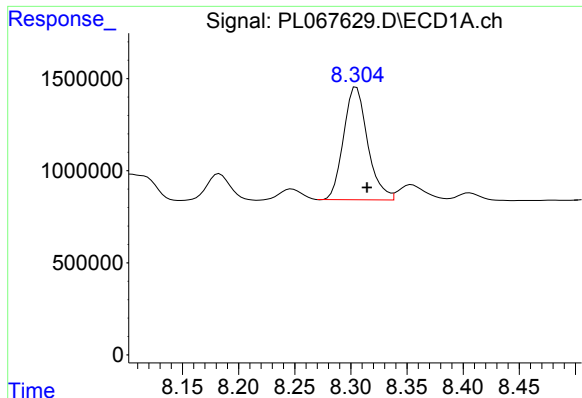


#17 4,4'-DDT

R.T.: 8.305 min
Delta R.T.: -0.009 min
Response: 9134674
Conc: 15.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
0249-AMND-COMP-N(CL-22)


Manual Integrations
APPROVED

Ankita
6/21/2021 12:10:11 PM

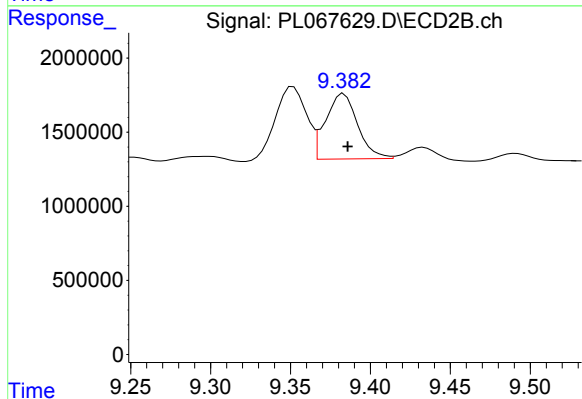


#17 4,4'-DDT

R.T.: 9.382 min
Delta R.T.: -0.004 min
Response: 6007459
Conc: 8.19 ng/ml m

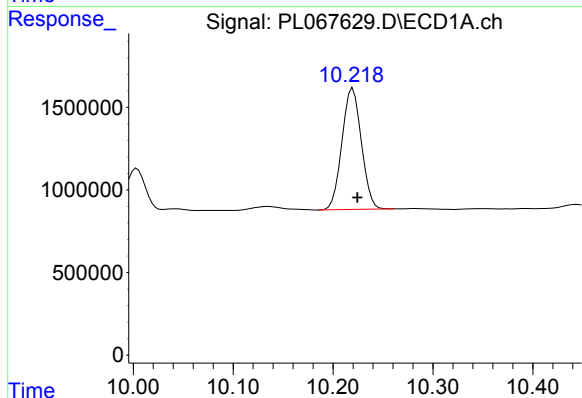

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 9928352
Conc: 14.01 ng/ml

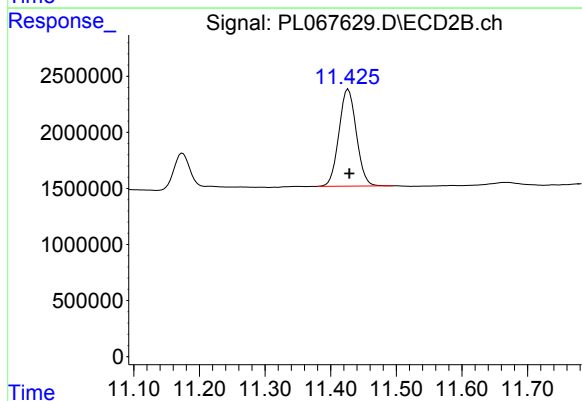

#28 Decachlorobiphenyl

R.T.: 11.427 min
Delta R.T.: -0.002 min
Response: 15953344
Conc: 16.02 ng/ml