

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061824\
Data File : PL090222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2024 14:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/19/2024
Supervised By :Ankita Jodhani 06/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:21:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.792	44567306	30857617	21.286m	21.521
28) SA Decachlor...	9.061	7.937	31898896	31192151	21.694	20.991

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061824\
Data File : PL090222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2024 14:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/19/2024
Supervised By : Ankita Jodhani 06/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:21:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

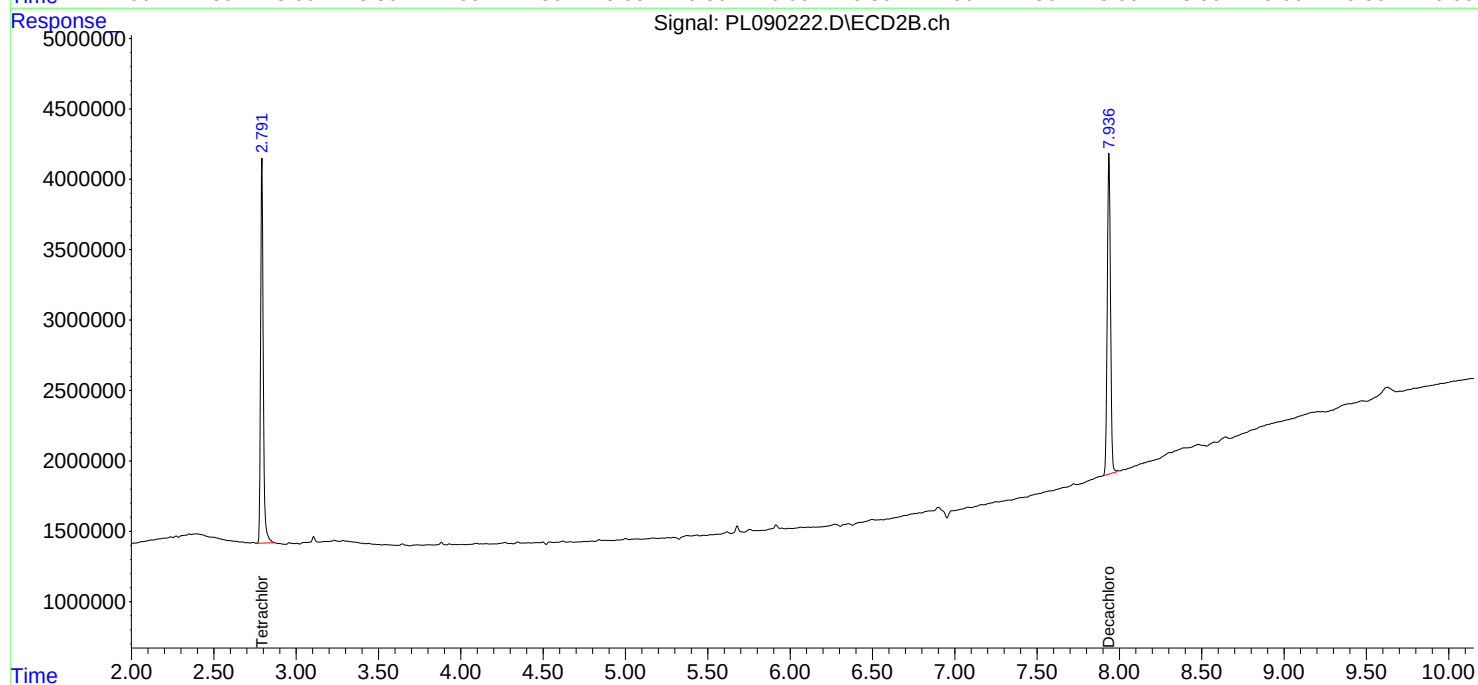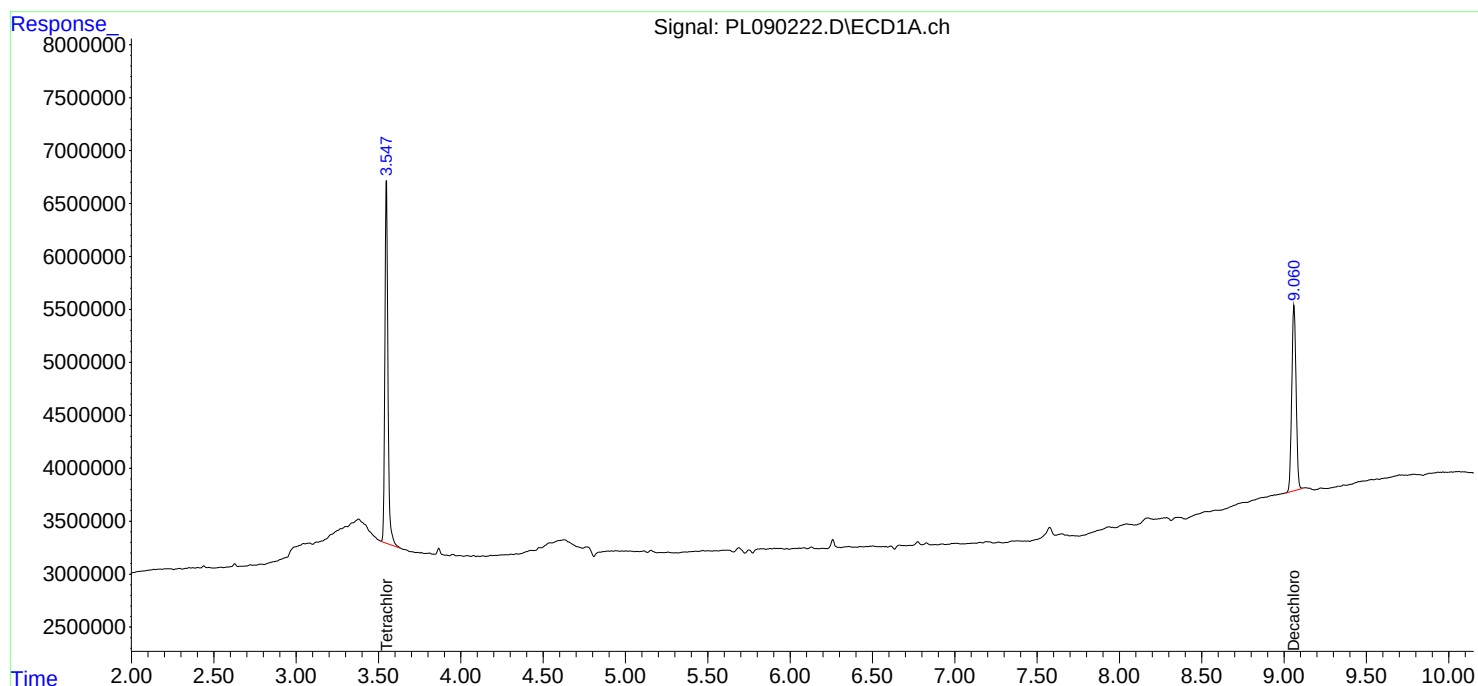

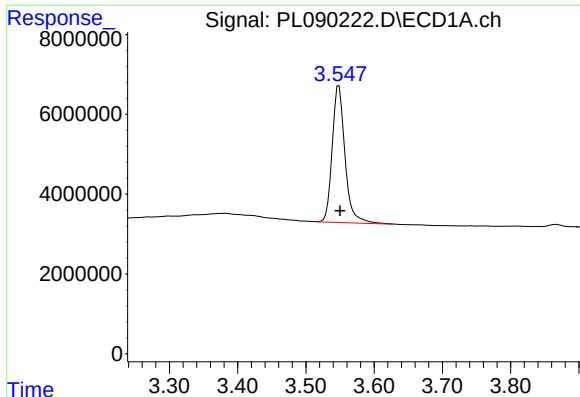


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: -0.003 min
Response: 44567306
Conc: 21.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/19/2024
Supervised By :Ankita Jodhani 06/19/2024

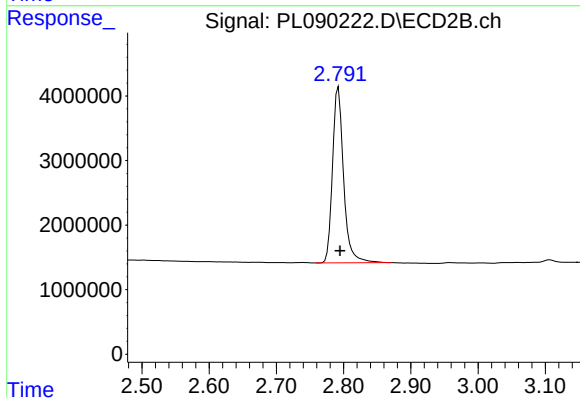


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: -0.002 min
Response: 30857617
Conc: 21.52 ng/ml

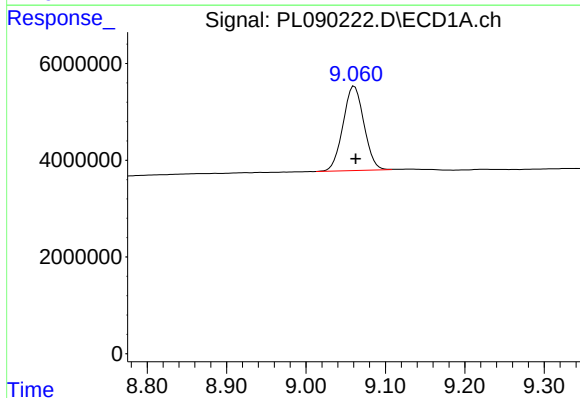

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: -0.002 min
Response: 31898896
Conc: 21.69 ng/ml

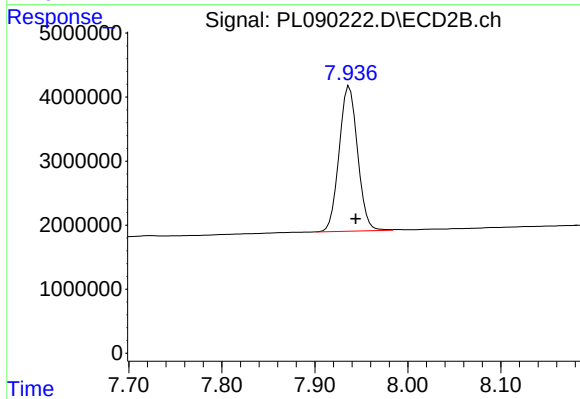

#28 Decachlorobiphenyl

R.T.: 7.937 min
Delta R.T.: -0.007 min
Response: 31192151
Conc: 20.99 ng/ml