

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL061825\  
 Data File : PL096095.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Jun 2025 11:08  
 Operator : AR\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 19 01:27:39 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL061725.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jun 17 17:11:36 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |       |          |          |       |          |
|------------------|--------------|--------|-------|----------|----------|-------|----------|
| 8) B             | Heptachlo... | 5.705  | 0.000 | 31625735 | 0        | 6.966 | N.D. #   |
| 10) B            | gamma-Chl... | 5.945f | 0.000 | 3976018  | 0        | 0.854 | N.D. #   |
| 13) MA           | Dieldrin     | 0.000  | 5.505 | 0        | 18270645 | N.D.  | 2.785 #  |
| 14) MA           | Endrin       | 0.000  | 5.785 | 0        | 14637677 | N.D.  | 2.466 #  |
| 24)              | Chlordane-2  | 0.000  | 4.471 | 0        | 13721179 | N.D.  | 52.706 # |
| 25)              | Chlordane-3  | 5.945f | 0.000 | 3976018  | 0        | 4.764 | N.D. #   |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL061825\  
Data File : PL096095.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Jun 2025 11:08  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 19 01:27:39 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL061725.M  
Quant Title : GC Extractables  
QLast Update : Tue Jun 17 17:11:36 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

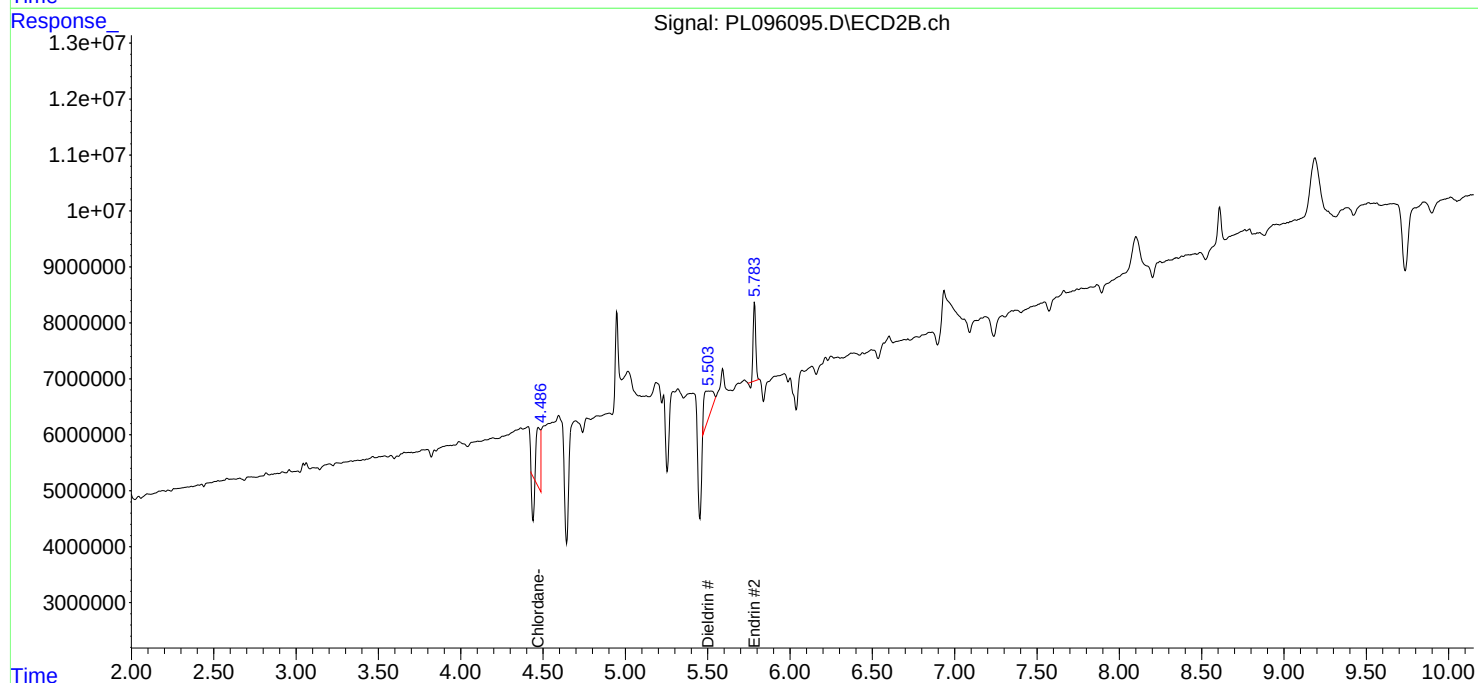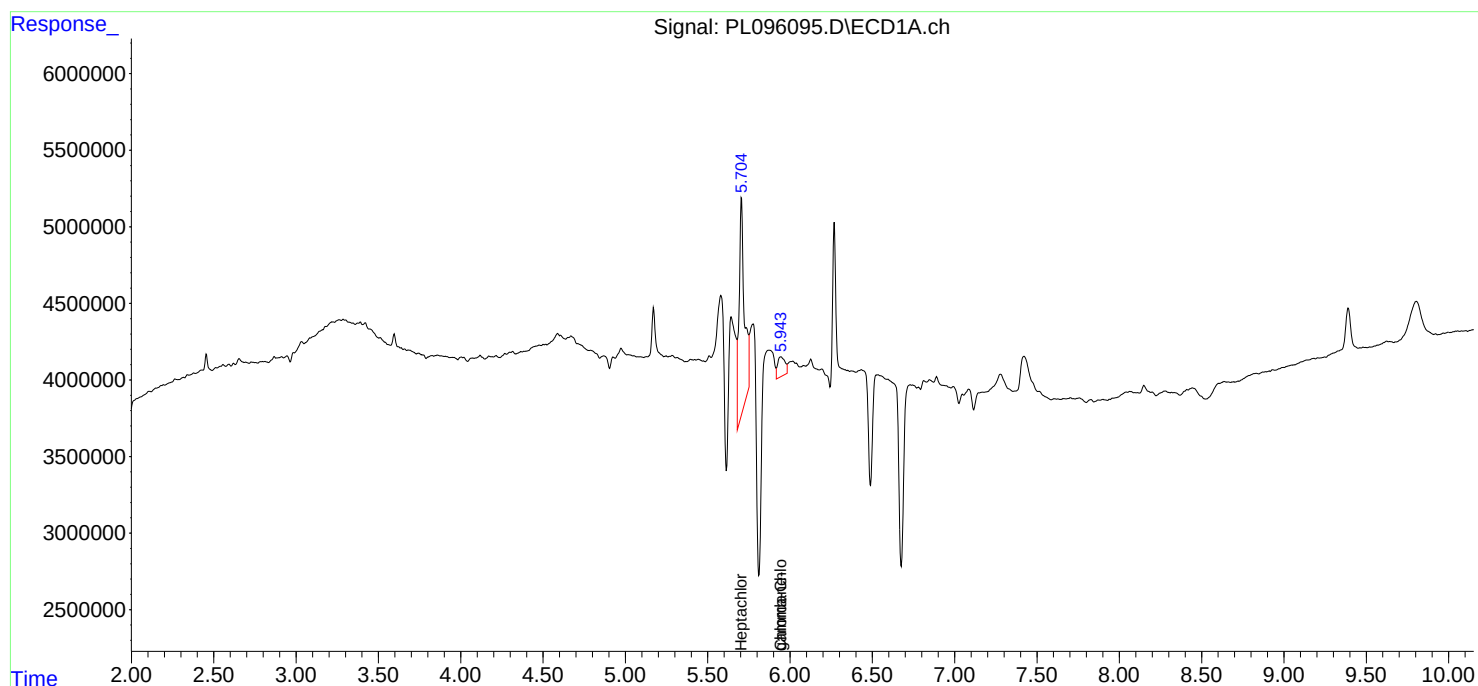


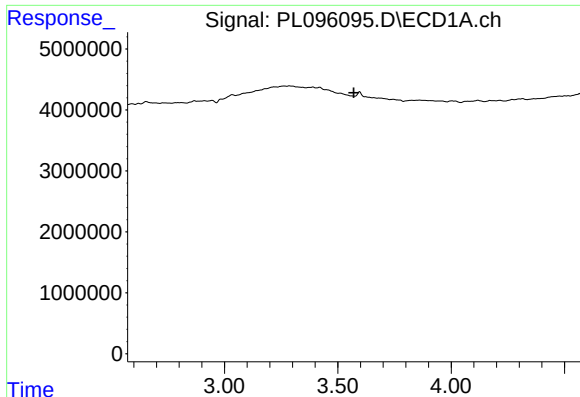

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T.: 3.570 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

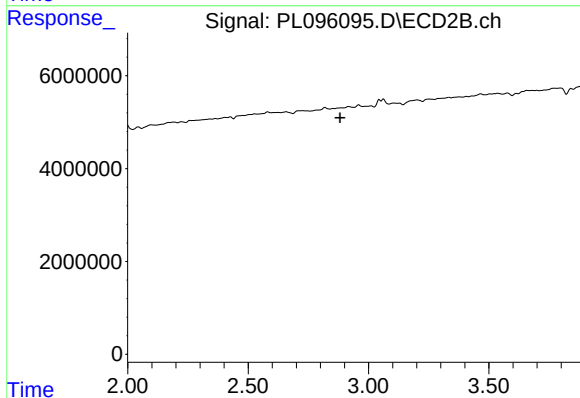


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T.: 2.882 min  
Response: 0  
Conc: N.D.

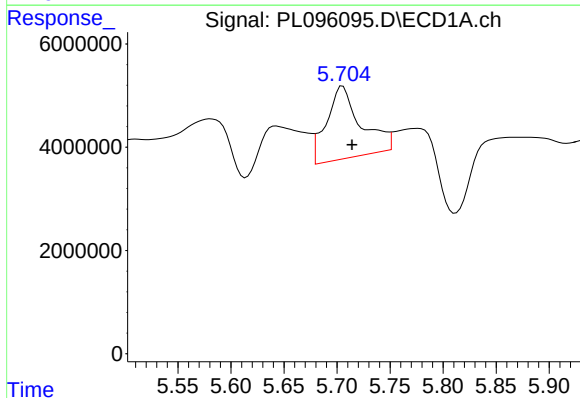


#8 Heptachlor epoxide

R.T.: 5.705 min  
Delta R.T.: -0.009 min  
Response: 31625735  
Conc: 6.97 ng/ml

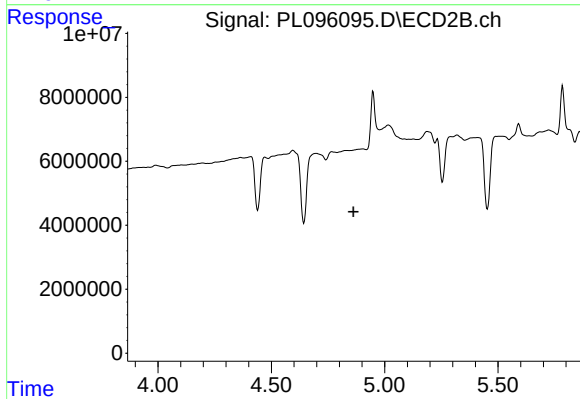

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T.: 4.863 min  
Response: 0  
Conc: N.D.

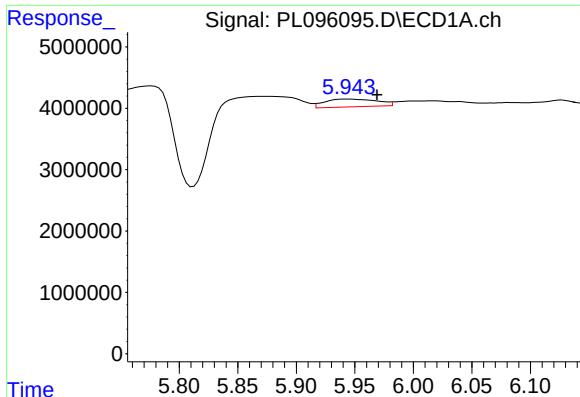

#10 gamma-Chlordane


R.T.: 5.945 min  
Delta R.T.: -0.024 min  
Response: 3976018  
Conc: 0.85 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

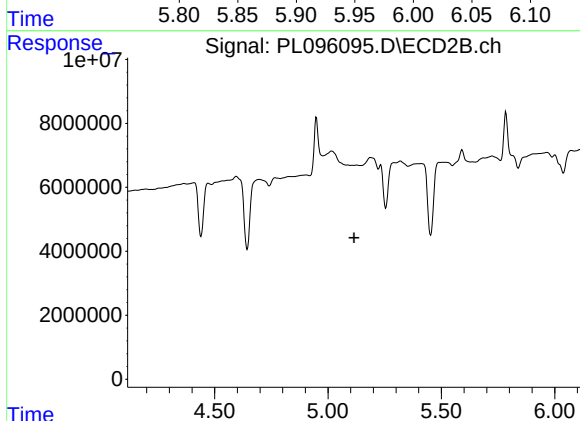


#10 gamma-Chlordane

R.T.: 0.000 min  
Exp R.T. : 5.116 min  
Response: 0  
Conc: N.D.

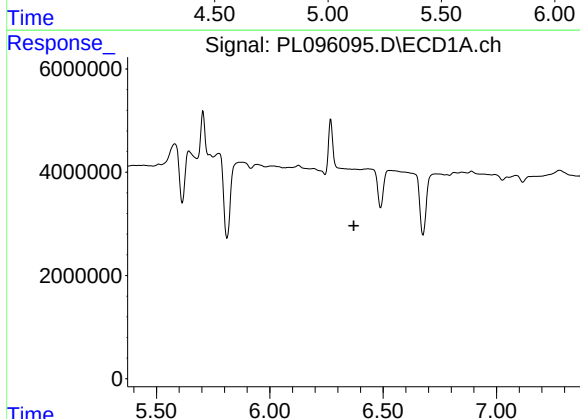


#13 Dieldrin

R.T.: 0.000 min  
Exp R.T. : 6.371 min  
Response: 0  
Conc: N.D.

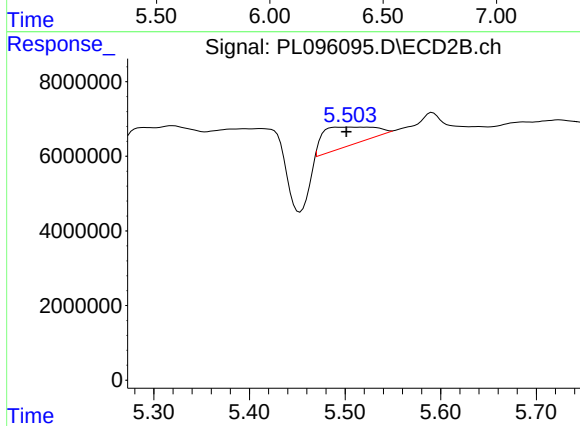

#13 Dieldrin


R.T.: 5.505 min  
Delta R.T.: 0.004 min  
Response: 18270645  
Conc: 2.78 ng/ml

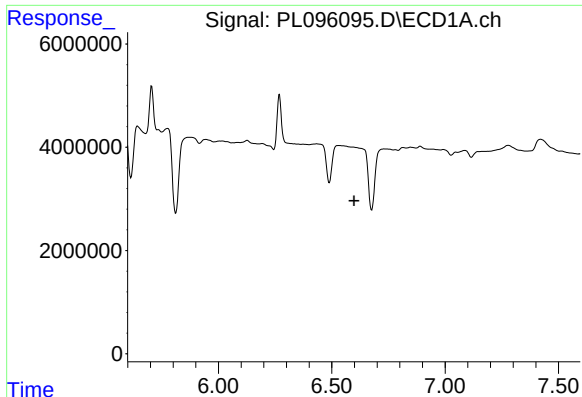

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.598 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

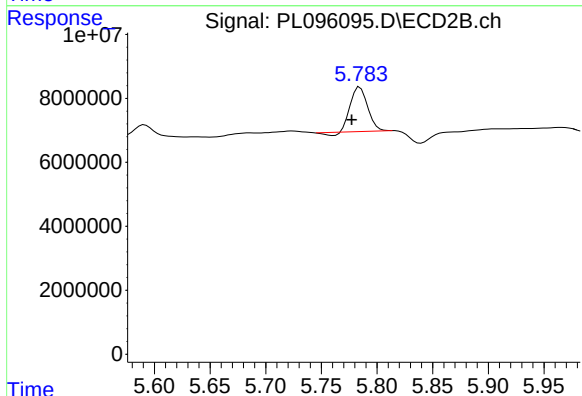


#14 Endrin

R.T.: 5.785 min  
Delta R.T.: 0.007 min  
Response: 14637677  
Conc: 2.47 ng/ml

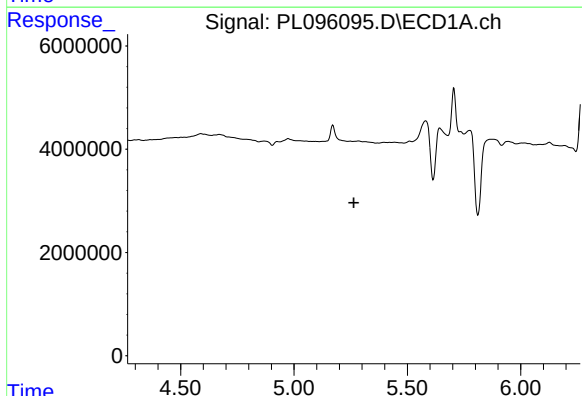


#24 Chlordane-2

R.T.: 0.000 min  
Exp R.T.: 5.264 min  
Response: 0  
Conc: N.D.

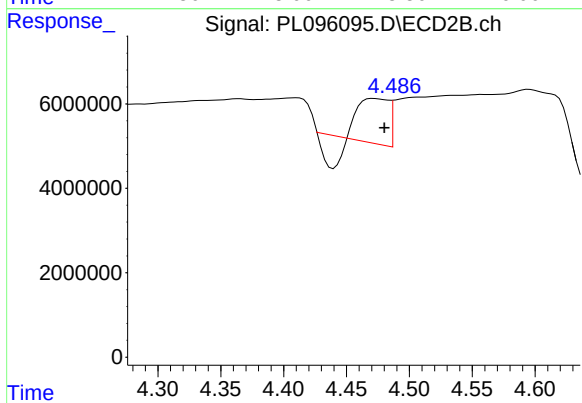

#24 Chlordane-2


R.T.: 4.471 min  
Delta R.T.: -0.009 min  
Response: 13721179  
Conc: 52.71 ng/ml

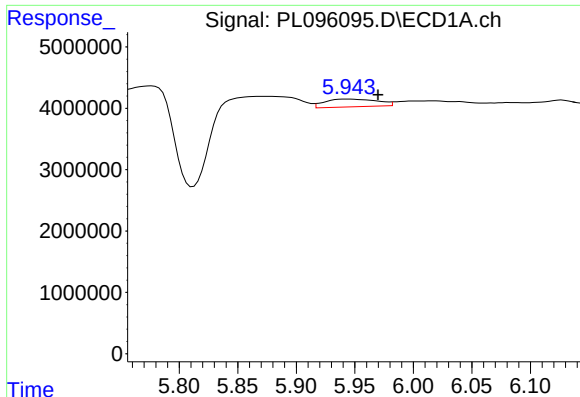

#25 Chlordane-3


R.T.: 5.945 min  
Delta R.T.: -0.025 min  
Response: 3976018  
Conc: 4.76 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

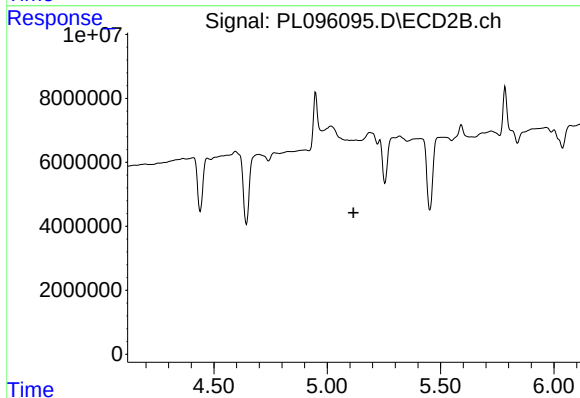


#25 Chlordane-3

R.T.: 0.000 min  
Exp R.T. : 5.116 min  
Response: 0  
Conc: N.D.

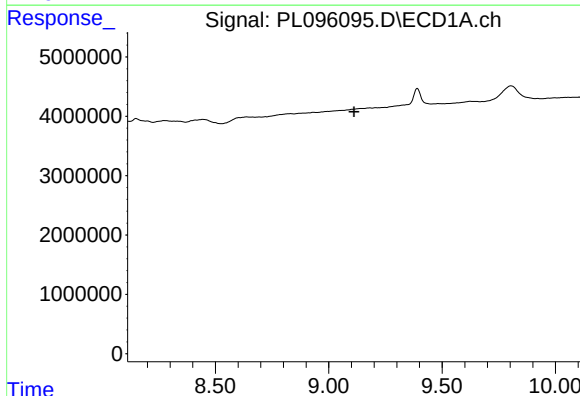

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.112 min  
Response: 0  
Conc: N.D.

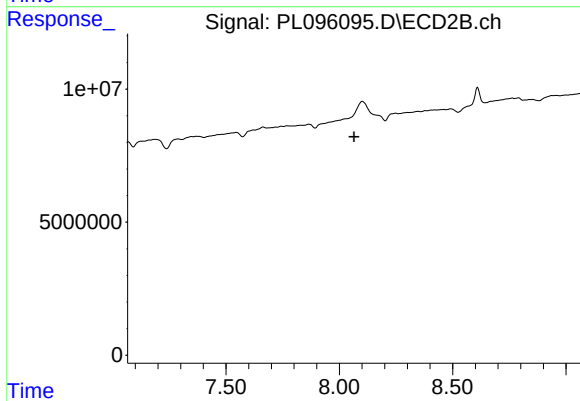

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.065 min  
Response: 0  
Conc: N.D.