

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
 Data File : PL096096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 11:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:27:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.899	66166832	83118521	18.183	17.524
28)	SA Decachlor...	9.113	8.081	50861211	100.1E6	17.761	16.602
Target Compounds							
24)	Chlordane-2	0.000	4.491	0	11869883	N.D.	45.595 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
Data File : PL096096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 11:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:27:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

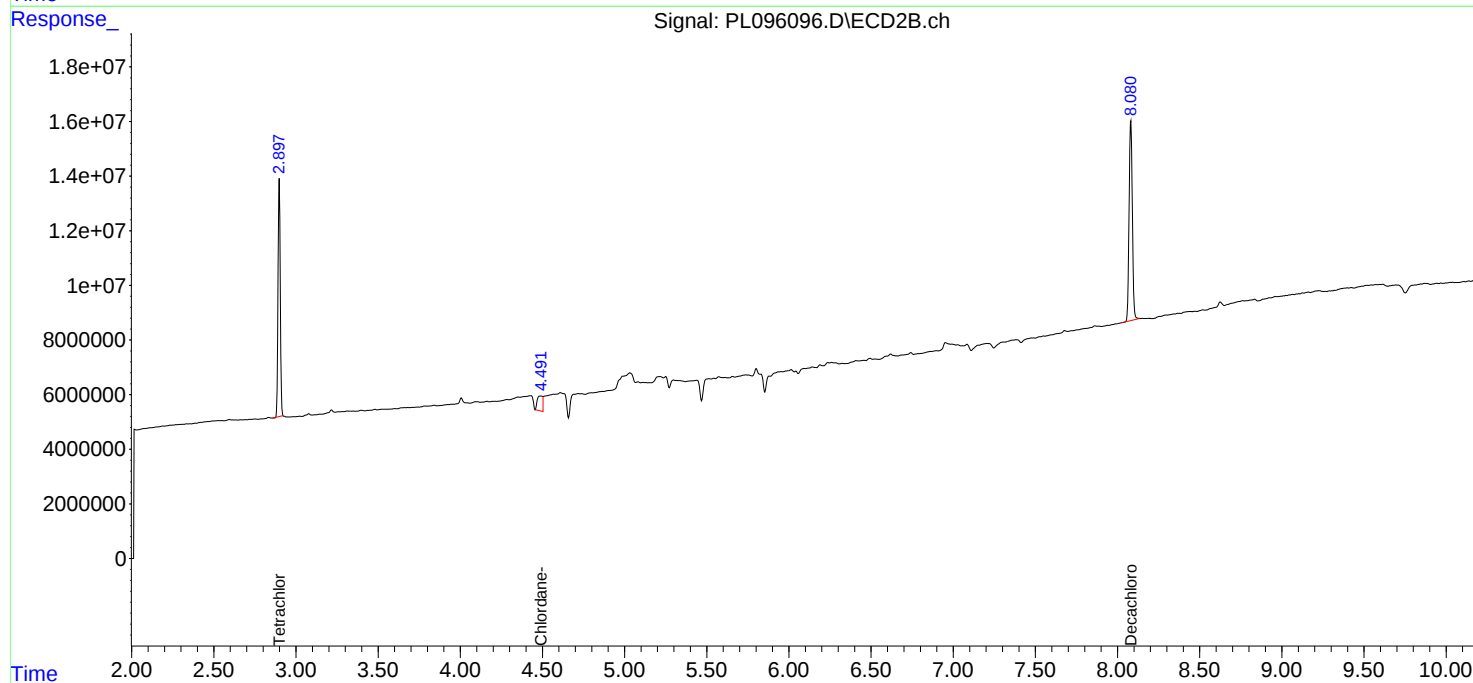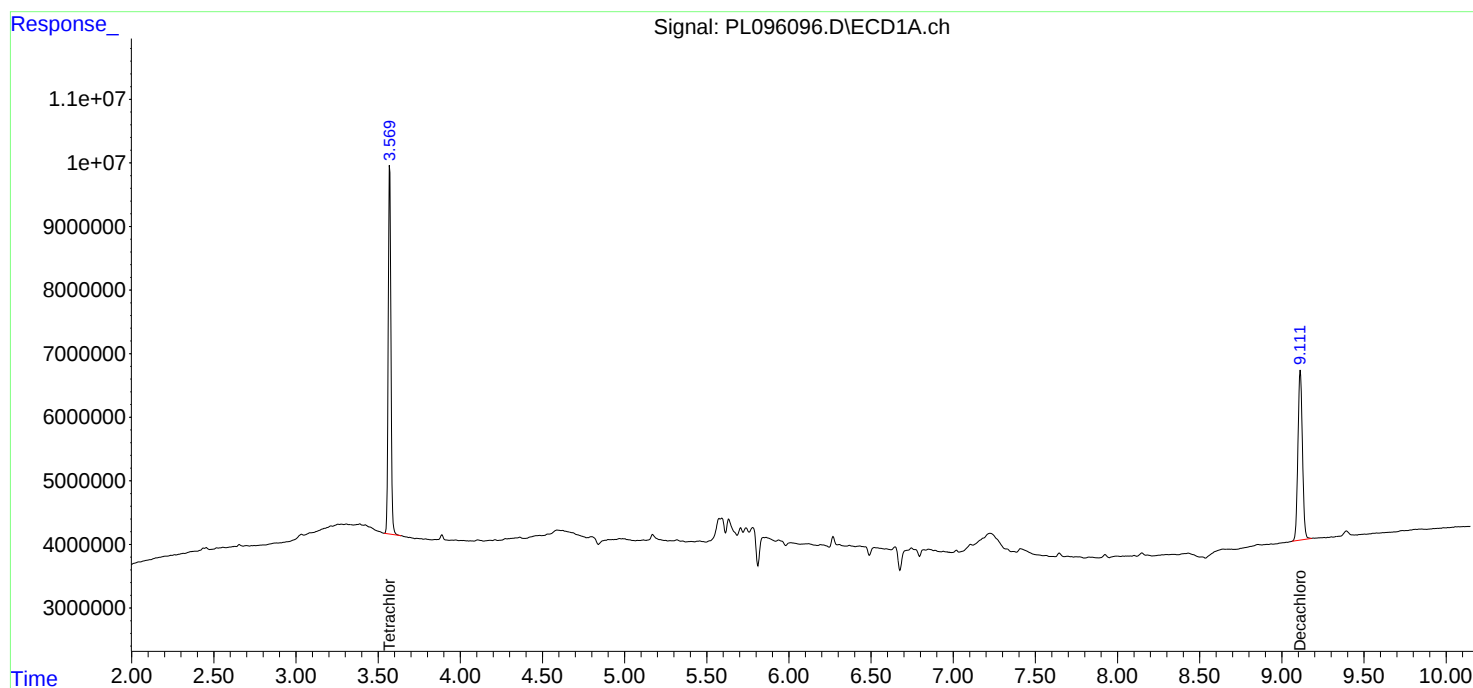


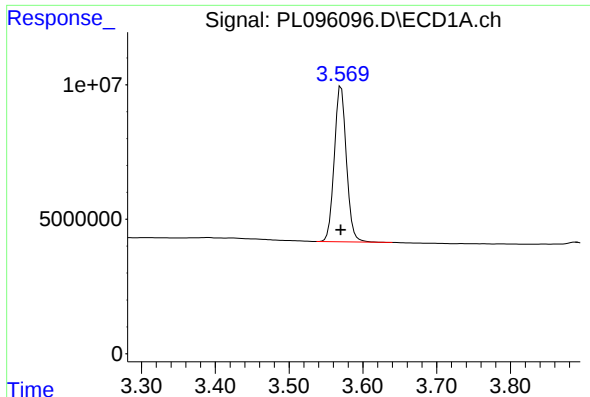

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 66166832
Conc: 18.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

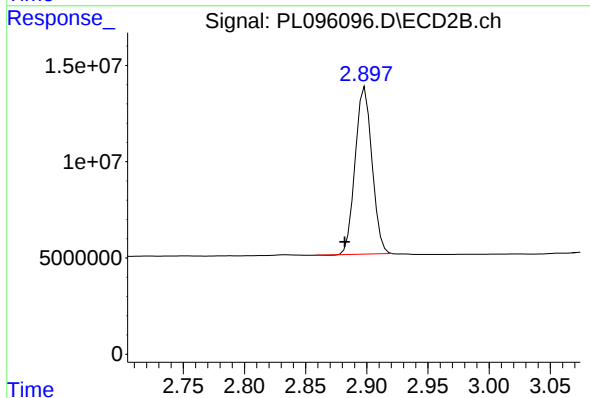


#1 Tetrachloro-m-xylene

R.T.: 2.899 min
Delta R.T.: 0.017 min
Response: 83118521
Conc: 17.52 ng/ml

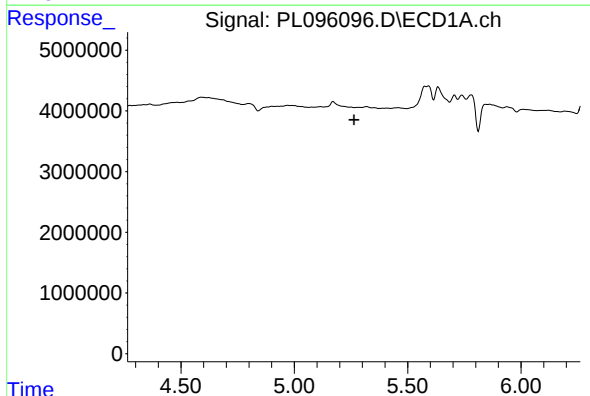


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.264 min
Response: 0
Conc: N.D.

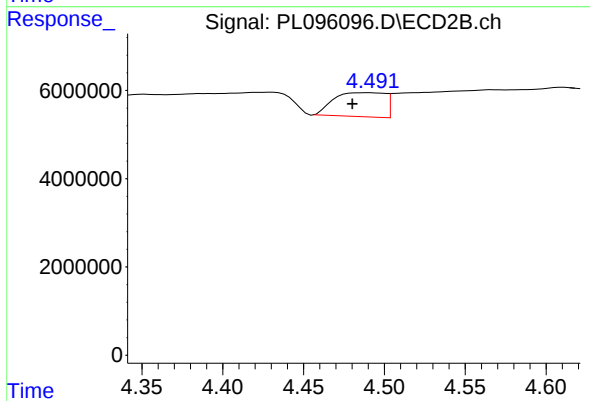

#24 Chlordane-2


R.T.: 4.491 min
Delta R.T.: 0.011 min
Response: 11869883
Conc: 45.59 ng/ml

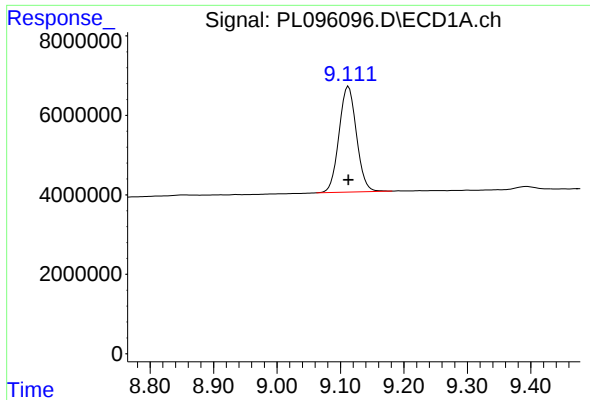

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 50861211
Conc: 17.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

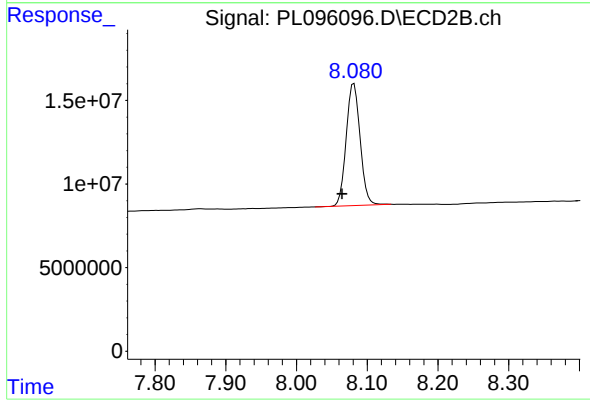

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 100071093
Conc: 16.60 ng/ml