

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
Data File : PL096111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 17:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:30:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.881	65512071	82813452	18.003	17.460
28)	SA Decachlor...	9.114	8.065	47986514	93295638	16.758	15.478
Target Compounds							
24)	Chlordane-2	0.000	4.469	0	6805643	N.D.	26.142 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
Data File : PL096111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 17:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:30:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

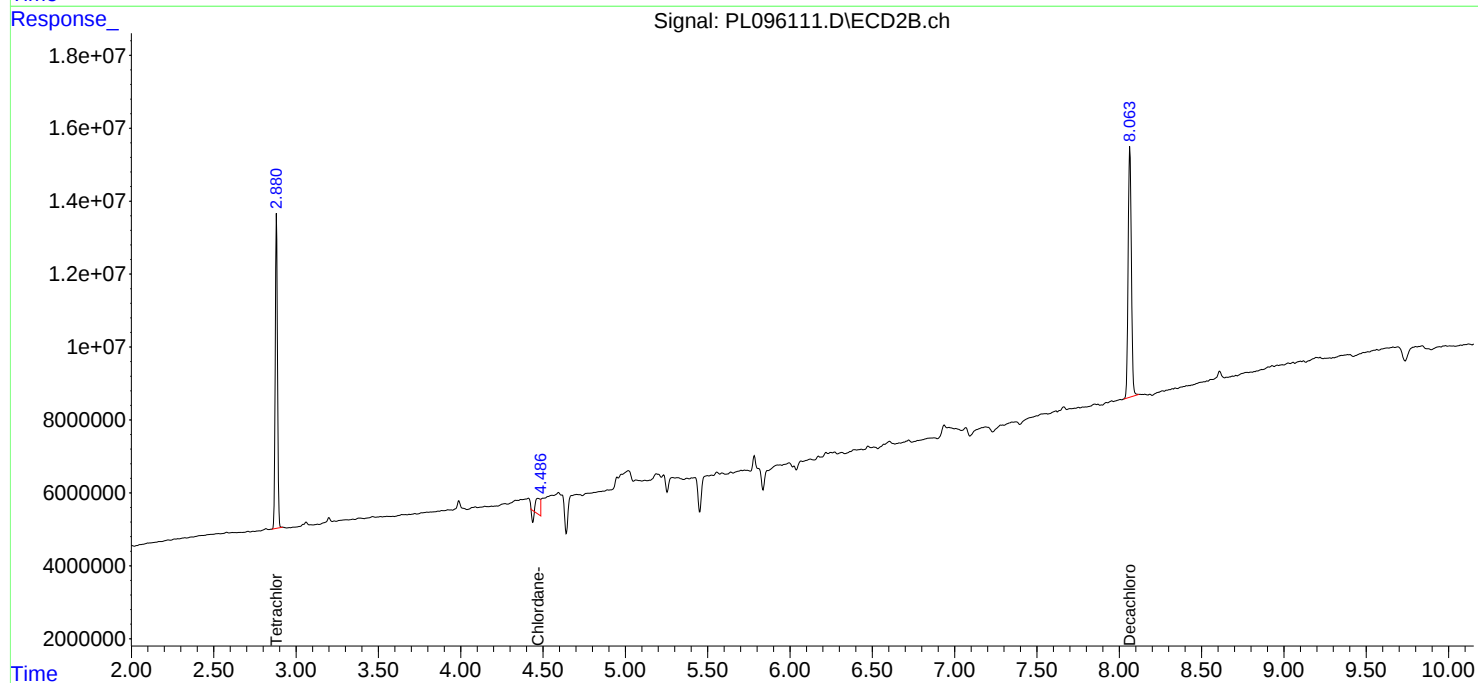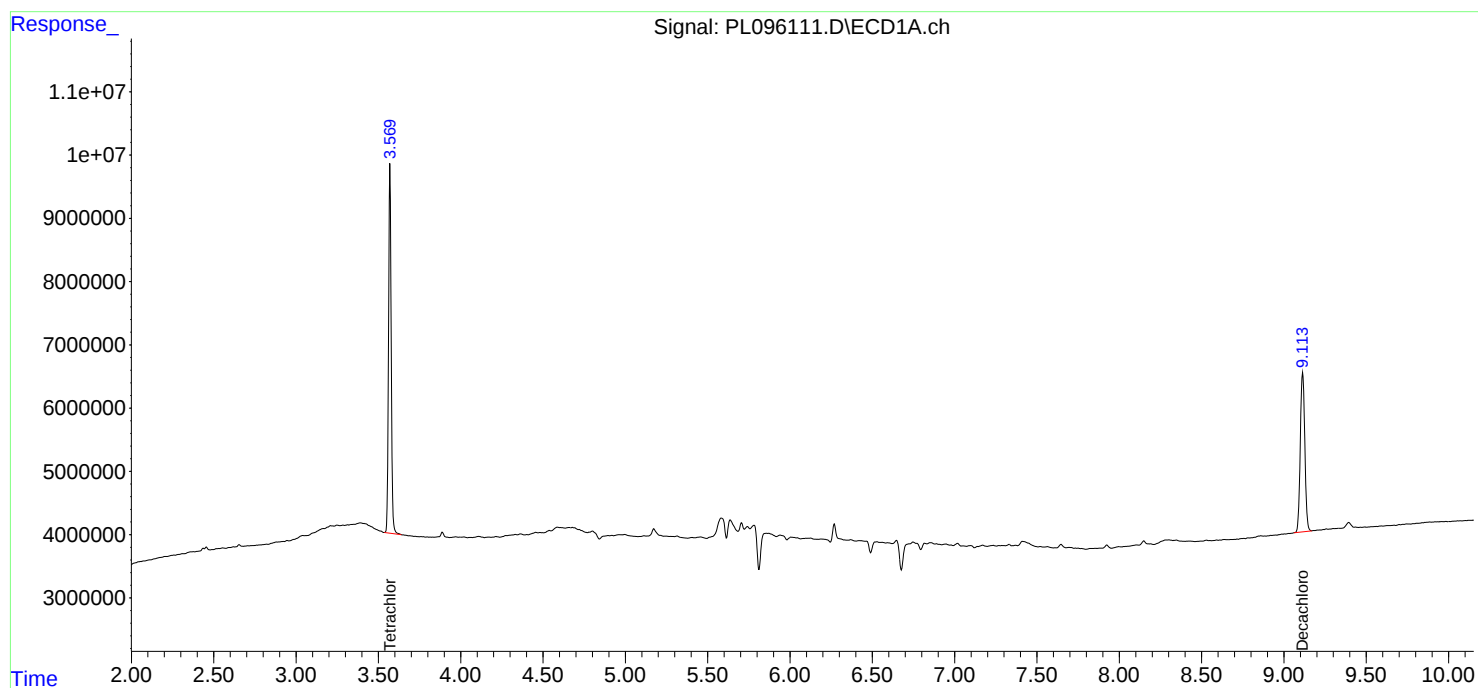


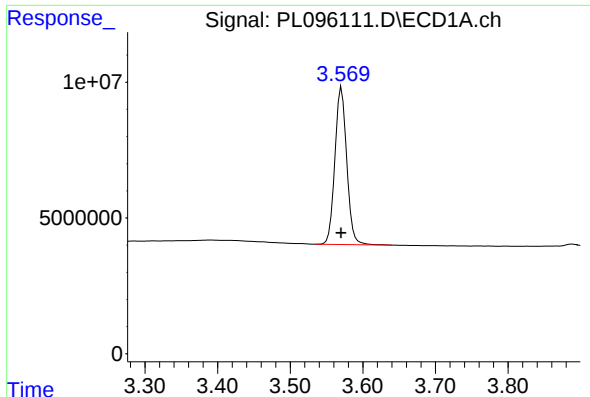

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.000 min
Response: 65512071
Conc: 18.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

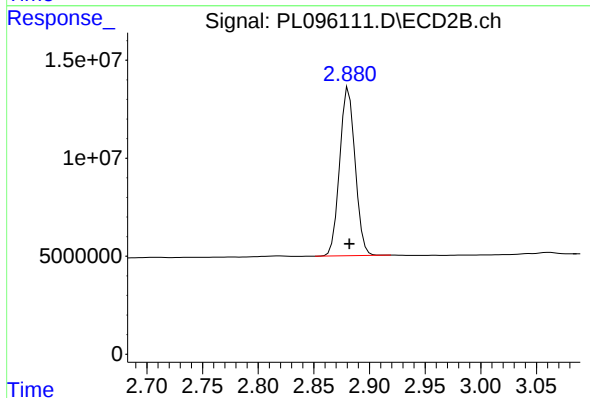


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 82813452
Conc: 17.46 ng/ml

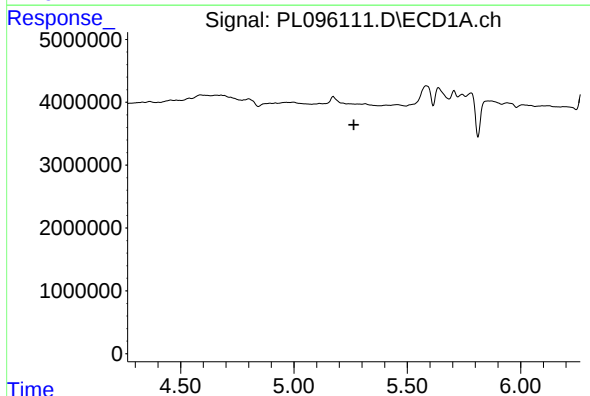


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.264 min
Response: 0
Conc: N.D.

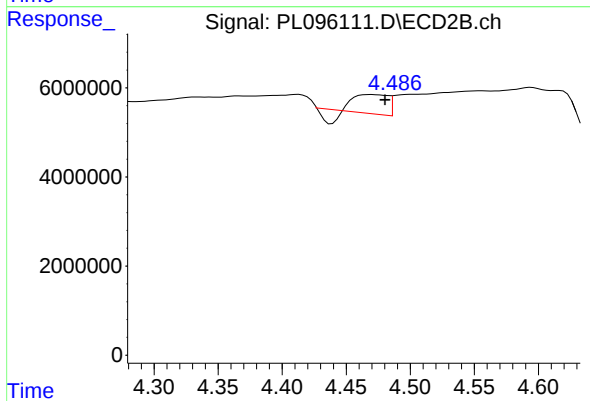

#24 Chlordane-2


R.T.: 4.469 min
Delta R.T.: -0.011 min
Response: 6805643
Conc: 26.14 ng/ml

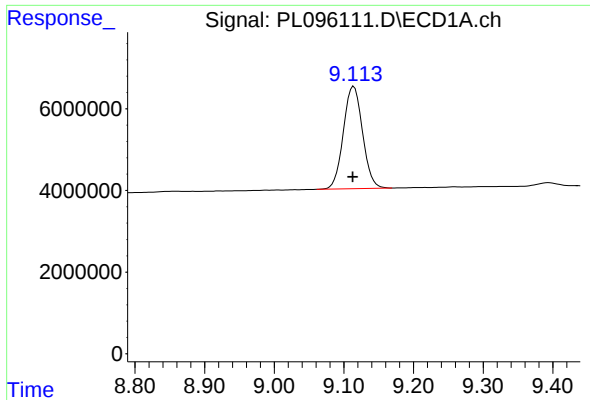

#28 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: 0.002 min
Response: 47986514
Conc: 16.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

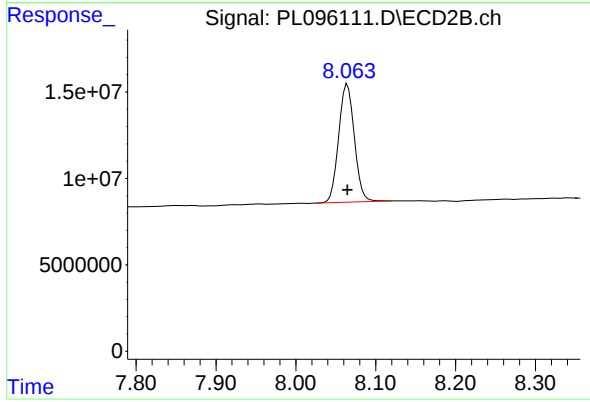

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 93295638
Conc: 15.48 ng/ml