

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
 Data File : PL096099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 12:12
 Operator : AR\AJ
 Sample : Q2338-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-061625

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/19/2025
 Supervised By : mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 01:28:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.576	2.879	41386357	54452842	11.373m	11.481m
28) SA Decachlor...	9.140f	8.066	30343501	36668267	10.596m	6.084 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061825\
Data File : PL096099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 12:12
Operator : AR\AJ
Sample : Q2338-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-061625


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/19/2025
Supervised By : mohammad ahmed 06/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 01:28:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

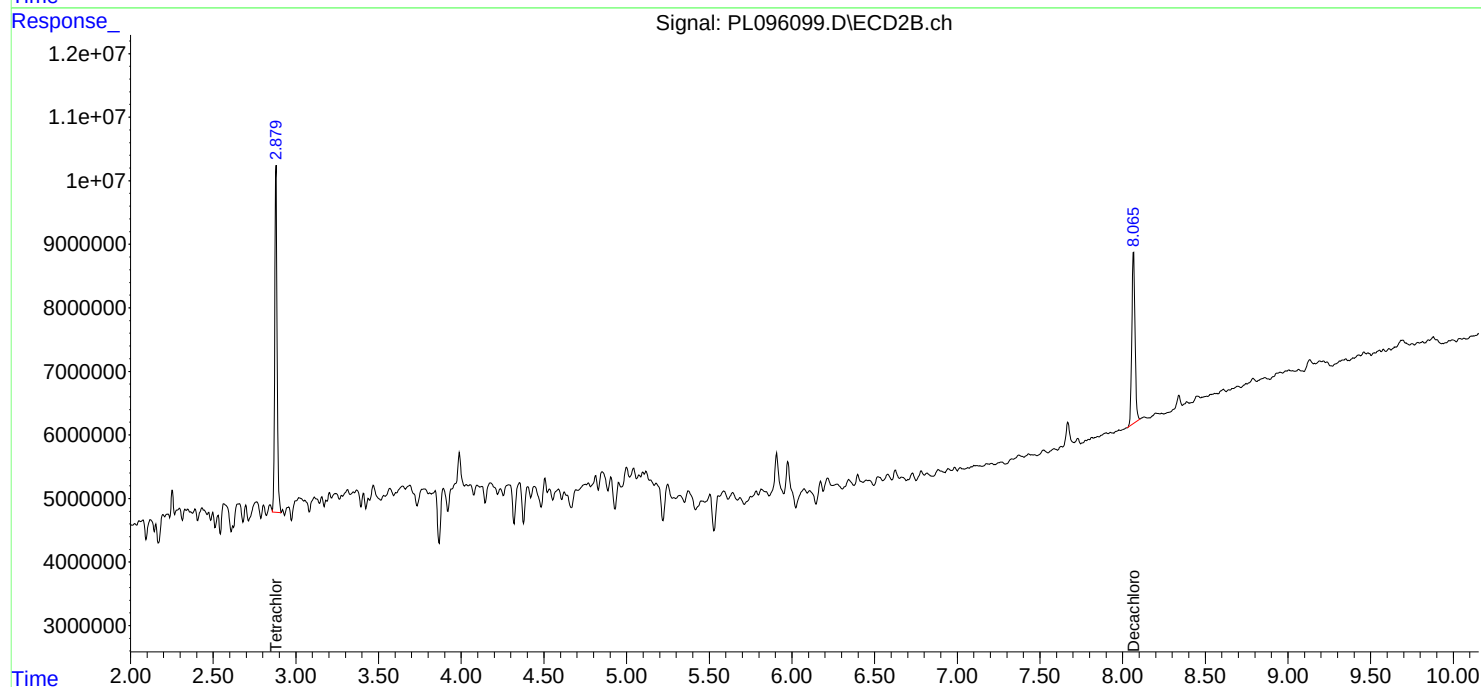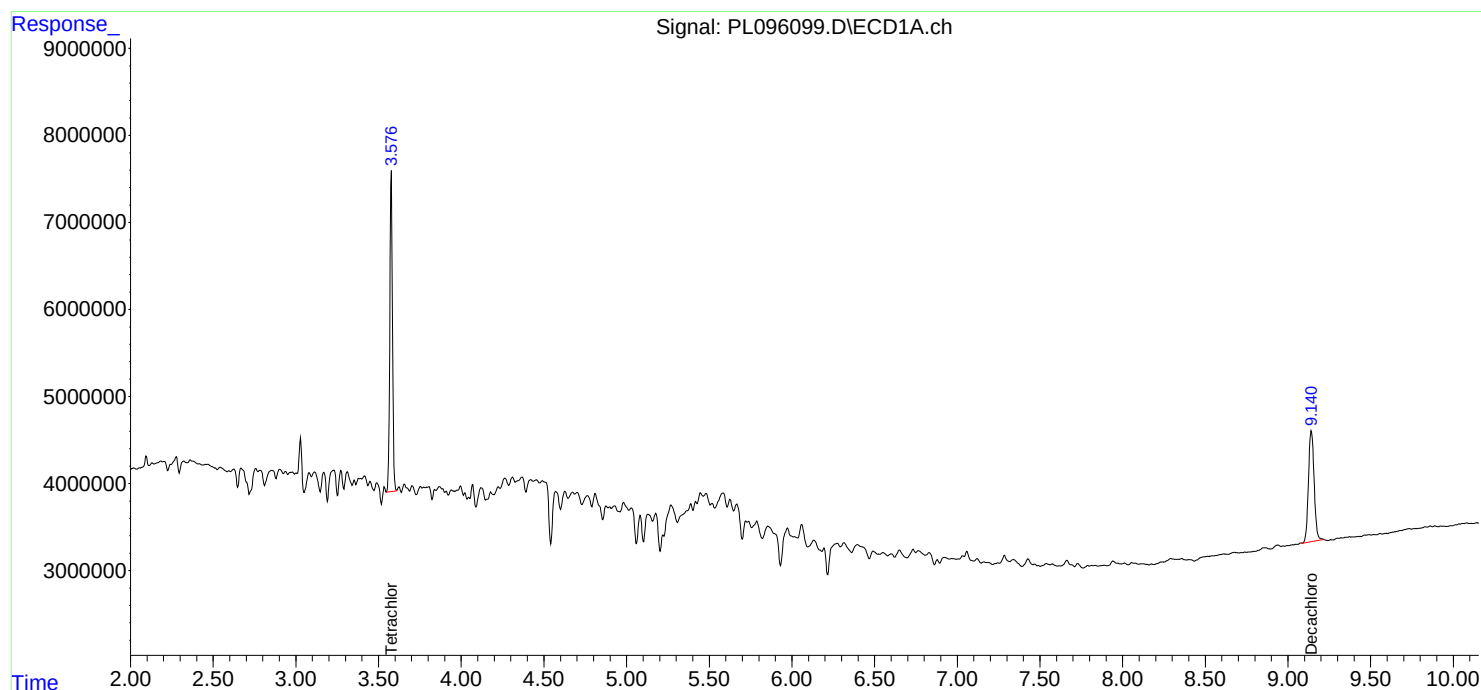

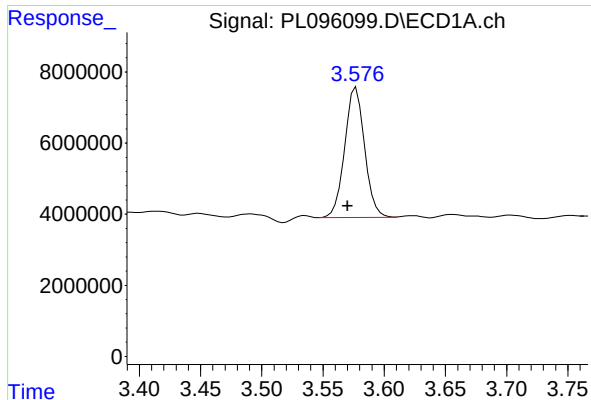


#1 Tetrachloro-m-xylene

R.T.: 3.576 min
Delta R.T.: 0.006 min
Response: 41386357
Conc: 11.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061625


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/19/2025
Supervised By :mohammad ahmed 06/23/2025

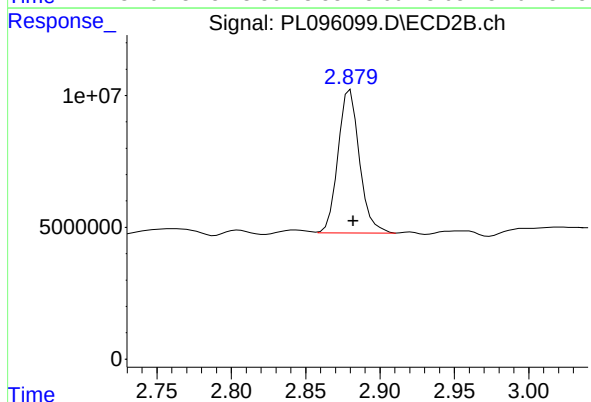


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: -0.003 min
Response: 54452842
Conc: 11.48 ng/ml m

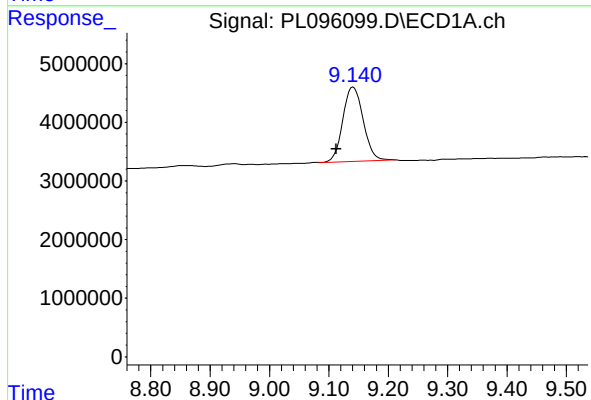

#28 Decachlorobiphenyl

R.T.: 9.140 min
Delta R.T.: 0.027 min
Response: 30343501
Conc: 10.60 ng/ml m

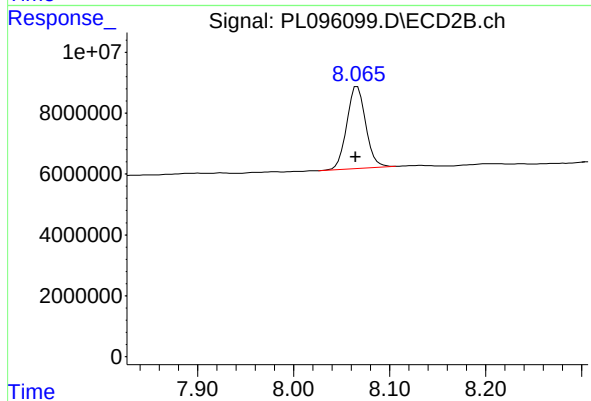

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.002 min
Response: 36668267
Conc: 6.08 ng/ml