

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
 Data File : PL049620.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 09:29
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 00:59:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	4.008f	0.000	19546926	0	1.153	N.D.	#
8) B	Heptachlo...	0.000	5.798	0	10184568	N.D.	3.116	#
12) B	4,4'-DDE	5.457f	0.000	9455116	0	0.604	N.D.	#
14) MA	Endrin	5.790f	0.000	64934414	0	4.502	N.D.	#
16) A	4,4'-DDD	5.957	0.000	34318758	0	2.884	N.D.	#
17) MA	4,4'-DDT	6.183	0.000	199.1E6	0	16.174	N.D.	#
18) B	Endrin al...	6.277f	0.000	173.7E6	0	15.868	N.D.	#
19) B	Endosulfa...	0.000	7.183	0	2625278	N.D.	0.863	#
20) A	Methoxychlor	6.748f	0.000	245.4E6	0	38.265	N.D.	#
21) B	Endrin ke...	6.941	0.000	81618527	0	5.735	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049620.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 09:29
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 00:59:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

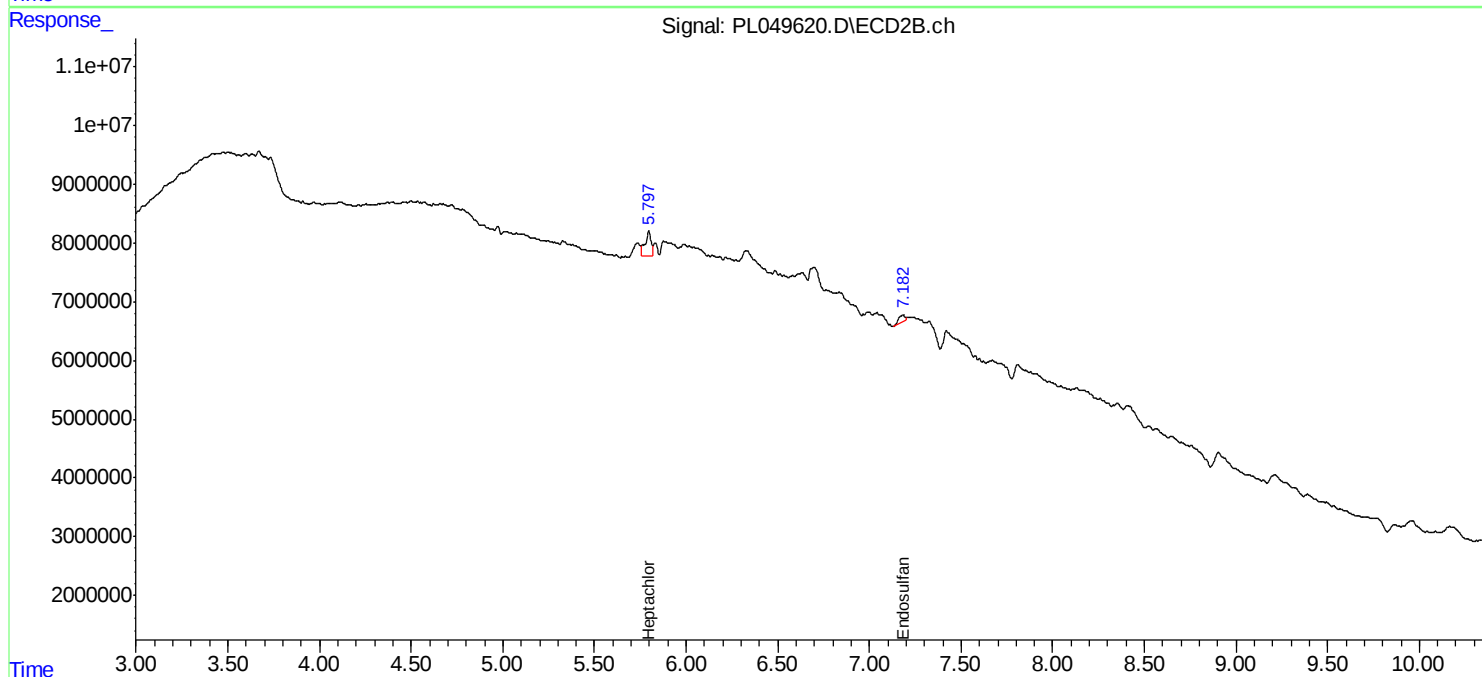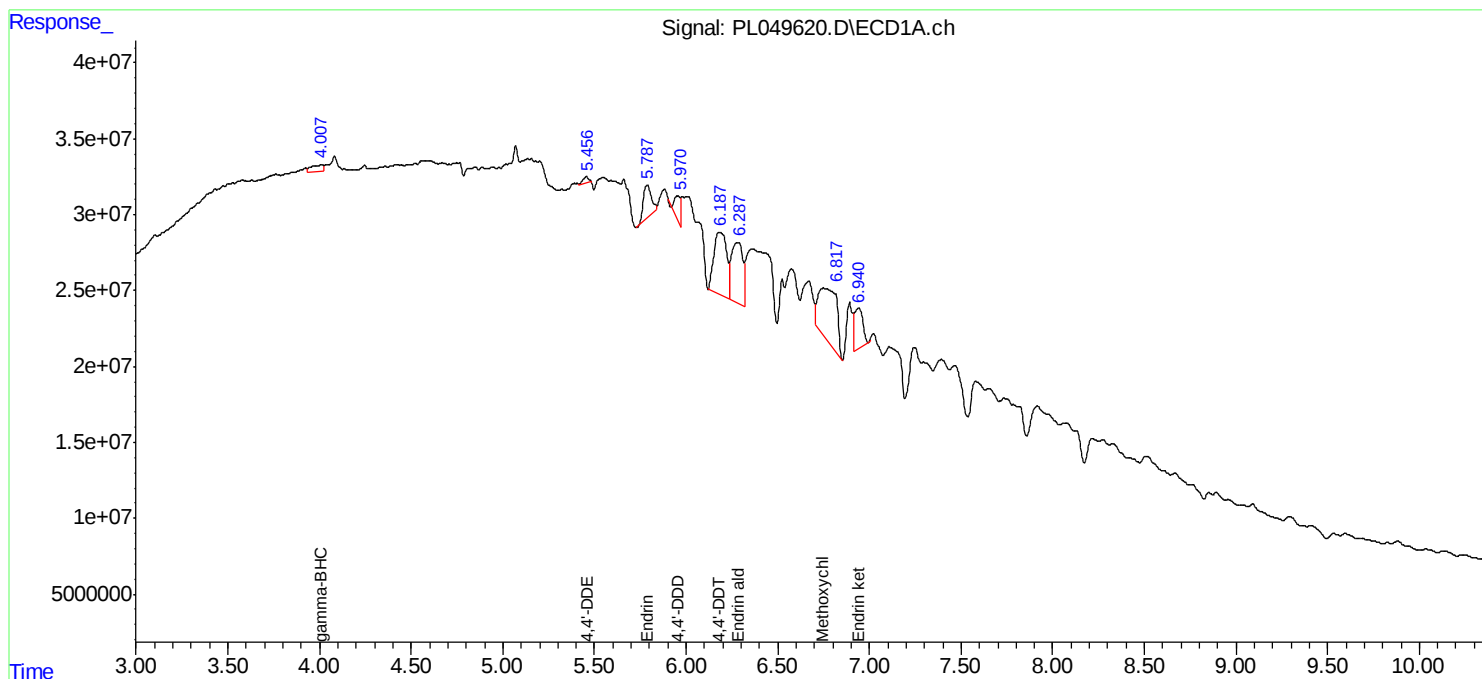


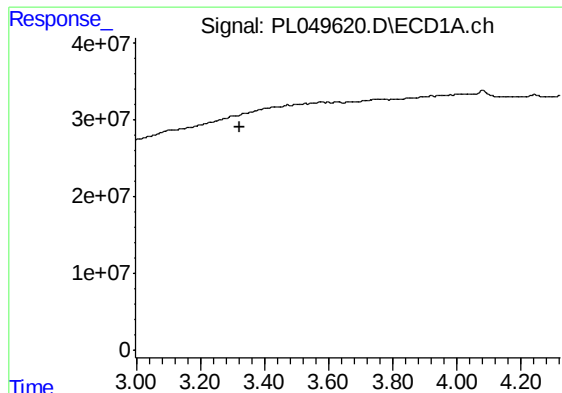

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

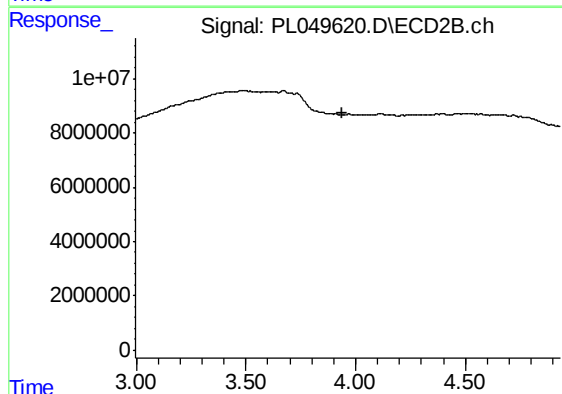


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

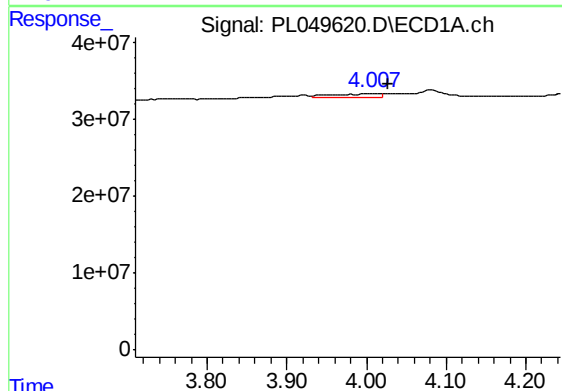


#3 gamma-BHC (Lindane)

R.T.: 4.008 min
Delta R.T.: -0.019 min
Response: 19546926
Conc: 1.15 ng/ml

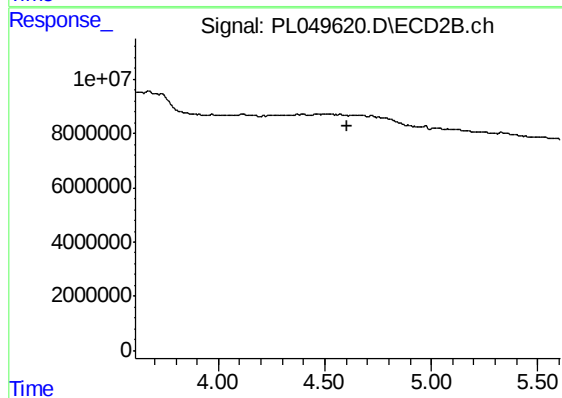

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

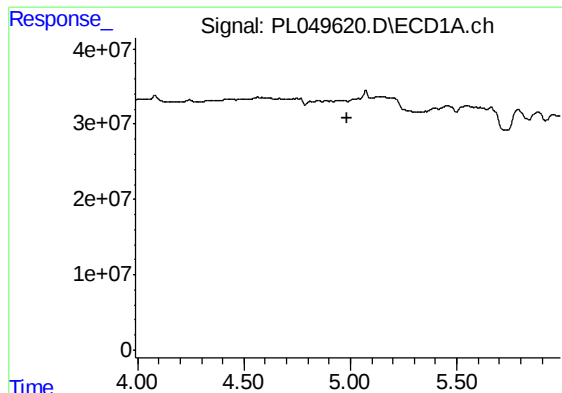

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

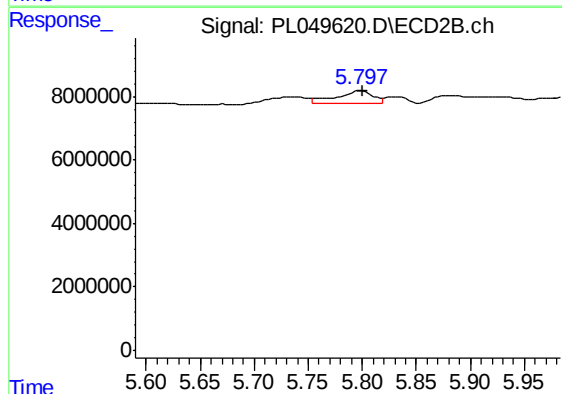


#8 Heptachlor epoxide

R.T.: 5.798 min
Delta R.T.: -0.002 min
Response: 10184568
Conc: 3.12 ng/ml

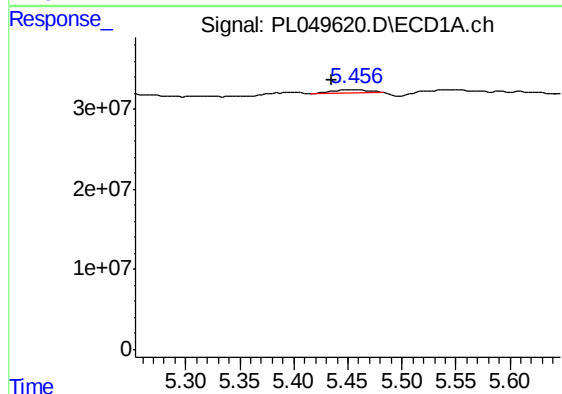


#12 4,4'-DDE

R.T.: 5.457 min
Delta R.T.: 0.022 min
Response: 9455116
Conc: 0.60 ng/ml

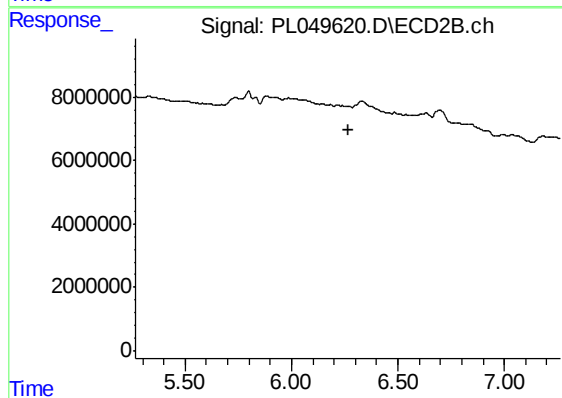

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.267 min
Response: 0
Conc: N.D.

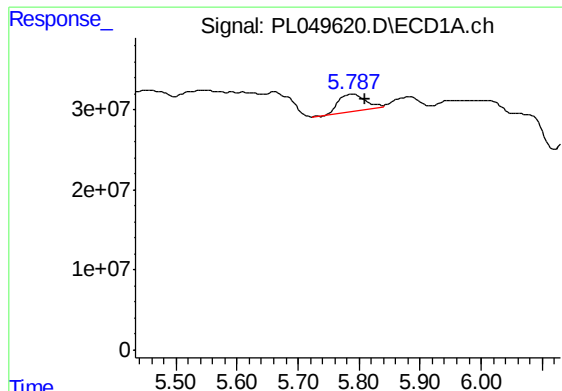

#14 Endrin


R.T.: 5.790 min
Delta R.T.: -0.021 min
Response: 64934414
Conc: 4.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

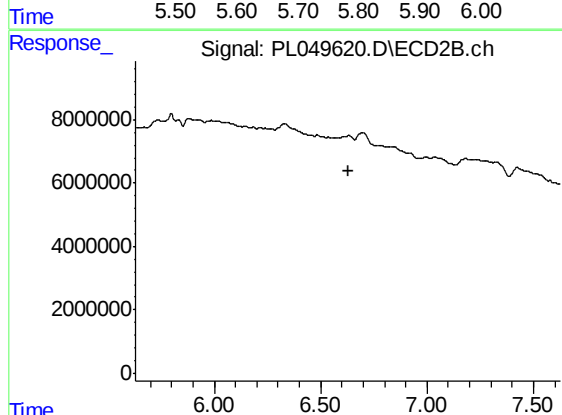


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

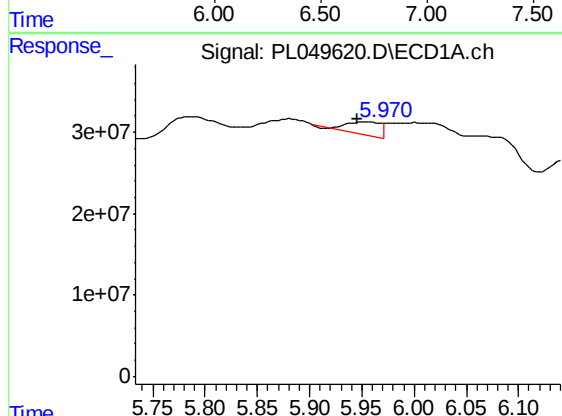


#16 4,4'-DDD

R.T.: 5.957 min
Delta R.T.: 0.012 min
Response: 34318758
Conc: 2.88 ng/ml

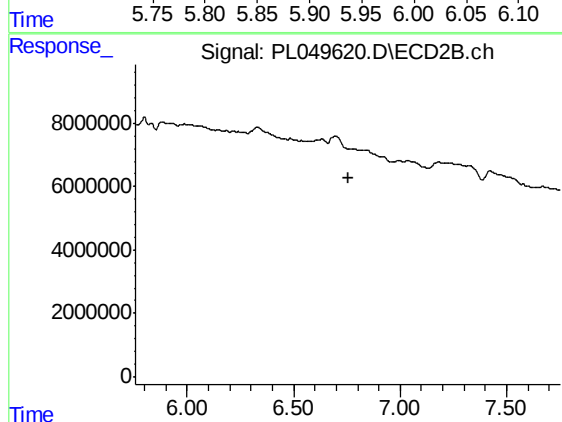

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

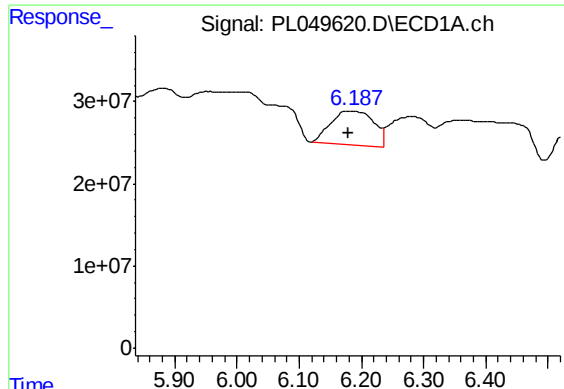

#17 4,4'-DDT


R.T.: 6.183 min
Delta R.T.: 0.003 min
Response: 199148643
Conc: 16.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

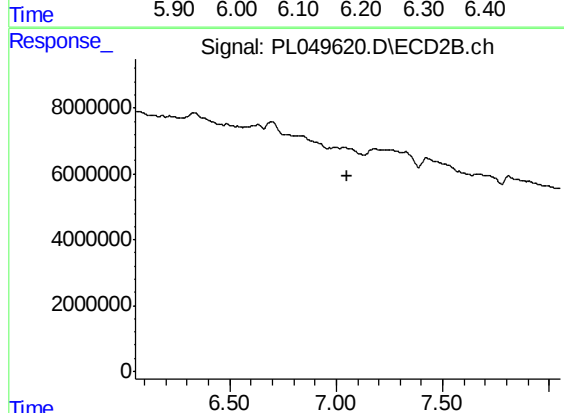


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

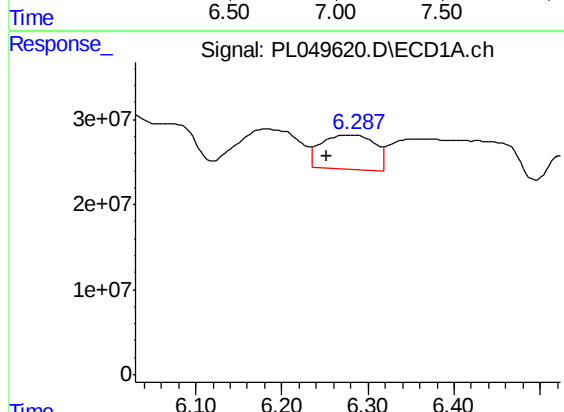


#18 Endrin aldehyde

R.T.: 6.277 min
Delta R.T.: 0.024 min
Response: 173664119
Conc: 15.87 ng/ml

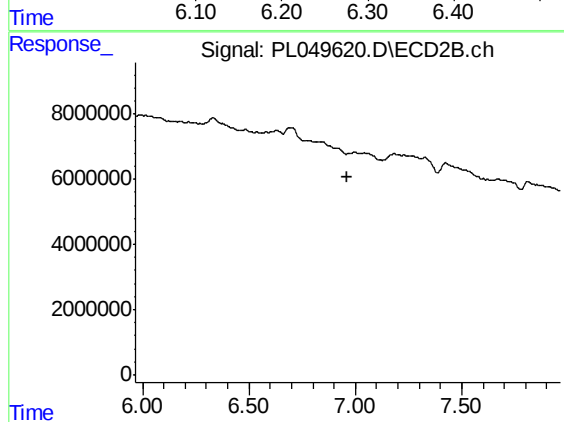

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.965 min
Response: 0
Conc: N.D.

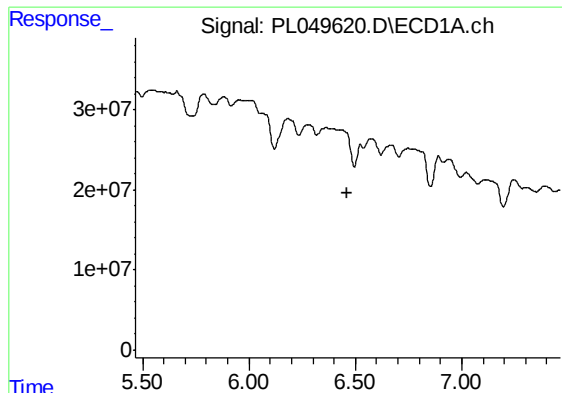

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

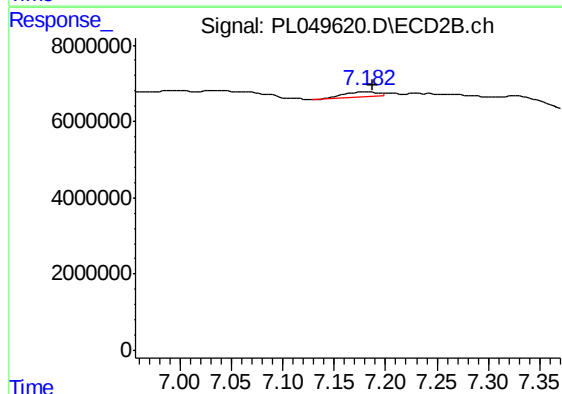


#19 Endosulfan Sulfate

R.T.: 7.183 min
Delta R.T.: -0.005 min
Response: 2625278
Conc: 0.86 ng/ml

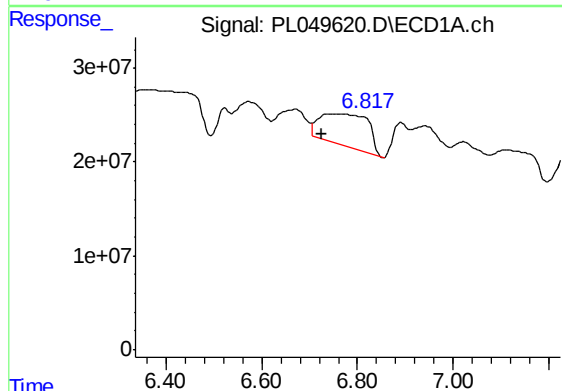


#20 Methoxychlor

R.T.: 6.748 min
Delta R.T.: 0.023 min
Response: 245421253
Conc: 38.27 ng/ml

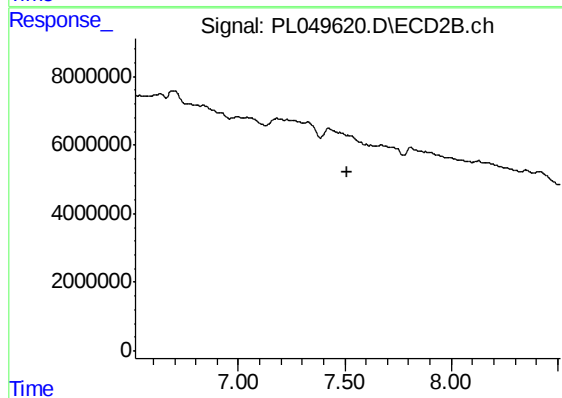

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

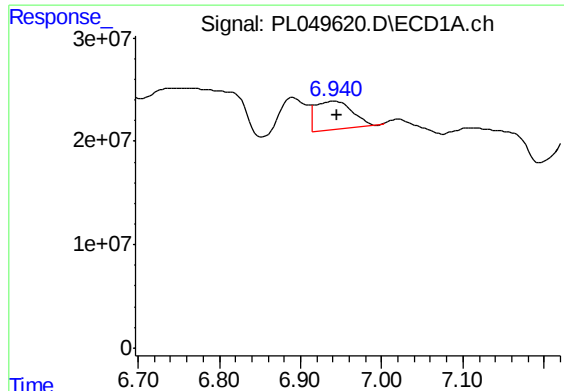

#21 Endrin ketone


R.T.: 6.941 min
Delta R.T.: -0.005 min
Response: 81618527
Conc: 5.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

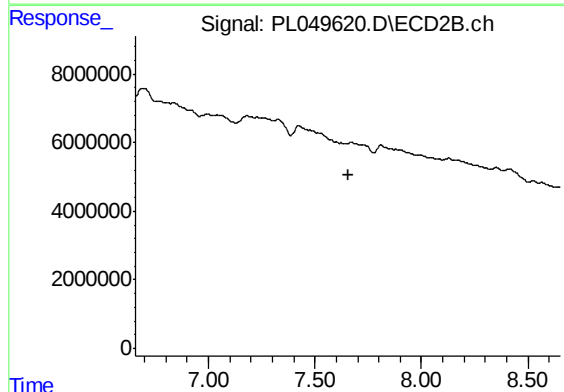


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

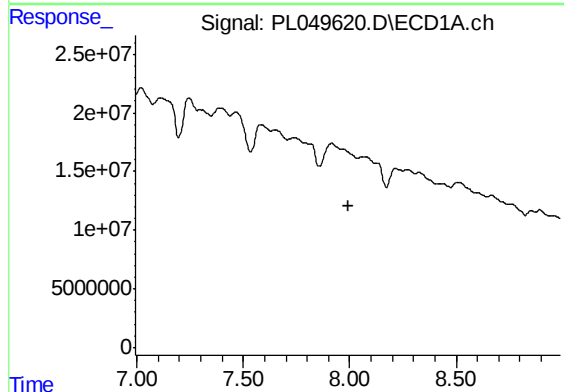

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

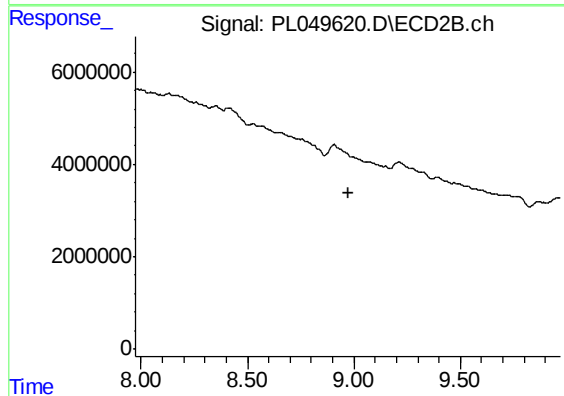

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.972 min
Response: 0
Conc: N.D.