

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
 Data File : PL049669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 23:28
 Operator : SM\AJ
 Sample : K3441-02
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SAMPLE-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:12:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.936	214.6E6	59602336	19.480	20.630
28)	SA Decachlor...	7.990	8.971	216.6E6	63313637	17.037	18.958
Target Compounds							
3)	MA gamma-BHC...	4.037	0.000	133.5E6	0	7.877	N.D. #
4)	MA Heptachlor	4.330f	0.000	20338935	0	1.149	N.D. #
6)	B beta-BHC	0.000	4.797	0	6411026	N.D.	3.722 #
7)	B delta-BHC	0.000	4.991	0	4203483	N.D.	1.370 #
15)	B Endosulfa...	0.000	6.857f	0	4106566	N.D.	1.354 #
16)	A 4,4'-DDD	5.944	0.000	9338630	0	0.785	N.D. #
21)	B Endrin ke...	0.000	7.656	0	2603821	N.D.	0.819 #
22)	Mirex	7.124	0.000	2655952	0	0.252	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 23:28
Operator : SM\AJ
Sample : K3441-02
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SAMPLE-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:12:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

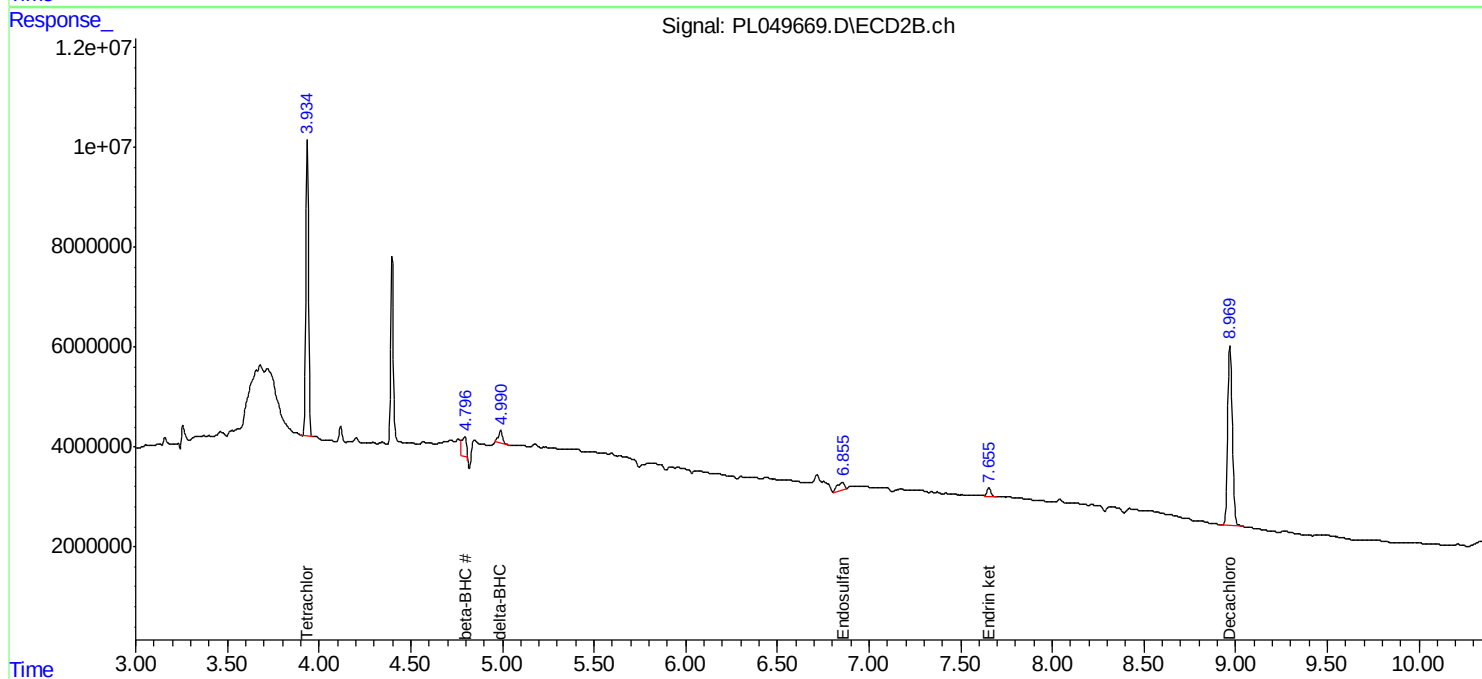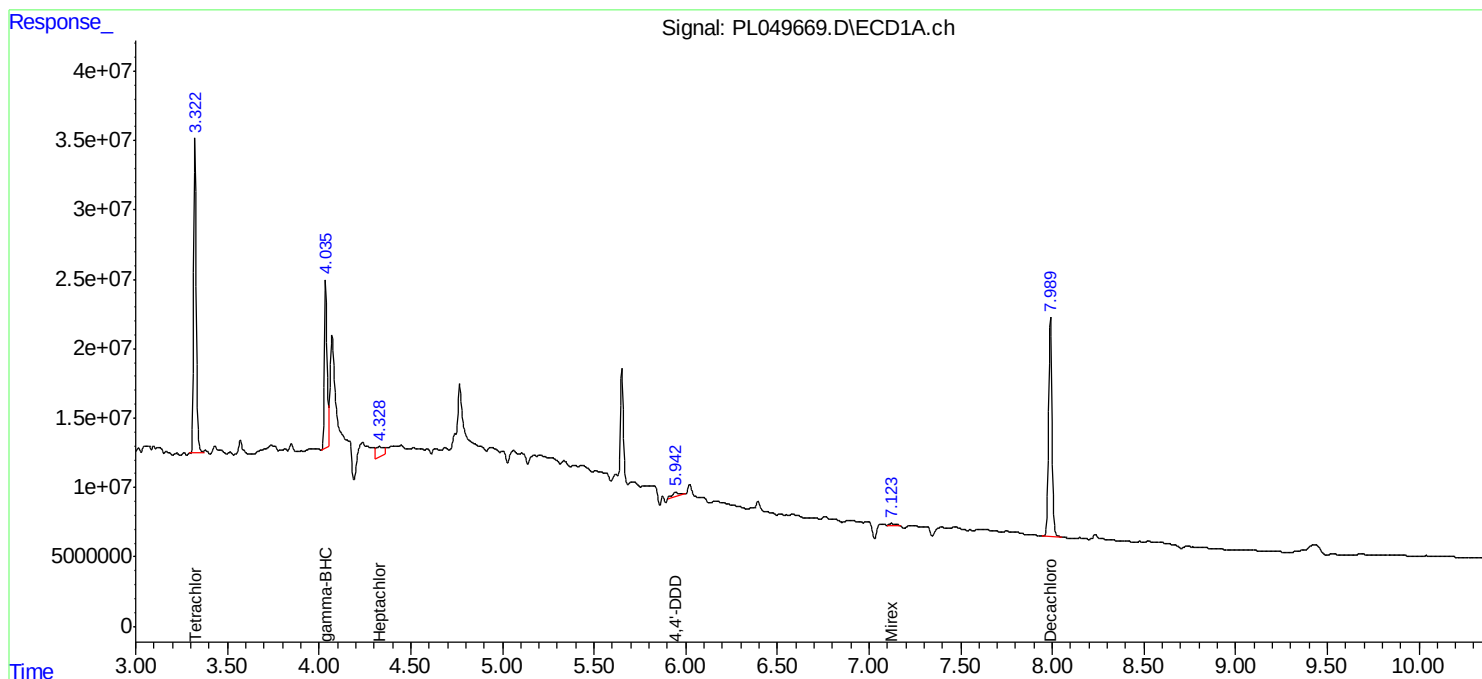


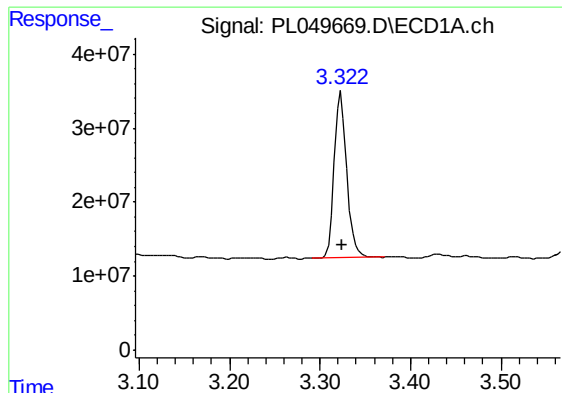

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 214642837
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-3

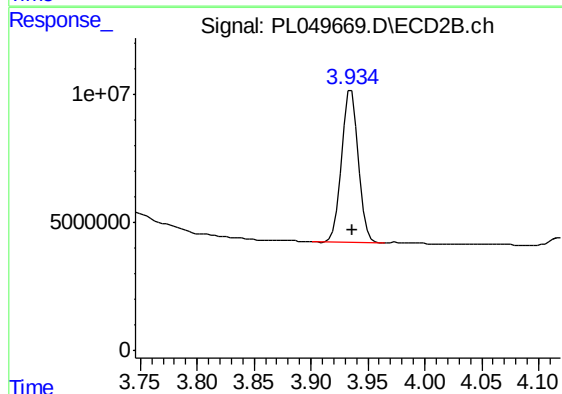


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 59602336
Conc: 20.63 ng/ml

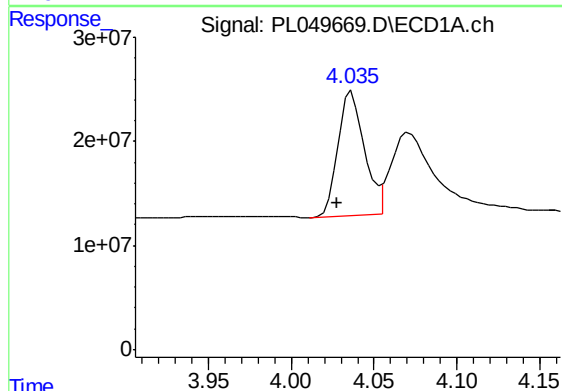


#3 gamma-BHC (Lindane)

R.T.: 4.037 min
Delta R.T.: 0.009 min
Response: 133507581
Conc: 7.88 ng/ml

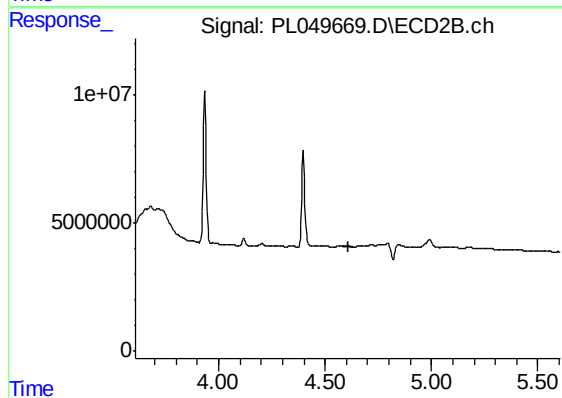

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

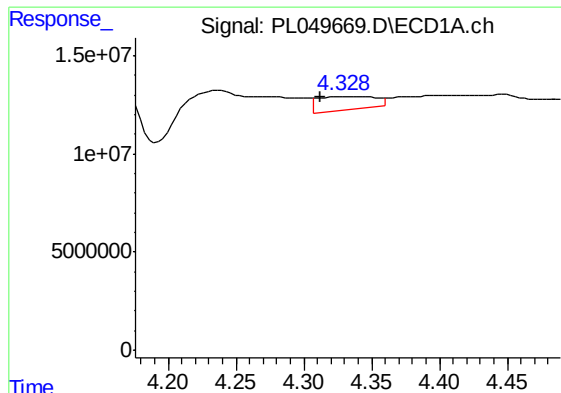

#4 Heptachlor


R.T.: 4.330 min
Delta R.T.: 0.018 min
Response: 20338935
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-3

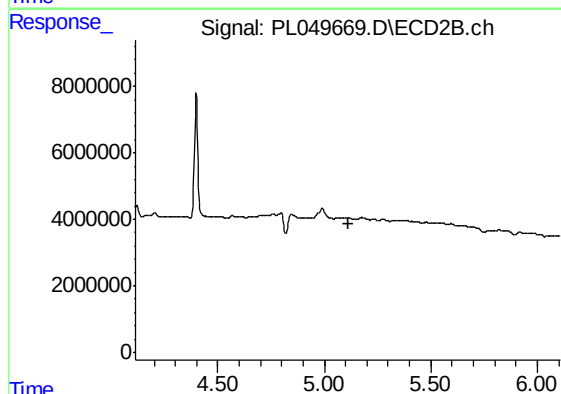


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

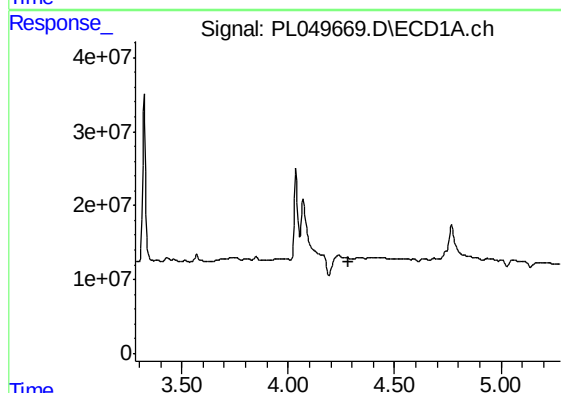


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

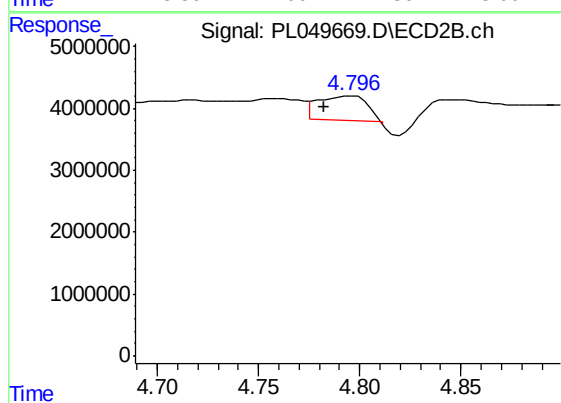

#6 beta-BHC


R.T.: 4.797 min
Delta R.T.: 0.014 min
Response: 6411026
Conc: 3.72 ng/ml

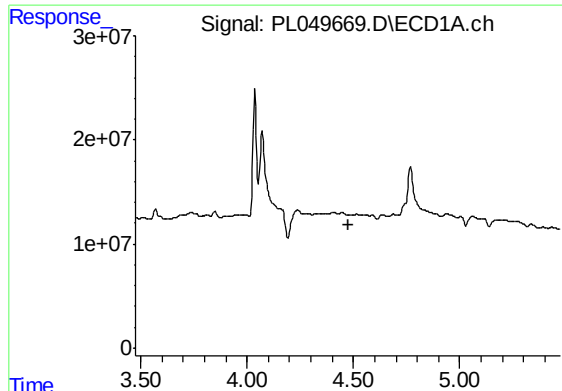

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SAMPLE-3

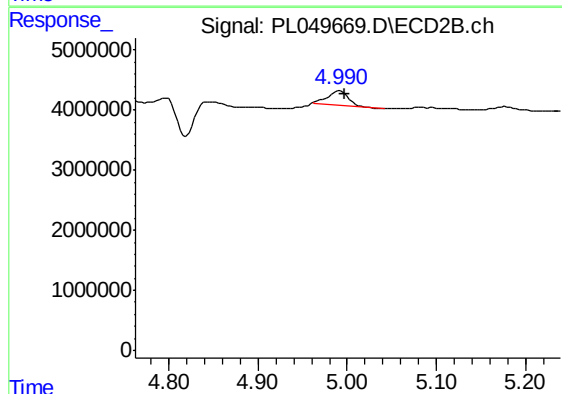


#7 delta-BHC

R.T.: 4.991 min
Delta R.T.: -0.005 min
Response: 4203483
Conc: 1.37 ng/ml

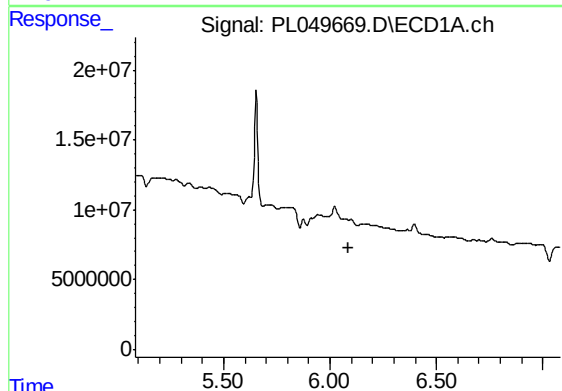


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

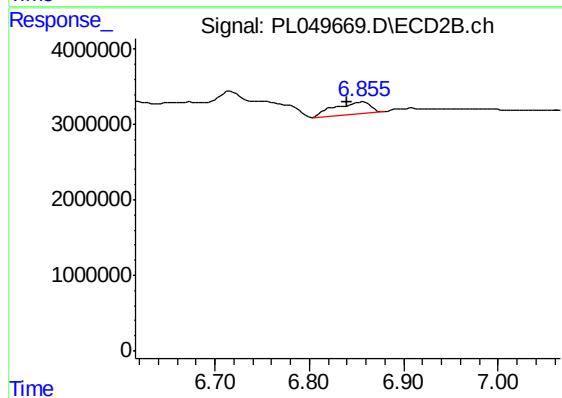

#15 Endosulfan II


R.T.: 6.857 min
Delta R.T.: 0.016 min
Response: 4106566
Conc: 1.35 ng/ml

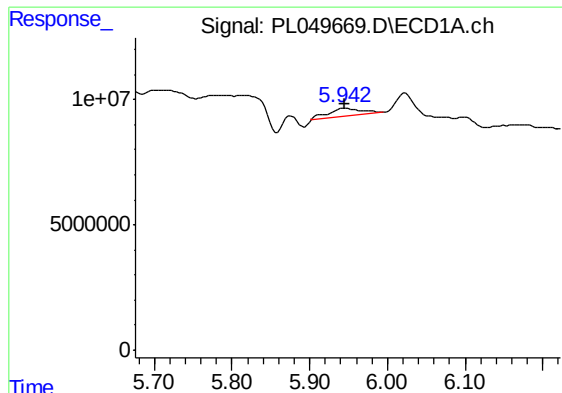

#16 4,4'-DDD


R.T.: 5.944 min
Delta R.T.: -0.001 min
Response: 9338630
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-3

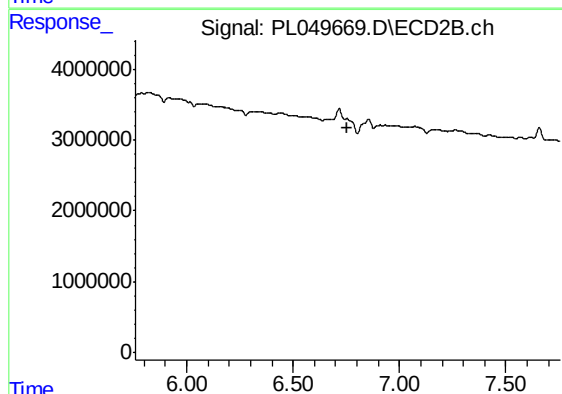


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.756 min
Response: 0
Conc: N.D.

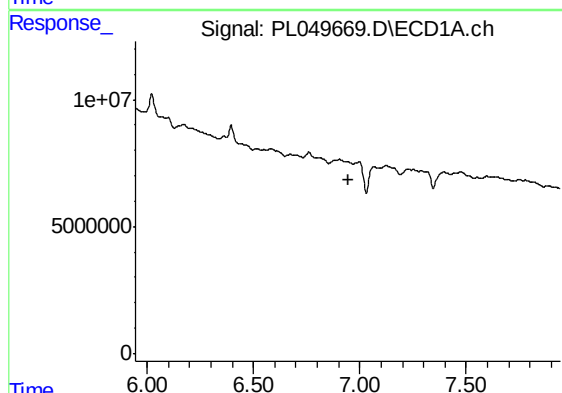


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.946 min
Response: 0
Conc: N.D.

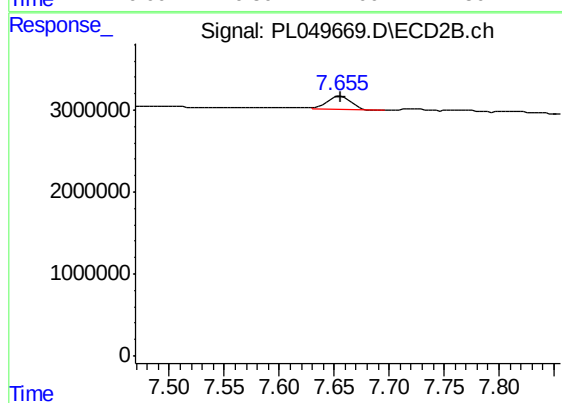

#21 Endrin ketone


R.T.: 7.656 min
Delta R.T.: 0.000 min
Response: 2603821
Conc: 0.82 ng/ml

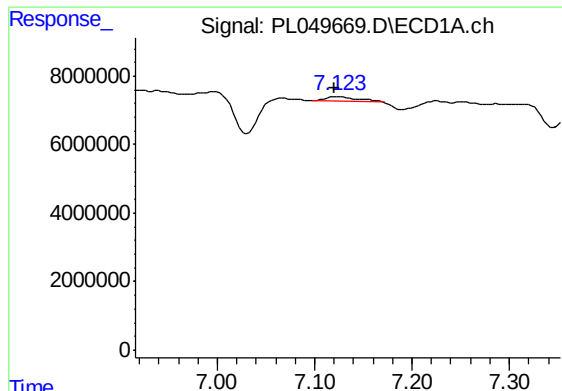

#22 Mirex


R.T.: 7.124 min
Delta R.T.: 0.004 min
Response: 2655952
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SAMPLE-3

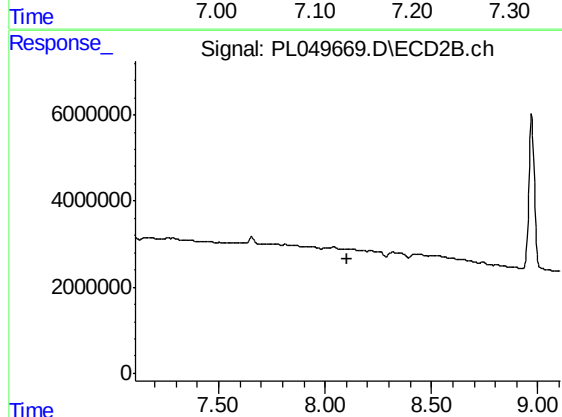


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.

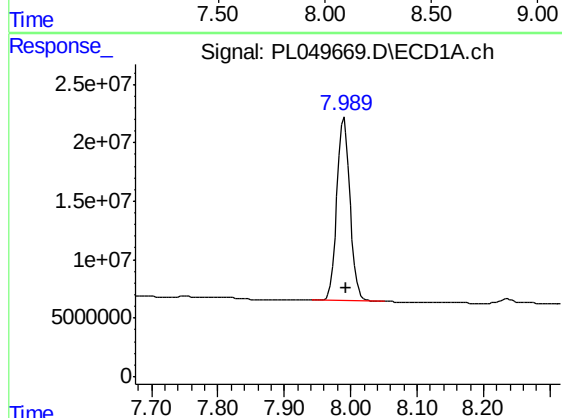

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 216634215
Conc: 17.04 ng/ml

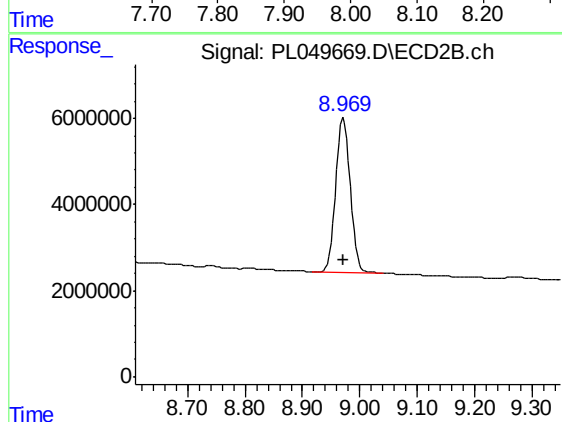

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.002 min
Response: 63313637
Conc: 18.96 ng/ml