Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 01:44
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument : ECD_L
ClientSampleId : I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 06:39:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

		Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
		System Monitoring Compounds							
1)	SA	Tetrachlo...	3.324	3.935	225.8E6	63735137	20.495	22.061	
28)	SA	Decachlor...	7.990	8.972	240.9E6	66685528	18.946	19.968	
		Target Compounds							
7)	B	delta-BHC	0.000	4.972f	0	886927	N.D.	0.289	#
8)	B	Heptachlo...	0.000	5.797	0	31088203	N.D.	9.511	#
9)	A	Endosulfan I	5.334f	0.000	18919098	0	1.293	N.D.	#
14)	MA	Endrin	5.823	0.000	10949110	0	0.759	N.D.	#
15)	B	Endosulfa...	6.070f	0.000	12474797	0	0.945	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 01:44
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 06:39:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

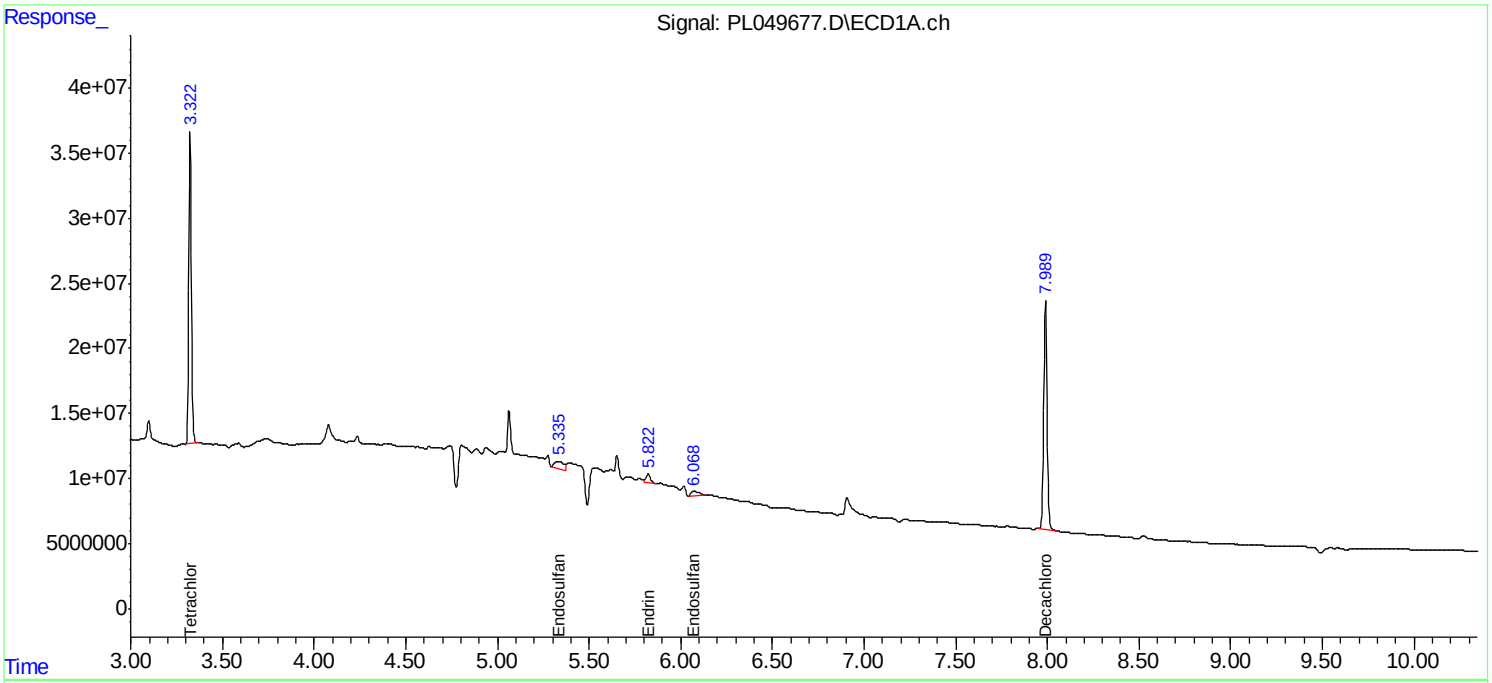

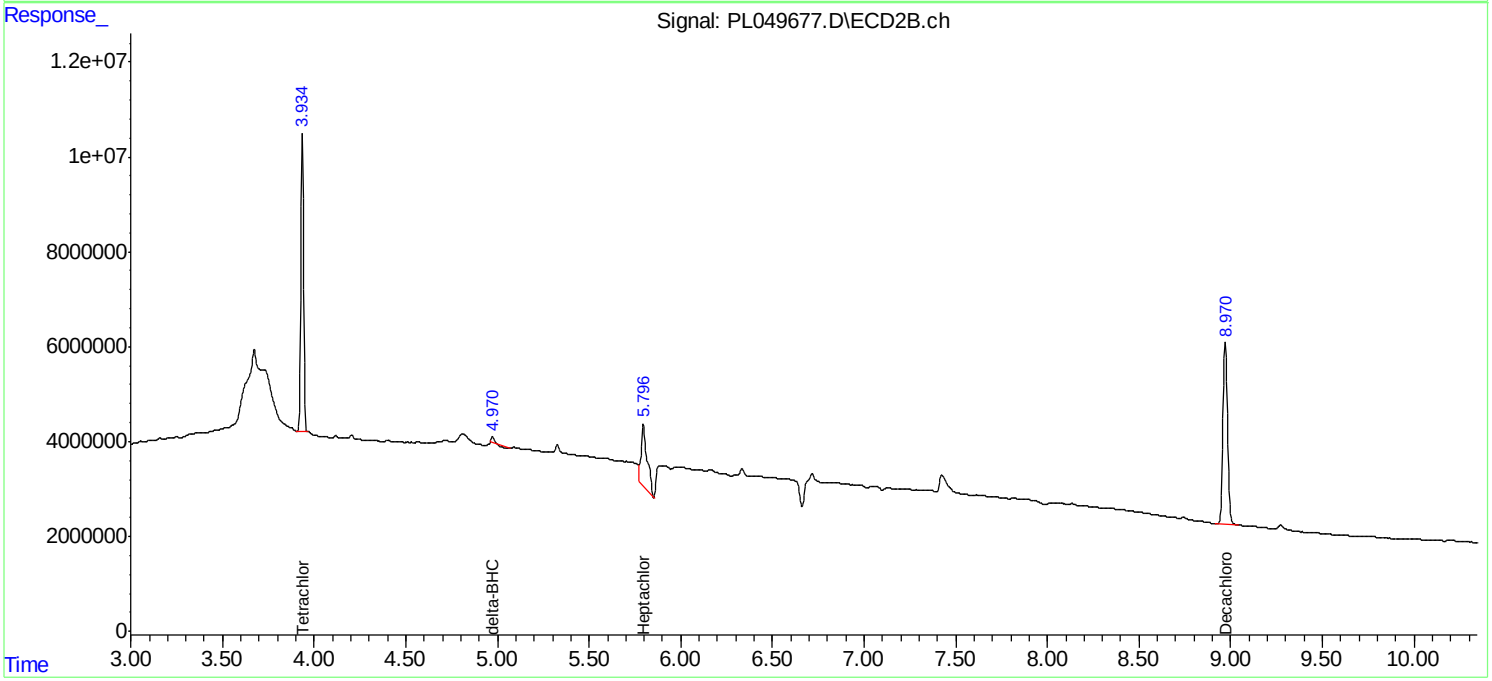

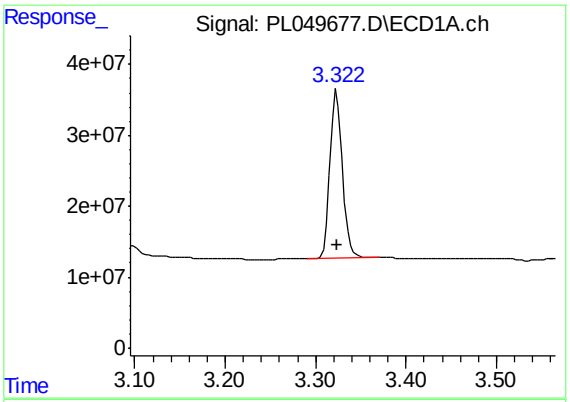

#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 225830758
Conc: 20.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

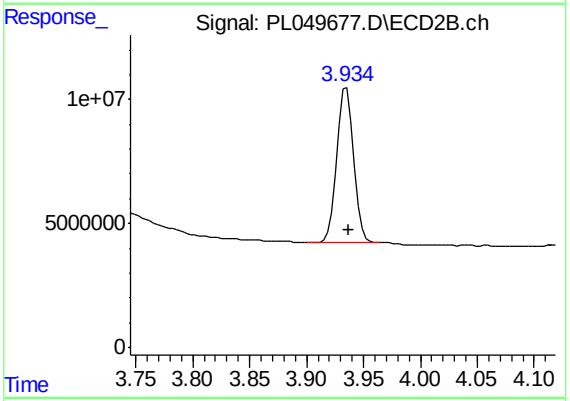

#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 63735137
Conc: 22.06 ng/ml

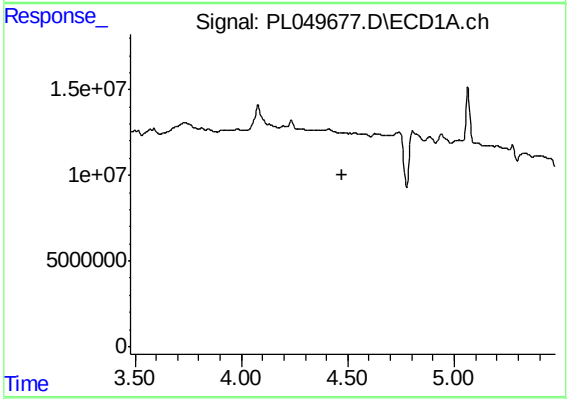

#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.475 min
Response: 0
Conc: N.D.

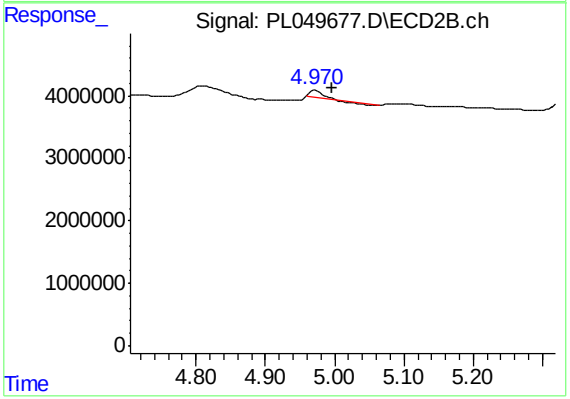

#7 delta-BHC

R.T.: 4.972 min
Delta R.T.: -0.025 min
Response: 886927
Conc: 0.29 ng/ml

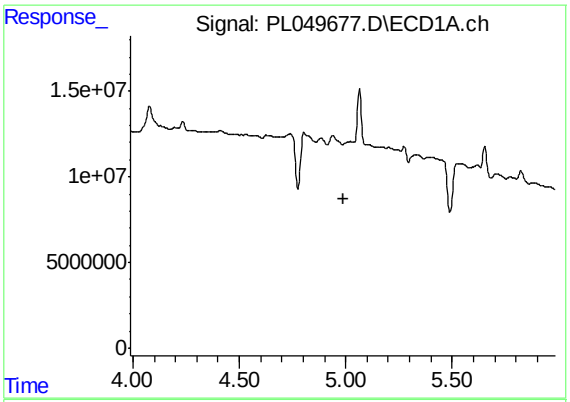

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

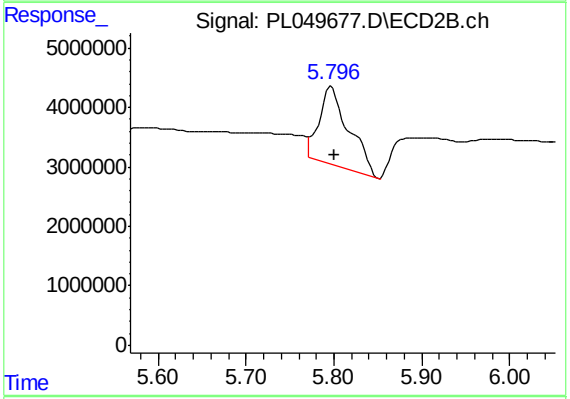

#8 Heptachlor epoxide

R.T.: 5.797 min
Delta R.T.: -0.003 min
Response: 31088203
Conc: 9.51 ng/ml

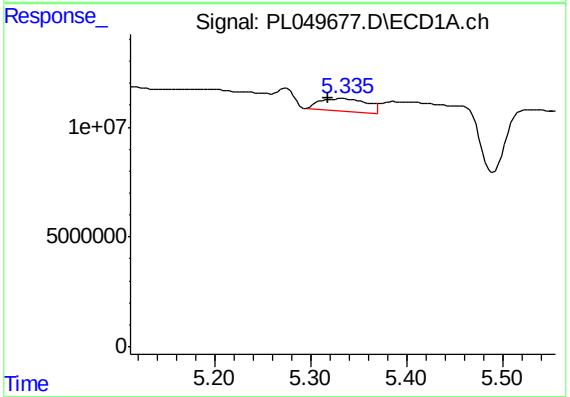

#9 Endosulfan I

R.T.: 5.334 min
Delta R.T.: 0.015 min
Response: 18919098
Conc: 1.29 ng/ml

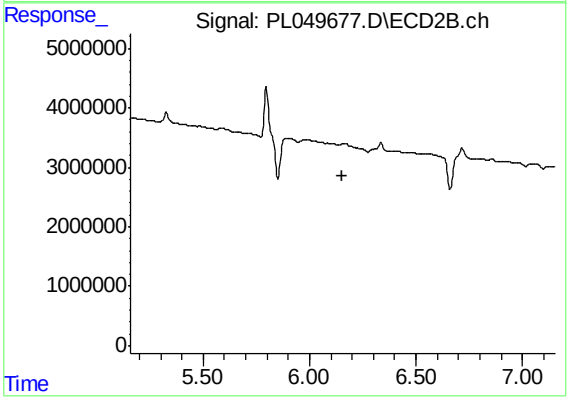

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.156 min
Response: 0
Conc: N.D.

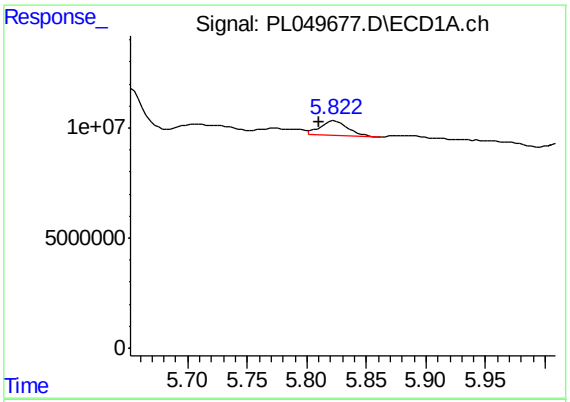

#14 Endrin

R.T.: 5.823 min
Delta R.T.: 0.013 min
Response: 10949110
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

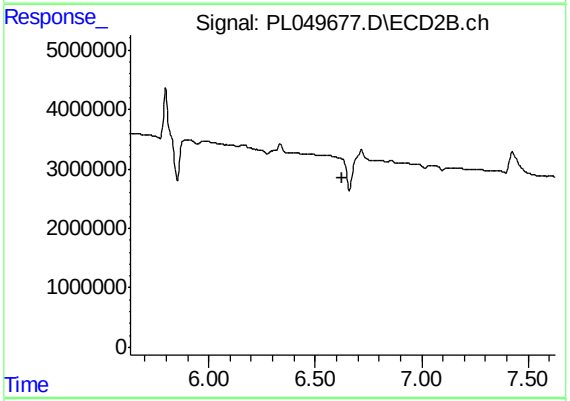

#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.630 min
Response: 0
Conc: N.D.

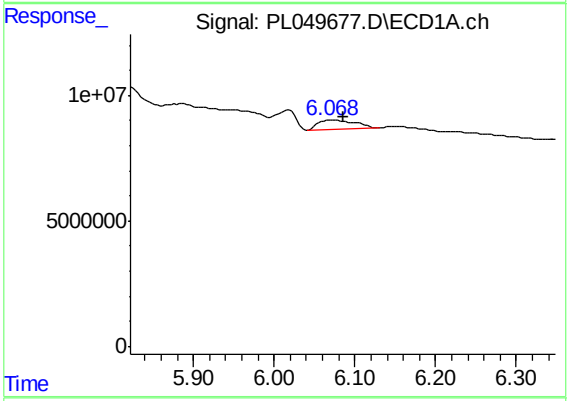

#15 Endosulfan II

R.T.: 6.070 min
Delta R.T.: -0.016 min
Response: 12474797
Conc: 0.94 ng/ml

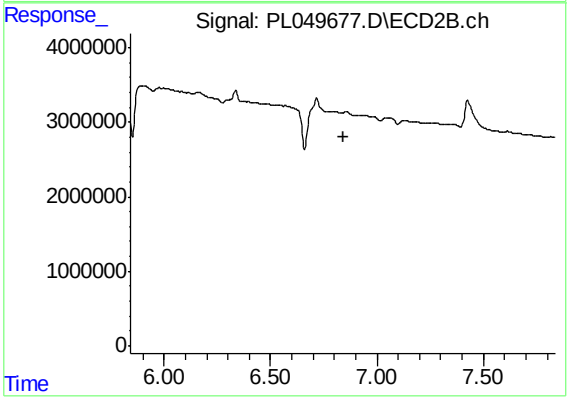

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.841 min
Response: 0
Conc: N.D.

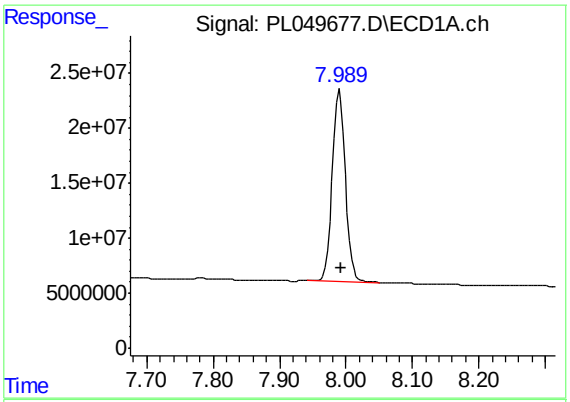

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 240905375
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

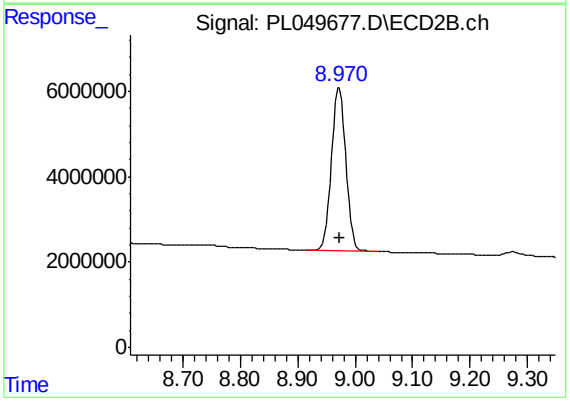

#28 Decachlorobiphenyl

R.T.: 8.972 min
Delta R.T.: 0.000 min
Response: 66685528
Conc: 19.97 ng/ml