

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
 Data File : PL049626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 12:22
 Operator : SM\AJ
 Sample : K3157-07RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-061719-DRE

Manual Integrations
 APPROVED

Ankita
 6/20/2019 10:01:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:01:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.934	47641447	14393862	4.324m	4.982m
28)	SA Decachlor...	7.991	8.971	69805653	23365179	5.490	6.996 #
Target Compounds							
12)	B 4,4'-DDE	5.432	6.264	12684726	3134061	0.811m	0.955

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 12:22
Operator : SM\AJ
Sample : K3157-07RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CL-01-061719-DRE


Manual Integrations
APPROVED

Ankita
6/20/2019 10:01:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:01:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

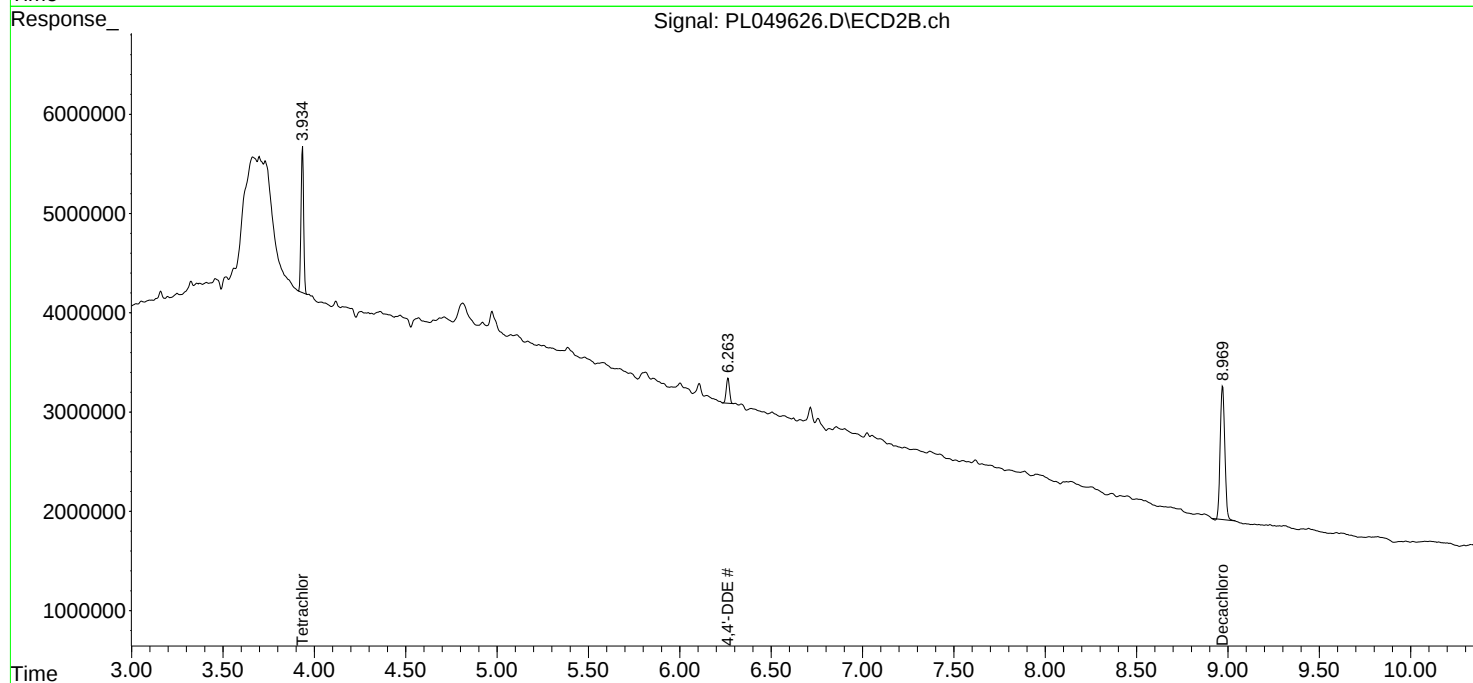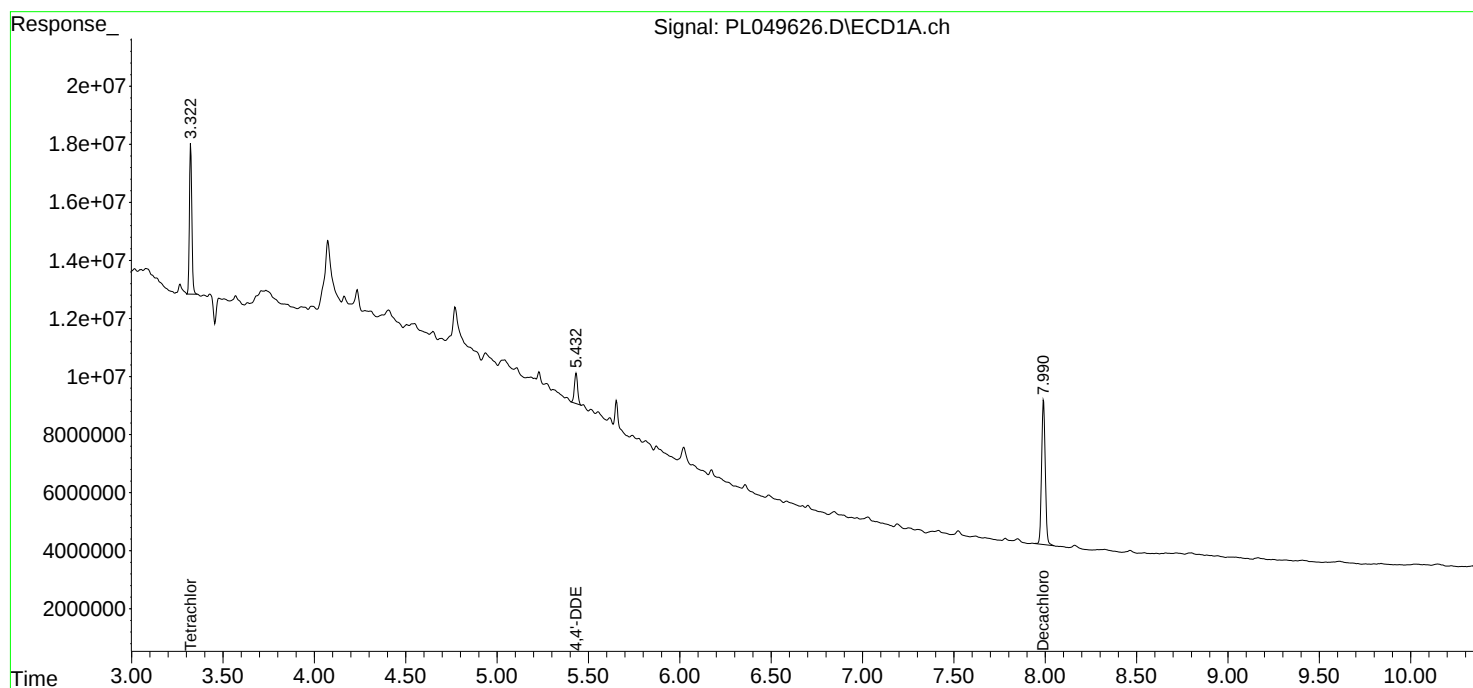

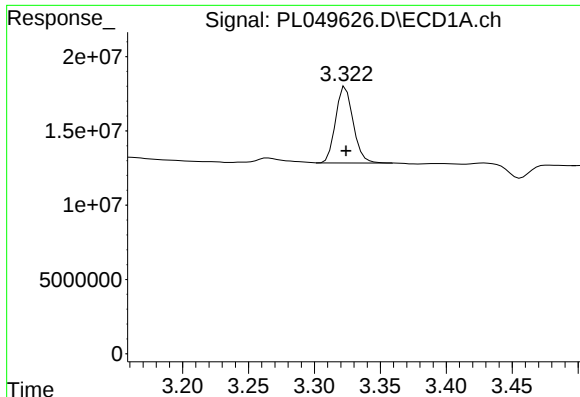


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 47641447
Conc: 4.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-01-061719-DRE


Manual Integrations
APPROVED

Ankita
6/20/2019 10:01:48 AM

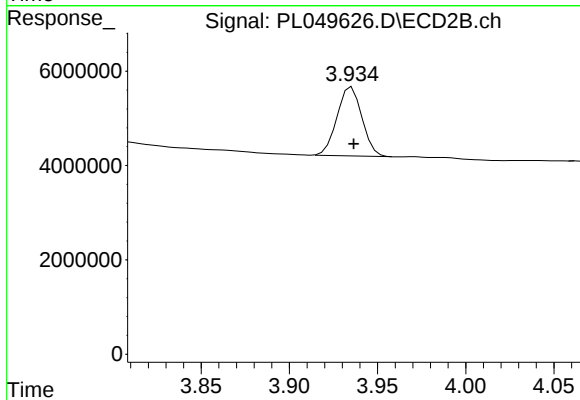


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.002 min
Response: 14393862
Conc: 4.98 ng/ml m

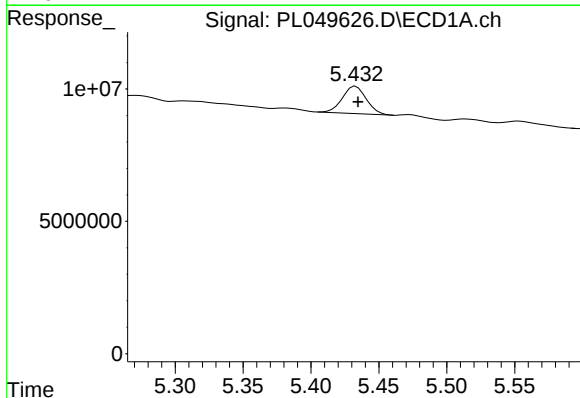


#12 4,4'-DDE

R.T.: 5.432 min
Delta R.T.: -0.003 min
Response: 12684726
Conc: 0.81 ng/ml m

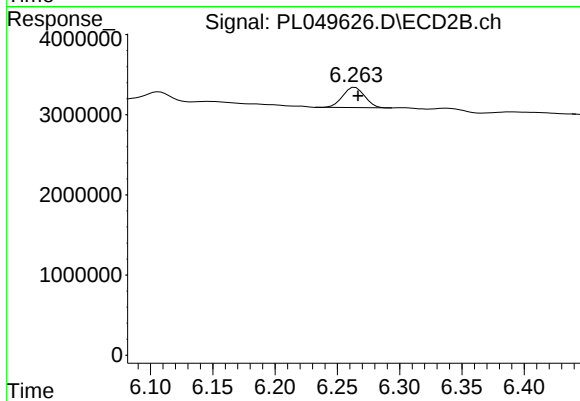

#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.002 min
Response: 3134061
Conc: 0.95 ng/ml

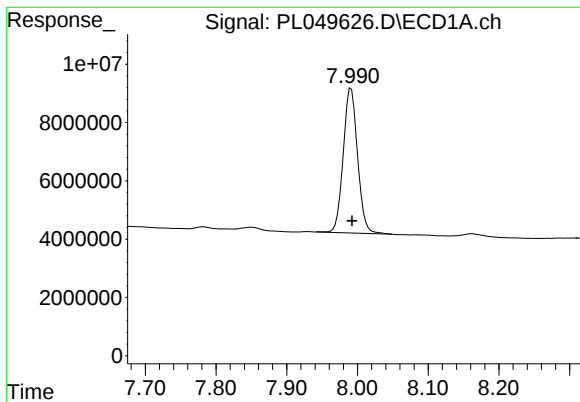


#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: -0.001 min
Response: 69805653
Conc: 5.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-061719-DRE

Manual Integrations
APPROVED

Ankita
6/20/2019 10:01:48 AM

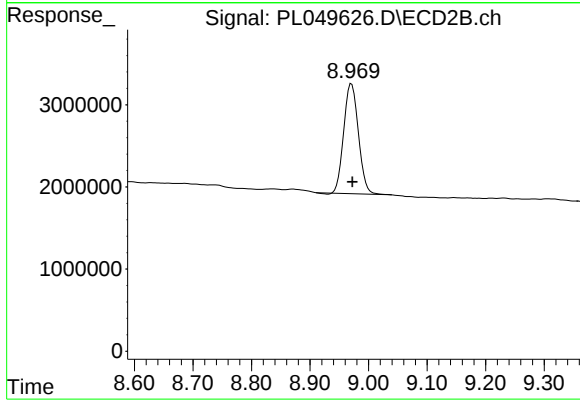

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.001 min
Response: 23365179
Conc: 7.00 ng/ml