

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
 Data File : PL049639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 15:39
 Operator : SM\AJ
 Sample : K3428-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-013-SW163-061319

Manual Integrations
 APPROVED

Ankita
 6/20/2019 10:02:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:04:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.935	185.0E6	48538846	16.791	16.801
28) SA Decachlor...	7.990	8.970	247.1E6	70952321	19.431	21.245
Target Compounds						
12) B 4,4'-DDE	5.431	6.263	69713639	13888574	4.457m	4.231
17) MA 4,4'-DDT	6.177	7.052	54159028	10107571	4.399	3.605

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 15:39
Operator : SM\AJ
Sample : K3428-09
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-013-SW163-061319


Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:04:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

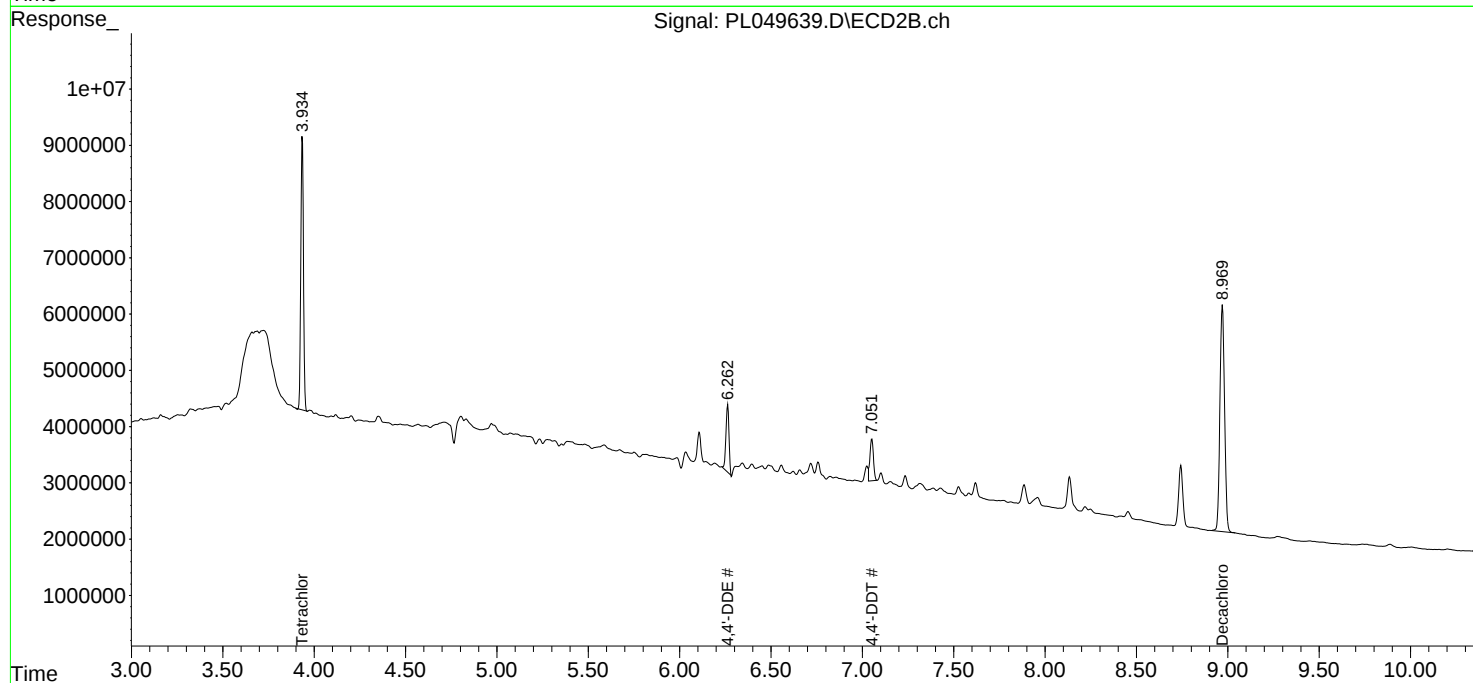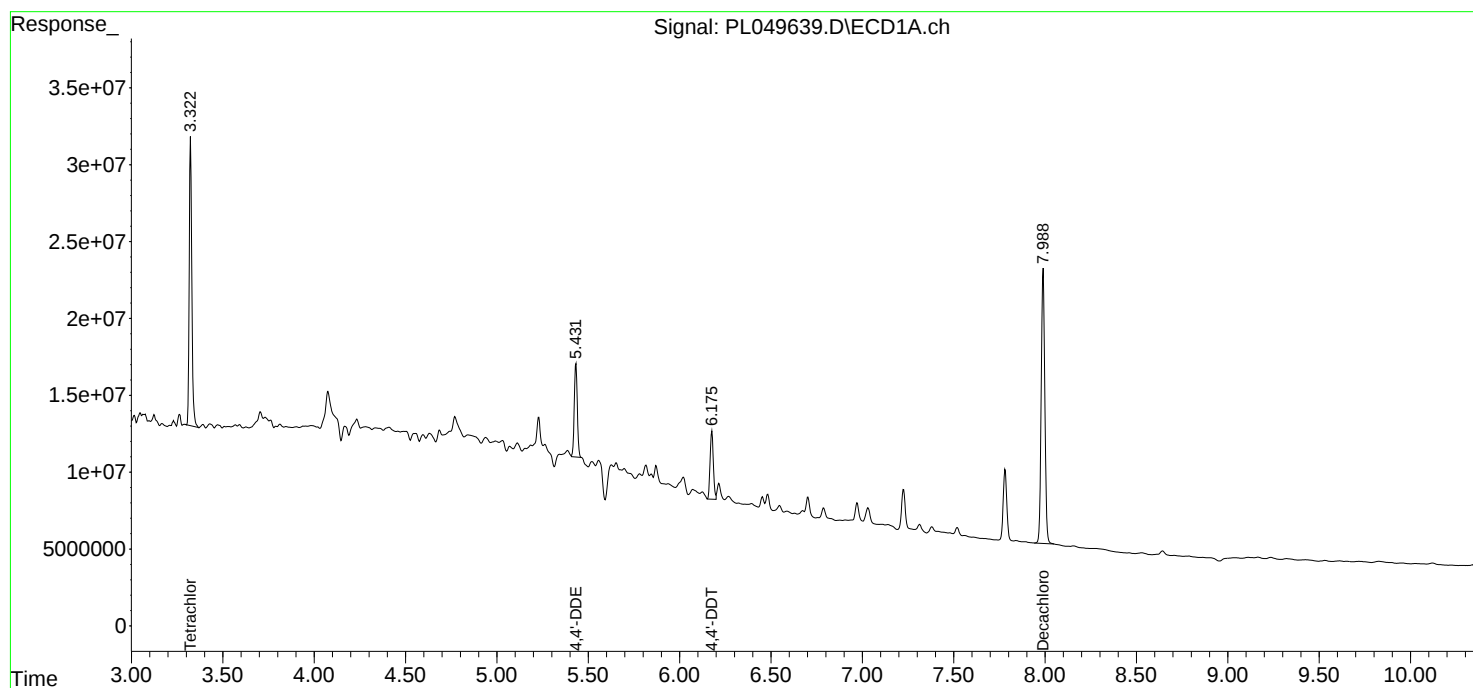

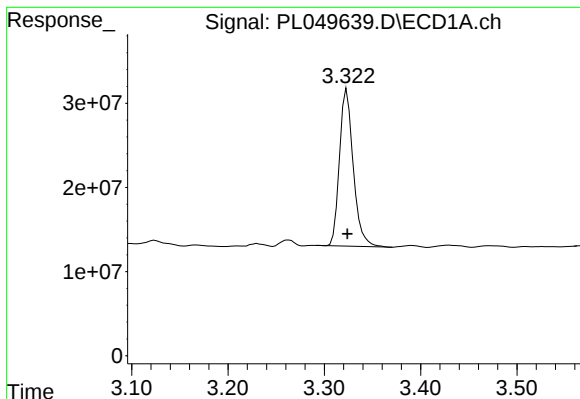


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 185019282
Conc: 16.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW163-061319


Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:03 AM

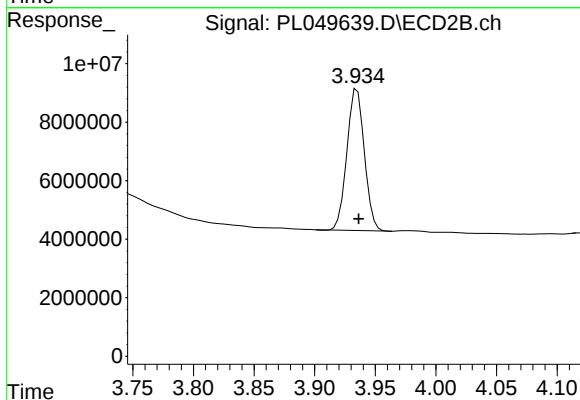


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.001 min
Response: 48538846
Conc: 16.80 ng/ml

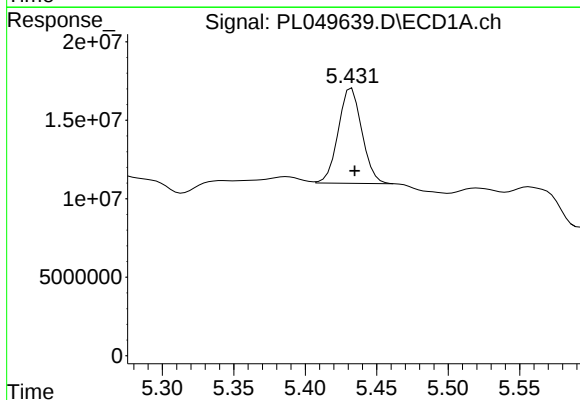


#12 4,4'-DDE

R.T.: 5.431 min
Delta R.T.: -0.004 min
Response: 69713639
Conc: 4.46 ng/ml m

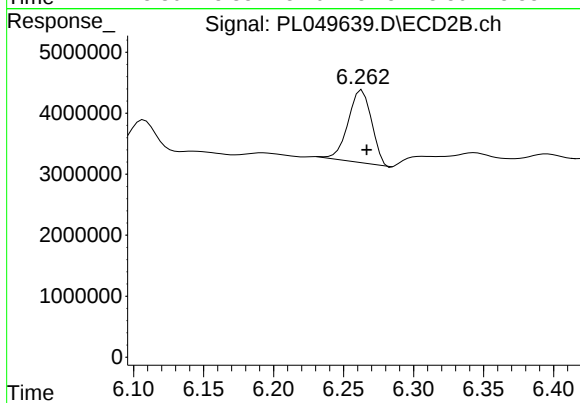

#12 4,4'-DDE

R.T.: 6.263 min
Delta R.T.: -0.003 min
Response: 13888574
Conc: 4.23 ng/ml

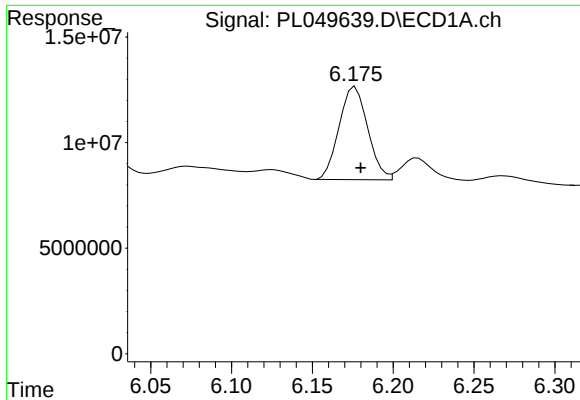


#17 4,4'-DDT

R.T.: 6.177 min
Delta R.T.: -0.003 min
Response: 54159028
Conc: 4.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW163-061319


Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:03 AM

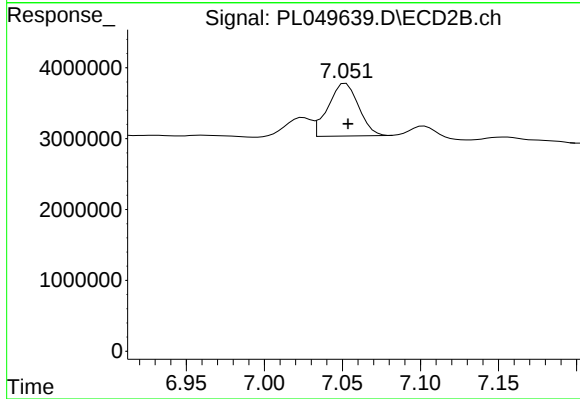


#17 4,4'-DDT

R.T.: 7.052 min
Delta R.T.: -0.001 min
Response: 10107571
Conc: 3.61 ng/ml

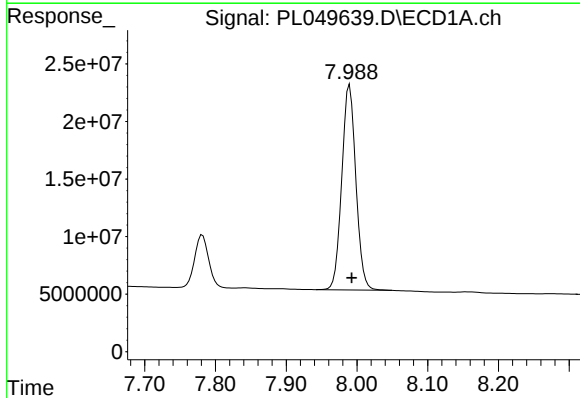

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.003 min
Response: 247075384
Conc: 19.43 ng/ml

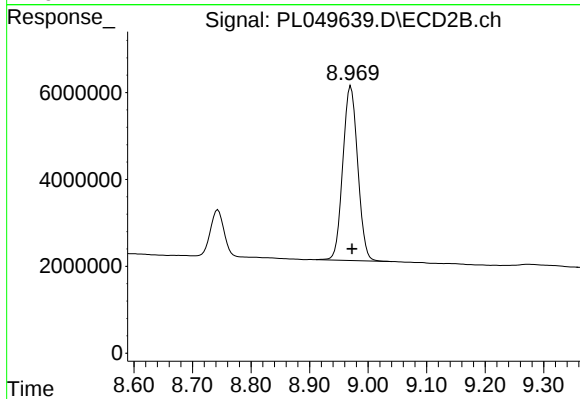

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: -0.002 min
Response: 70952321
Conc: 21.25 ng/ml