

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
 Data File : PL049640.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2019 15:55
 Operator : SM\AJ
 Sample : K3428-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-013-SW166-061319

Manual Integrations
 APPROVED

Ankita
 6/20/2019 10:02:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:04:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
 Quant Title : GC Extractables
 QLast Update : Fri May 31 01:35:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.934	183.7E6	45029546	16.674m	15.586m
28)	SA Decachlor...	7.990	8.971	223.0E6	63478298	17.536	19.007
Target Compounds							
17)	MA 4,4'-DDT	6.177	7.052	88575630	21633638	7.194	7.716

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061919\
Data File : PL049640.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2019 15:55
Operator : SM\AJ
Sample : K3428-10
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-013-SW166-061319


Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:04:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL053019.M
Quant Title : GC Extractables
QLast Update : Fri May 31 01:35:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

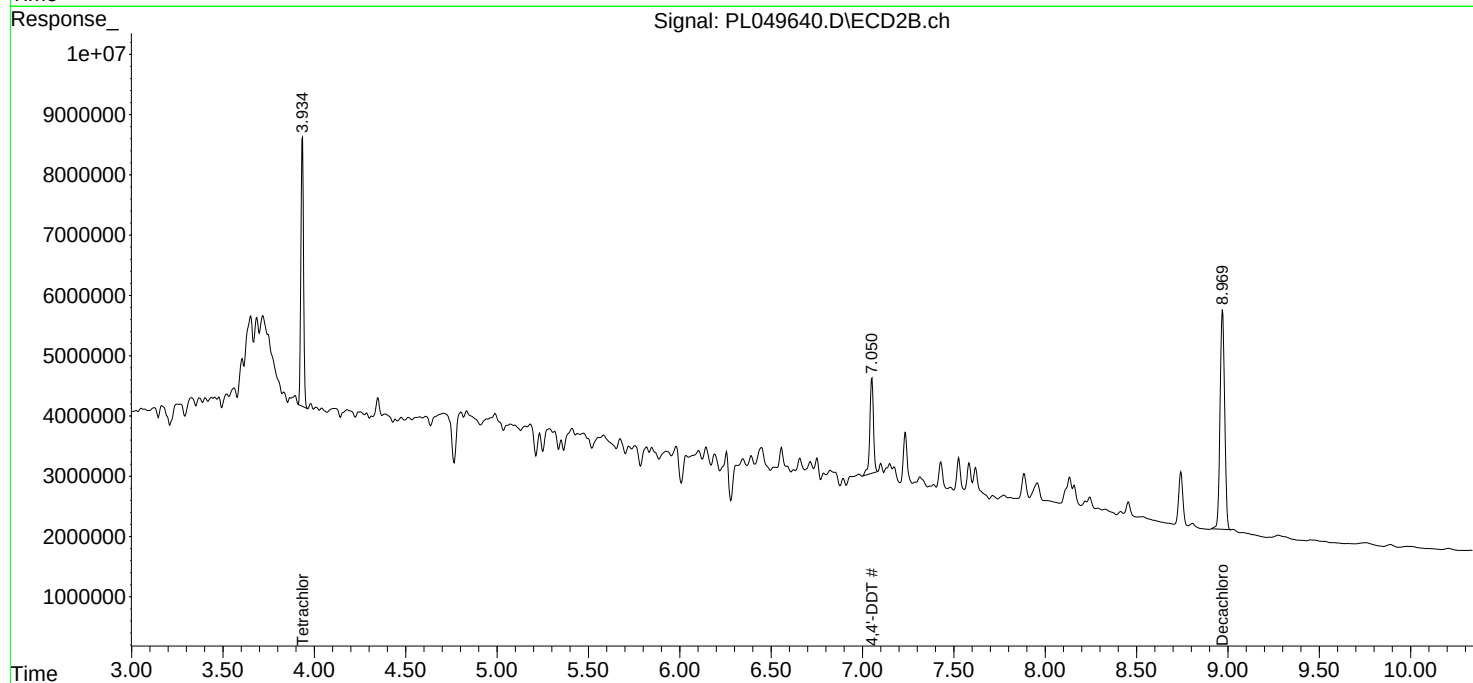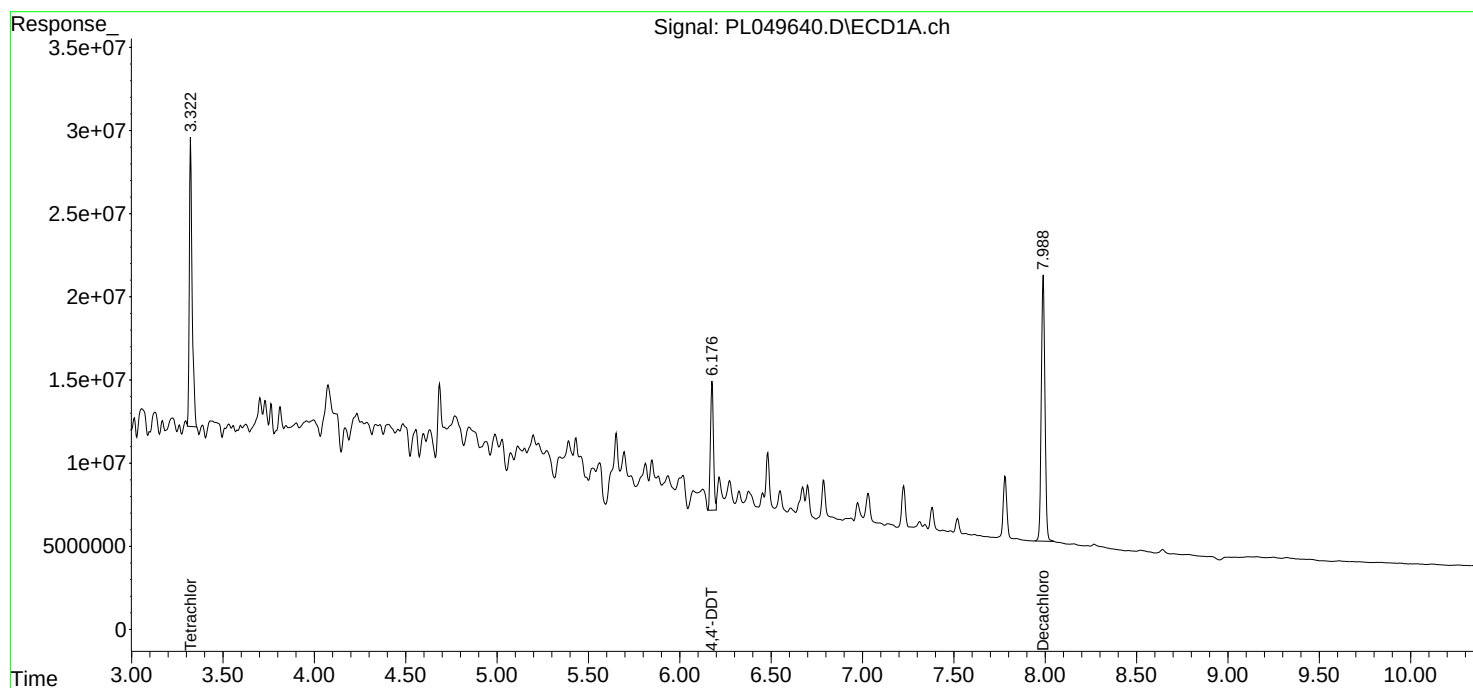

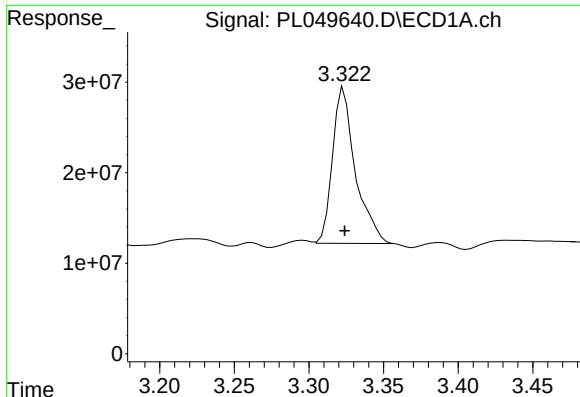


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 183724377
Conc: 16.67 ng/ml m

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW166-061319


Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:05 AM

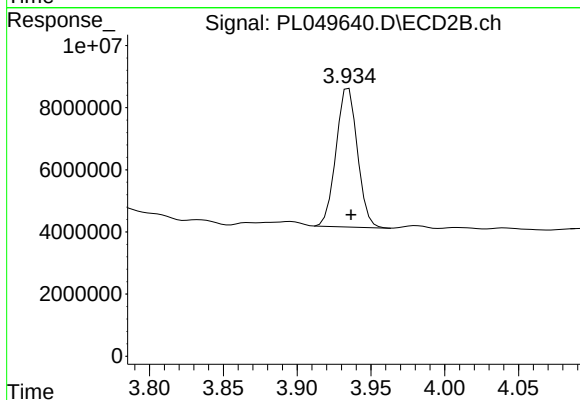


#1 Tetrachloro-m-xylene

R.T.: 3.934 min
Delta R.T.: -0.003 min
Response: 45029546
Conc: 15.59 ng/ml m

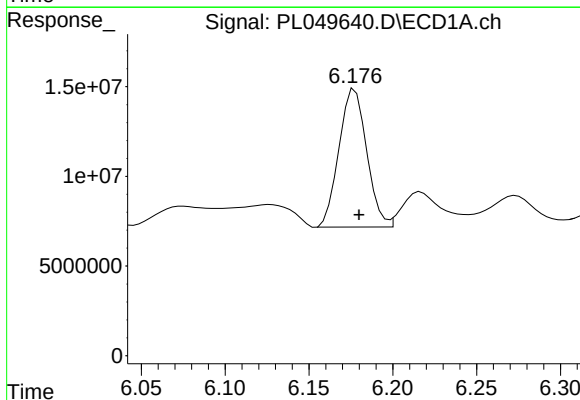


#17 4,4'-DDT

R.T.: 6.177 min
Delta R.T.: -0.002 min
Response: 88575630
Conc: 7.19 ng/ml

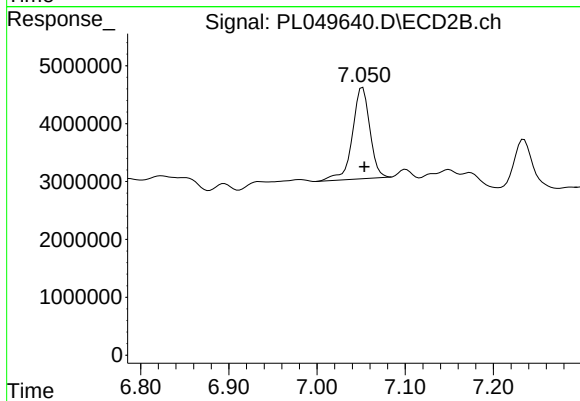

#17 4,4'-DDT

R.T.: 7.052 min
Delta R.T.: -0.002 min
Response: 21633638
Conc: 7.72 ng/ml

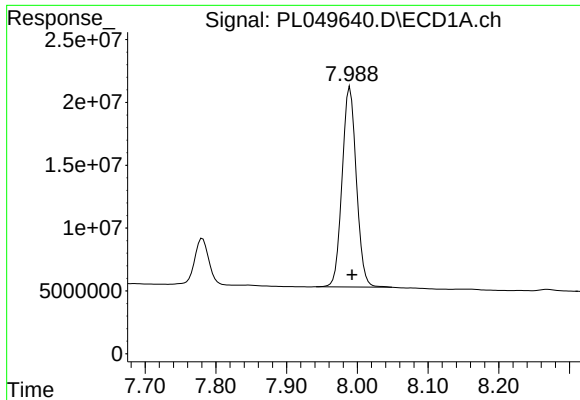


#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.003 min
Response: 222974579
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW166-061319

Manual Integrations
APPROVED

Ankita
6/20/2019 10:02:05 AM

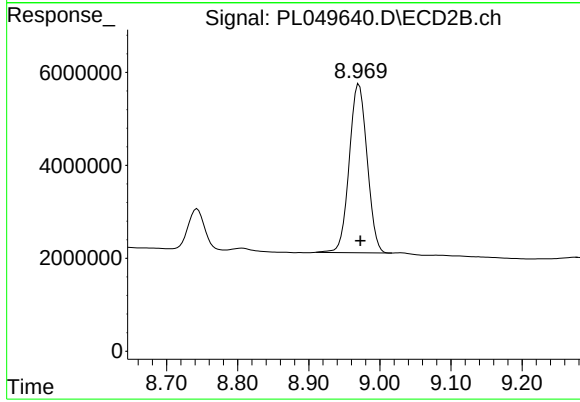

#28 Decachlorobiphenyl

R.T.: 8.971 min
Delta R.T.: -0.002 min
Response: 63478298
Conc: 19.01 ng/ml