

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061920\
 Data File : PL059387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 17:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:14:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.519	4.072	39801281	64148380	23.049	24.654
28)	SA Decachlor...	8.290	9.181	37630213	56812478	22.884	23.966
Target Compounds							
2)	A alpha-BHC	3.977	0.000	1088059	0	0.435	N.D. #
3)	MA gamma-BHC...	4.250	0.000	209843	0	0.096	N.D. #
4)	MA Heptachlor	0.000	5.261	0	533620	N.D.	0.155 #
8)	B Heptachlo...	0.000	5.952	0	25304036	N.D.	9.135 #
11)	B alpha-Chl...	0.000	6.275	0	7137391	N.D.	2.348 #
14)	MA Endrin	6.083	0.000	736943	0	0.486	N.D. #
23)	Chlordane-1	4.421f	0.000	1726522	0	34.323	N.D. #
26)	Chlordane-4	0.000	6.275	0	7137391	N.D.	15.685 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061920\
Data File : PL059387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 17:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:14:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

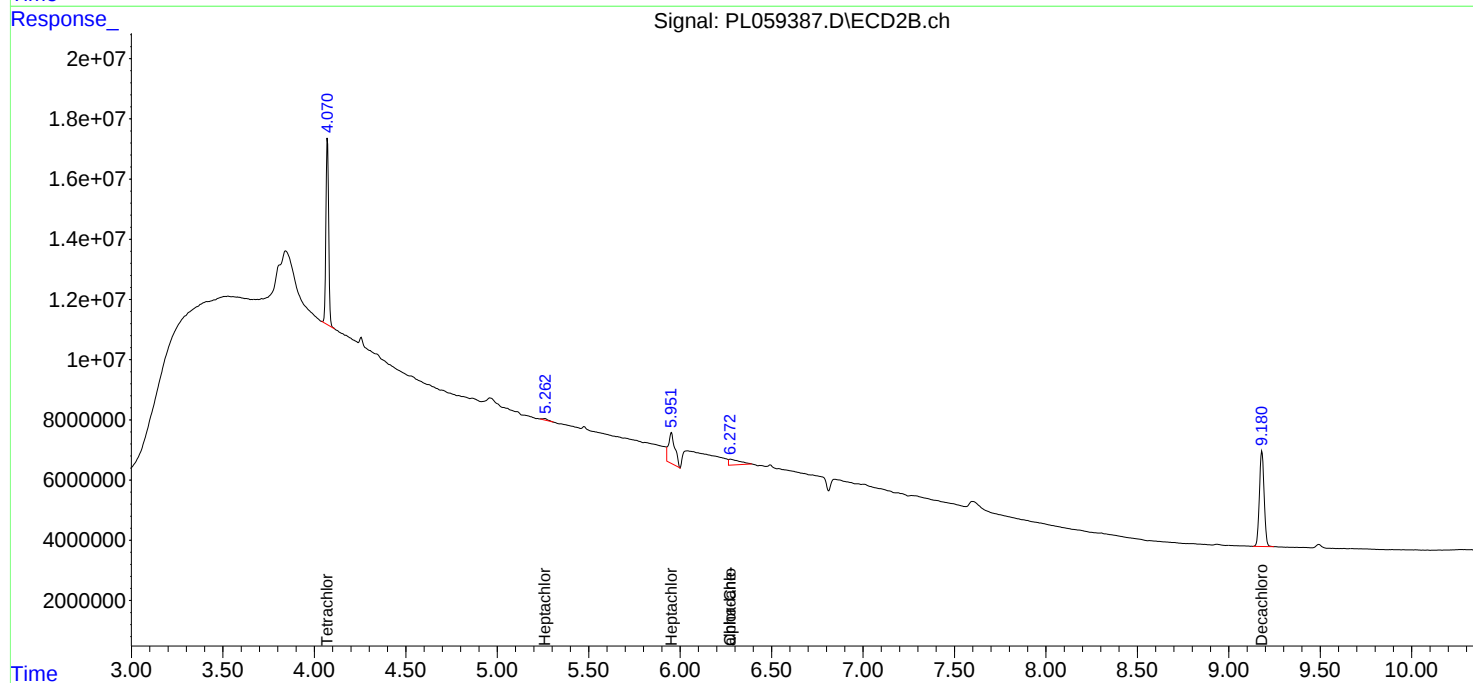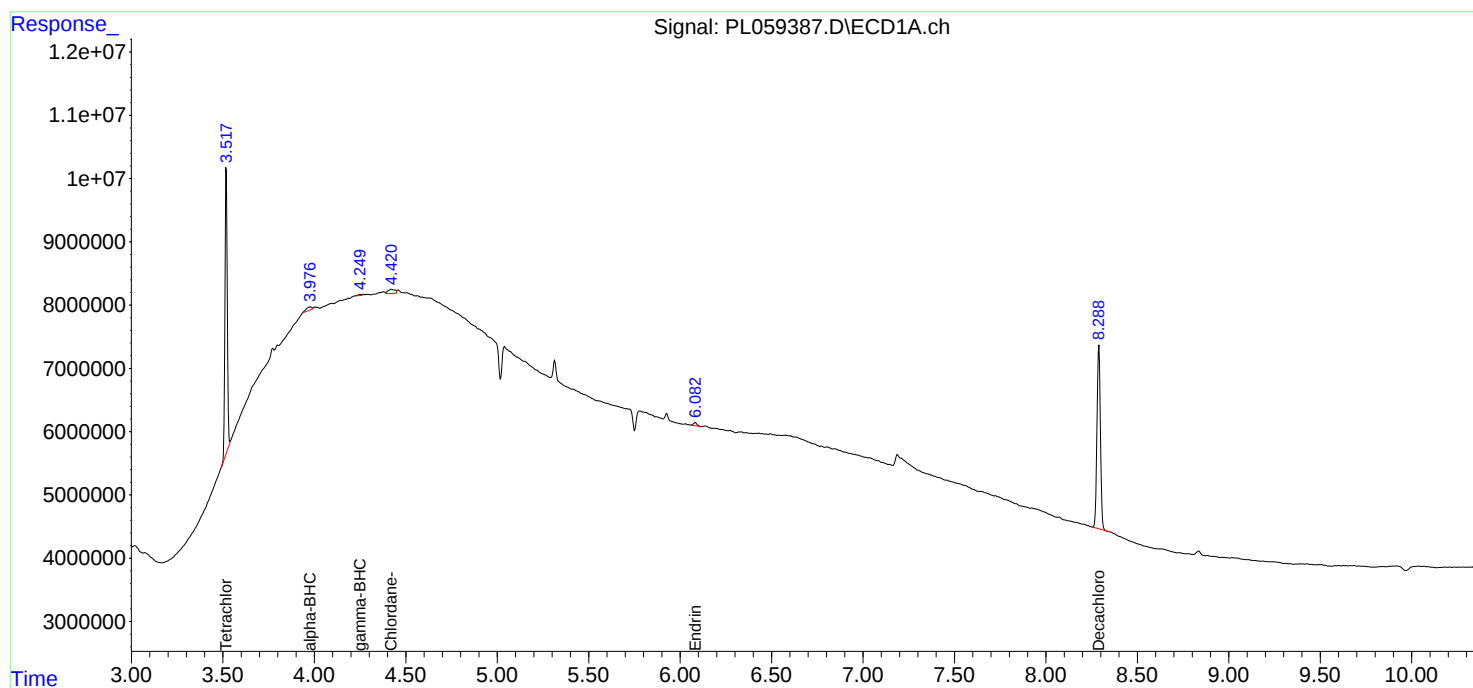


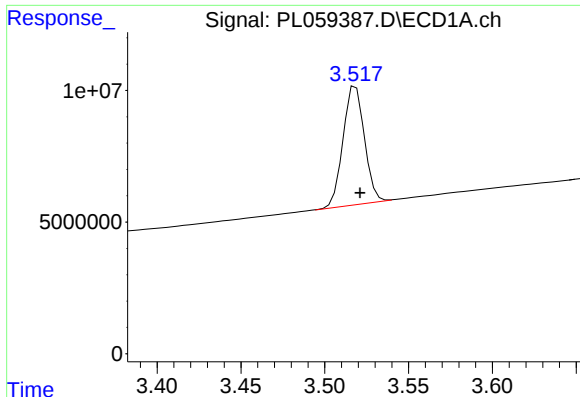

#1 Tetrachloro-m-xylene


R.T.: 3.519 min
Delta R.T.: -0.002 min
Response: 39801281
Conc: 23.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

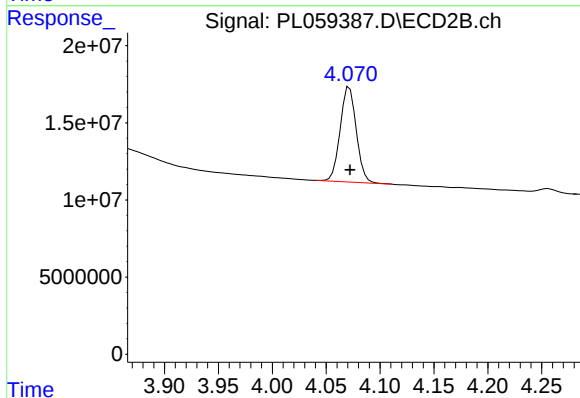


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 64148380
Conc: 24.65 ng/ml

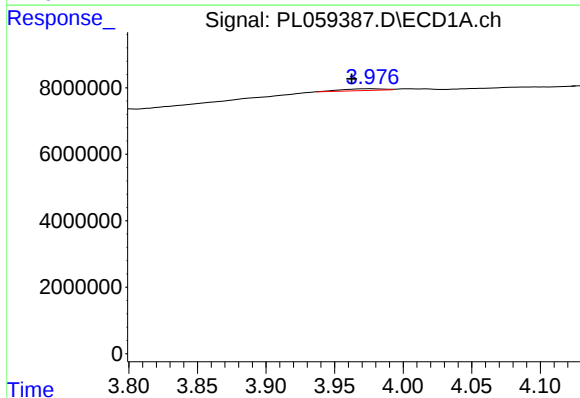


#2 alpha-BHC

R.T.: 3.977 min
Delta R.T.: 0.015 min
Response: 1088059
Conc: 0.43 ng/ml

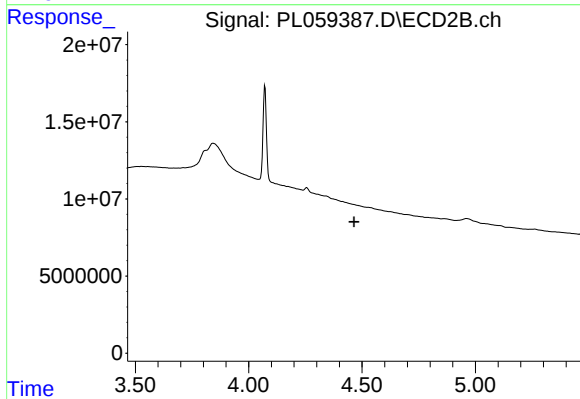

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.465 min
Response: 0
Conc: N.D.

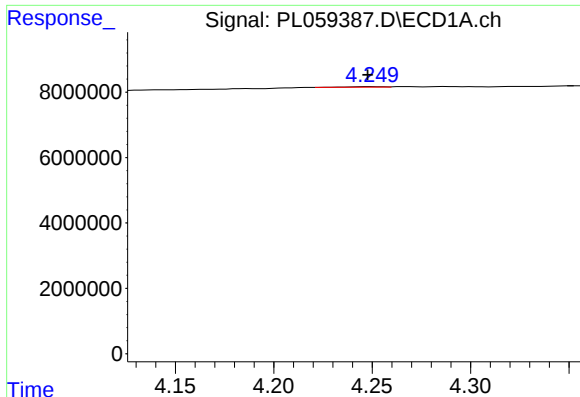

#3 gamma-BHC (Lindane)


R.T.: 4.250 min
Delta R.T.: 0.002 min
Response: 209843
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

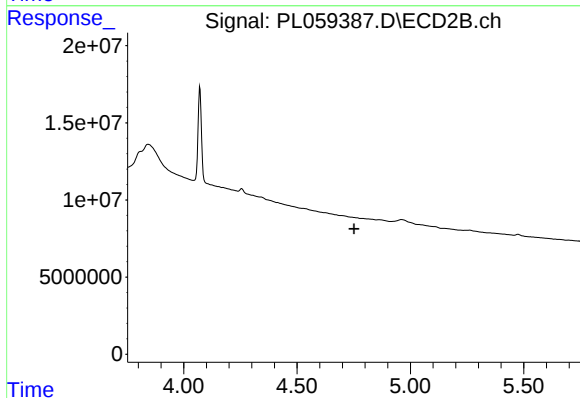


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.752 min
Response: 0
Conc: N.D.

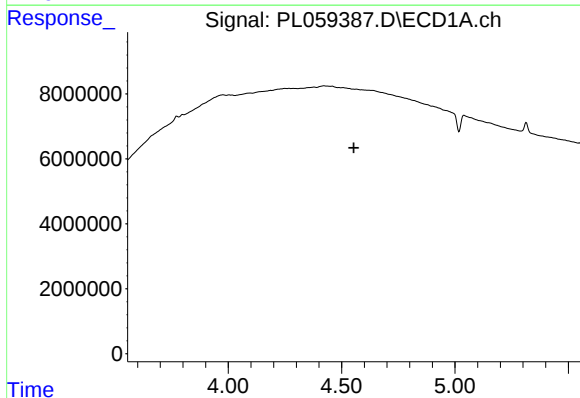


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.554 min
Response: 0
Conc: N.D.

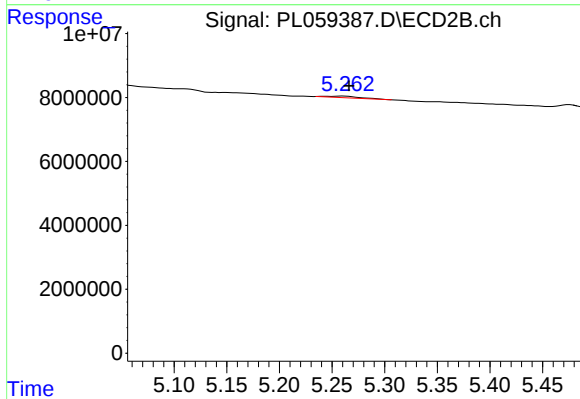

#4 Heptachlor


R.T.: 5.261 min
Delta R.T.: -0.005 min
Response: 533620
Conc: 0.15 ng/ml

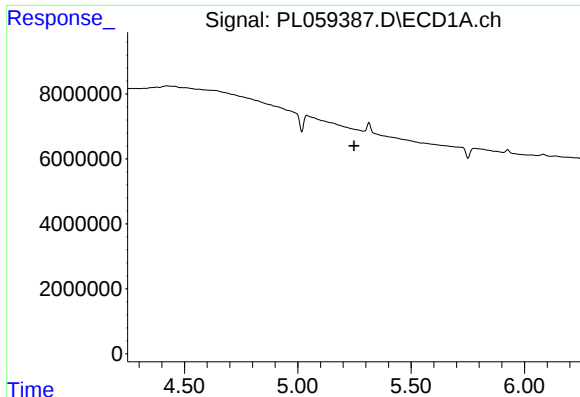

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.248 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

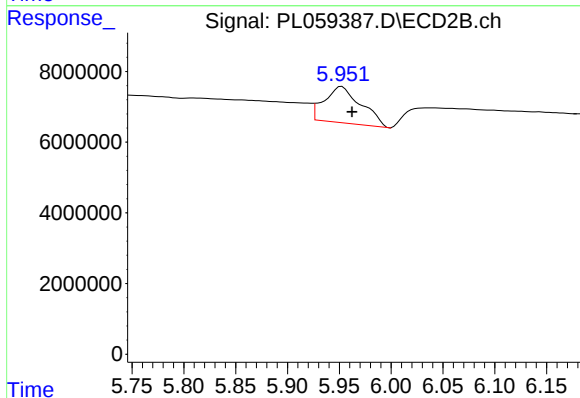


#8 Heptachlor epoxide

R.T.: 5.952 min
Delta R.T.: -0.010 min
Response: 25304036
Conc: 9.14 ng/ml

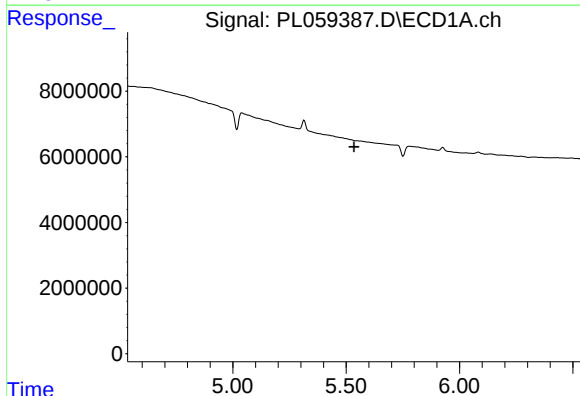


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.535 min
Response: 0
Conc: N.D.

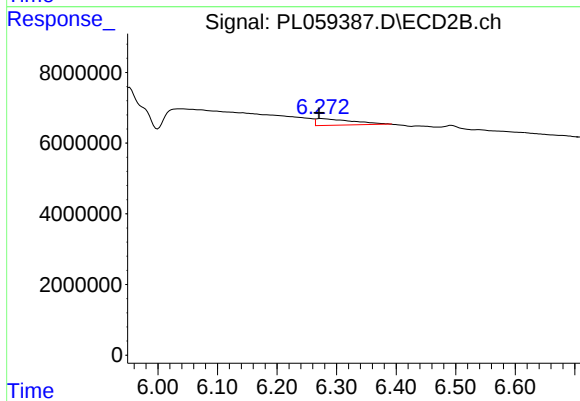

#11 alpha-Chlordane


R.T.: 6.275 min
Delta R.T.: 0.004 min
Response: 7137391
Conc: 2.35 ng/ml

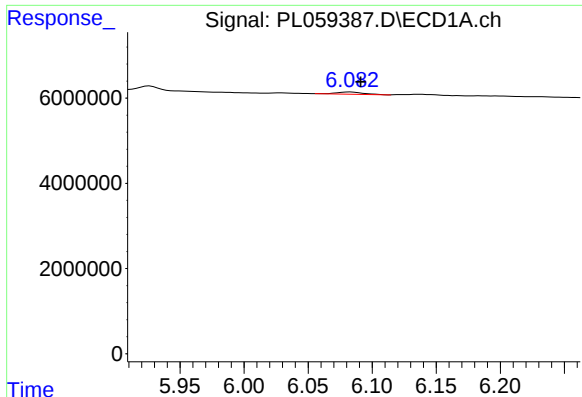

#14 Endrin


R.T.: 6.083 min
Delta R.T.: -0.008 min
Response: 736943
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

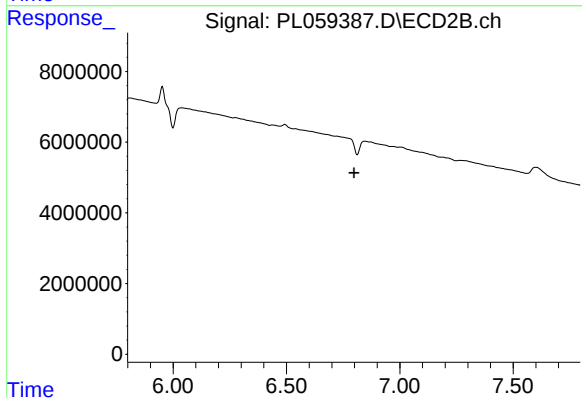


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.799 min
Response: 0
Conc: N.D.

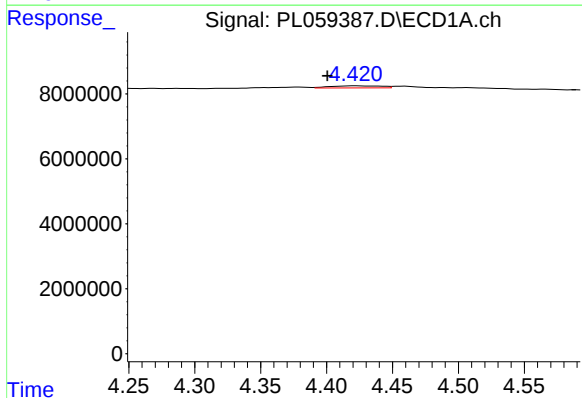


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.021 min
Response: 1726522
Conc: 34.32 ng/ml

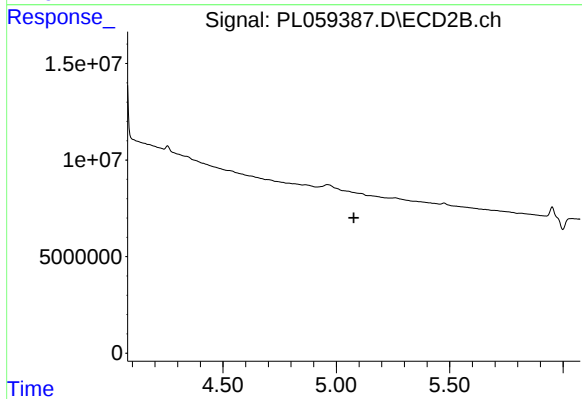

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.077 min
Response: 0
Conc: N.D.

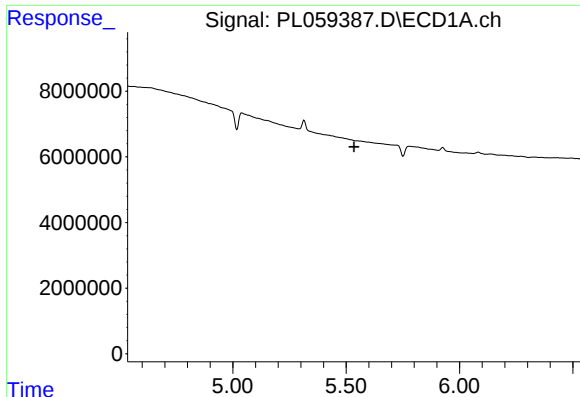

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

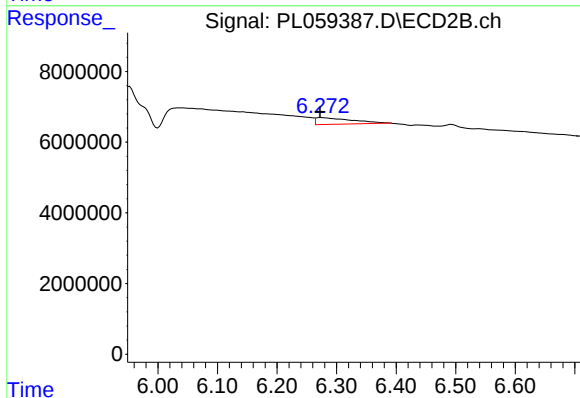


#26 Chlordane-4

R.T.: 6.275 min
Delta R.T.: 0.003 min
Response: 7137391
Conc: 15.68 ng/ml

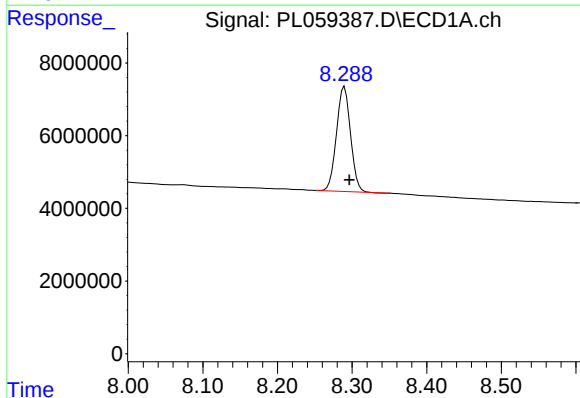

#28 Decachlorobiphenyl

R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 37630213
Conc: 22.88 ng/ml

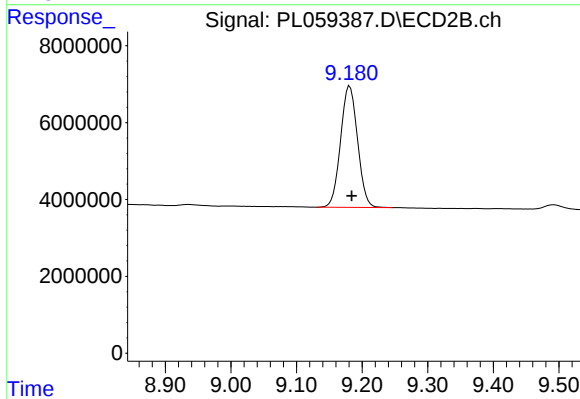

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 56812478
Conc: 23.97 ng/ml