

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061920\
 Data File : PL059378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2020 15:49
 Operator : AJ\MA
 Sample : L3053-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-228

Manual Integrations
 APPROVED

mohammad
 6/24/2020 11:43:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:12:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 04 08:16:22 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.520	4.071	2096067	3705888	1.214	1.424
28) SA Decachlor...	8.288	9.181	2576765	3813101	1.567m	1.609
Target Compounds						
10) B gamma-Chl...	5.471	6.195	821378	5031538	0.491	1.682 #
11) B alpha-Chl...	5.528	6.269	1566613	7816157	0.939m	2.572m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061920\
Data File : PL059378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2020 15:49
Operator : AJ\MA
Sample : L3053-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

mohammad
6/24/2020 11:43:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:12:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060320.M
Quant Title : GC Extractables
QLast Update : Thu Jun 04 08:16:22 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

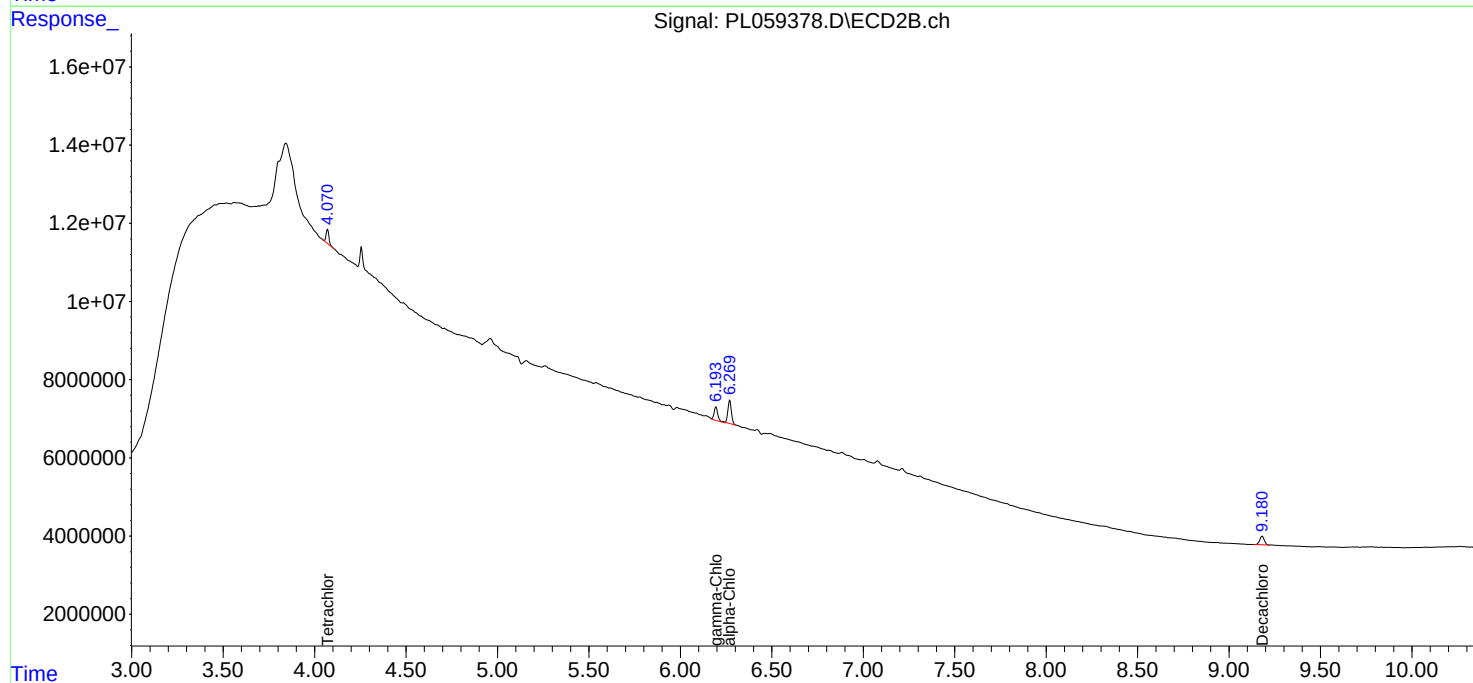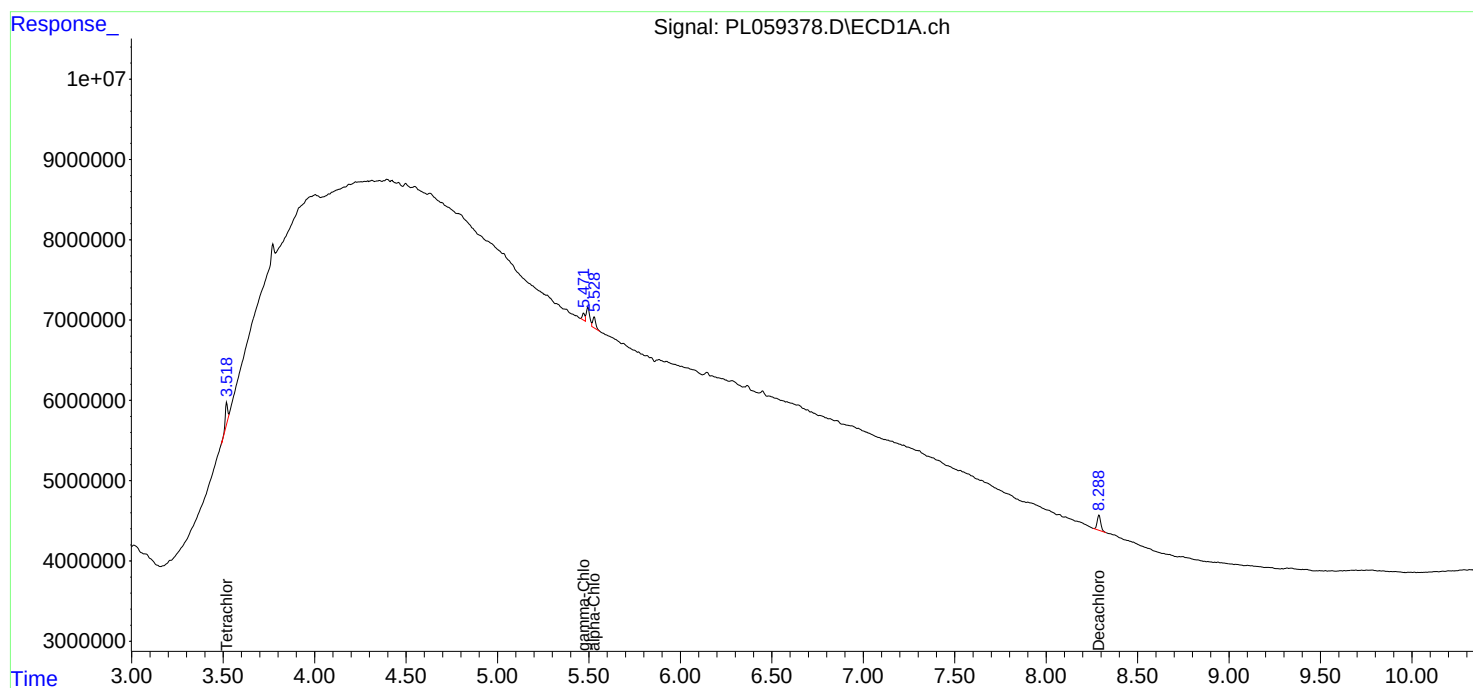

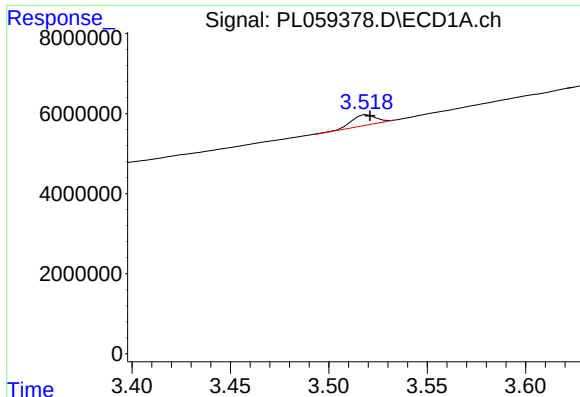


#1 Tetrachloro-m-xylene

R.T.: 3.520 min
Delta R.T.: -0.001 min
Response: 2096067
Conc: 1.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

mohammad
6/24/2020 11:43:13 AM

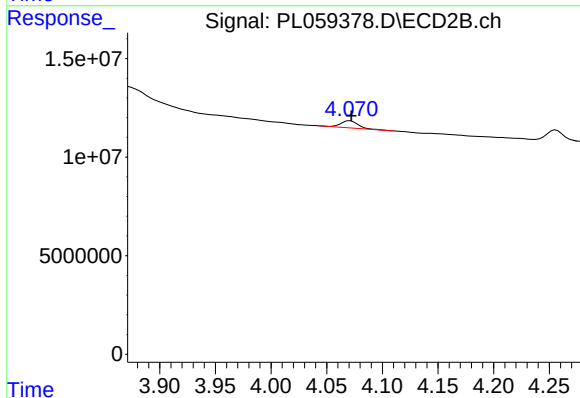


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.001 min
Response: 3705888
Conc: 1.42 ng/ml

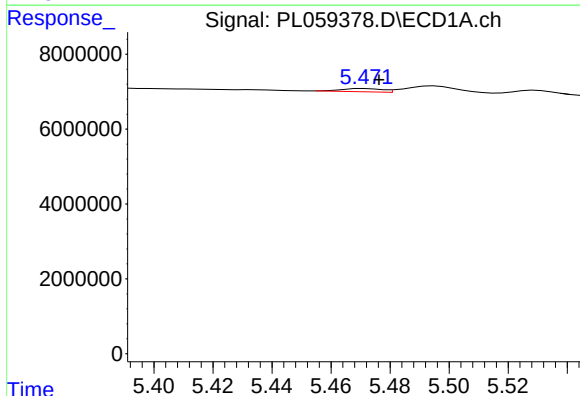


#10 gamma-Chlordane

R.T.: 5.471 min
Delta R.T.: -0.005 min
Response: 821378
Conc: 0.49 ng/ml

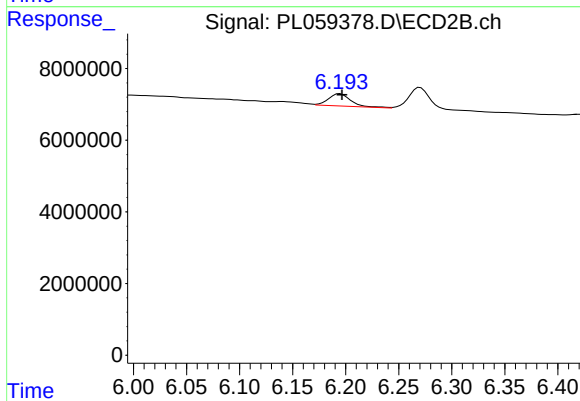

#10 gamma-Chlordane

R.T.: 6.195 min
Delta R.T.: -0.002 min
Response: 5031538
Conc: 1.68 ng/ml

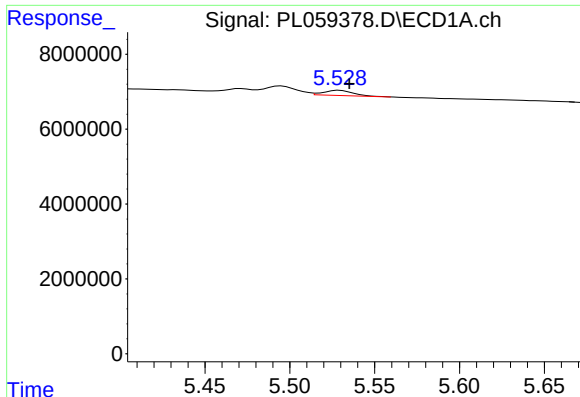


#11 alpha-Chlordane

R.T.: 5.528 min
Delta R.T.: -0.007 min
Response: 1566613
Conc: 0.94 ng/ml m

Instrument :
ECD_L
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

mohammad
6/24/2020 11:43:13 AM

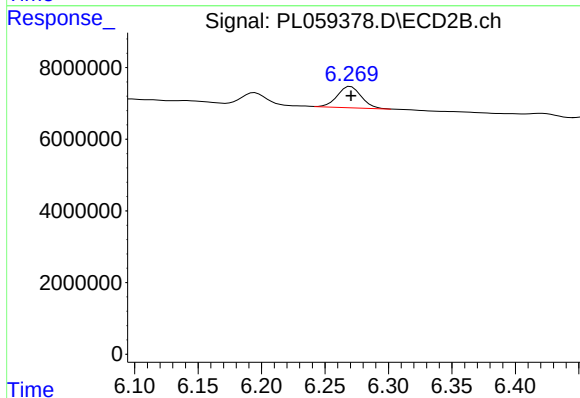


#11 alpha-Chlordane

R.T.: 6.269 min
Delta R.T.: -0.002 min
Response: 7816157
Conc: 2.57 ng/ml m

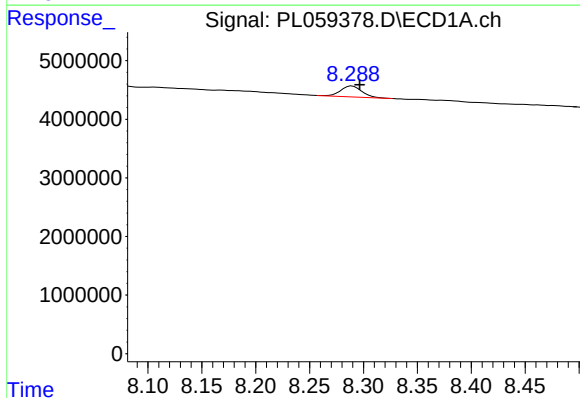

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: -0.009 min
Response: 2576765
Conc: 1.57 ng/ml m

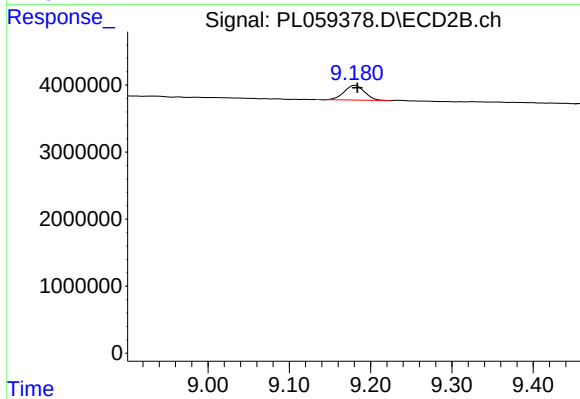

#28 Decachlorobiphenyl

R.T.: 9.181 min
Delta R.T.: -0.003 min
Response: 3813101
Conc: 1.61 ng/ml