

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG011923DDD\  
Data File : FG011281.D  
Signal(s) : FID1A.ch  
Acq On : 19 Jan 2023 13:46  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 28 03:40:10 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG123022.M  
Quant Title :  
QLast Update : Mon Jan 02 04:44:41 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.761  | 2753124  | 15.605 ug/ml |
| 12)                         | N-OCTACOSANE | 17.251 | 2610990  | 15.876 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG011923DDD\  
Data File : FG011281.D  
Signal(s) : FID1A.ch  
Acq On : 19 Jan 2023 13:46  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 28 03:40:10 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG123022.M  
Quant Title :  
QLast Update : Mon Jan 02 04:44:41 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

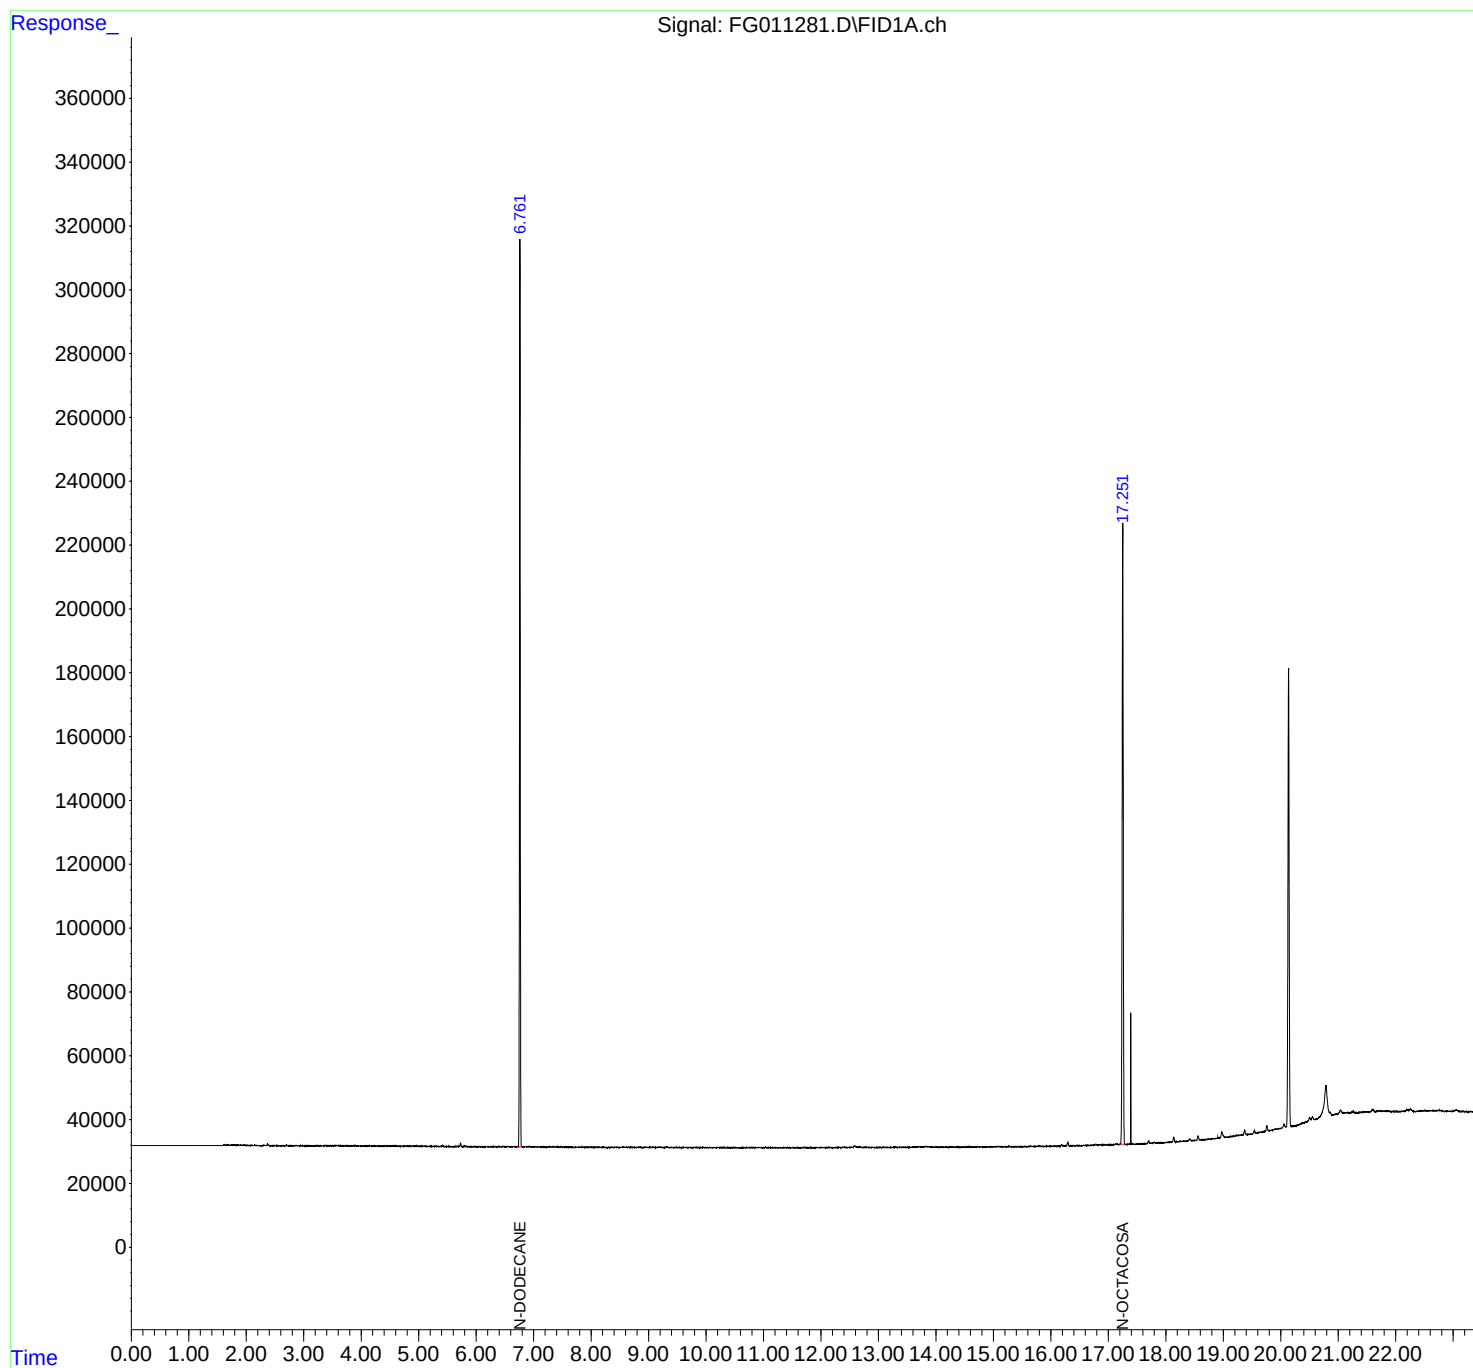


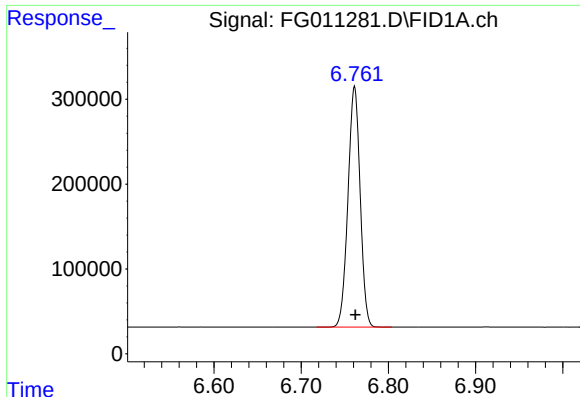

#3 N-DODECANE


R.T.: 6.761 min  
Delta R.T.: 0.000 min  
Response: 2753124  
Conc: 15.61 ug/ml

Instrument :  
ECD\_L  
ClientSampleId :

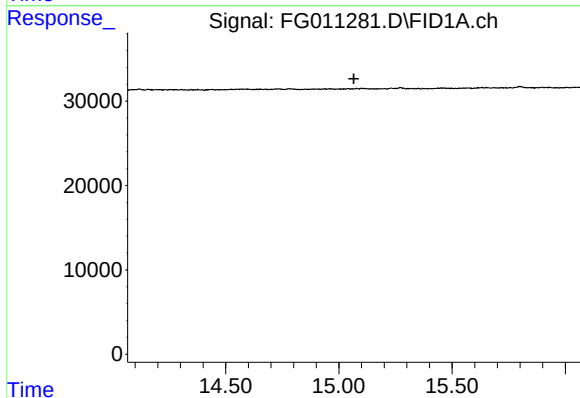

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 15.066 min  
Response: 0  
Conc: N.D.

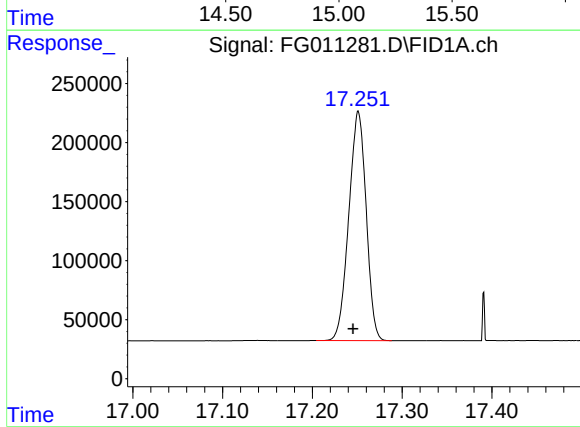

#12 N-OCTACOSANE

R.T.: 17.251 min  
Delta R.T.: 0.006 min  
Response: 2610990  
Conc: 15.88 ug/ml