

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011923DDD\
 Data File : FG011286.D
 Signal(s) : FID1A.ch
 Acq On : 19 Jan 2023 16:18
 Operator : YP\AJ
 Sample : 01214-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TJRC-011723-B3-0-10-DUP

Integration File: autoint1.e
 Quant Time: Jun 28 03:42:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
 Quant Title :
 QLast Update : Mon Jan 02 04:44:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.070	1471890	9.605 ug/ml
Target Compounds			
4) N-TETRADECANE	8.591	72656	0.407 ug/ml
5) N-HEXADECANE	10.204	96643	0.533 ug/ml
6) N-OCTADECANE	11.651	110138	0.600 ug/ml
7) N-EICOSANE	12.965	106972	0.596 ug/ml
8) N-DOCOSANE	14.167	95808	0.542 ug/ml
10) N-TETRACOSANE	15.245	139857	0.802 ug/ml
11) N-HEXACOSANE	16.298	59103	0.347 ug/ml
12) N-OCTACOSANE	17.248	142949	0.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG011923DDD\
Data File : FG011286.D
Signal(s) : FID1A.ch
Acq On : 19 Jan 2023 16:18
Operator : YP\AJ
Sample : 01214-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TJRC-011723-B3-0-10-DUP

Integration File: autoint1.e
Quant Time: Jun 28 03:42:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

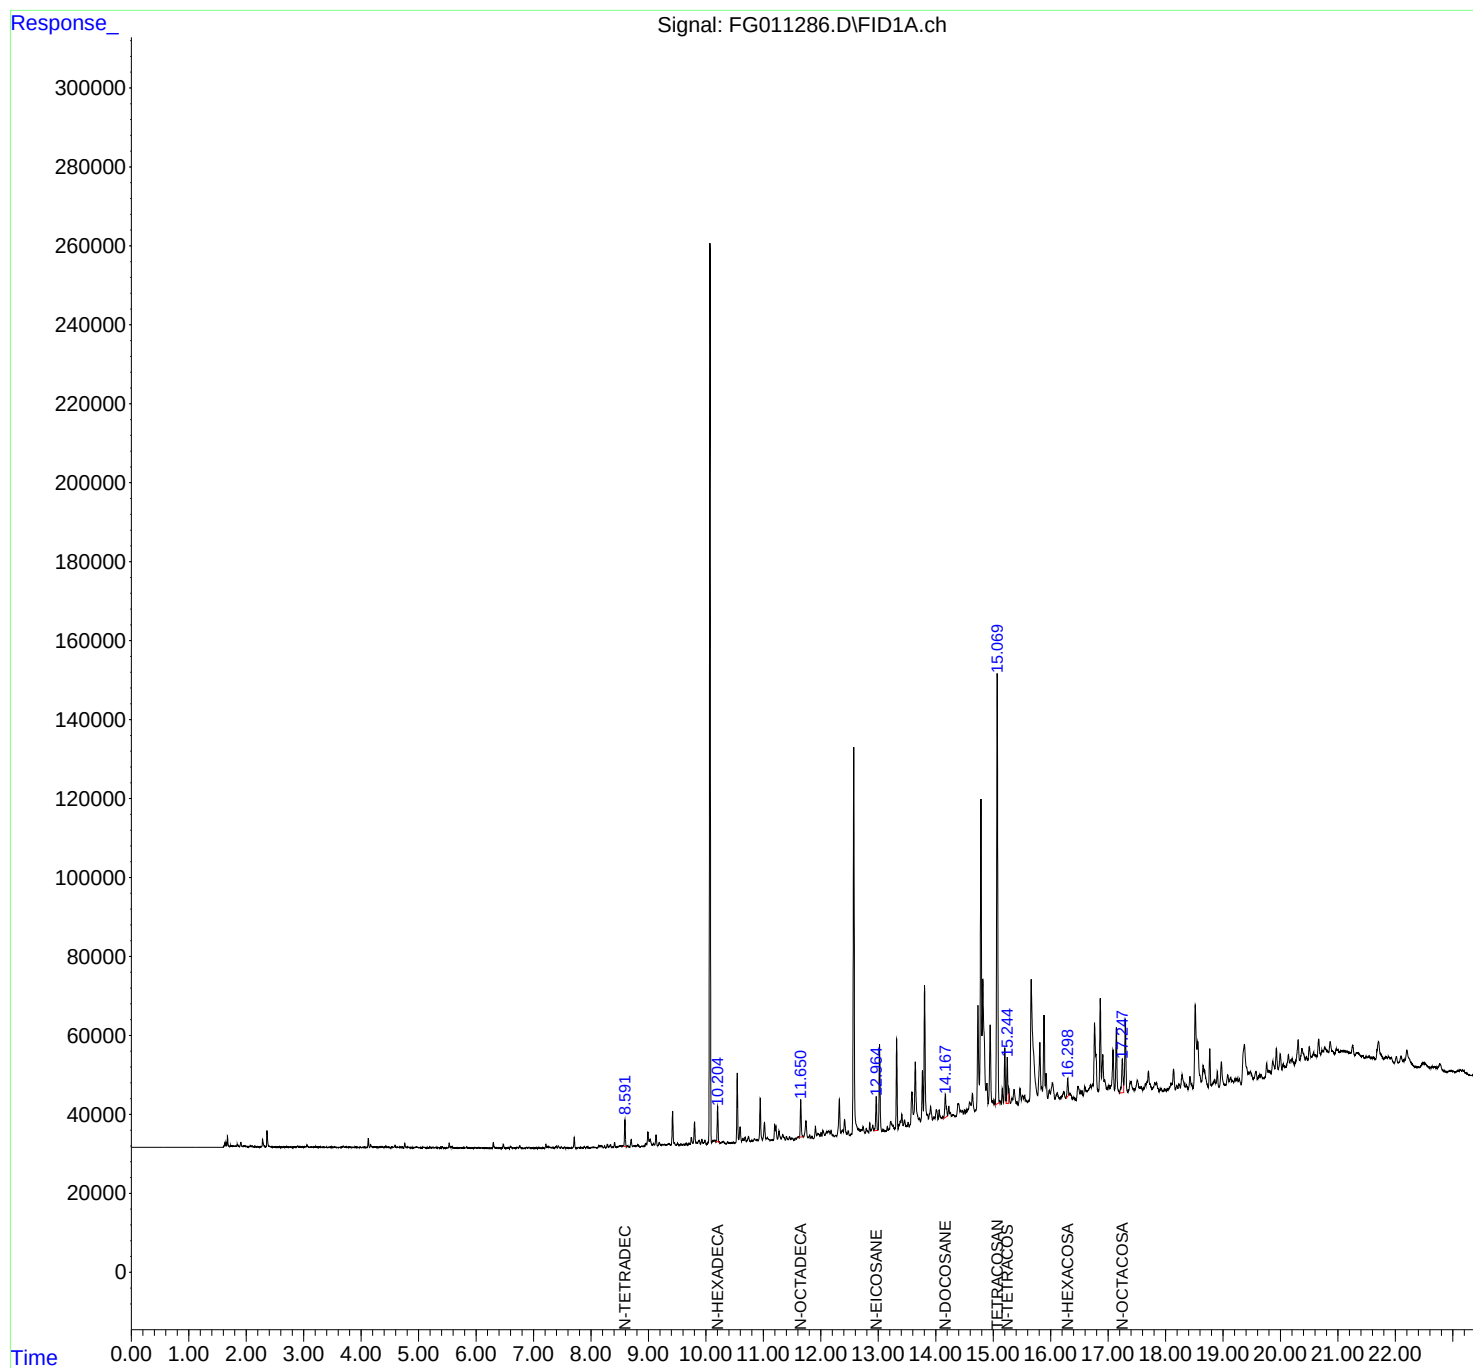


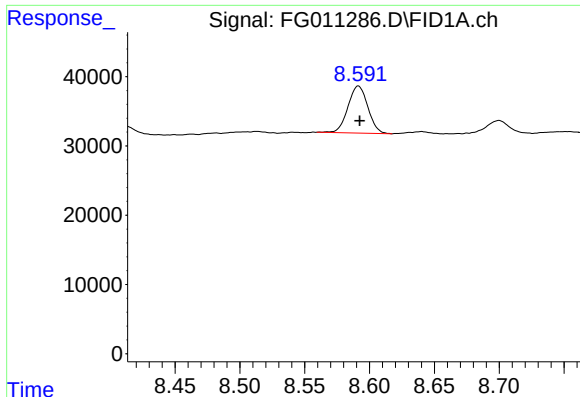

#4 N-TETRADECANE


R.T.: 8.591 min
Delta R.T.: -0.001 min
Response: 72656
Conc: 0.41 ug/ml

Instrument :
ECD_L
ClientSampleId :
TJRC-011723-B3-0-10-DUP

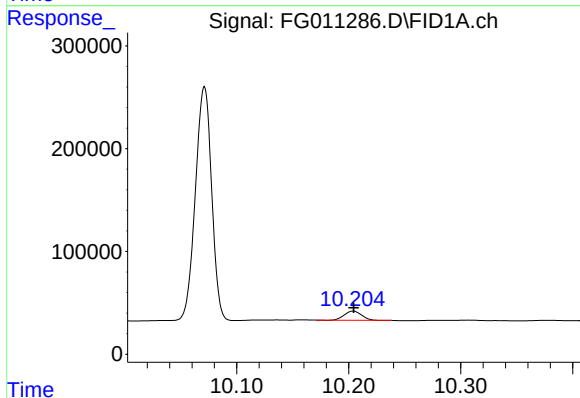


#5 N-HEXADECANE

R.T.: 10.204 min
Delta R.T.: 0.000 min
Response: 96643
Conc: 0.53 ug/ml

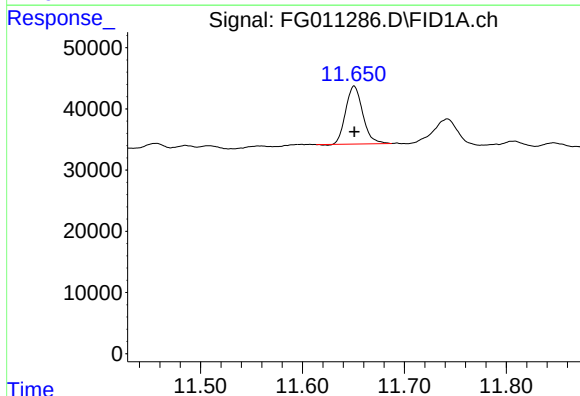


#6 N-OCTADECANE

R.T.: 11.651 min
Delta R.T.: 0.000 min
Response: 110138
Conc: 0.60 ug/ml

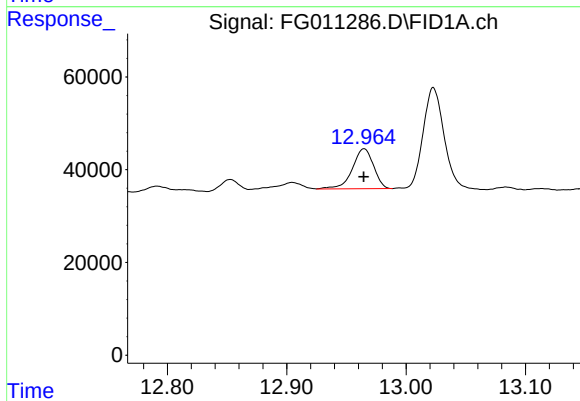

#7 N-EICOSANE


R.T.: 12.965 min
Delta R.T.: 0.000 min
Response: 106972
Conc: 0.60 ug/ml

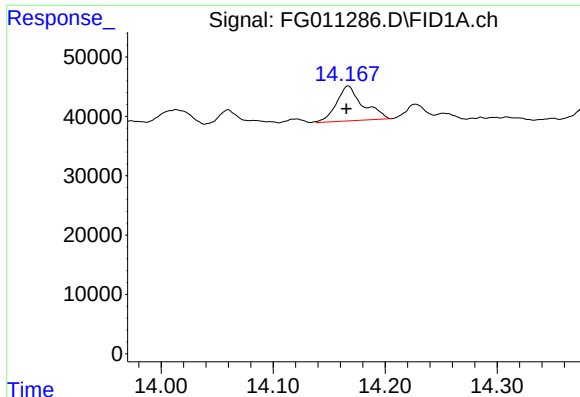

#8 N-DOCOSANE


R.T.: 14.167 min
Delta R.T.: 0.002 min
Response: 95808
Conc: 0.54 ug/ml

Instrument :
ECD_L
ClientSampleId :
TJRC-011723-B3-0-10-DUP

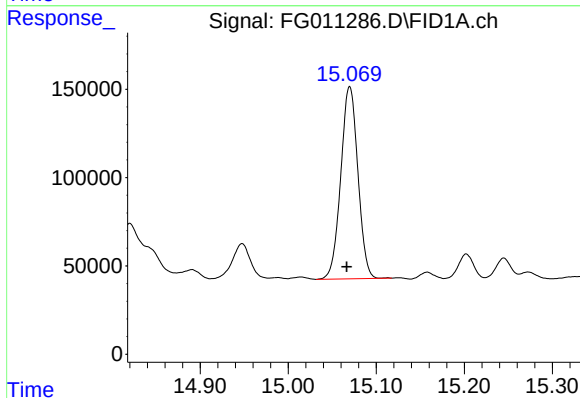


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.070 min
Delta R.T.: 0.003 min
Response: 1471890
Conc: 9.60 ug/ml

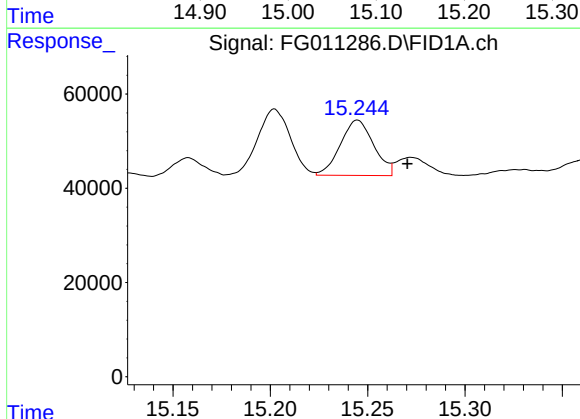


#10 N-TETRACOSANE

R.T.: 15.245 min
Delta R.T.: -0.026 min
Response: 139857
Conc: 0.80 ug/ml

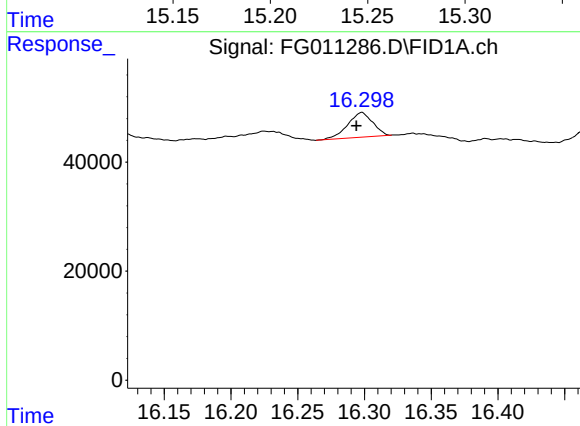

#11 N-HEXACOSANE

R.T.: 16.298 min
Delta R.T.: 0.004 min
Response: 59103
Conc: 0.35 ug/ml

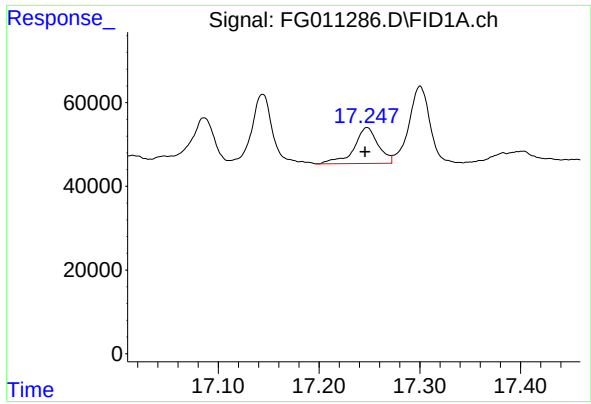

#12 N-OCTACOSANE

R.T.: 17.248 min
Delta R.T.: 0.002 min
Response: 142949
Conc: 0.87 ug/ml

Instrument :

ECD_L

ClientSampleId :

TJRC-011723-B3-0-10-DUP