

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012523DDD\
Data File : FG011295.D
Signal(s) : FID1A.ch
Acq On : 25 Jan 2023 14:28
Operator : YP\AJ
Sample : PB150448BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB150448BL

Integration File: autoint1.e
Quant Time: Jun 28 04:28:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.069	1802623	11.763 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012523DDD\
Data File : FG011295.D
Signal(s) : FID1A.ch
Acq On : 25 Jan 2023 14:28
Operator : YP\AJ
Sample : PB150448BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB150448BL

Integration File: autoint1.e
Quant Time: Jun 28 04:28:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

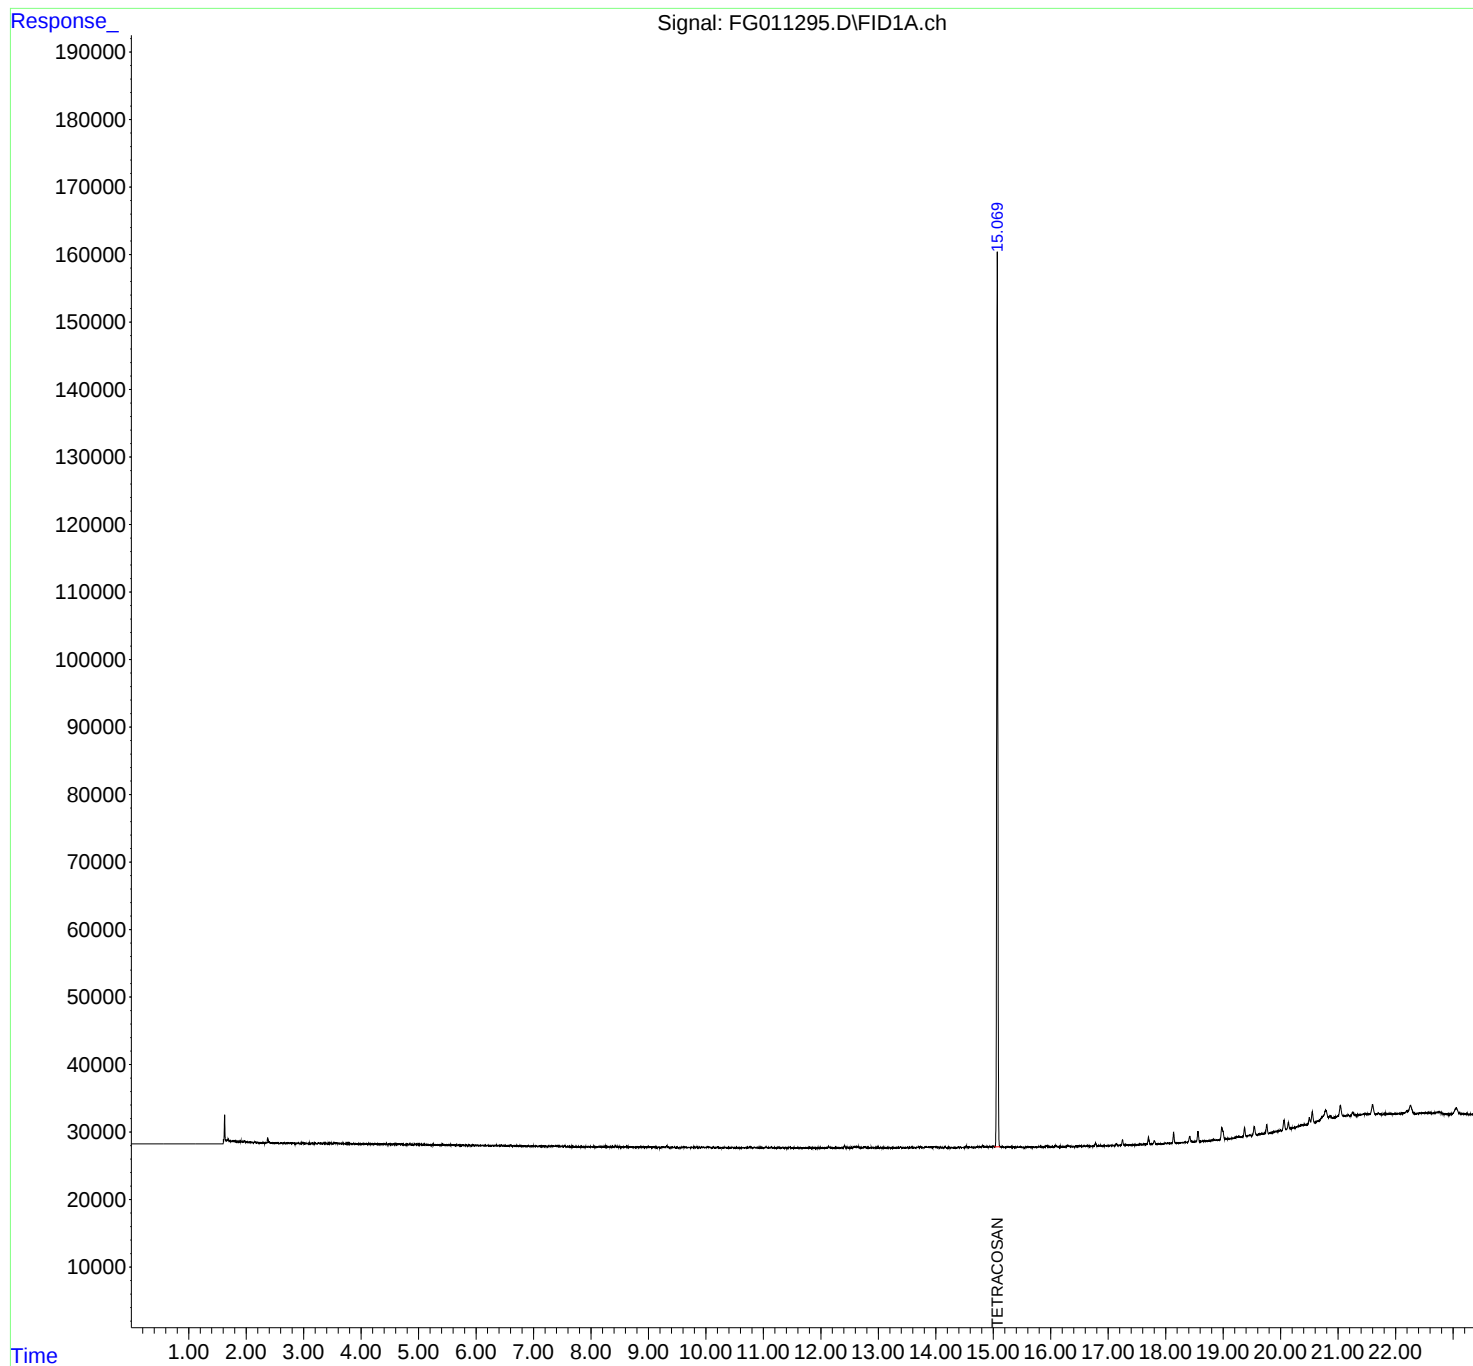

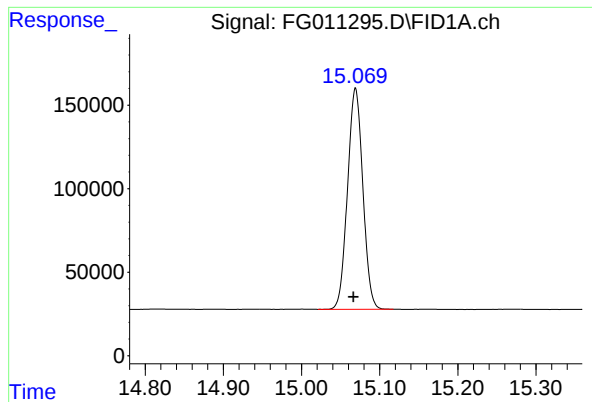

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.069 min
Delta R.T.: 0.003 min
Response: 1802623
Conc: 11.76 ug/ml

Instrument :
ECD_L
ClientSampleId :
PB150448BL