

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012623DDD\
Data File : FG011303.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2023 08:11
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 06:07:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.963	130767	0.728 ug/ml
8)	N-DOCOSANE	14.177	129108	0.730 ug/ml
10)	N-TETRACOSANE	15.283	161061	0.923 ug/ml
11)	N-HEXACOSANE	16.311	59252	0.348 ug/ml
12)	N-OCTACOSANE	17.267	50325	0.306 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG012623DDD\
Data File : FG011303.D
Signal(s) : FID1A.ch
Acq On : 26 Jan 2023 08:11
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 06:07:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG123022.M
Quant Title :
QLast Update : Mon Jan 02 04:44:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

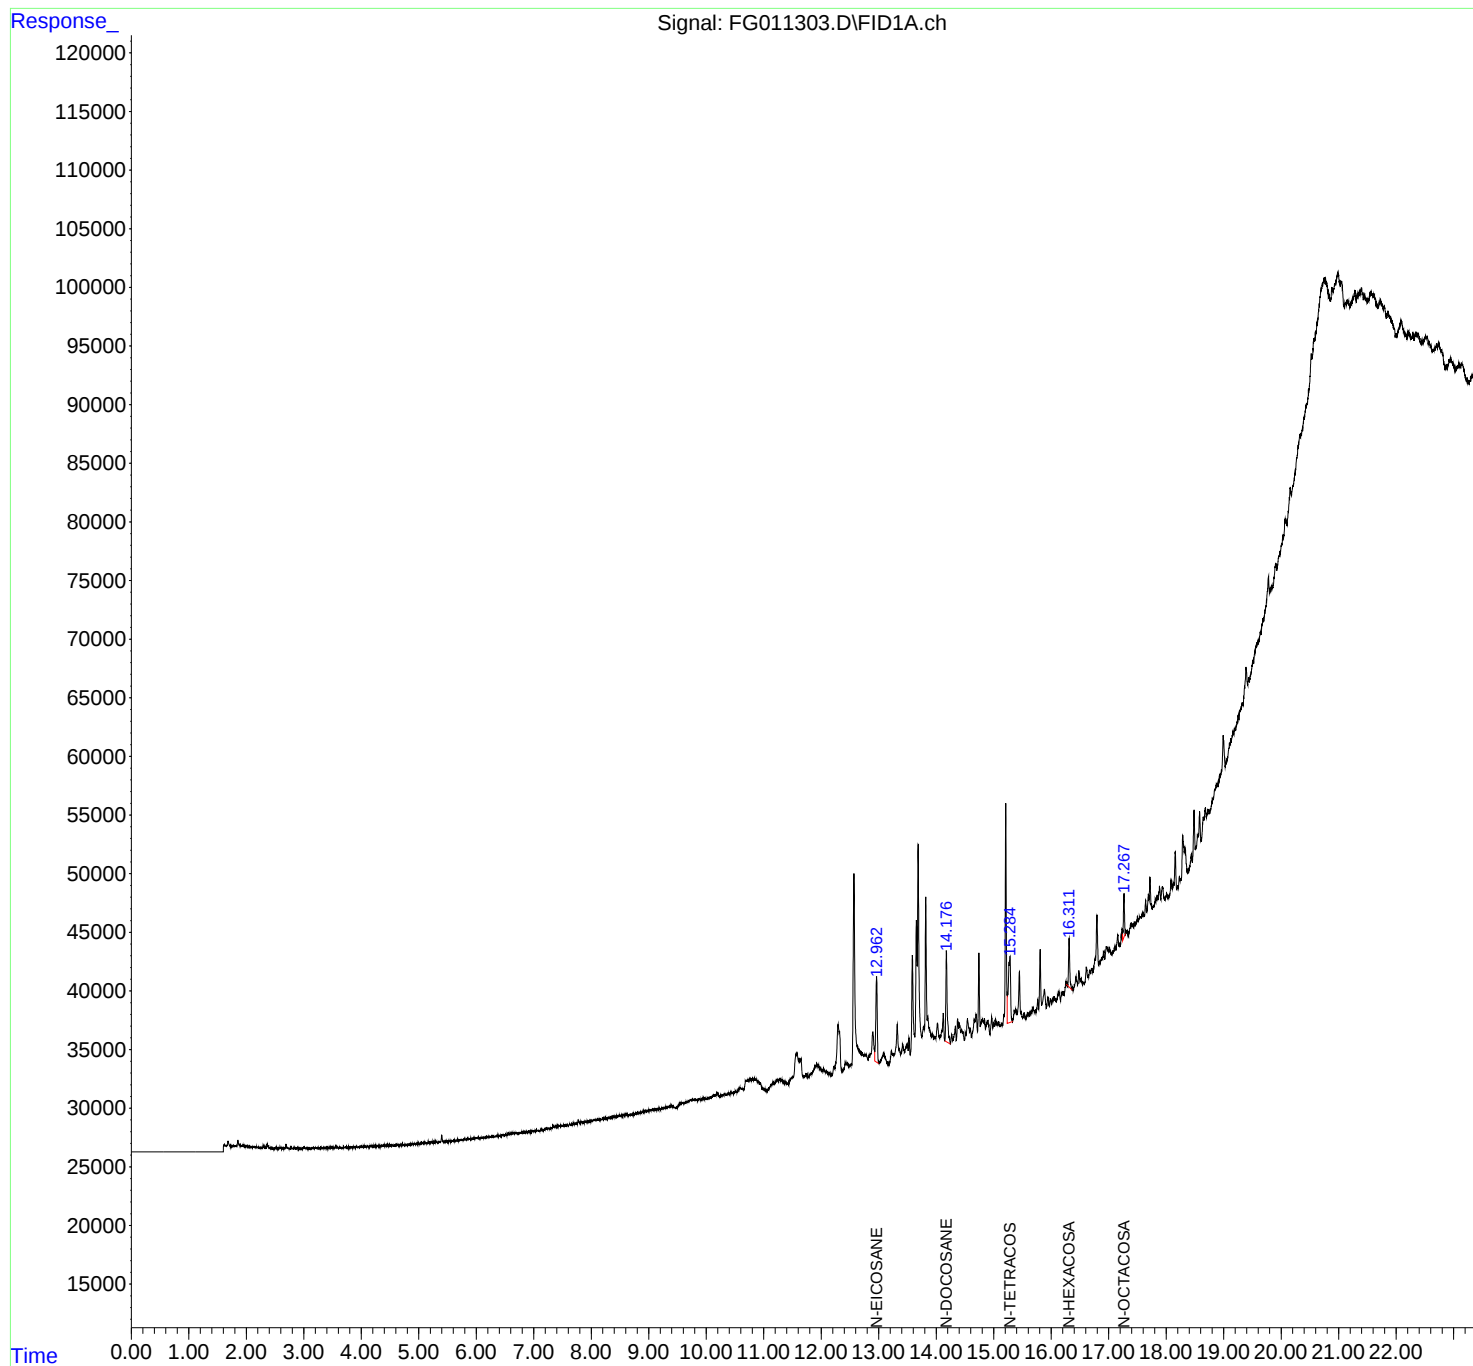


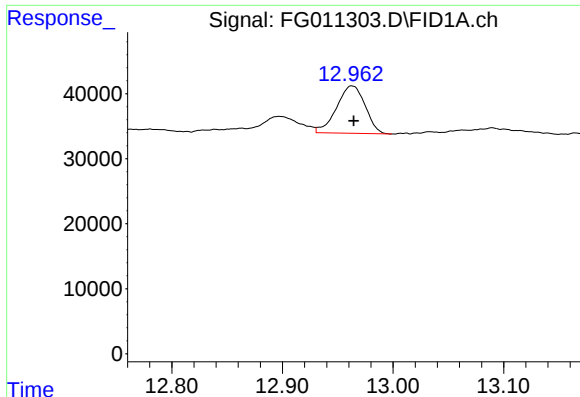

#7 N-EICOSANE


R.T.: 12.963 min
Delta R.T.: -0.002 min
Response: 130767
Conc: 0.73 ug/ml

Instrument :
ECD_L
ClientSampleId :

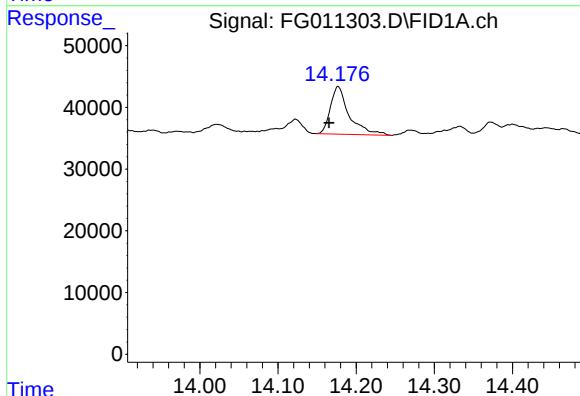


#8 N-DOCOSANE

R.T.: 14.177 min
Delta R.T.: 0.011 min
Response: 129108
Conc: 0.73 ug/ml

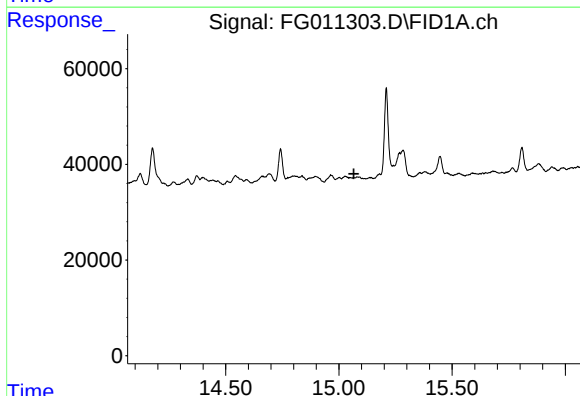


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

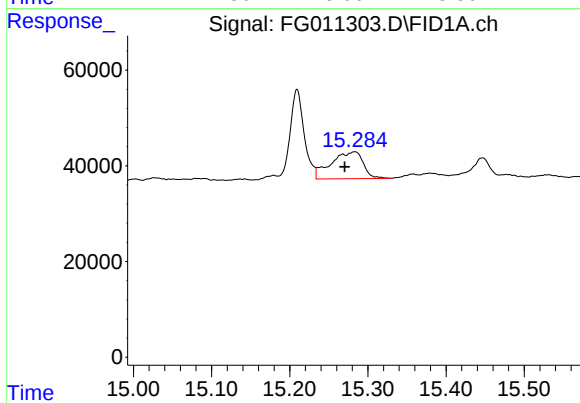

#10 N-TETRACOSANE


R.T.: 15.283 min
Delta R.T.: 0.013 min
Response: 161061
Conc: 0.92 ug/ml

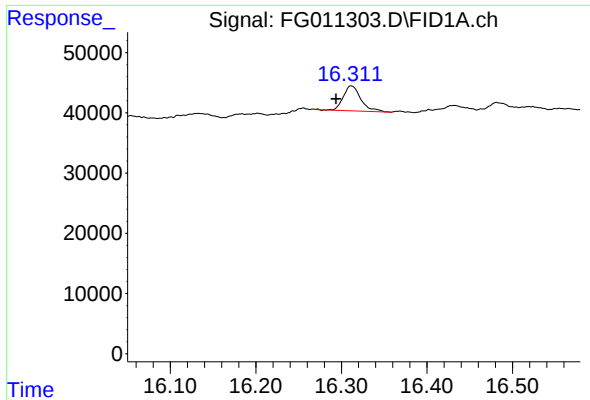

#11 N-HEXACOSANE

R.T.: 16.311 min
Delta R.T.: 0.018 min
Response: 59252
Conc: 0.35 ug/ml

Instrument :
ECD_L
ClientSampleId :

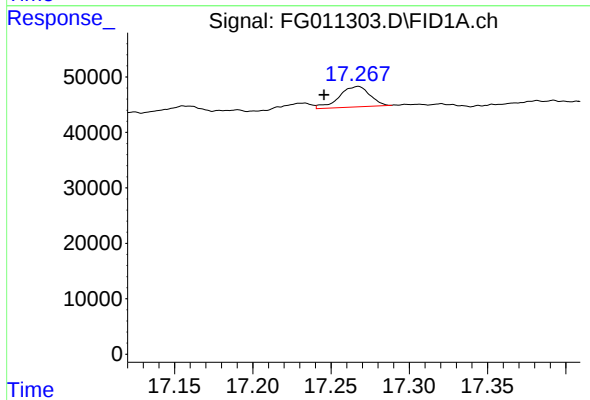

#12 N-OCTACOSANE

R.T.: 17.267 min
Delta R.T.: 0.022 min
Response: 50325
Conc: 0.31 ug/ml