

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041723DDD\
Data File : FG011837.D
Signal(s) : FID1A.ch
Acq On : 17 Apr 2023 21:49
Operator : YP\AJ
Sample :
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 07:51:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041323.M
Quant Title :
QLast Update : Wed Apr 12 18:20:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.942	56833	0.545 ug/ml
15) N-TETRATRIACONTANE	19.727	57701	0.562 ug/ml
16) N-HEXATRIACONTANE	20.468	61993	0.606 ug/ml
17) N-OCTATRIACONTANE	21.214	80543	0.772 ug/ml
18) N-TETRACONTANE	22.145	117592	1.109 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG041723DDD\
Data File : FG011837.D
Signal(s) : FID1A.ch
Acq On : 17 Apr 2023 21:49
Operator : YP\AJ
Sample :
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 07:51:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG041323.M
Quant Title :
QLast Update : Wed Apr 12 18:20:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

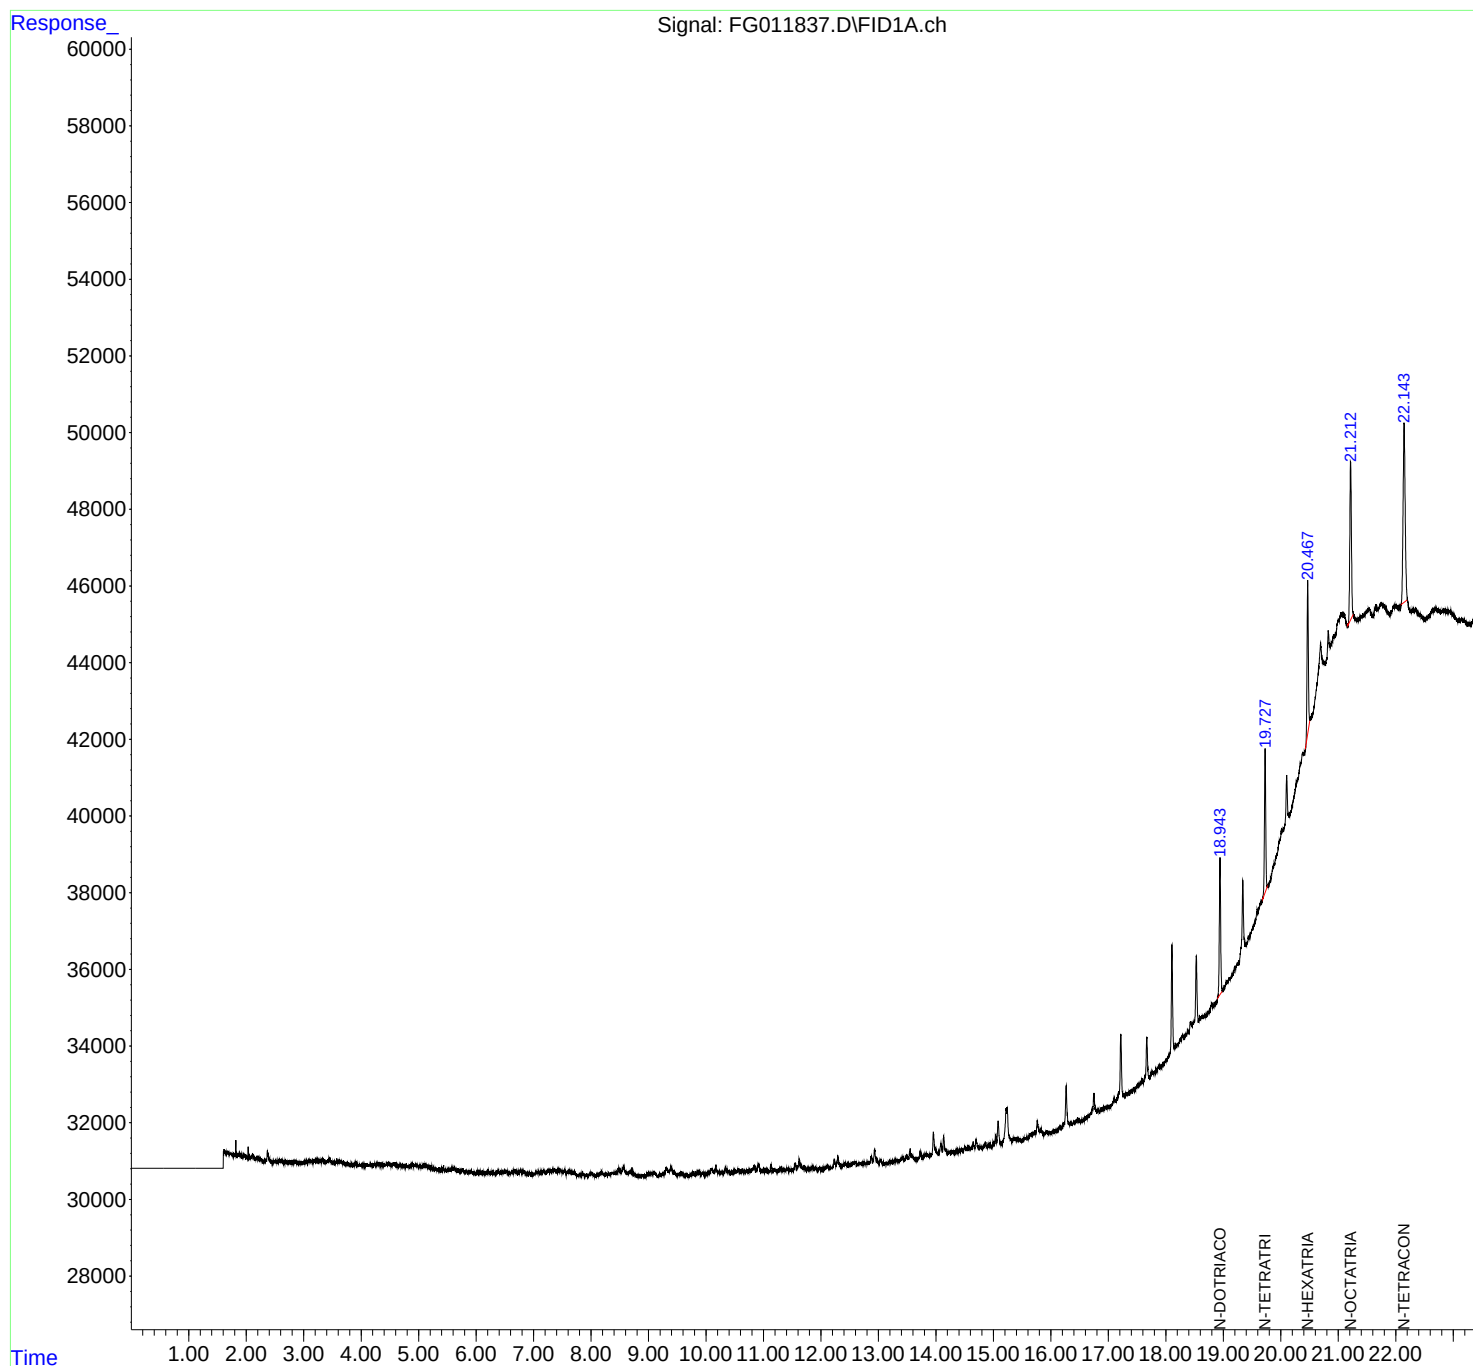


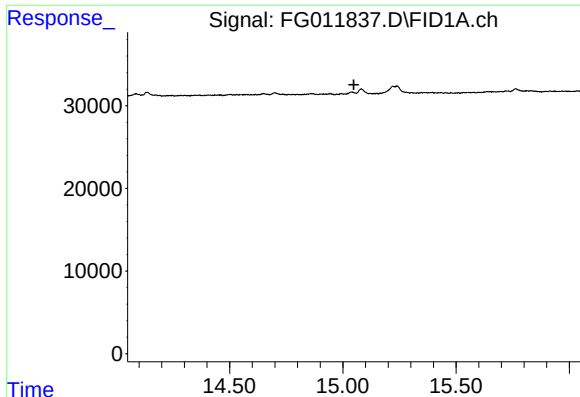

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

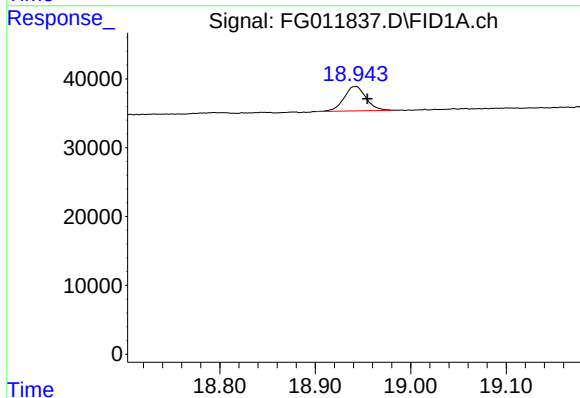


#14 N-DOTRIACONTANE

R.T.: 18.942 min
Delta R.T.: -0.012 min
Response: 56833
Conc: 0.55 ug/ml

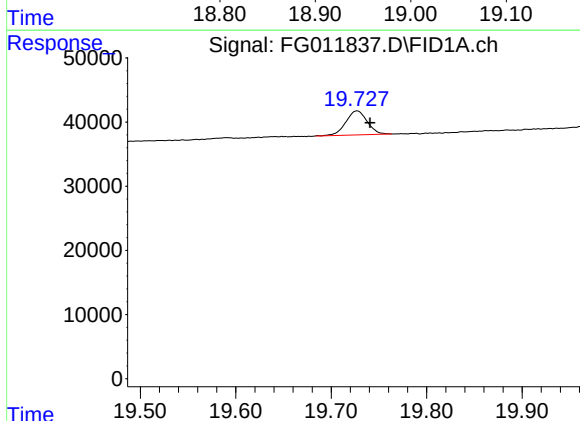


#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: -0.014 min
Response: 57701
Conc: 0.56 ug/ml

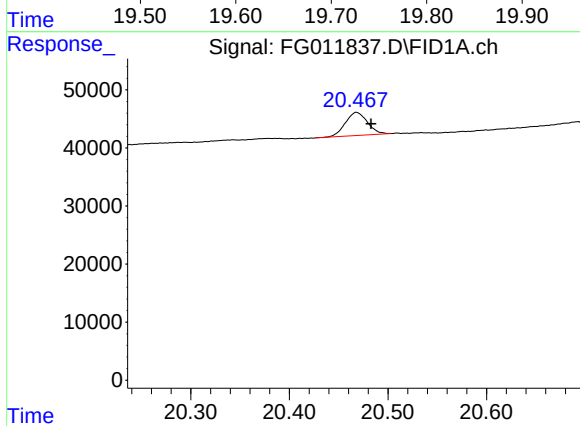

#16 N-HEXATRIACONTANE


R.T.: 20.468 min
Delta R.T.: -0.015 min
Response: 61993
Conc: 0.61 ug/ml

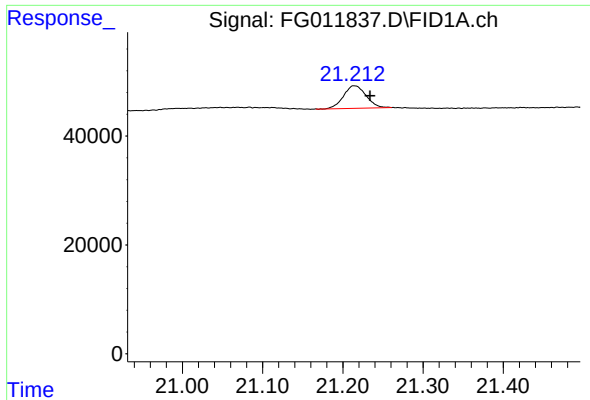

#17 N-OCTATRIACONTANE

R.T.: 21.214 min
Delta R.T.: -0.020 min
Response: 80543
Conc: 0.77 ug/ml

Instrument :
ECD_L
ClientSampleId :

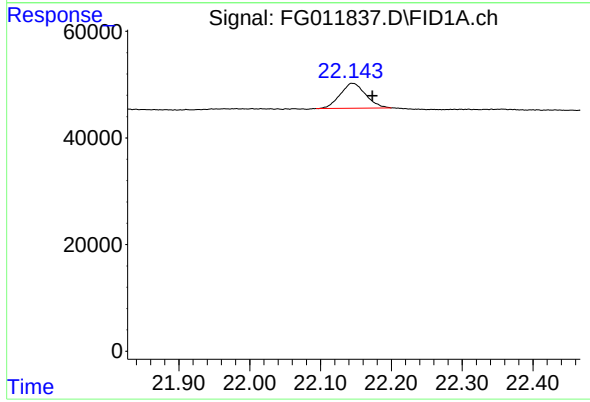

#18 N-TETRACONTANE

R.T.: 22.145 min
Delta R.T.: -0.029 min
Response: 117592
Conc: 1.11 ug/ml