

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061923\
 Data File : PL083550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 18:18
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 04:15:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 17 12:34:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	2.754	98964638	130.9E6	44.774	56.190 #
28)	SA Decachlor...	8.994	7.964	80843263	101.3E6	42.425	41.254
Target Compounds							
23)	Chlordane-1	4.624	3.767	41270015	48146002	429.014	491.177
24)	Chlordane-2	5.155	4.353	47409100	57074269	436.964	474.634
25)	Chlordane-3	5.868	4.991	165.8E6	156.3E6	433.942	477.161
26)	Chlordane-4	5.951	5.055	203.6E6	156.3E6	440.275	463.712
27)	Chlordane-5	6.799	5.956	30748102	48495555	387.392	436.199



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061923\
Data File : PL083550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 18:18
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 04:15:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061723.M
Quant Title : GC Extractables
QLast Update : Sat Jun 17 12:34:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

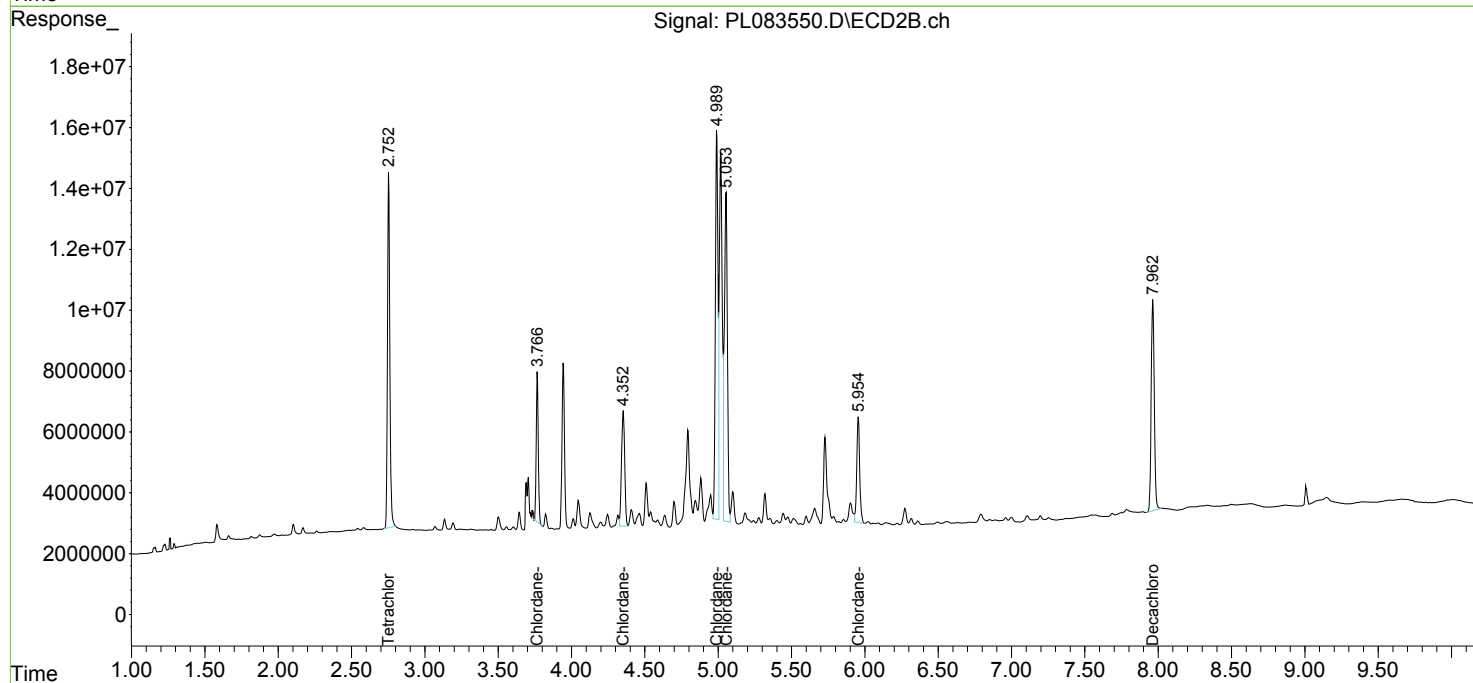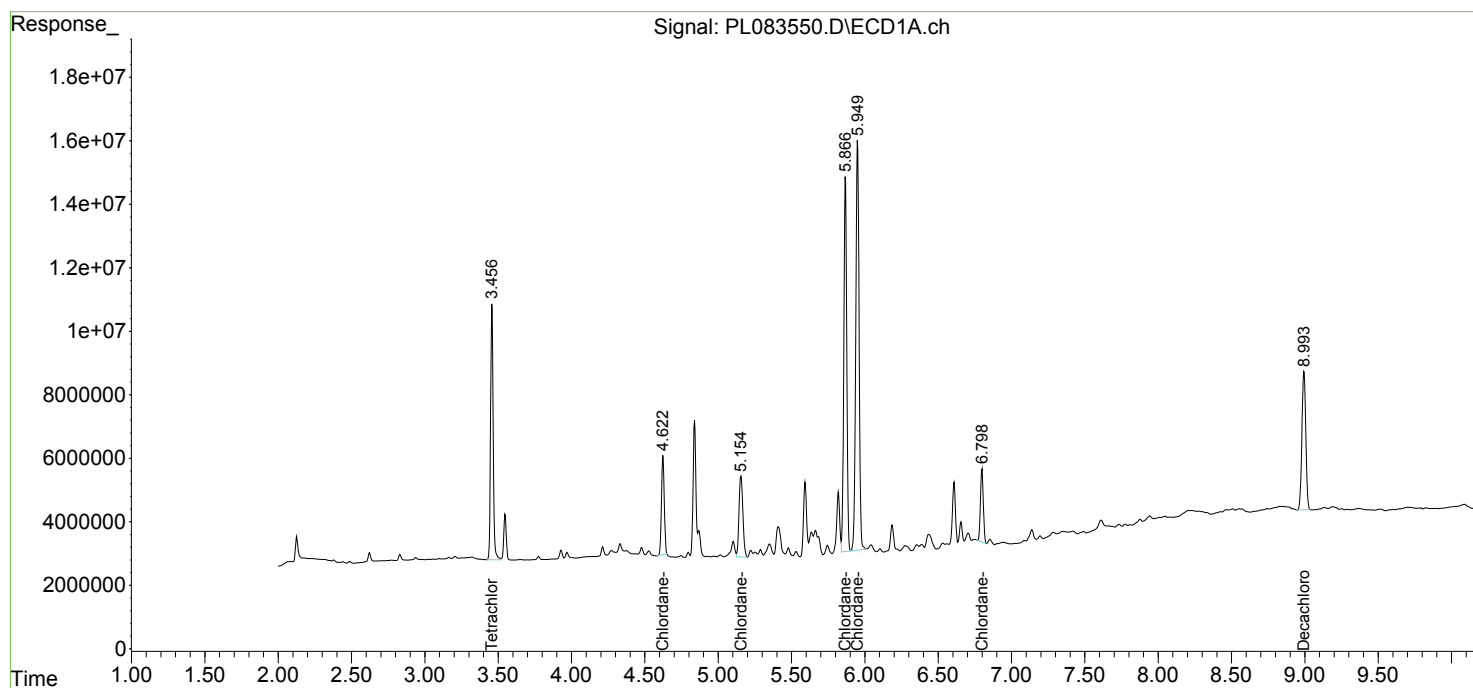


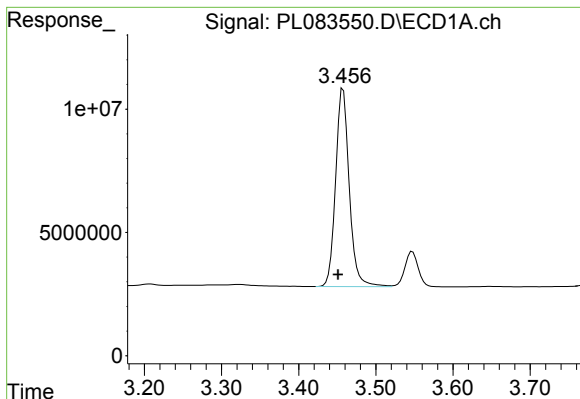

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.007 min
Response: 98964638
Conc: 44.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

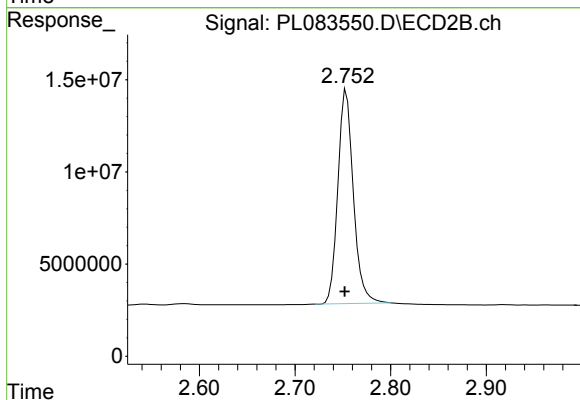


#1 Tetrachloro-m-xylene

R.T.: 2.754 min
Delta R.T.: 0.002 min
Response: 130887917
Conc: 56.19 ng/ml

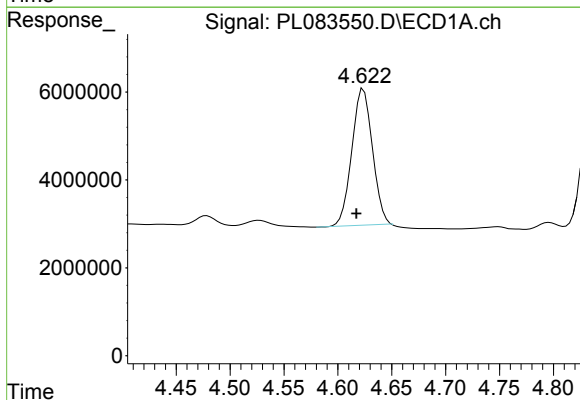


#23 Chlordane-1

R.T.: 4.624 min
Delta R.T.: 0.007 min
Response: 41270015
Conc: 429.01 ng/ml

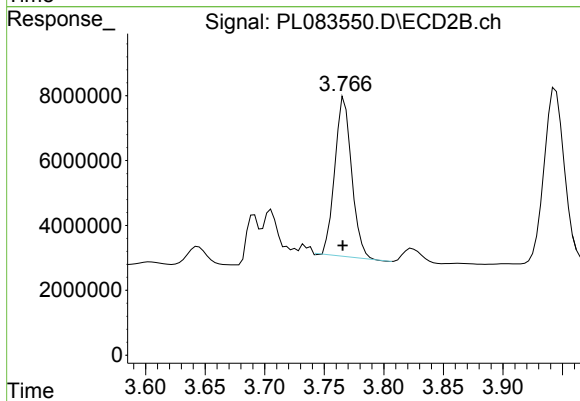

#23 Chlordane-1


R.T.: 3.767 min
Delta R.T.: 0.002 min
Response: 48146002
Conc: 491.18 ng/ml

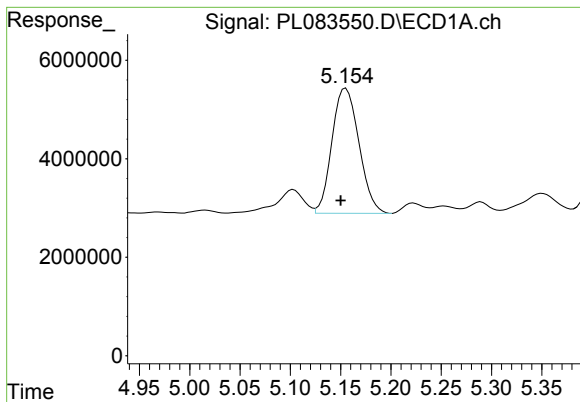

#24 Chlordane-2


R.T.: 5.155 min
Delta R.T.: 0.005 min
Response: 47409100
Conc: 436.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

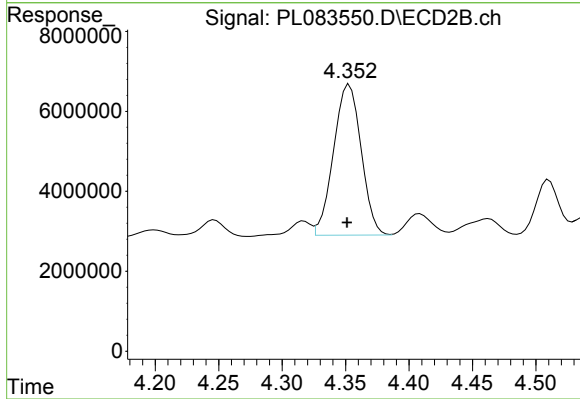


#24 Chlordane-2

R.T.: 4.353 min
Delta R.T.: 0.002 min
Response: 57074269
Conc: 474.63 ng/ml

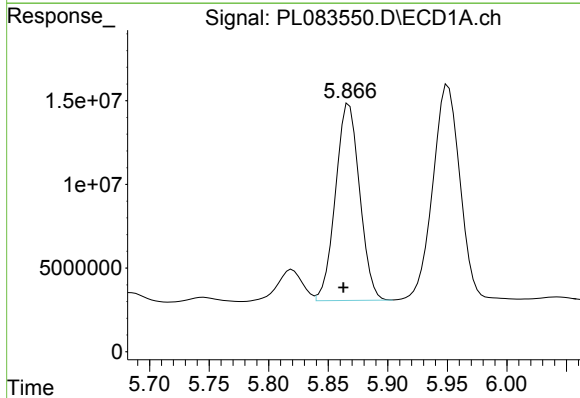


#25 Chlordane-3

R.T.: 5.868 min
Delta R.T.: 0.005 min
Response: 165810808
Conc: 433.94 ng/ml

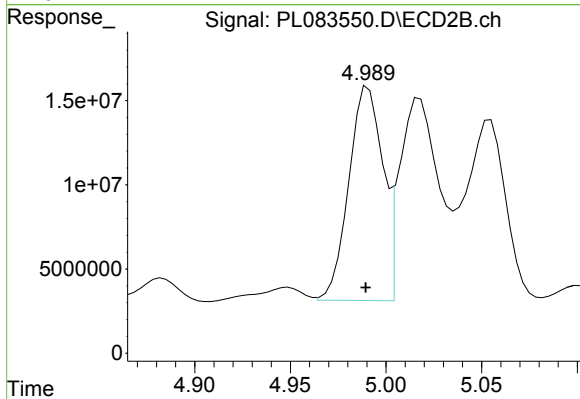

#25 Chlordane-3


R.T.: 4.991 min
Delta R.T.: 0.001 min
Response: 156344262
Conc: 477.16 ng/ml

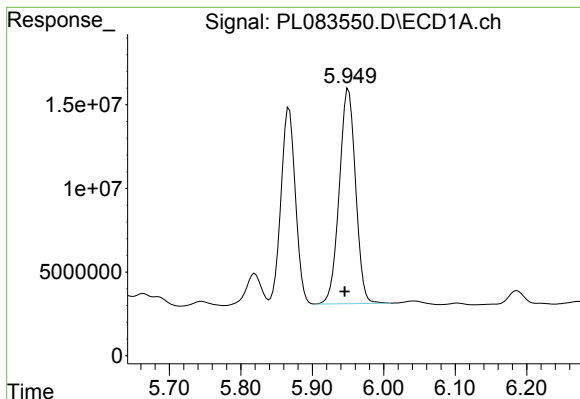

#26 Chlordane-4


R.T.: 5.951 min
Delta R.T.: 0.005 min
Response: 203593881
Conc: 440.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

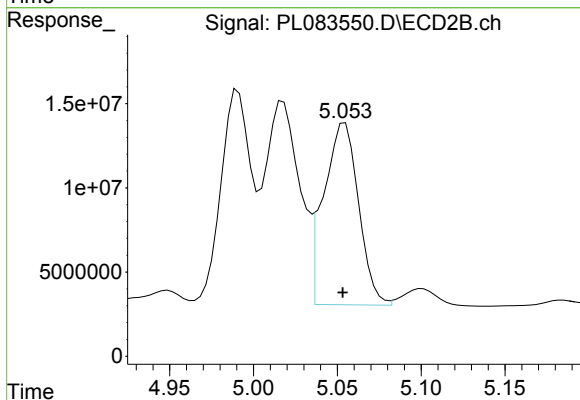


#26 Chlordane-4

R.T.: 5.055 min
Delta R.T.: 0.001 min
Response: 156307650
Conc: 463.71 ng/ml

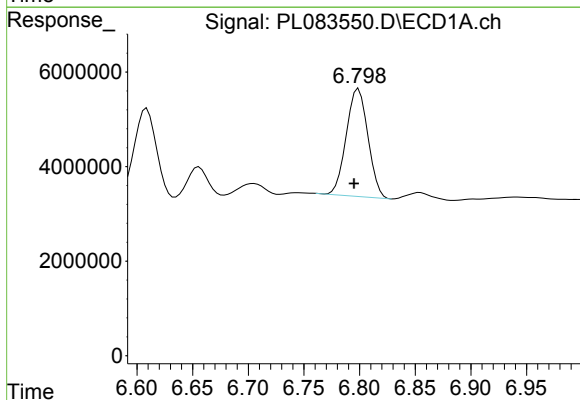


#27 Chlordane-5

R.T.: 6.799 min
Delta R.T.: 0.004 min
Response: 30748102
Conc: 387.39 ng/ml

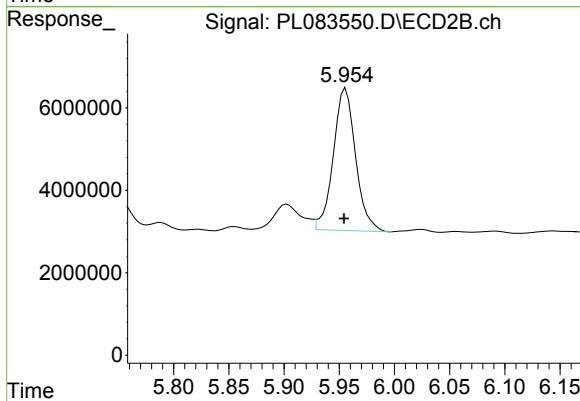

#27 Chlordane-5


R.T.: 5.956 min
Delta R.T.: 0.001 min
Response: 48495555
Conc: 436.20 ng/ml

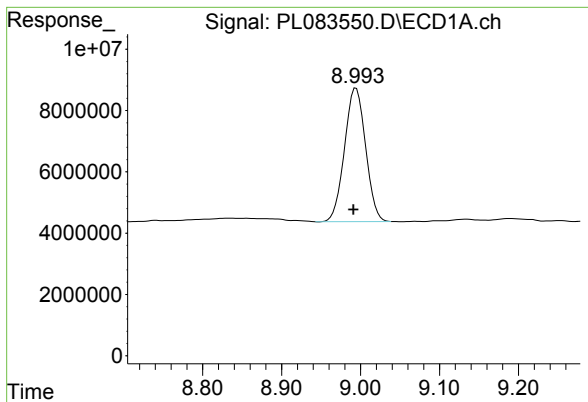

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.003 min
Response: 80843263
Conc: 42.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

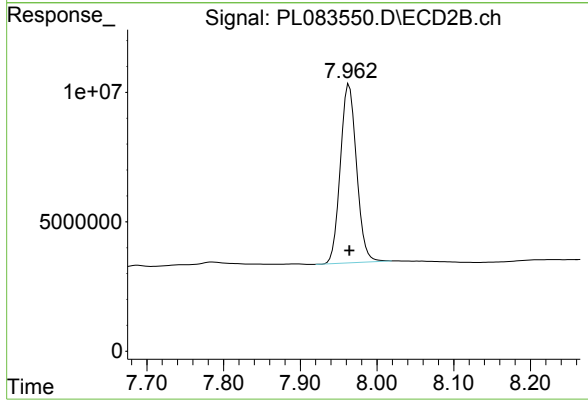

#28 Decachlorobiphenyl

R.T.: 7.964 min
Delta R.T.: 0.000 min
Response: 101323054
Conc: 41.25 ng/ml