

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061924\
 Data File : PL090234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 13:37
 Operator : AR\AJ
 Sample : P2943-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-212

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/20/2024
 Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:23:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.791	24031796	15266055	11.478m	10.647
28)	SA Decachlor...	9.055	7.933	15357872	15498321	10.445	10.429
Target Compounds							
12)	B 4,4'-DDE	6.196	5.250	109.0E6	92353087	50.095	55.279m
15)	B Endosulfa...	6.800	5.956	615039	1457209	0.295	0.905 #
16)	A 4,4'-DDD	6.713	5.805	7491721	3811351	4.277m	2.704 #
17)	MA 4,4'-DDT	7.026	6.056	59541401	47247551	32.340	31.113

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061924\
Data File : PL090234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 13:37
Operator : AR\AJ
Sample : P2943-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/20/2024
Supervised By : Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:23:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

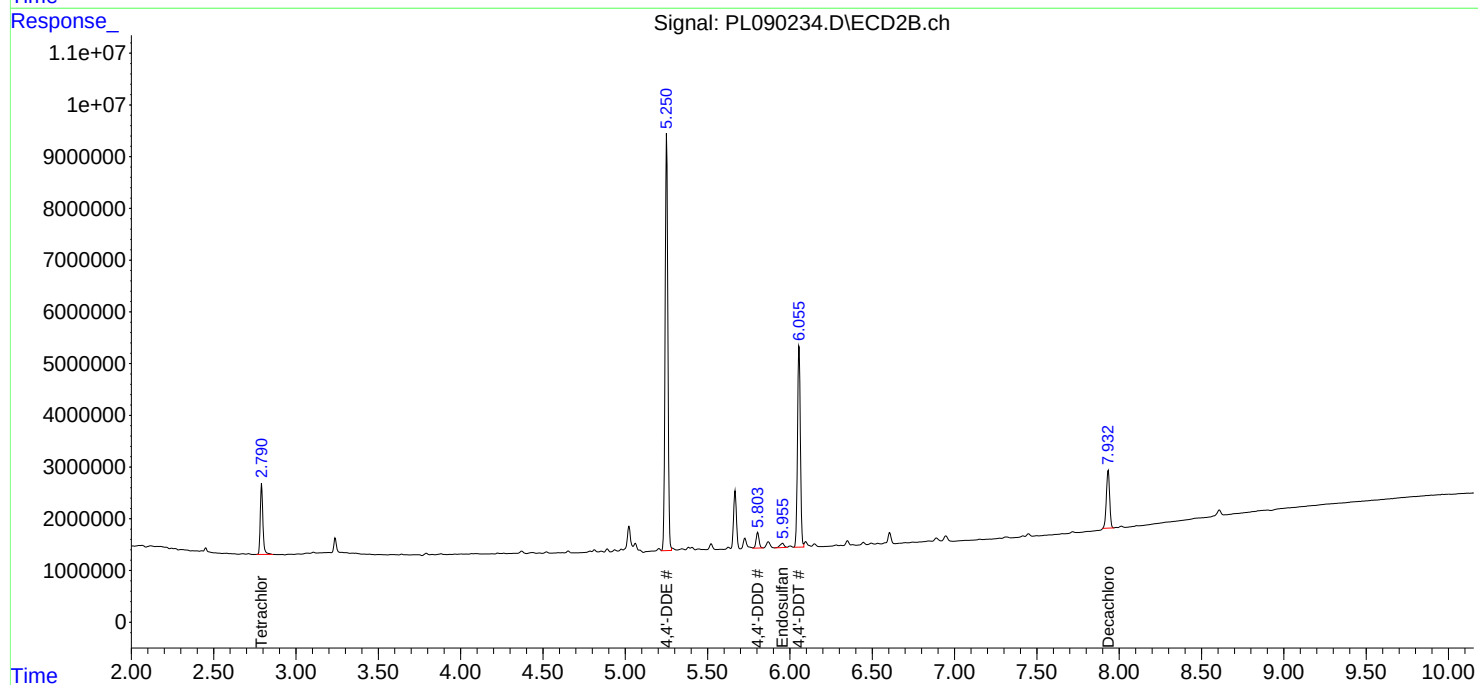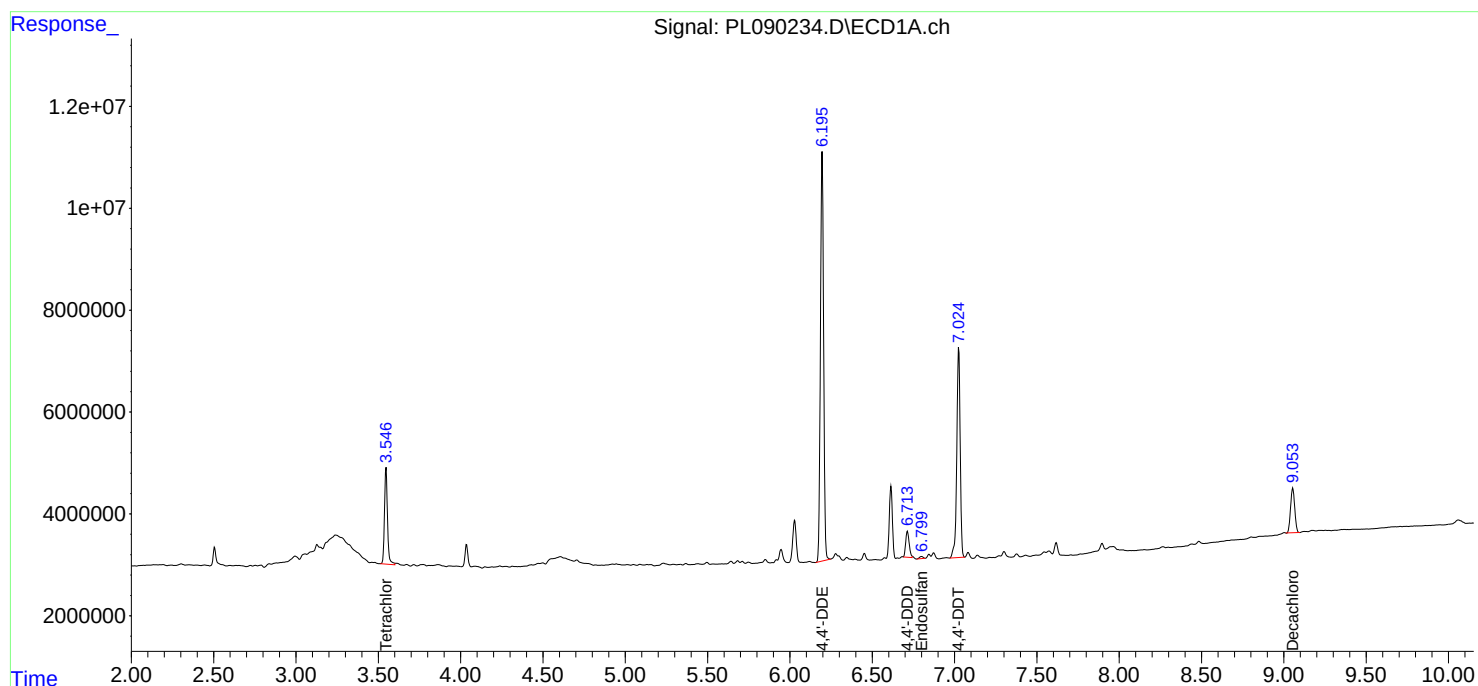

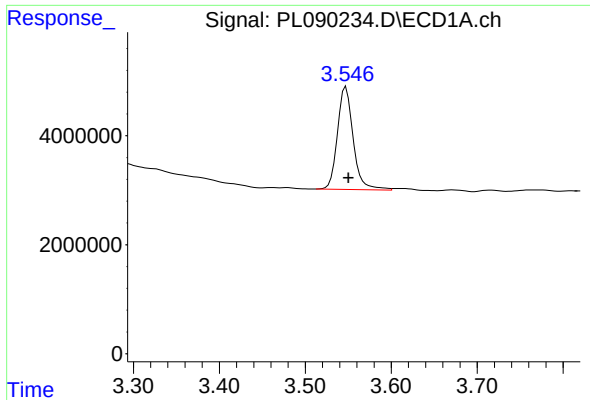


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.004 min
Response: 24031796
Conc: 11.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

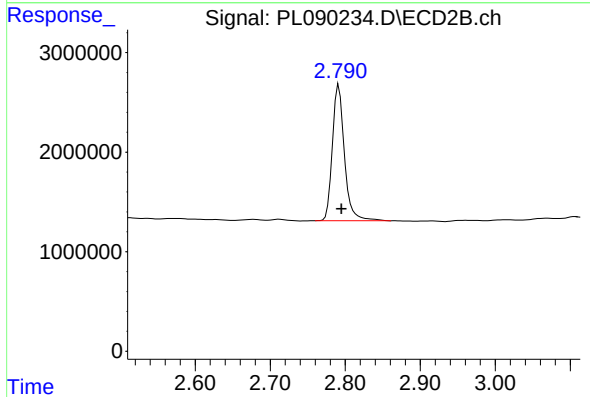


#1 Tetrachloro-m-xylene

R.T.: 2.791 min
Delta R.T.: -0.003 min
Response: 15266055
Conc: 10.65 ng/ml

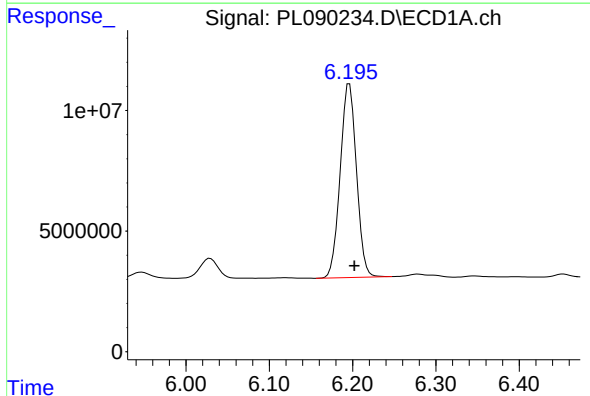


#12 4,4'-DDE

R.T.: 6.196 min
Delta R.T.: -0.006 min
Response: 108975482
Conc: 50.10 ng/ml

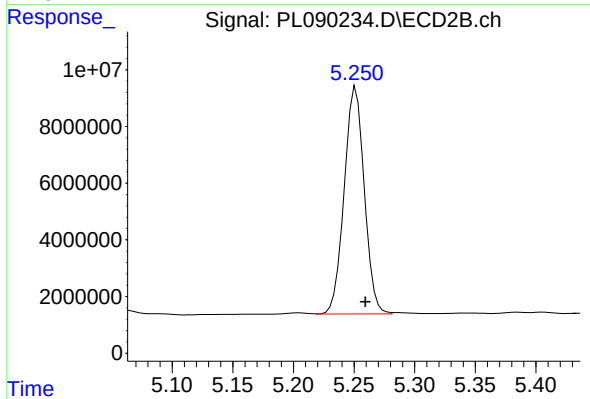

#12 4,4'-DDE

R.T.: 5.250 min
Delta R.T.: -0.009 min
Response: 92353087
Conc: 55.28 ng/ml m

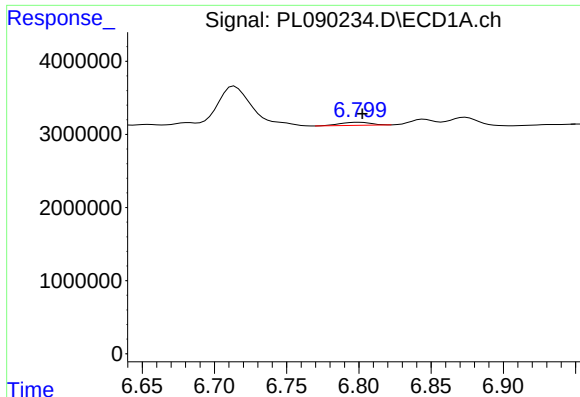


#15 Endosulfan II

R.T.: 6.800 min
Delta R.T.: -0.002 min
Response: 615039
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

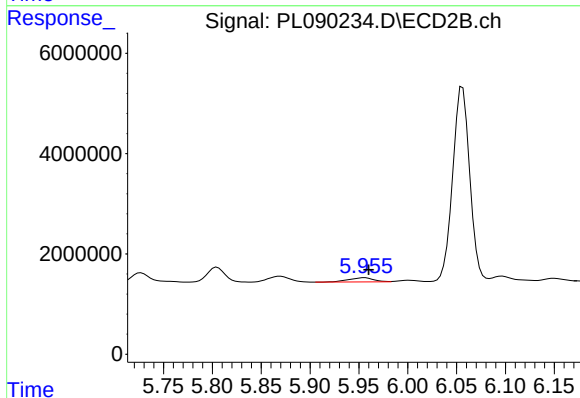


#15 Endosulfan II

R.T.: 5.956 min
Delta R.T.: -0.004 min
Response: 1457209
Conc: 0.90 ng/ml

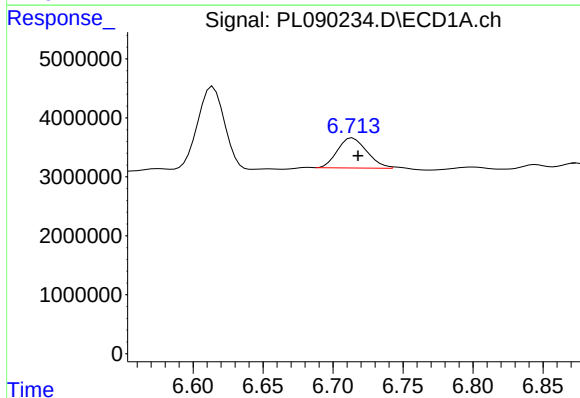


#16 4,4'-DDD

R.T.: 6.713 min
Delta R.T.: -0.005 min
Response: 7491721
Conc: 4.28 ng/ml m

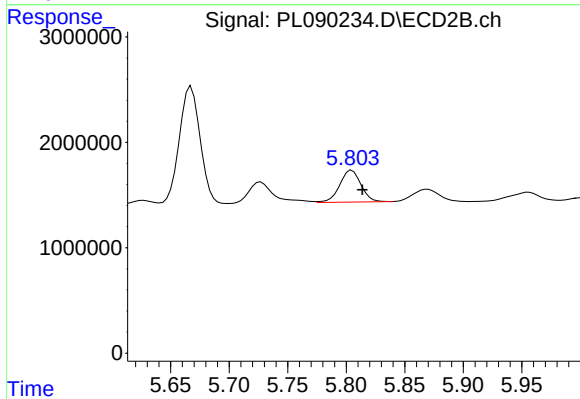

#16 4,4'-DDD

R.T.: 5.805 min
Delta R.T.: -0.009 min
Response: 3811351
Conc: 2.70 ng/ml

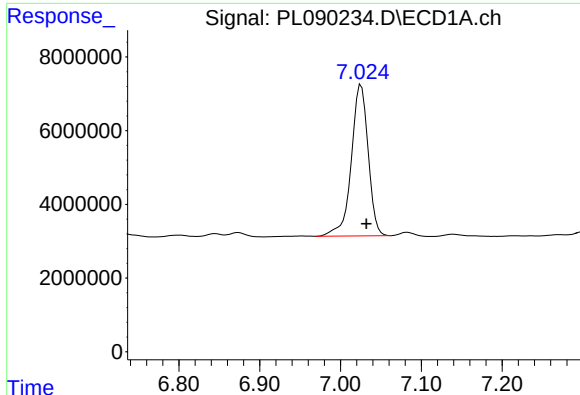


#17 4,4'-DDT

R.T.: 7.026 min
Delta R.T.: -0.007 min
Response: 59541401
Conc: 32.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-212


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

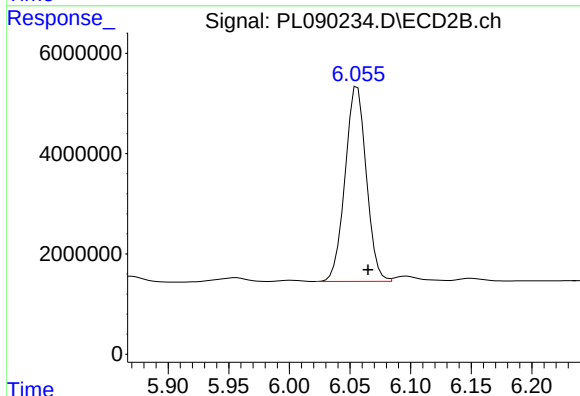


#17 4,4'-DDT

R.T.: 6.056 min
Delta R.T.: -0.009 min
Response: 47247551
Conc: 31.11 ng/ml

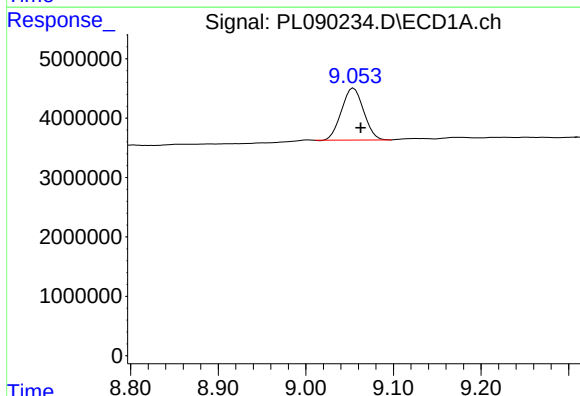

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: -0.008 min
Response: 15357872
Conc: 10.44 ng/ml

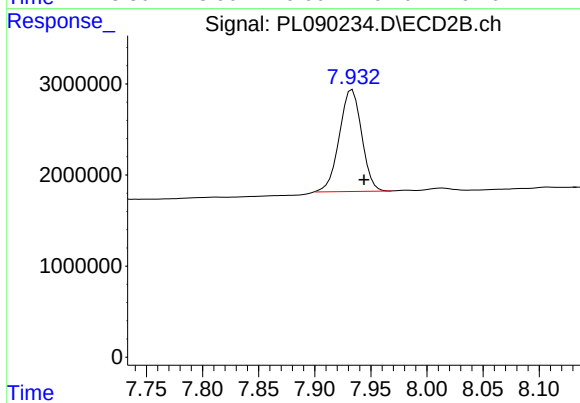

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: -0.010 min
Response: 15498321
Conc: 10.43 ng/ml