

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061924\
 Data File : PL090247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 17:53
 Operator : AR\AJ
 Sample : P2956-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-W-01-202406

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/20/2024
 Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:28:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:57:01 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.790	41585409	29893241	19.862m	20.848
28) SA Decachlor...	9.053	7.932	25566434	24604473	17.388	16.557

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061924\
Data File : PL090247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 17:53
Operator : AR\AJ
Sample : P2956-02
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-W-01-202406


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/20/2024
Supervised By : Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:28:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:57:01 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

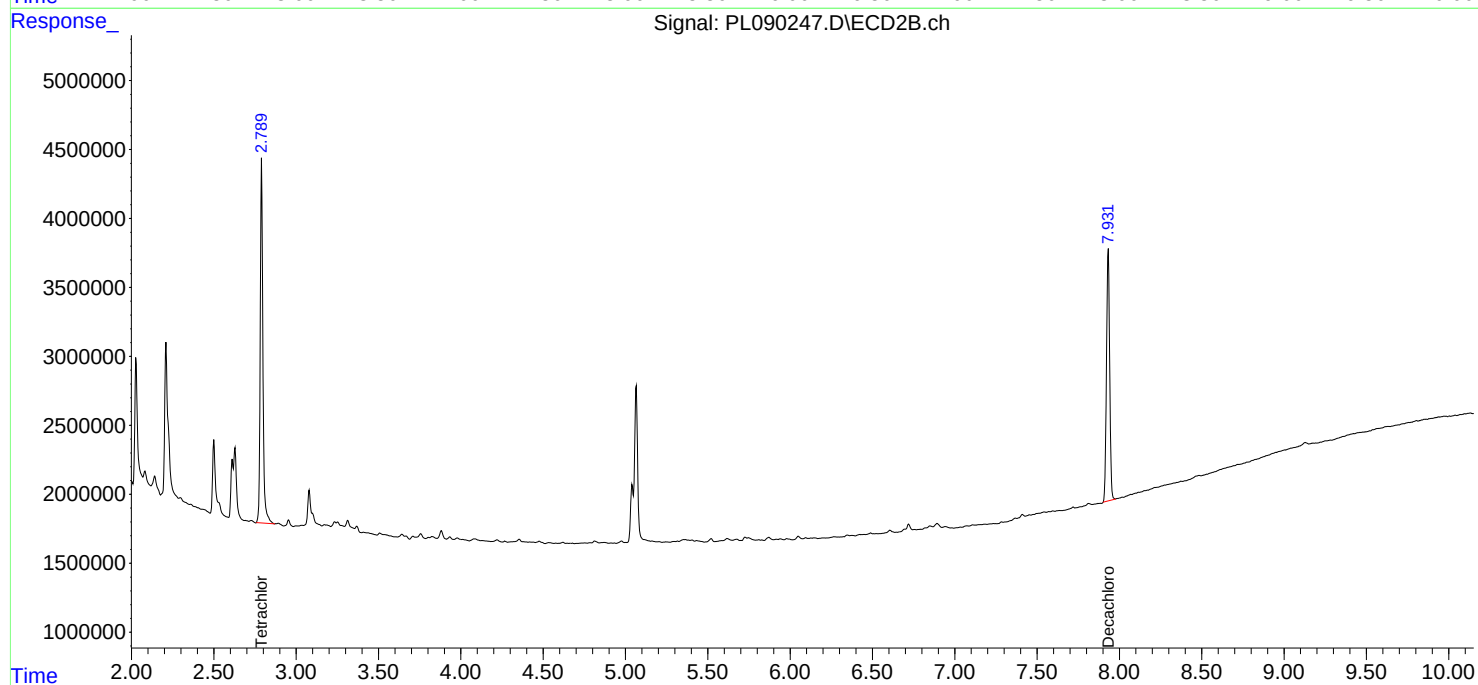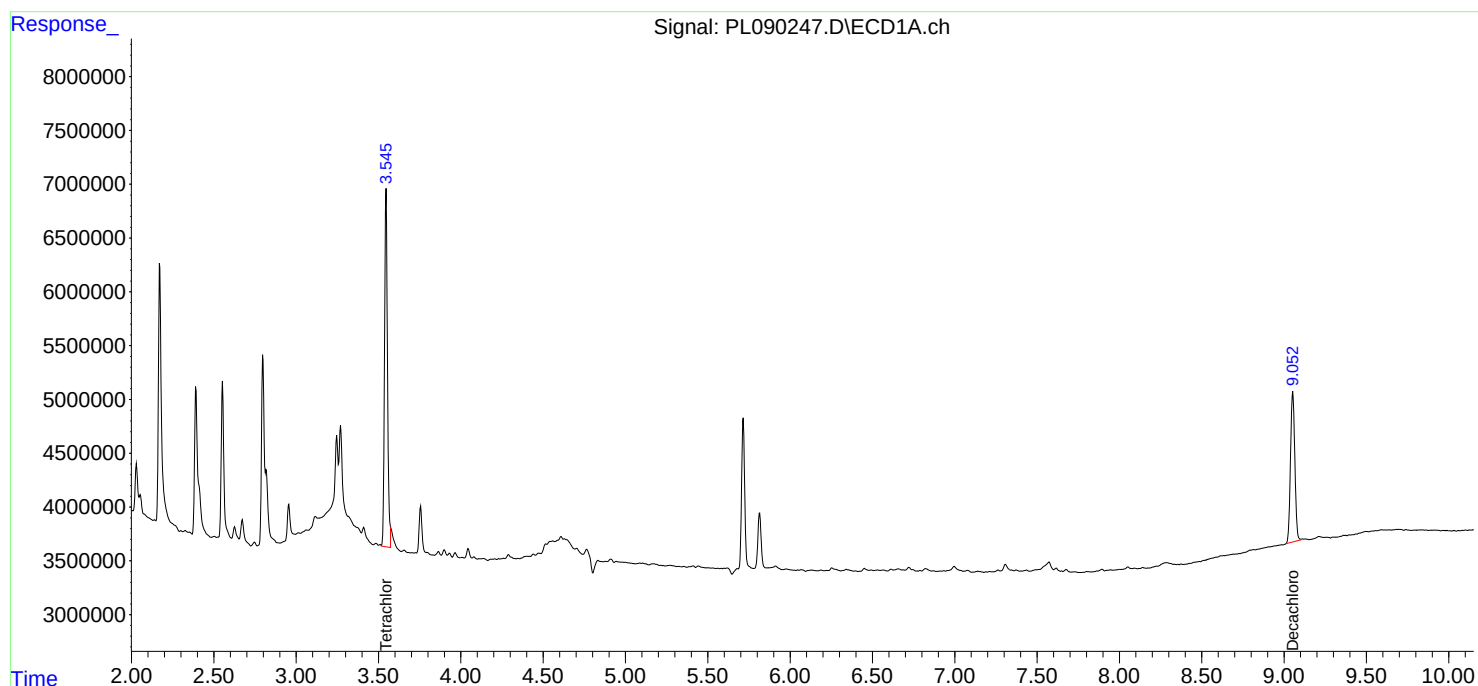

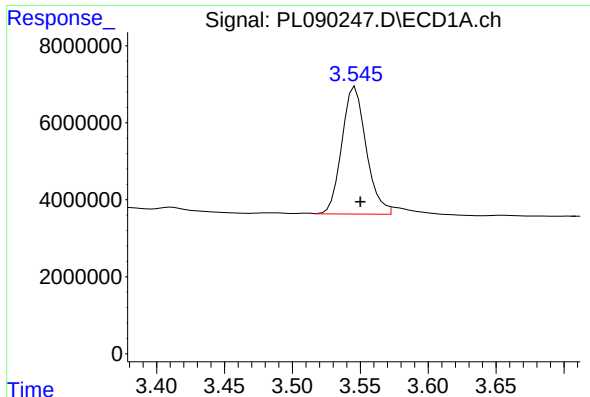


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.005 min
Response: 41585409
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-W-01-202406


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024

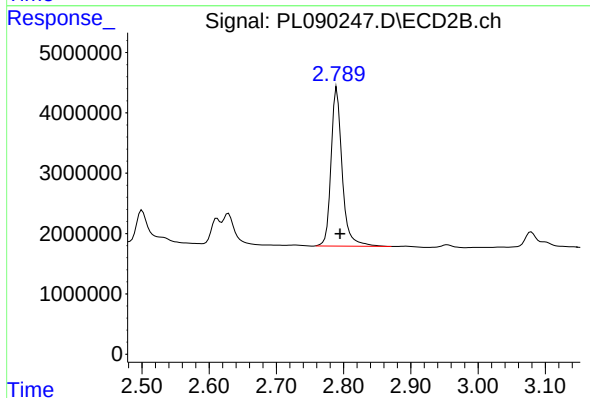


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: -0.005 min
Response: 29893241
Conc: 20.85 ng/ml

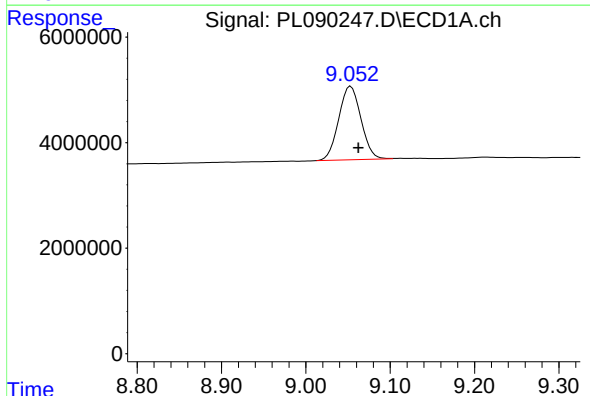

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.009 min
Response: 25566434
Conc: 17.39 ng/ml

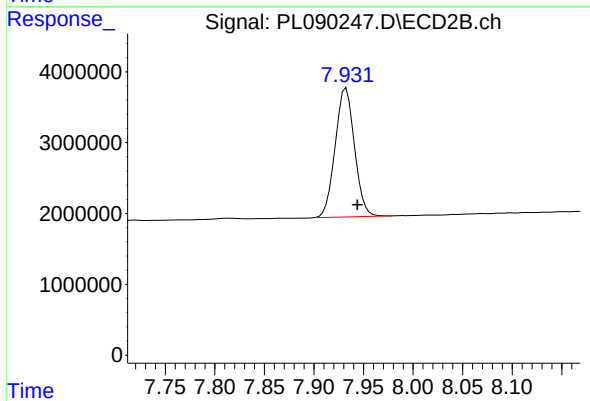

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.011 min
Response: 24604473
Conc: 16.56 ng/ml