

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
 Data File : PL096113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 09:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:57:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	5.718	0.000	40666880	0	8.957	N.D.	#
10) B	gamma-Chl...	5.973	0.000	8117536	0	1.743	N.D.	#
13) MA	Dieldrin	0.000	5.528f	0	24130588	N.D.	3.678	#
14) MA	Endrin	0.000	5.786	0	26102661	N.D.	4.398	#
15) B	Endosulfa...	0.000	6.075	0	7978173	N.D.	1.342	#
24)	Chlordane-2	0.000	4.475	0	18534143	N.D.	71.194	#
25)	Chlordane-3	5.973	0.000	8117536	0	9.727	N.D.	#
27)	Chlordane-5	6.910	6.075	35707499	7978173	200.356	26.109	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
Data File : PL096113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 09:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:57:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

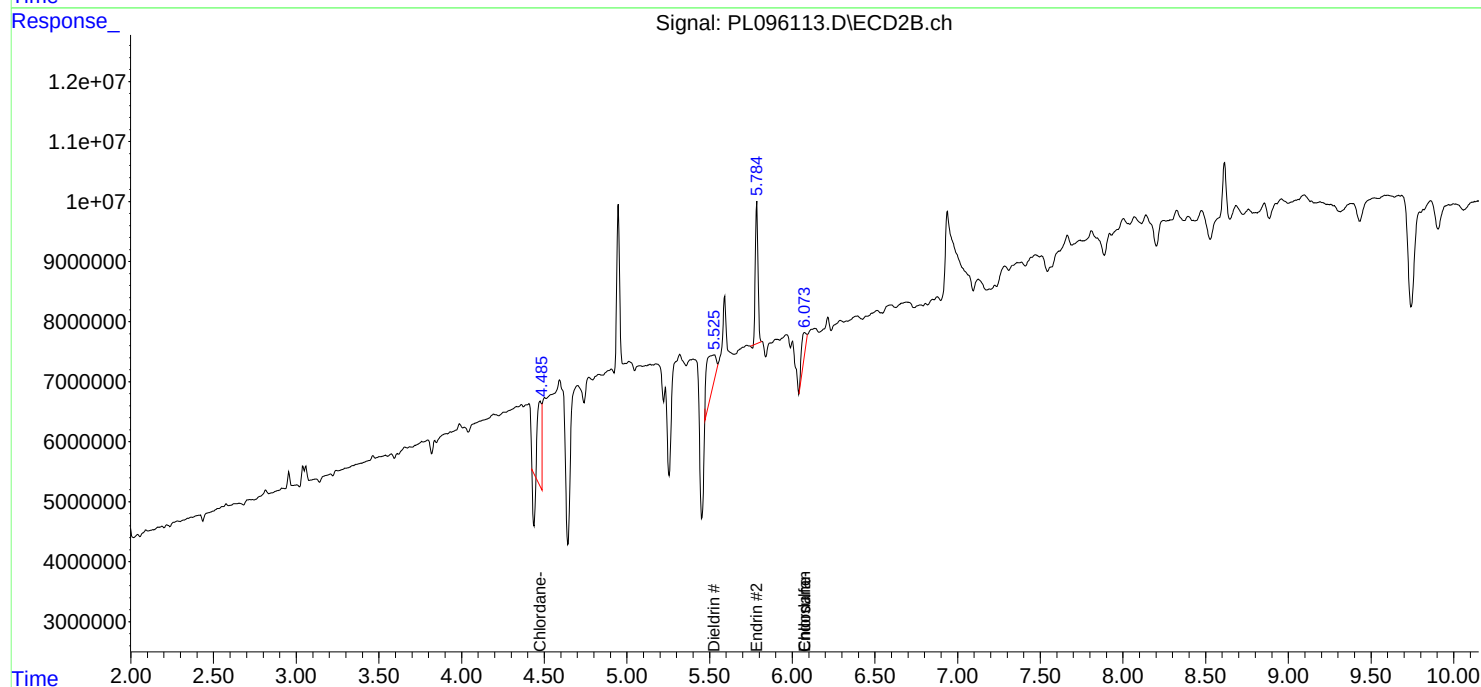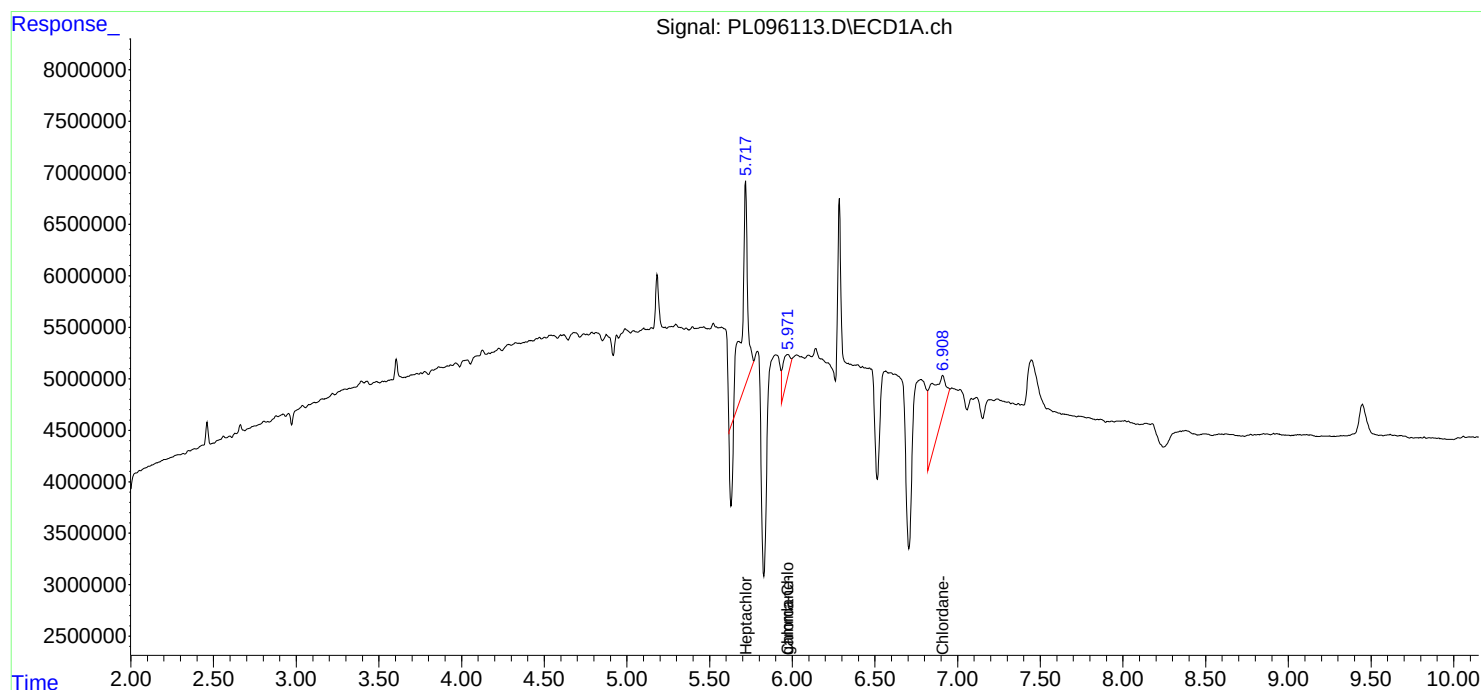


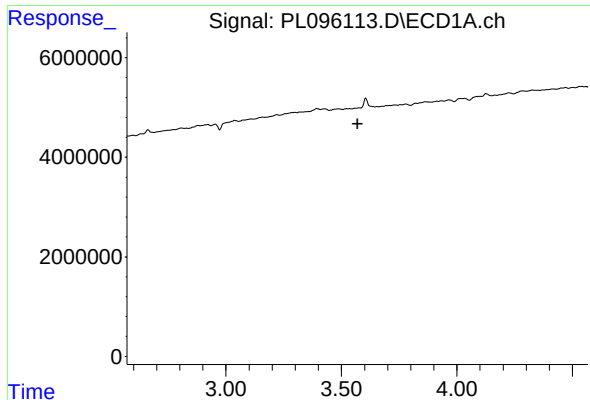

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.570 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

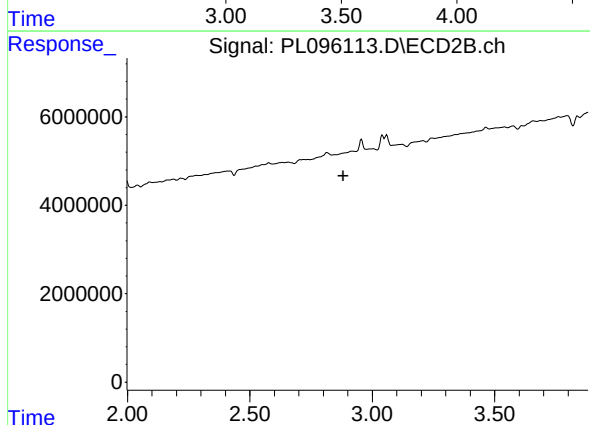


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.882 min
Response: 0
Conc: N.D.

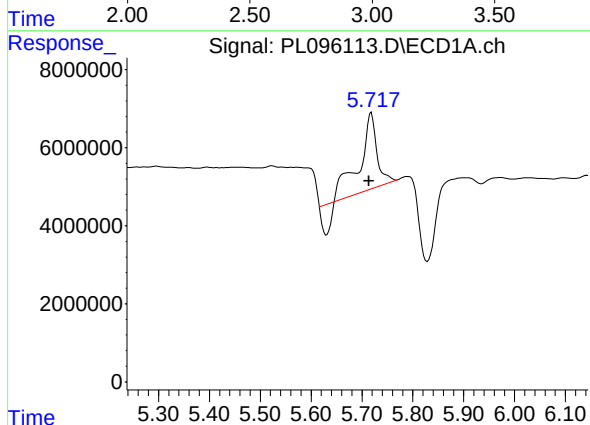


#8 Heptachlor epoxide

R.T.: 5.718 min
Delta R.T.: 0.004 min
Response: 40666880
Conc: 8.96 ng/ml

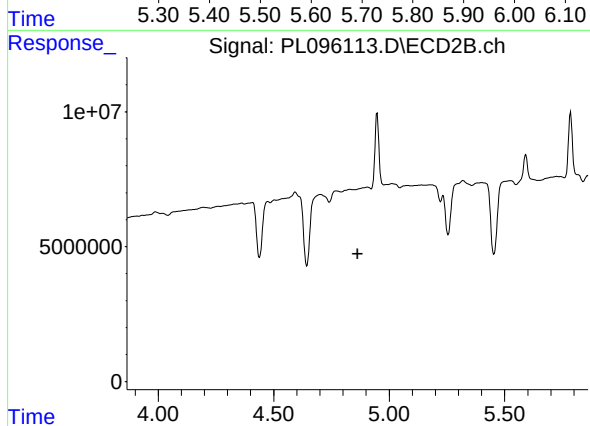

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.863 min
Response: 0
Conc: N.D.

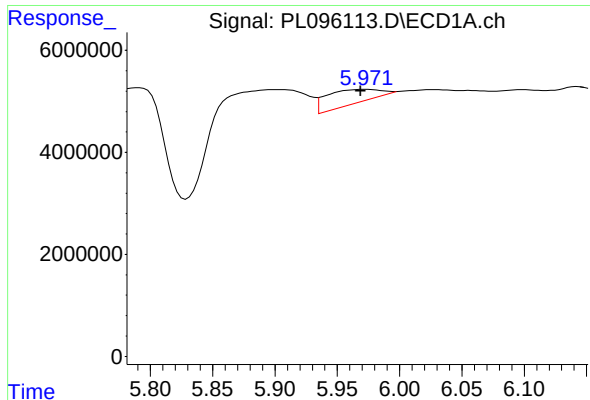

#10 gamma-Chlordane


R.T.: 5.973 min
Delta R.T.: 0.004 min
Response: 8117536
Conc: 1.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

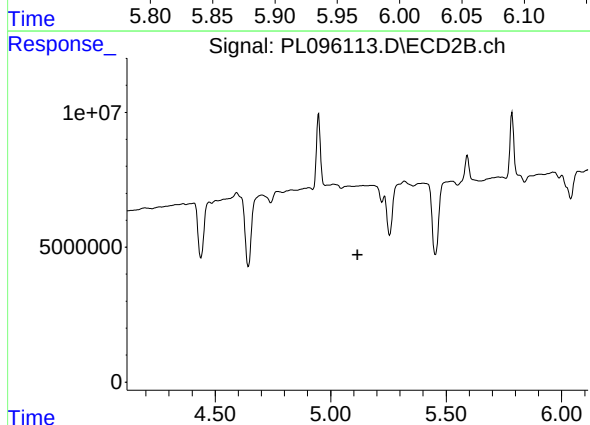


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

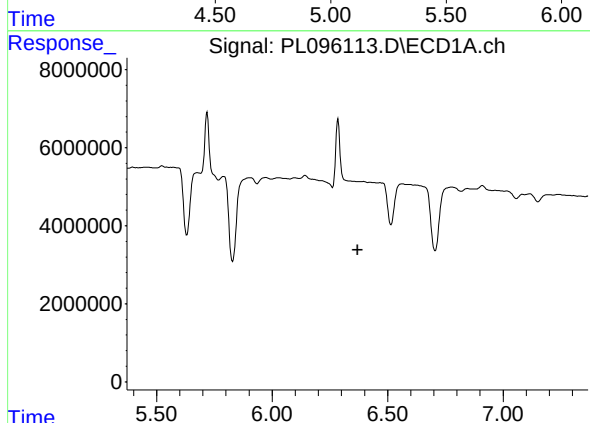


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

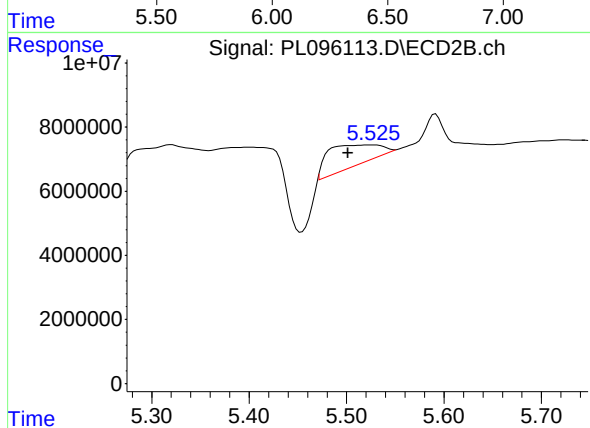

#13 Dieldrin


R.T.: 5.528 min
Delta R.T.: 0.026 min
Response: 24130588
Conc: 3.68 ng/ml

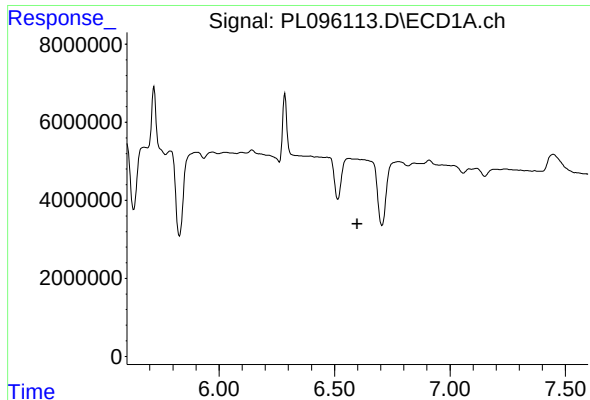

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.598 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

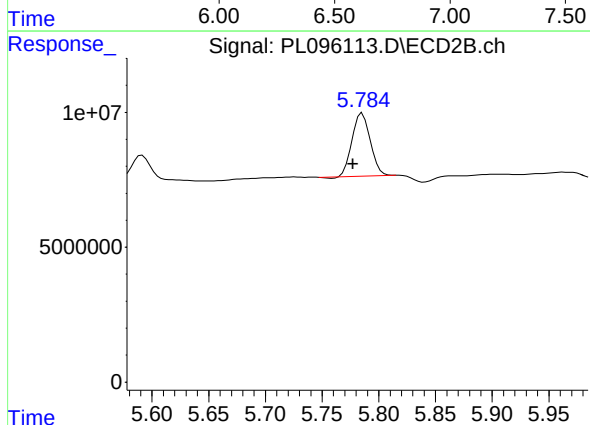


#14 Endrin

R.T.: 5.786 min
Delta R.T.: 0.008 min
Response: 26102661
Conc: 4.40 ng/ml

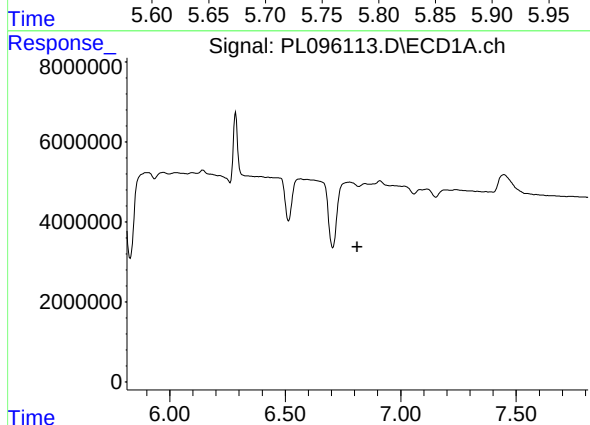


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.812 min
Response: 0
Conc: N.D.

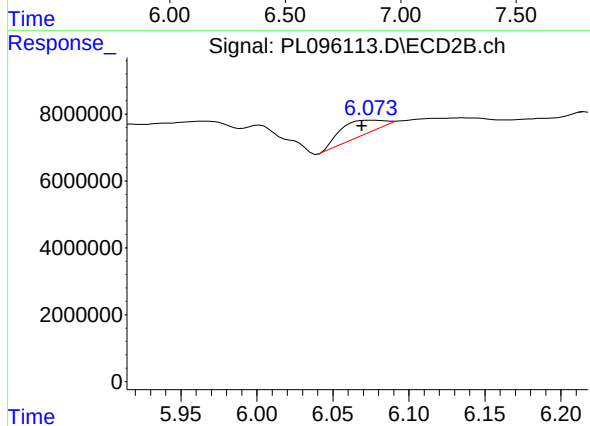

#15 Endosulfan II


R.T.: 6.075 min
Delta R.T.: 0.006 min
Response: 7978173
Conc: 1.34 ng/ml

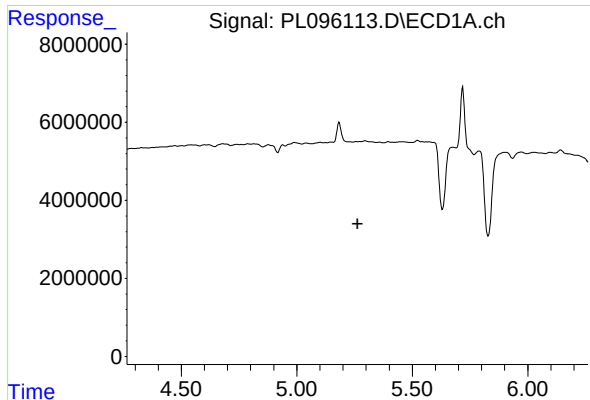

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

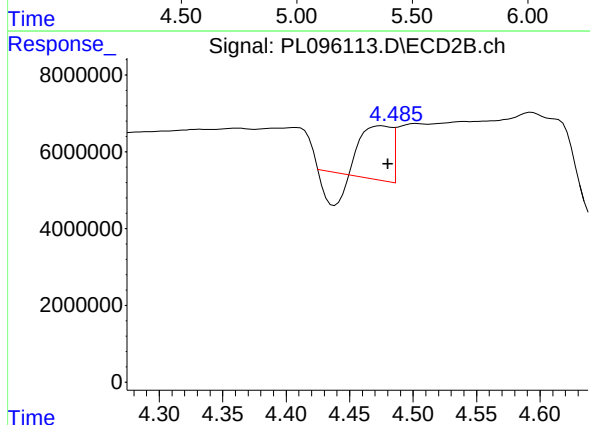


#24 Chlordane-2

R.T.: 4.475 min
Delta R.T.: -0.005 min
Response: 18534143
Conc: 71.19 ng/ml

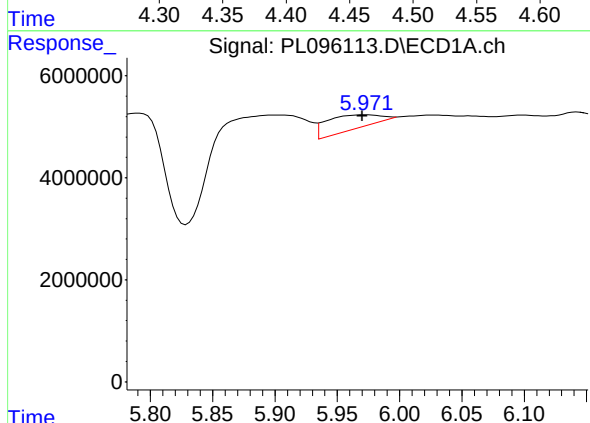


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.003 min
Response: 8117536
Conc: 9.73 ng/ml

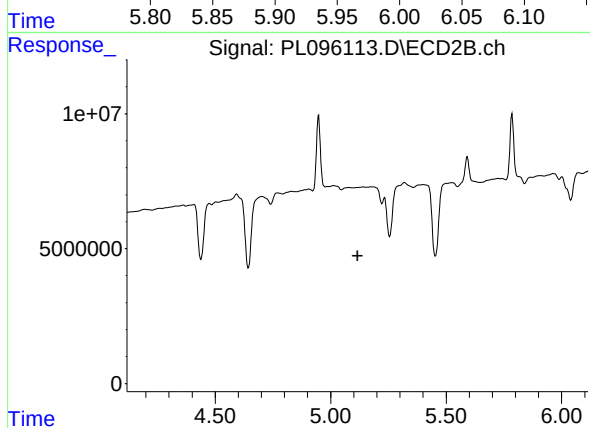

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

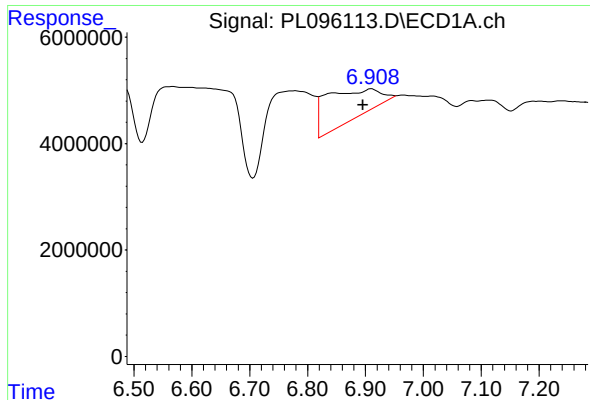

#27 Chlordane-5


R.T.: 6.910 min
Delta R.T.: 0.014 min
Response: 35707499
Conc: 200.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

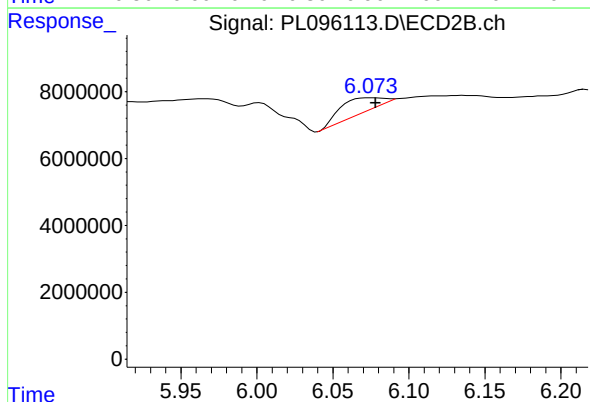


#27 Chlordane-5

R.T.: 6.075 min
Delta R.T.: -0.003 min
Response: 7978173
Conc: 26.11 ng/ml

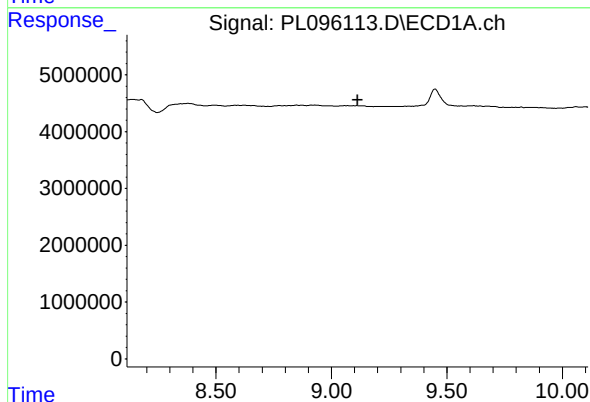

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.112 min
Response: 0
Conc: N.D.

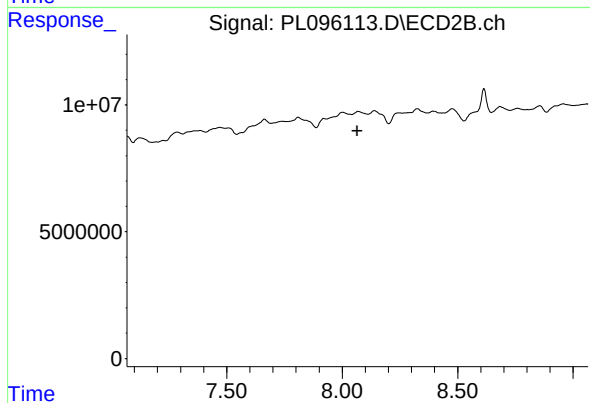

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.065 min
Response: 0
Conc: N.D.