

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
 Data File : PL096114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 10:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:58:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.572	2.881	74242329	89343234	20.402	18.837
28) SA Decachlor...	9.125	8.065	52343913	98734483	18.279	16.381
Target Compounds						
10) B gamma-Chl...	5.946f	0.000	2529316	0	0.543	N.D. #
25) Chlordane-3	5.946f	0.000	2529316	0	3.031	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
Data File : PL096114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 10:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:58:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

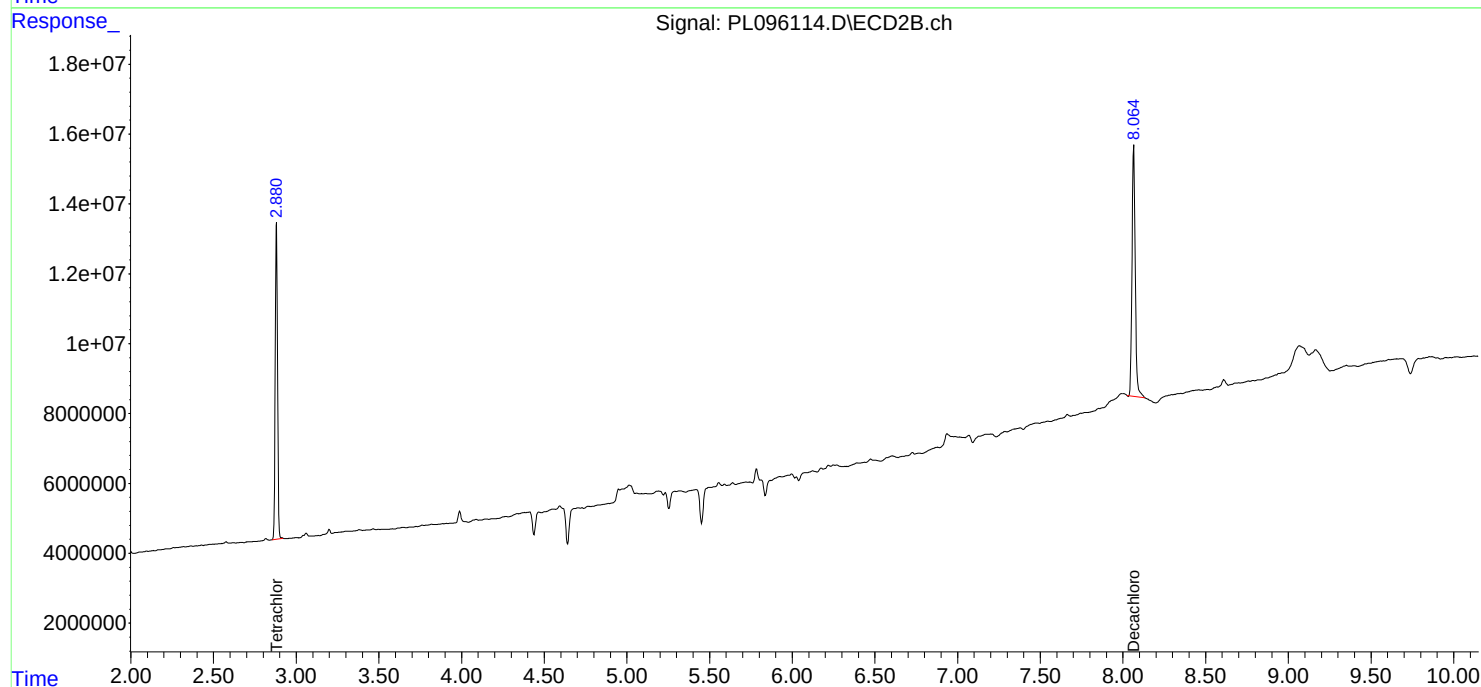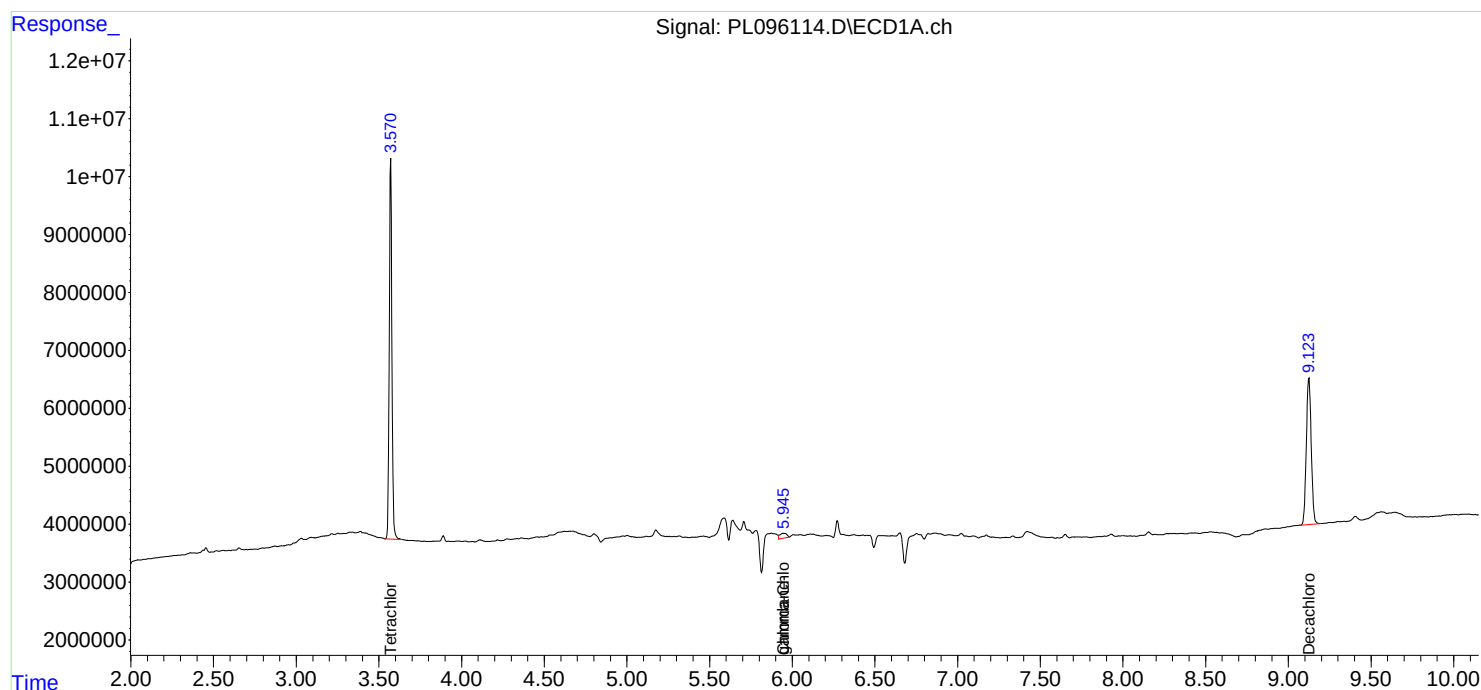


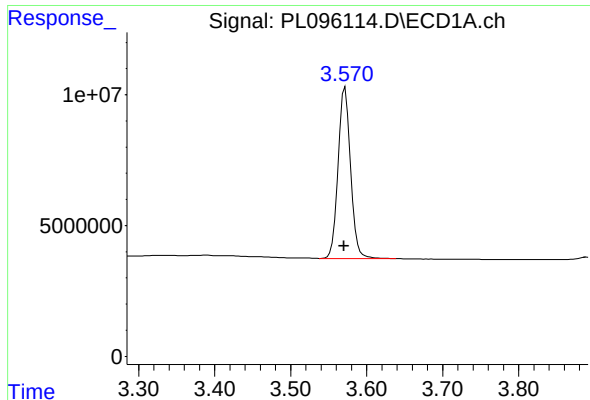

#1 Tetrachloro-m-xylene


R.T.: 3.572 min
Delta R.T.: 0.002 min
Response: 74242329
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

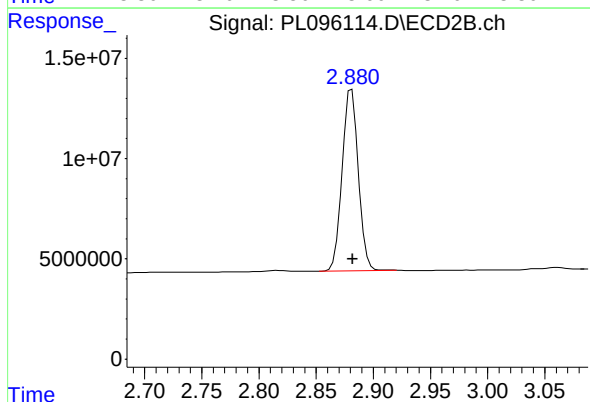


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 89343234
Conc: 18.84 ng/ml

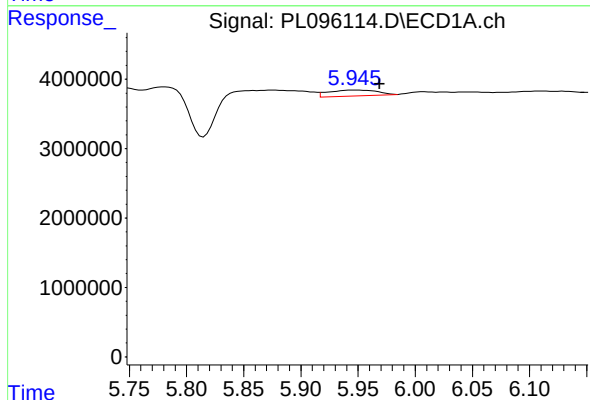


#10 gamma-Chlordane

R.T.: 5.946 min
Delta R.T.: -0.022 min
Response: 2529316
Conc: 0.54 ng/ml

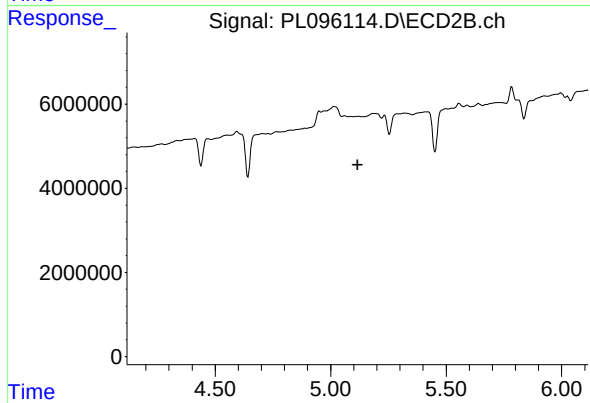

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

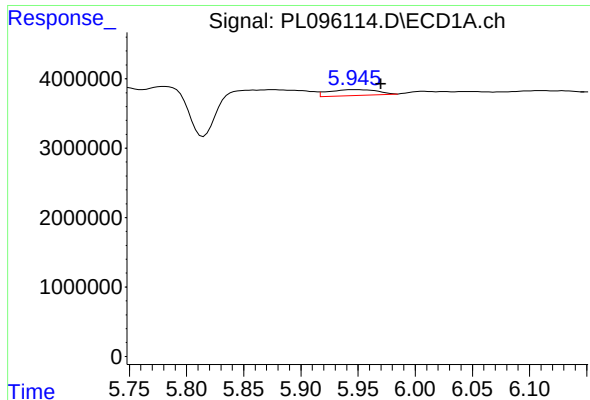

#25 Chlordane-3


R.T.: 5.946 min
Delta R.T.: -0.024 min
Response: 2529316
Conc: 3.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

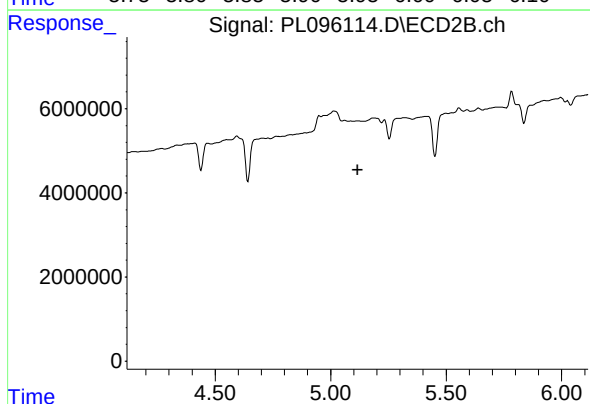


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

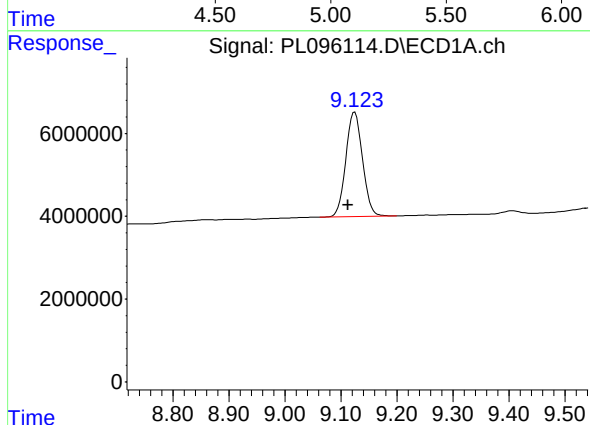

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.012 min
Response: 52343913
Conc: 18.28 ng/ml

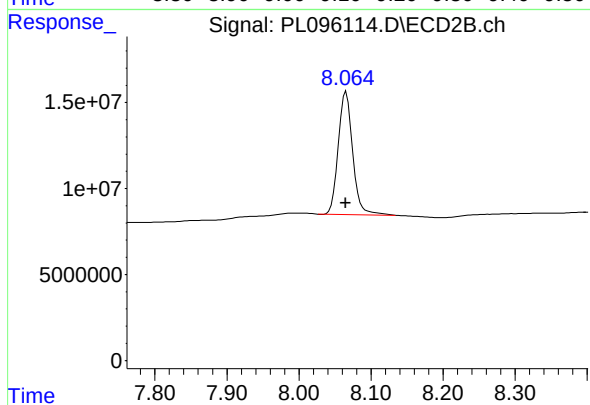

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: 0.000 min
Response: 98734483
Conc: 16.38 ng/ml