

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
 Data File : PL096117.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2025 10:53
 Operator : AR\AJ
 Sample : Q2338-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-061625

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:58:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 17 17:11:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.571	2.882	42713278	54668560	11.738	11.526
28)	SA Decachlor...	9.118	8.066	30963352	37873160	10.813	6.283 #
Target Compounds							
5)	MB Aldrin	5.264f	4.354	19332692	11827254	3.792	1.798 #
9)	A Endosulfan I	0.000	5.249	0	5846916	N.D.	0.912 #
10)	B gamma-Chl...	5.968	0.000	7084494	0	1.521	N.D. #
16)	A 4,4'-DDD	0.000	5.908	0	10207647	N.D.	1.856 #
23)	Chlordane-1	0.000	3.893	0	10483669	N.D.	45.451 #
24)	Chlordane-2	5.264	4.508f	19332692	3592537	89.077	13.800 #
25)	Chlordane-3	5.968	0.000	7084494	0	8.489	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL061925\
Data File : PL096117.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2025 10:53
Operator : AR\AJ
Sample : Q2338-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:58:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061725.M
Quant Title : GC Extractables
QLast Update : Tue Jun 17 17:11:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

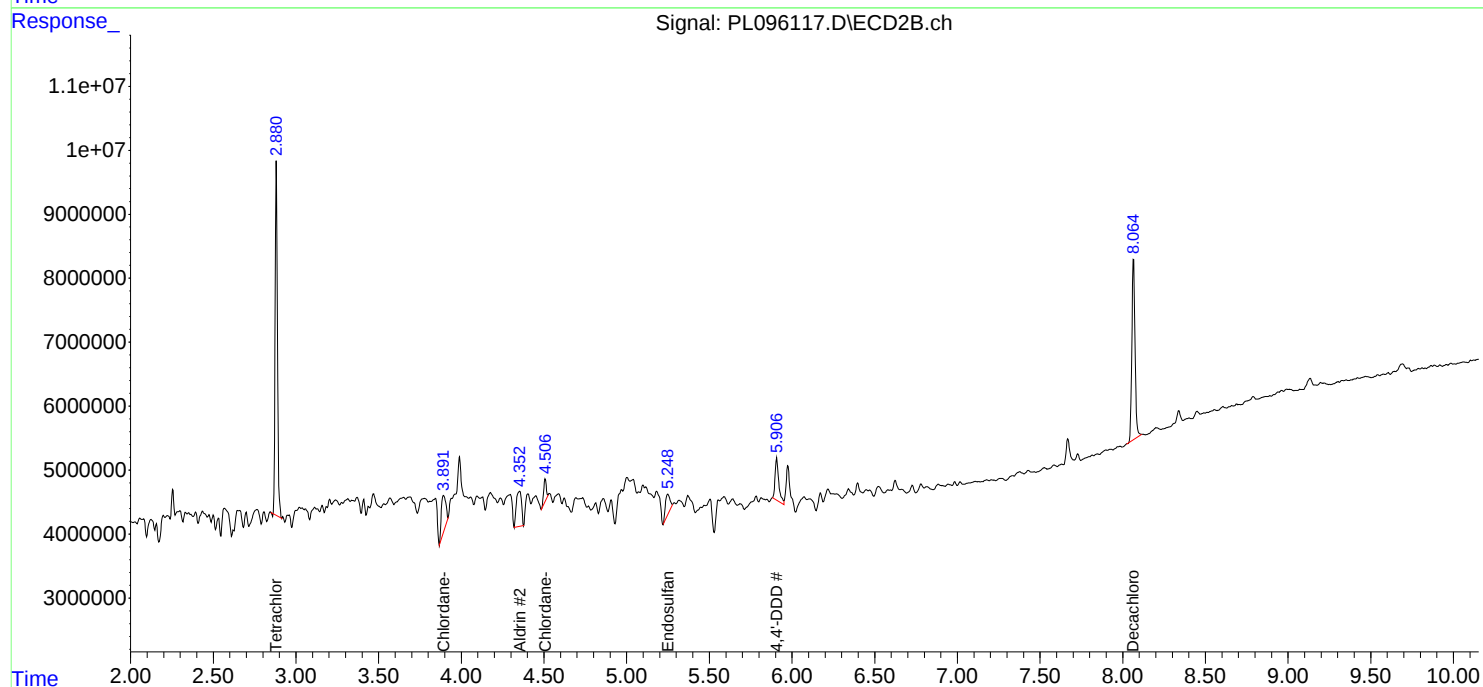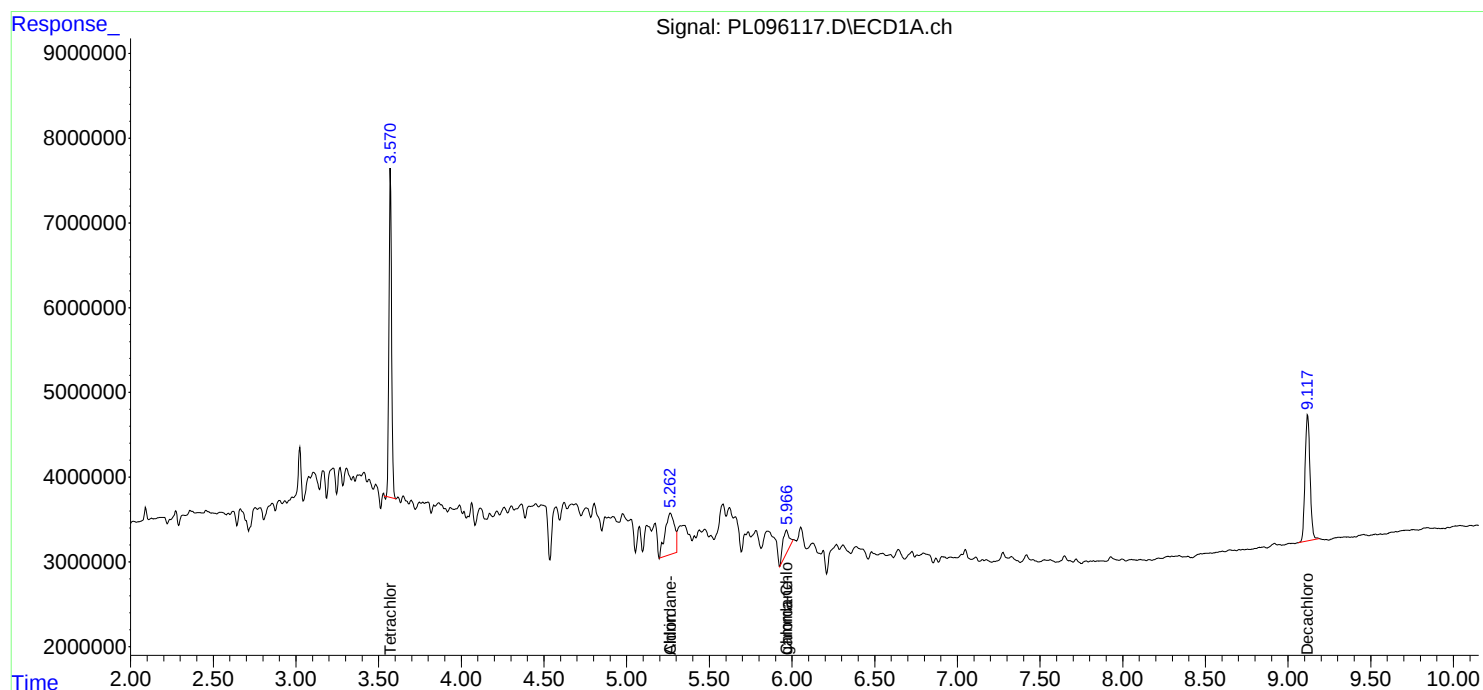


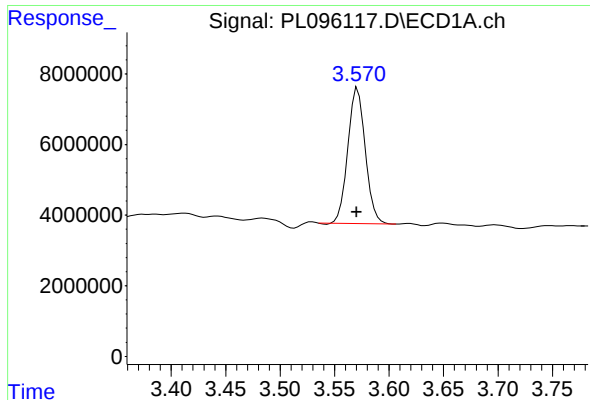

#1 Tetrachloro-m-xylene


R.T.: 3.571 min
Delta R.T.: 0.001 min
Response: 42713278
Conc: 11.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

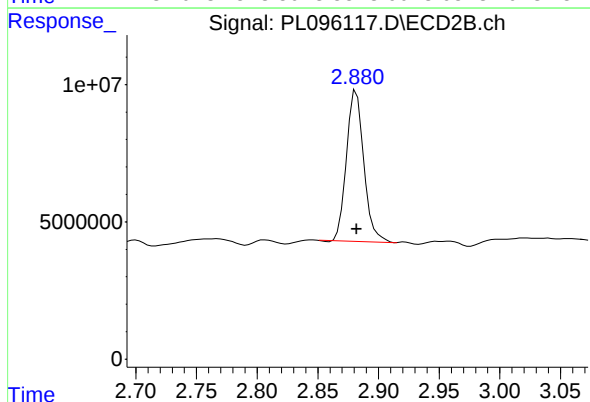


#1 Tetrachloro-m-xylene

R.T.: 2.882 min
Delta R.T.: 0.000 min
Response: 54668560
Conc: 11.53 ng/ml

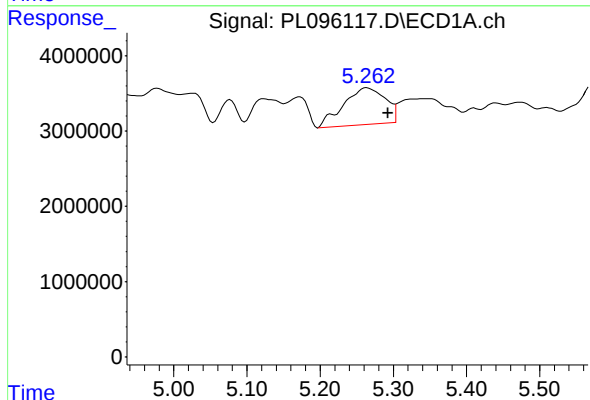


#5 Aldrin

R.T.: 5.264 min
Delta R.T.: -0.029 min
Response: 19332692
Conc: 3.79 ng/ml

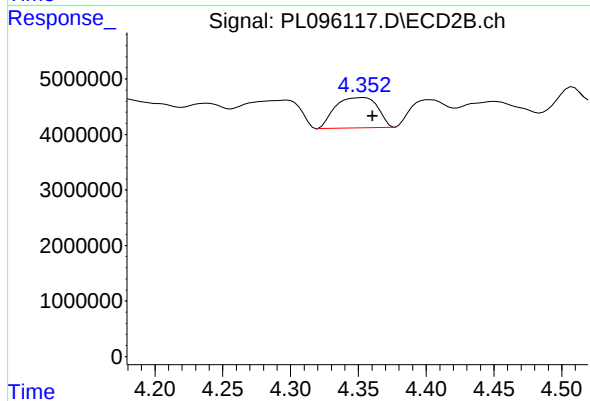

#5 Aldrin


R.T.: 4.354 min
Delta R.T.: -0.007 min
Response: 11827254
Conc: 1.80 ng/ml

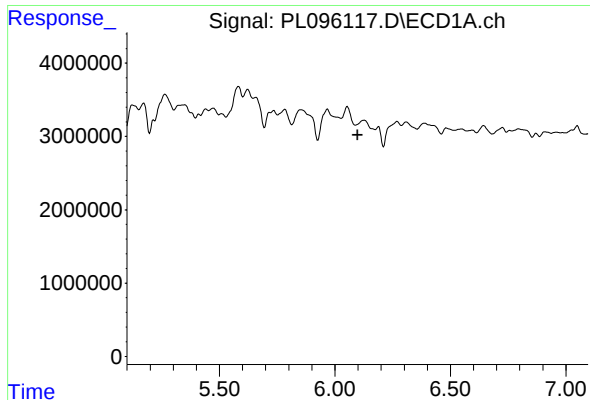

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

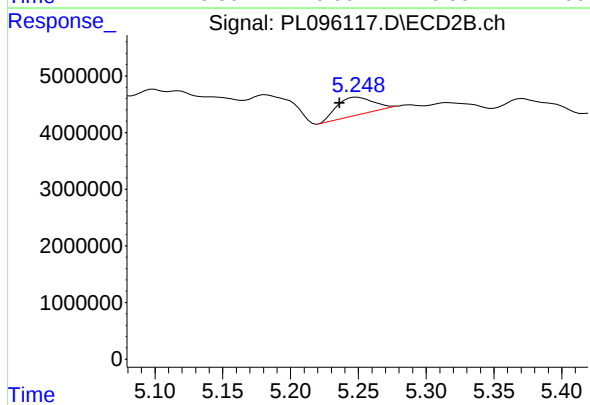


#9 Endosulfan I

R.T.: 5.249 min
Delta R.T.: 0.013 min
Response: 5846916
Conc: 0.91 ng/ml

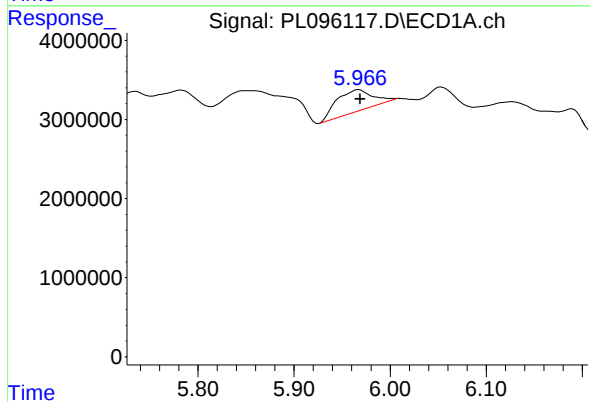


#10 gamma-Chlordane

R.T.: 5.968 min
Delta R.T.: -0.001 min
Response: 7084494
Conc: 1.52 ng/ml

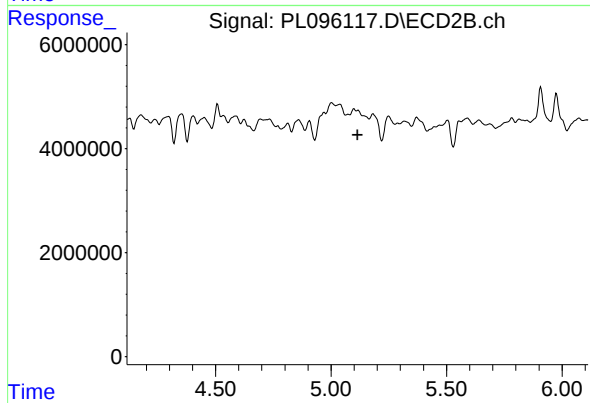

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

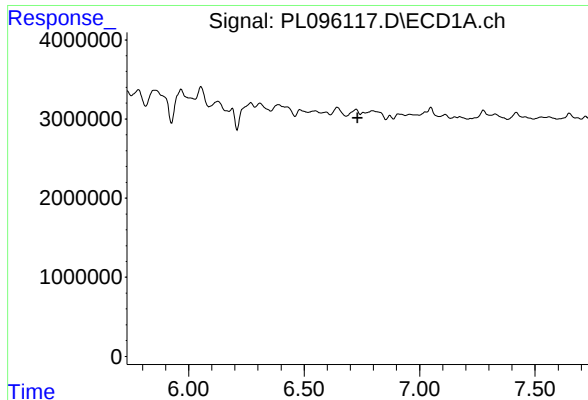

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

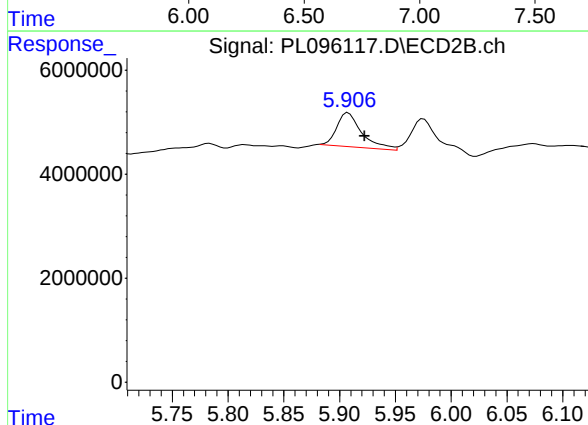


#16 4,4'-DDD

R.T.: 5.908 min
Delta R.T.: -0.015 min
Response: 10207647
Conc: 1.86 ng/ml

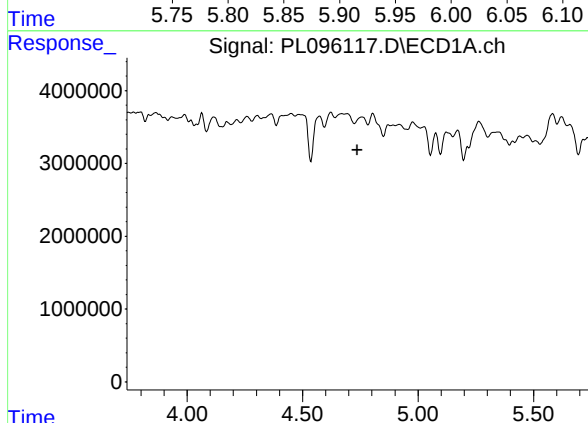


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.737 min
Response: 0
Conc: N.D.

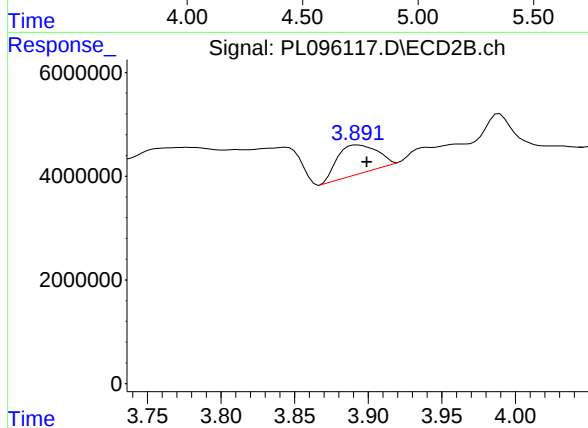

#23 Chlordane-1


R.T.: 3.893 min
Delta R.T.: -0.006 min
Response: 10483669
Conc: 45.45 ng/ml

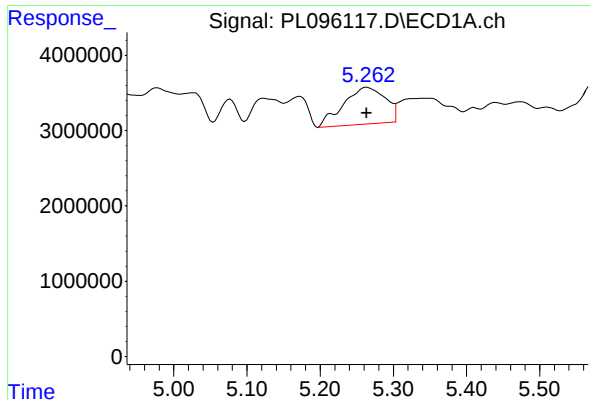

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 19332692
Conc: 89.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

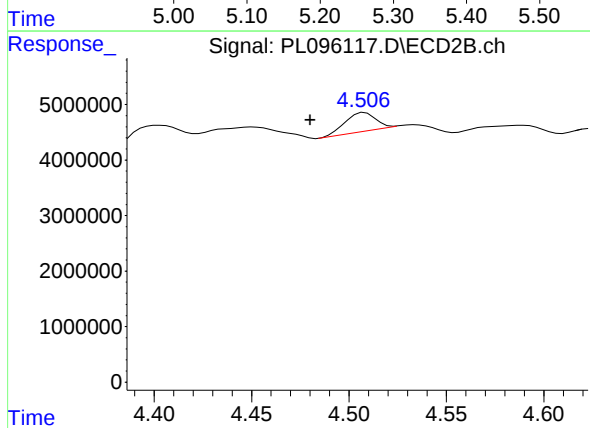


#24 Chlordane-2

R.T.: 4.508 min
Delta R.T.: 0.028 min
Response: 3592537
Conc: 13.80 ng/ml

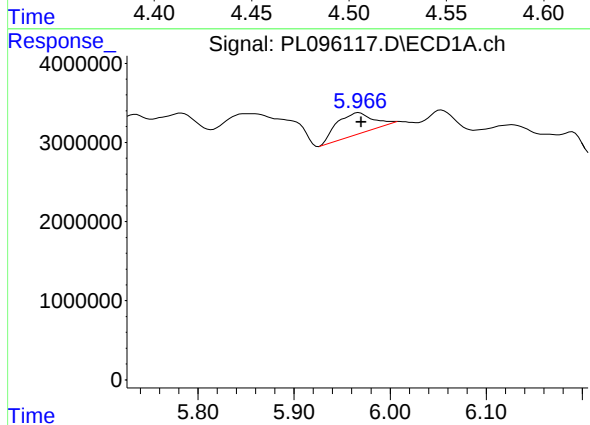


#25 Chlordane-3

R.T.: 5.968 min
Delta R.T.: -0.002 min
Response: 7084494
Conc: 8.49 ng/ml

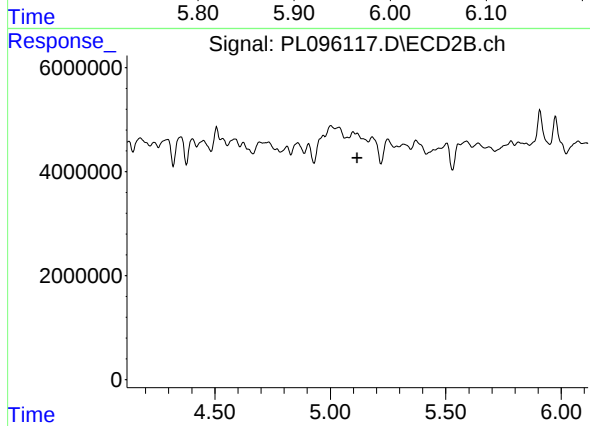

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

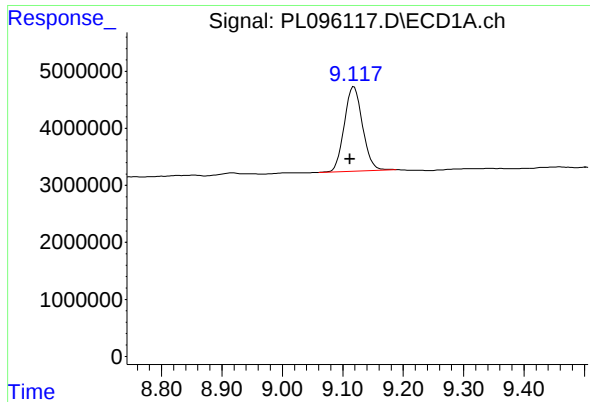

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.006 min
Response: 30963352
Conc: 10.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-061625

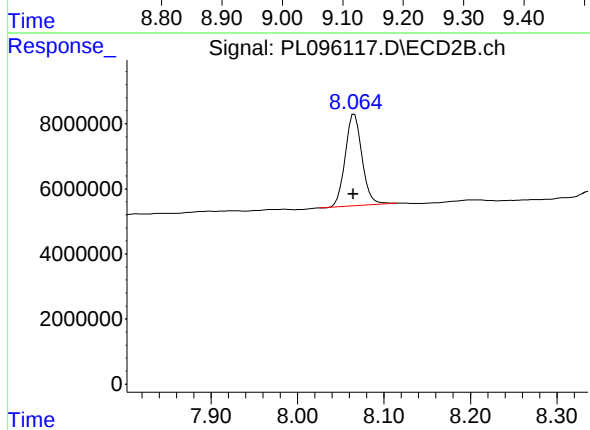

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.001 min
Response: 37873160
Conc: 6.28 ng/ml