

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062019\
 Data File : PL049682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 14:56
 Operator : SM\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:27:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	136.1E6	36741009	12.066	12.000
28)	SA Decachlor...	7.991	8.973	164.5E6	45286308	12.946	13.490
Target Compounds							
7)	B delta-BHC	0.000	4.972f	0	14723338	N.D.	3.738 #
9)	A Endosulfan I	5.318	6.155	89562758	20490237	5.789	6.031
10)	B gamma-Chl...	5.209	6.034	98106473	21835970	5.741	5.860
12)	B 4,4'-DDE	5.433	6.266	188.4E6	40745215	11.310	11.742
13)	MA Dieldrin	5.556	6.412	196.9E6	42124775	11.819	11.874
19)	B Endosulfa...	6.464	7.188	151.9E6	37090257	11.718	12.324
20)	A Methoxychlor	6.725	7.515	397.2E6	100.4E6	60.941	60.224
21)	B Endrin ke...	6.946	7.657	142.8E6	33452458	10.162	10.735
25)	Chlordane-3	5.209	6.034	98106473	21835970	52.234	43.880



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062019\
Data File : PL049682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 14:56
Operator : SM\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:27:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

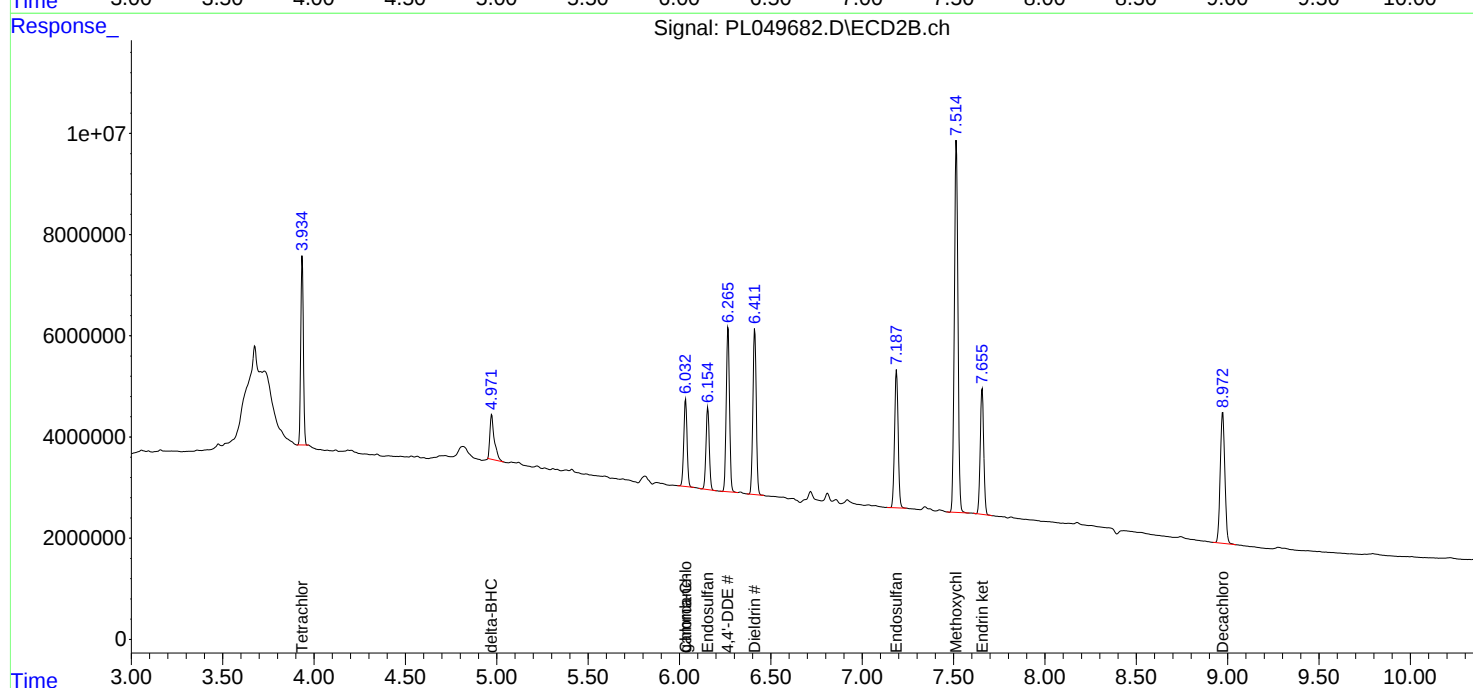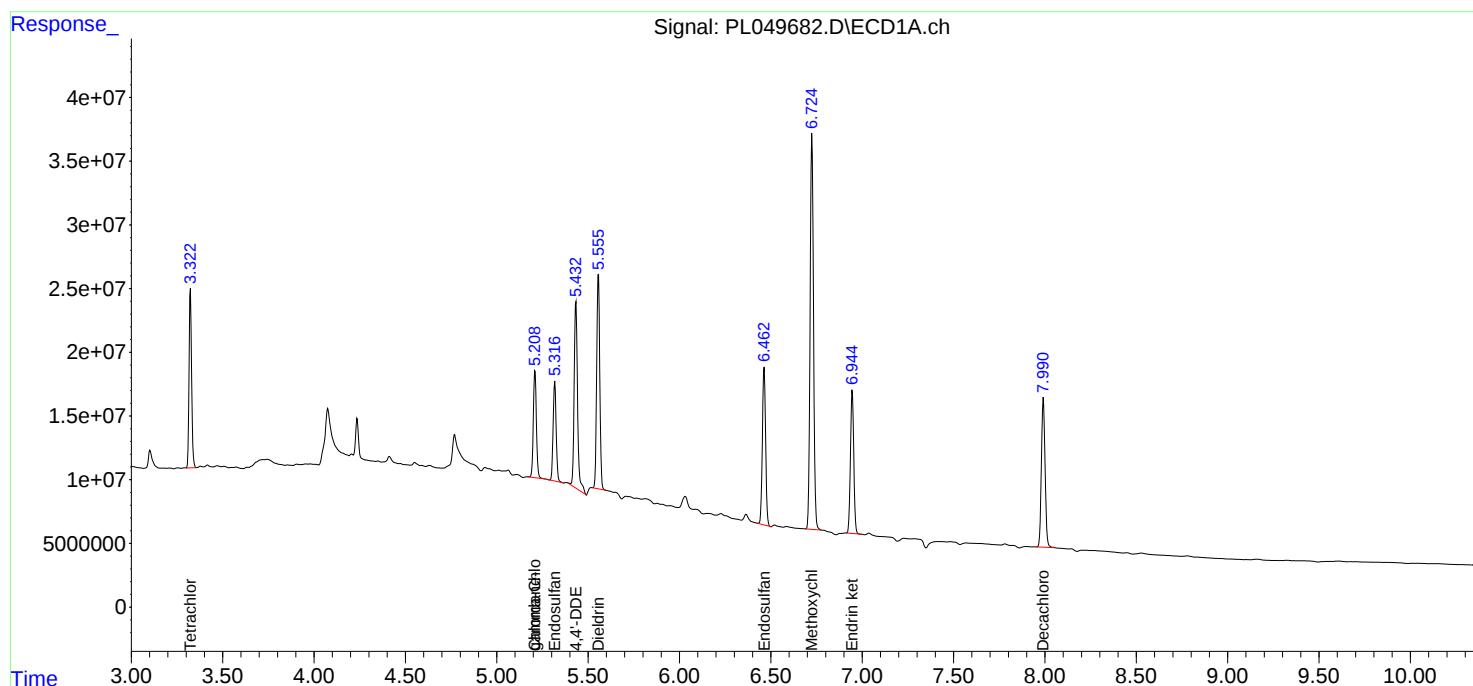


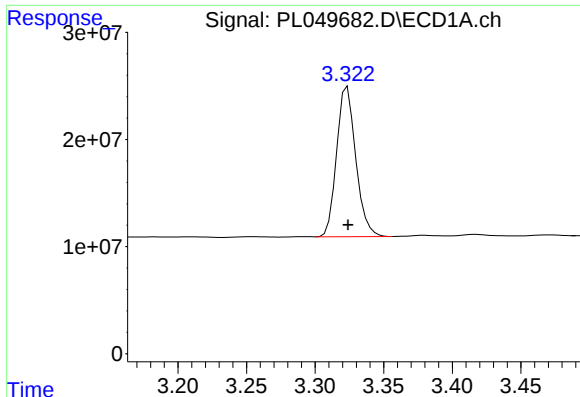

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 136077335
Conc: 12.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

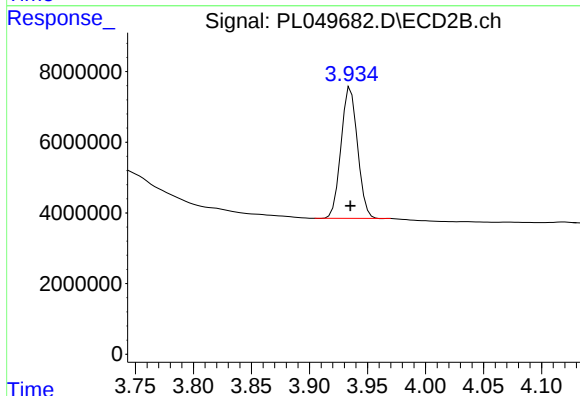


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 36741009
Conc: 12.00 ng/ml

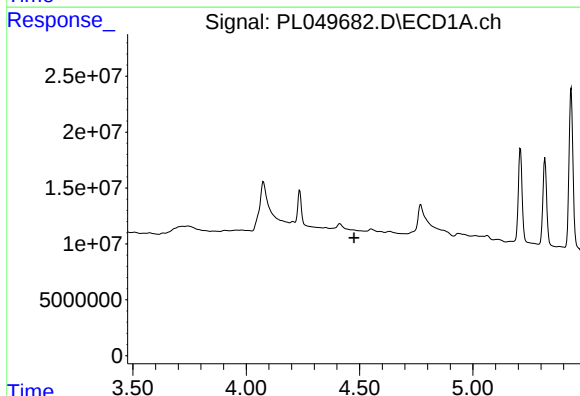


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.476 min
Response: 0
Conc: N.D.

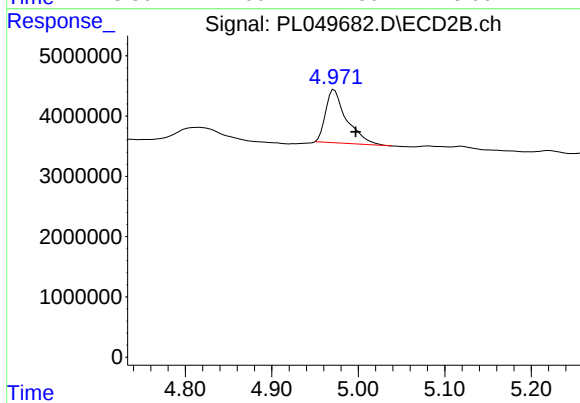

#7 delta-BHC


R.T.: 4.972 min
Delta R.T.: -0.025 min
Response: 14723338
Conc: 3.74 ng/ml

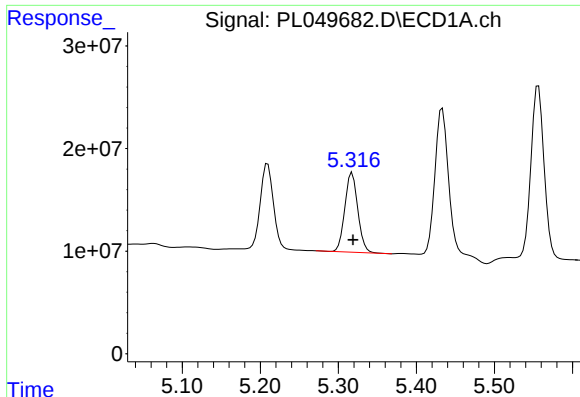

#9 Endosulfan I


R.T.: 5.318 min
Delta R.T.: 0.000 min
Response: 89562758
Conc: 5.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

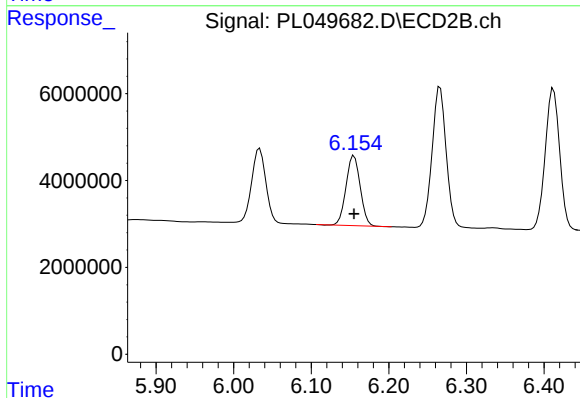


#9 Endosulfan I

R.T.: 6.155 min
Delta R.T.: 0.000 min
Response: 20490237
Conc: 6.03 ng/ml

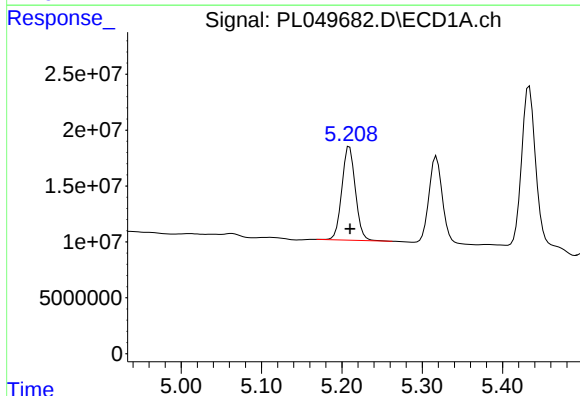


#10 gamma-Chlordane

R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 98106473
Conc: 5.74 ng/ml

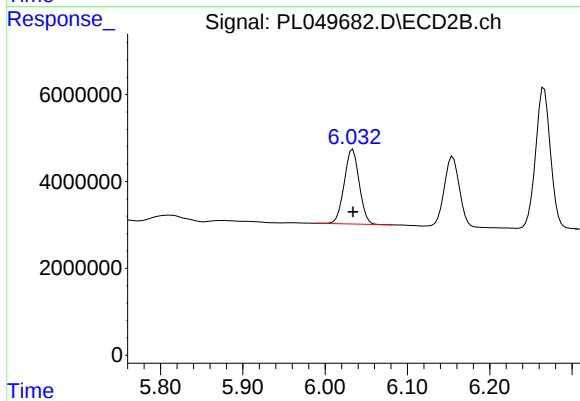

#10 gamma-Chlordane


R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 21835970
Conc: 5.86 ng/ml

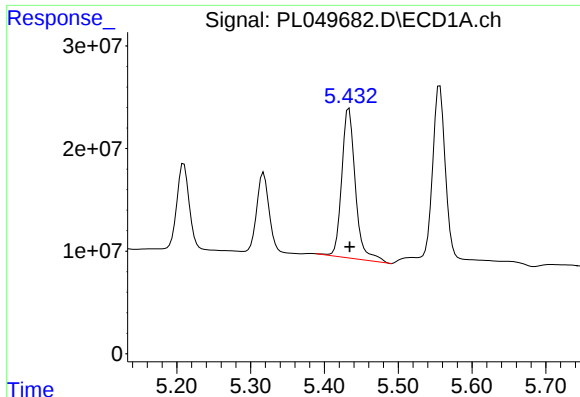

#12 4,4'-DDE


R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 188407079
Conc: 11.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

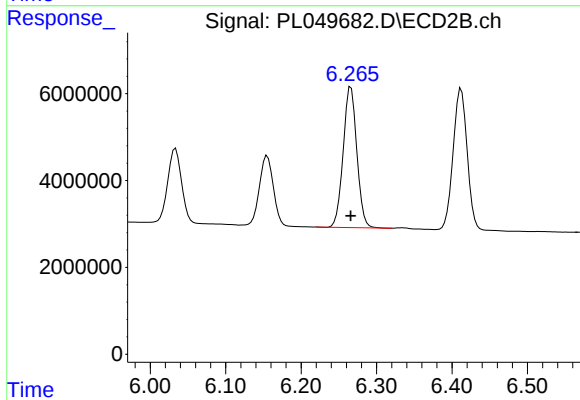


#12 4,4'-DDE

R.T.: 6.266 min
Delta R.T.: 0.000 min
Response: 40745215
Conc: 11.74 ng/ml

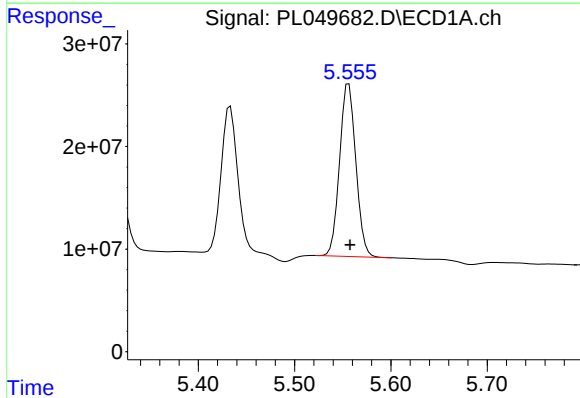


#13 Dieldrin

R.T.: 5.556 min
Delta R.T.: -0.001 min
Response: 196872820
Conc: 11.82 ng/ml

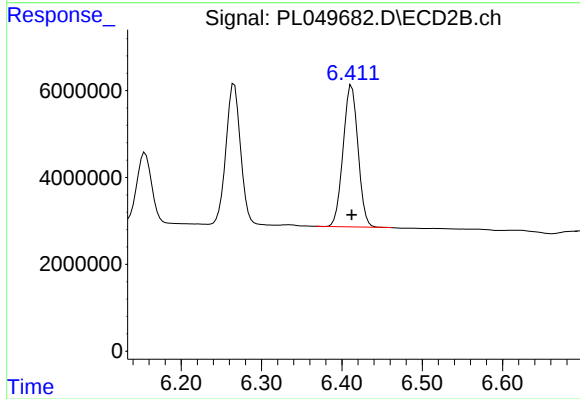

#13 Dieldrin


R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 42124775
Conc: 11.87 ng/ml

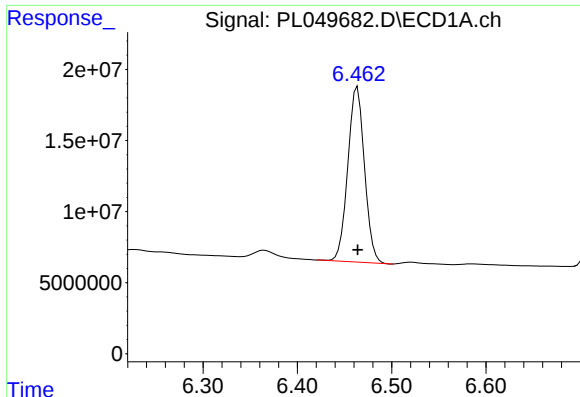

#19 Endosulfan Sulfate


R.T.: 6.464 min
Delta R.T.: 0.000 min
Response: 151934079
Conc: 11.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

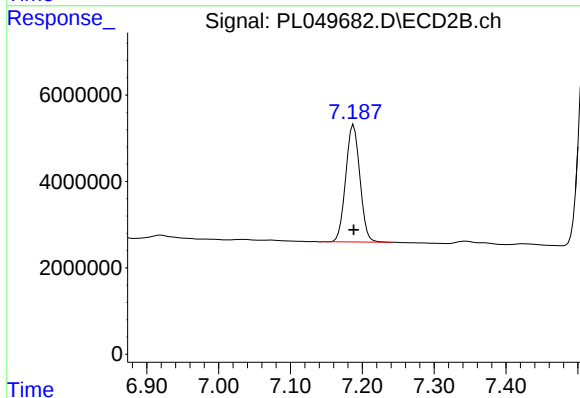


#19 Endosulfan Sulfate

R.T.: 7.188 min
Delta R.T.: 0.000 min
Response: 37090257
Conc: 12.32 ng/ml

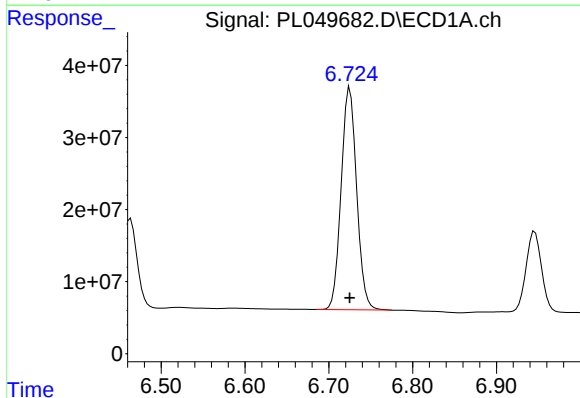


#20 Methoxychlor

R.T.: 6.725 min
Delta R.T.: 0.000 min
Response: 397229173
Conc: 60.94 ng/ml

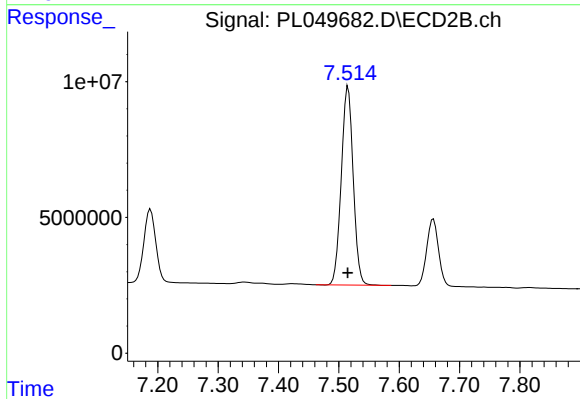

#20 Methoxychlor


R.T.: 7.515 min
Delta R.T.: 0.000 min
Response: 100380702
Conc: 60.22 ng/ml

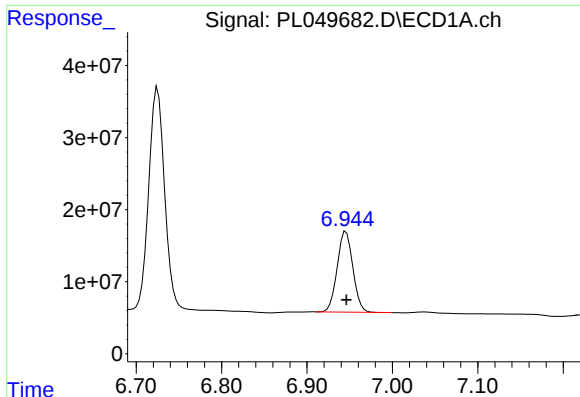

#21 Endrin ketone


R.T.: 6.946 min
Delta R.T.: 0.000 min
Response: 142834510
Conc: 10.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

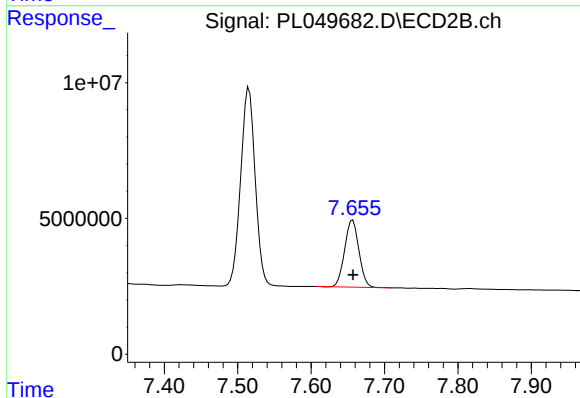


#21 Endrin ketone

R.T.: 7.657 min
Delta R.T.: 0.000 min
Response: 33452458
Conc: 10.74 ng/ml

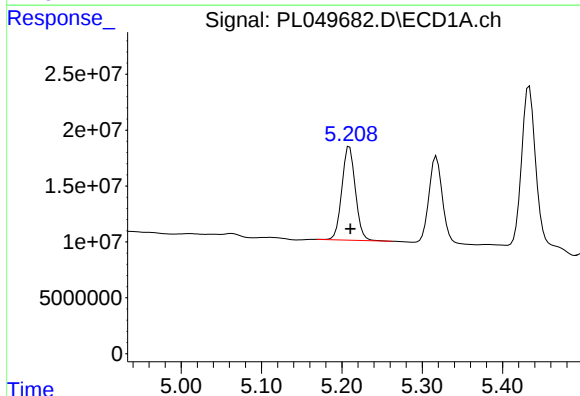


#25 Chlordane-3

R.T.: 5.209 min
Delta R.T.: -0.001 min
Response: 98106473
Conc: 52.23 ng/ml

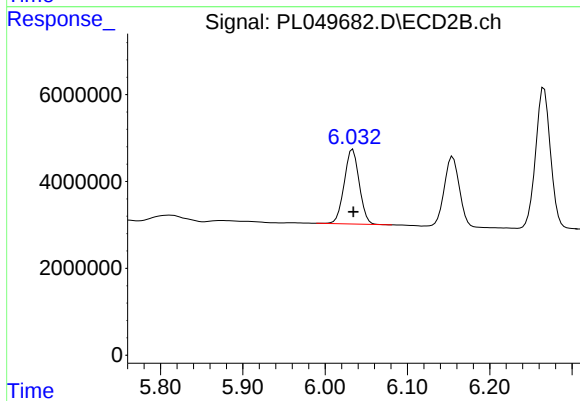

#25 Chlordane-3

R.T.: 6.034 min
Delta R.T.: -0.001 min
Response: 21835970
Conc: 43.88 ng/ml

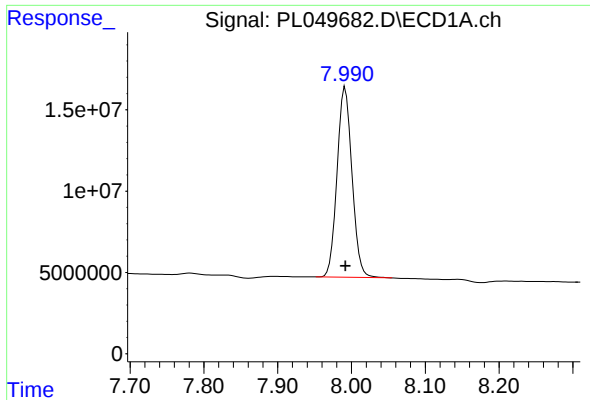

#28 Decachlorobiphenyl


R.T.: 7.991 min

Delta R.T.: 0.000 min

Response: 164499099

Conc: 12.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

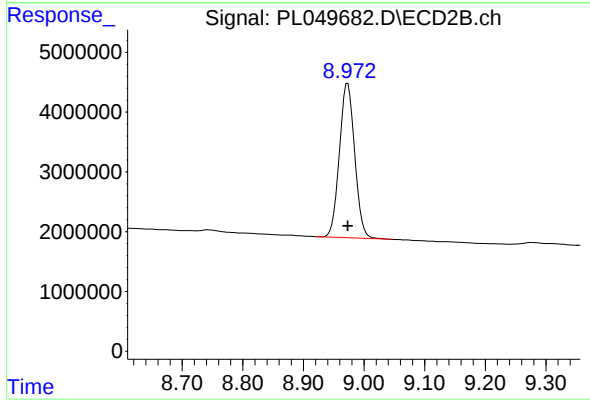

#28 Decachlorobiphenyl

R.T.: 8.973 min

Delta R.T.: 0.000 min

Response: 45286308

Conc: 13.49 ng/ml