

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062019\
 Data File : PL049694.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2019 17:57
 Operator : SM\AJ
 Sample : K3428-06RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-013-SW160-061319

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:48:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.935	159.4E6	41745696	14.133	13.635
28)	SA Decachlor...	7.991	8.974	158.6E6	42205837	12.482	12.572
Target Compounds							
6)	B beta-BHC	0.000	4.810f	0	10187383	N.D.	5.259 #
10)	B gamma-Chl...	5.230f	6.034	113.6E6	8003136	6.649	2.148 #
11)	B alpha-Chl...	5.266	6.108	50944570	27719417	3.069	7.495 #
12)	B 4,4'-DDE	5.434	6.264	64635381	10204205	3.880	2.941
17)	MA 4,4'-DDT	6.178	7.054	50112649	13677280	3.775	4.670
25)	Chlordane-3	5.230f	6.034	113.6E6	8003136	60.498	16.083 #
26)	Chlordane-4	5.266	6.108	50944570	27719417	29.192	46.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062019\
Data File : PL049694.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2019 17:57
Operator : SM\AJ
Sample : K3428-06RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:48:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

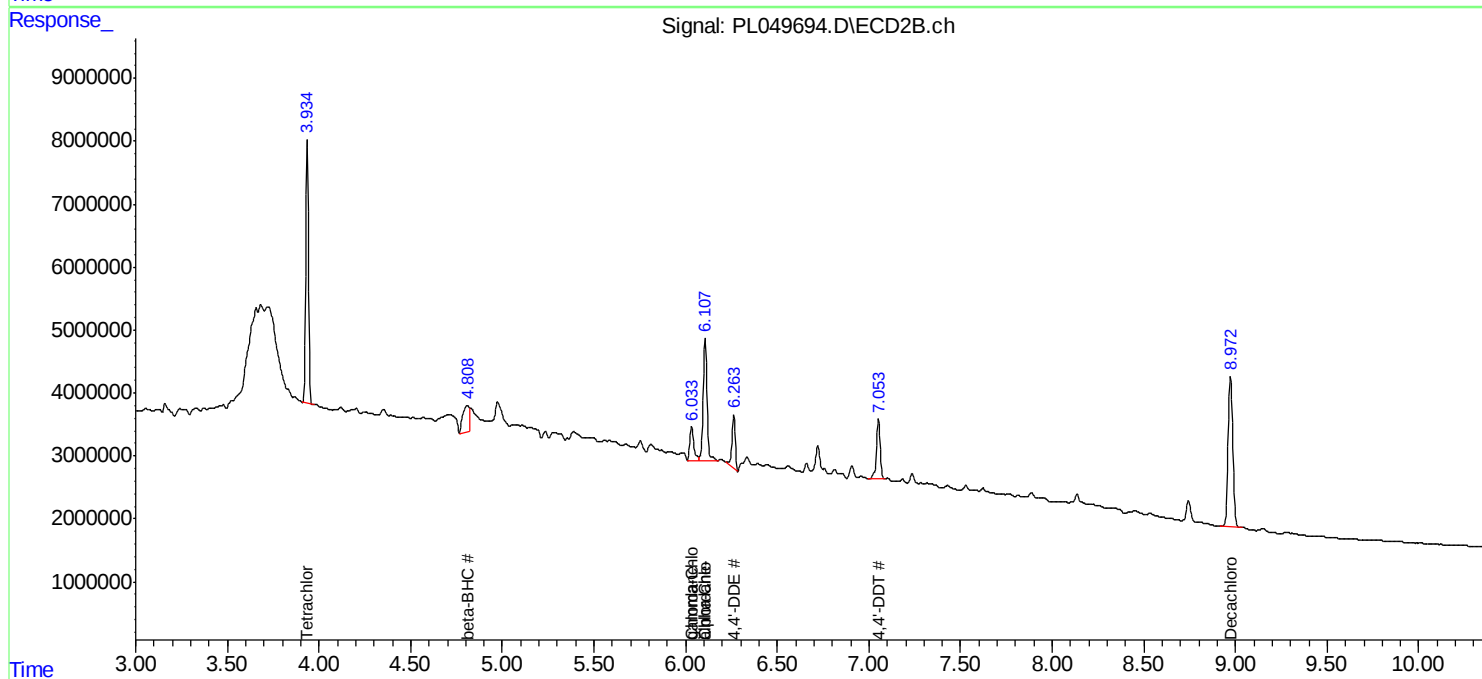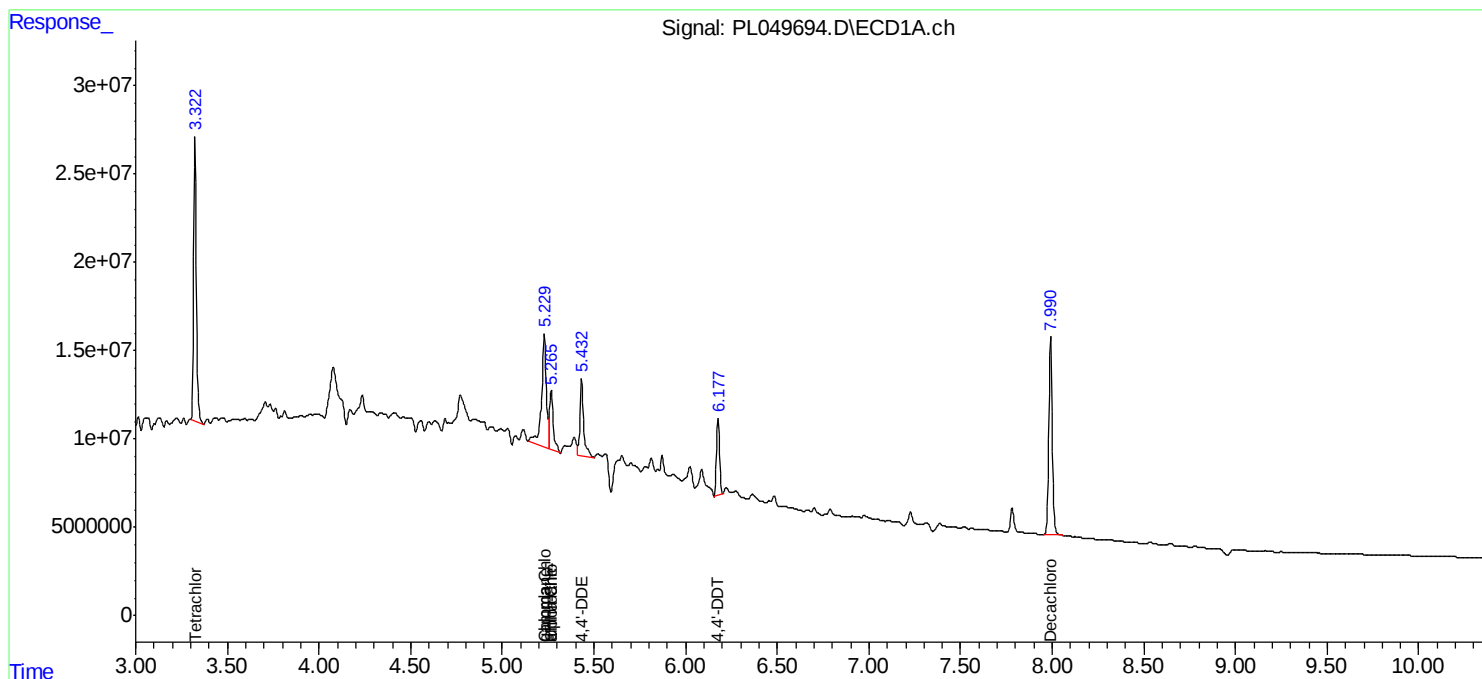


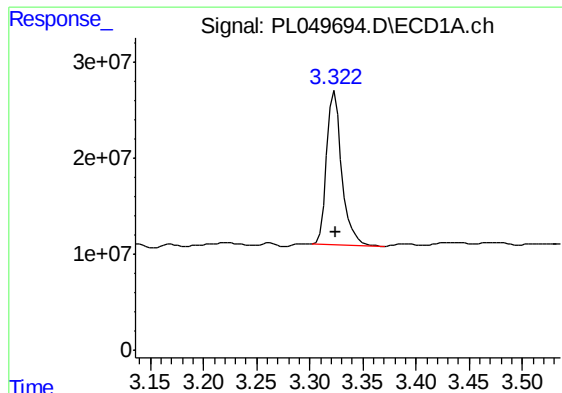

#1 Tetrachloro-m-xylene


R.T.: 3.324 min
Delta R.T.: 0.000 min
Response: 159388782
Conc: 14.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

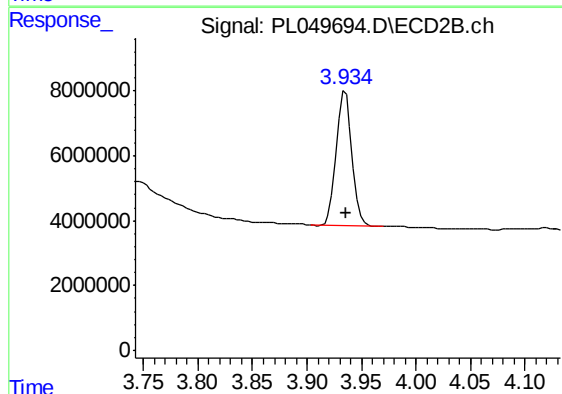


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 41745696
Conc: 13.63 ng/ml

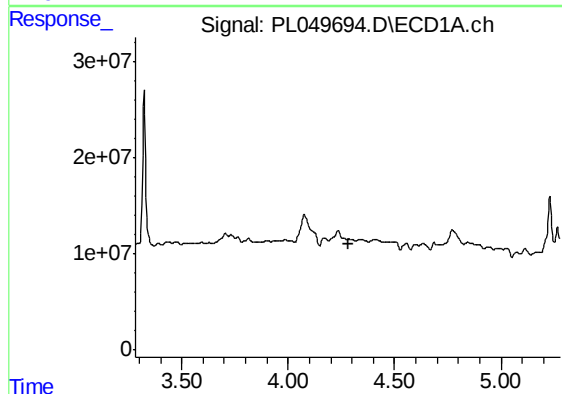


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.282 min
Response: 0
Conc: N.D.

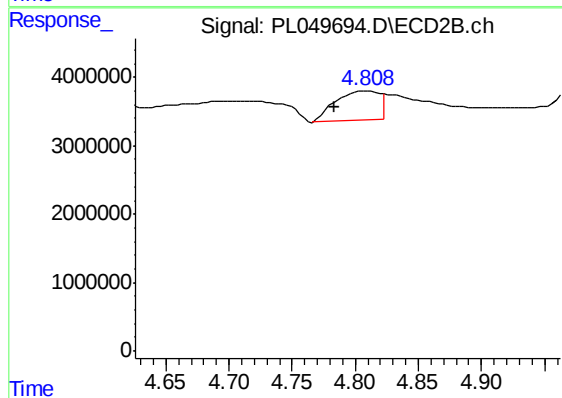

#6 beta-BHC


R.T.: 4.810 min
Delta R.T.: 0.027 min
Response: 10187383
Conc: 5.26 ng/ml

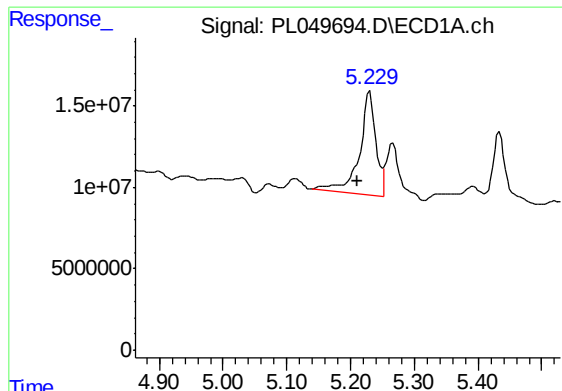

#10 gamma-Chlordane


R.T.: 5.230 min
Delta R.T.: 0.020 min
Response: 113628835
Conc: 6.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

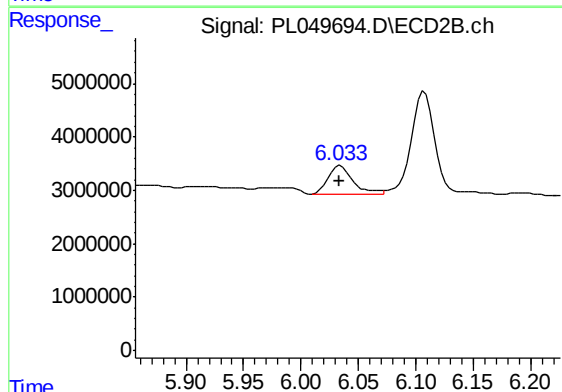


#10 gamma-Chlordane

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 8003136
Conc: 2.15 ng/ml

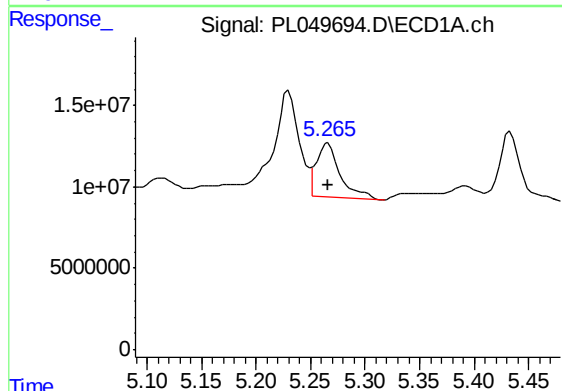


#11 alpha-Chlordane

R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 50944570
Conc: 3.07 ng/ml

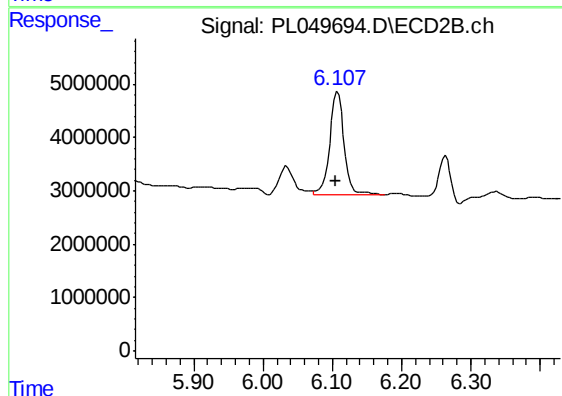

#11 alpha-Chlordane


R.T.: 6.108 min
Delta R.T.: 0.003 min
Response: 27719417
Conc: 7.49 ng/ml

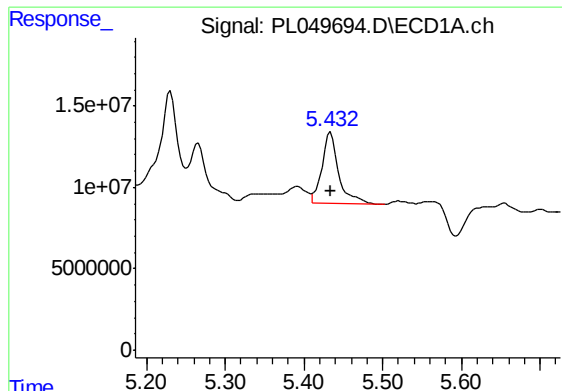

#12 4,4'-DDE


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 64635381
Conc: 3.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

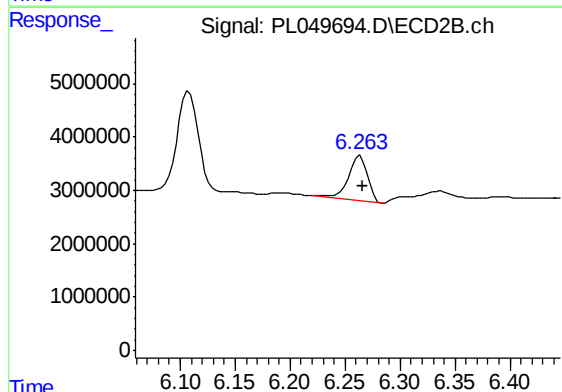


#12 4,4'-DDE

R.T.: 6.264 min
Delta R.T.: -0.002 min
Response: 10204205
Conc: 2.94 ng/ml

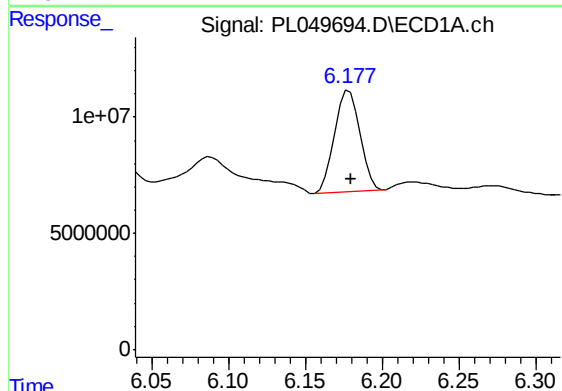


#17 4,4'-DDT

R.T.: 6.178 min
Delta R.T.: -0.001 min
Response: 50112649
Conc: 3.77 ng/ml

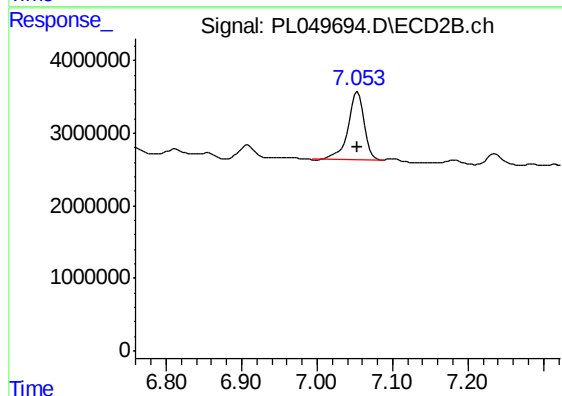

#17 4,4'-DDT


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 13677280
Conc: 4.67 ng/ml

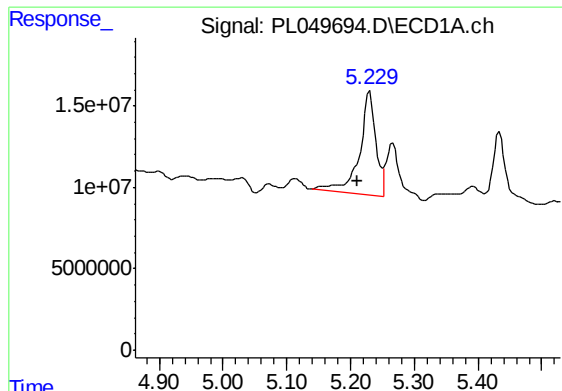

#25 Chlordane-3


R.T.: 5.230 min
Delta R.T.: 0.019 min
Response: 113628835
Conc: 60.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

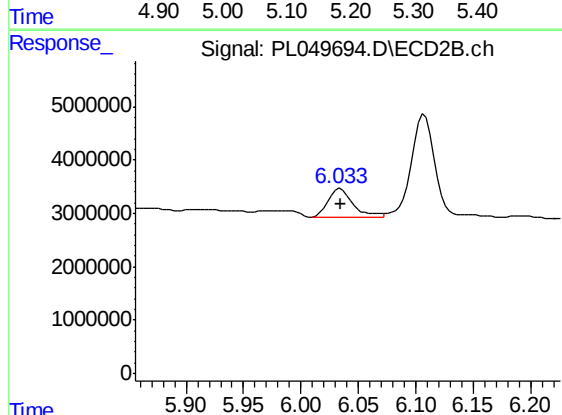


#25 Chlordane-3

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 8003136
Conc: 16.08 ng/ml

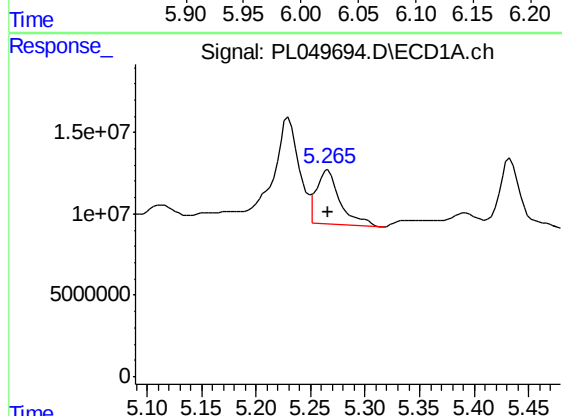


#26 Chlordane-4

R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 50944570
Conc: 29.19 ng/ml

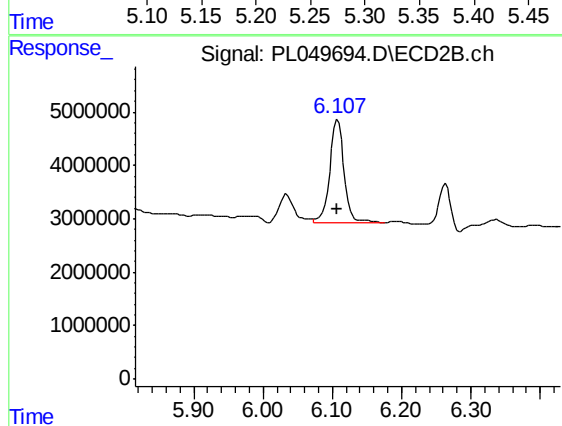

#26 Chlordane-4


R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 27719417
Conc: 46.64 ng/ml

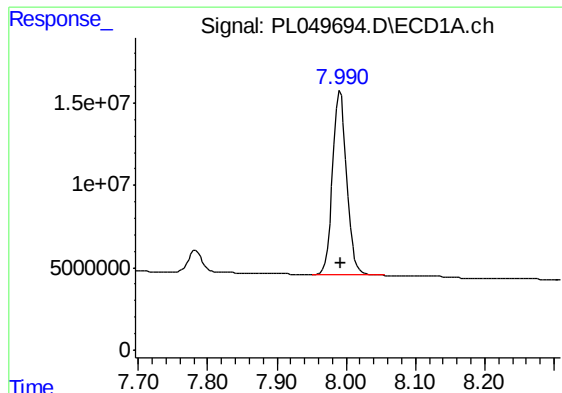

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 158595920
Conc: 12.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-013-SW160-061319

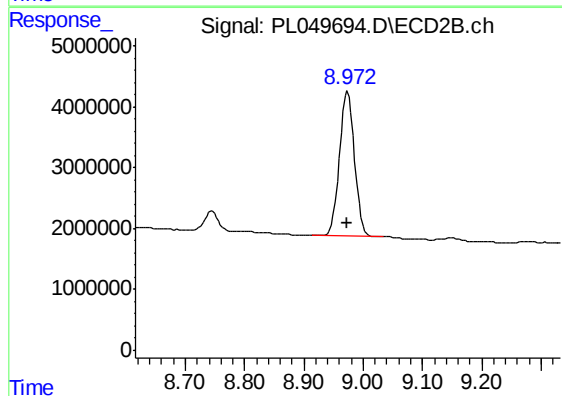

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: 0.000 min
Response: 42205837
Conc: 12.57 ng/ml