

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 08:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:45:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.637	14982776	34789168	22.200	20.730
28)	SA Decachlor...	11.634	10.379	-4717646	26398675	N.D.	18.736
Target Compounds							
7)	B delta-BHC	0.000	6.402	0	259041	N.D.	0.121 #
9)	A Endosulfan I	8.527	7.467	39991	62581	0.057	0.037 #
10)	B gamma-Chl...	8.389	7.336	610034	159534	0.786	0.087 #
11)	B alpha-Chl...	8.471	7.407	111408	180157	0.146	0.099 #
14)	MA Endrin	0.000	8.064f	0	486228	N.D.	0.356 #
15)	B Endosulfa...	9.306	0.000	519499	0	0.835	N.D. #
19)	B Endosulfa...	9.667	0.000	130419	0	0.208	N.D. #
22)	Mirex	10.627	0.000	297530	0	0.529	N.D. #
25)	Chlordane-3	8.389	7.336	610034	159534	5.908	0.928 #
26)	Chlordane-4	8.471	7.407	111408	180157	0.880	0.979



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 08:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:45:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

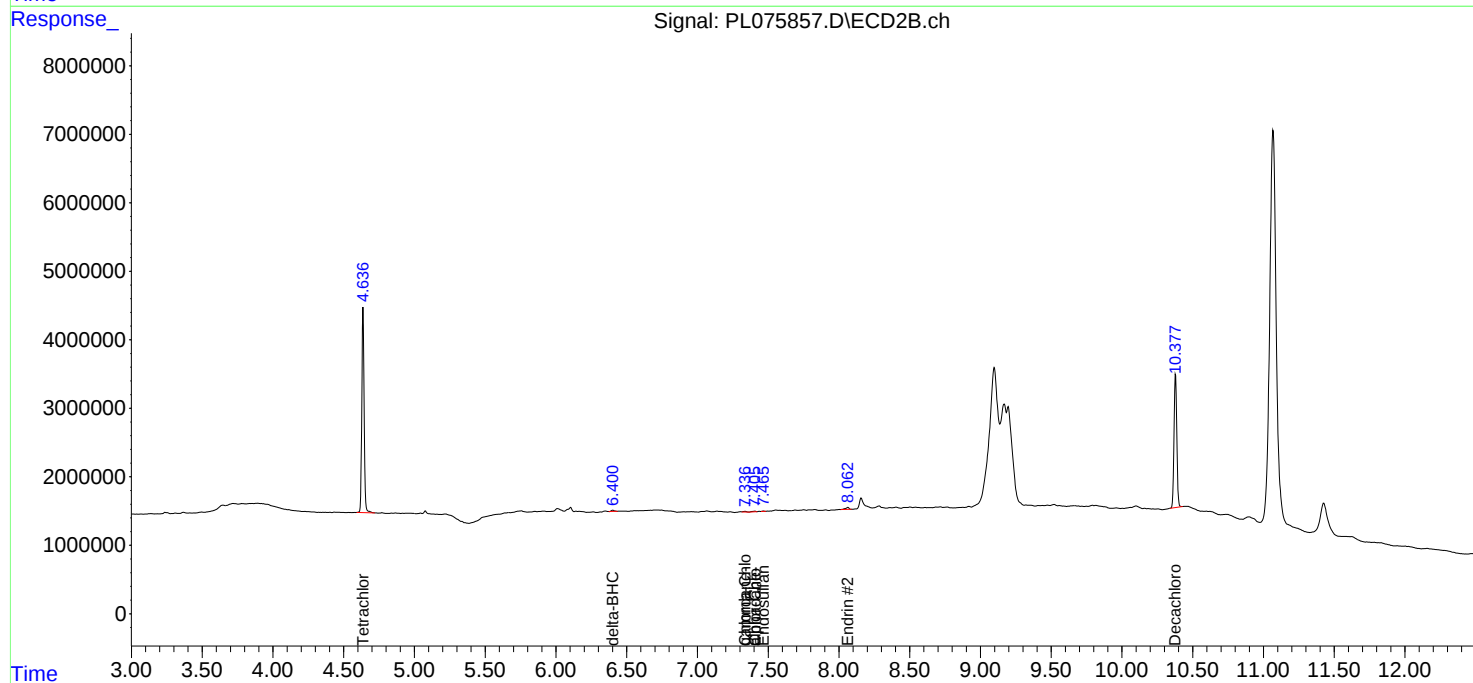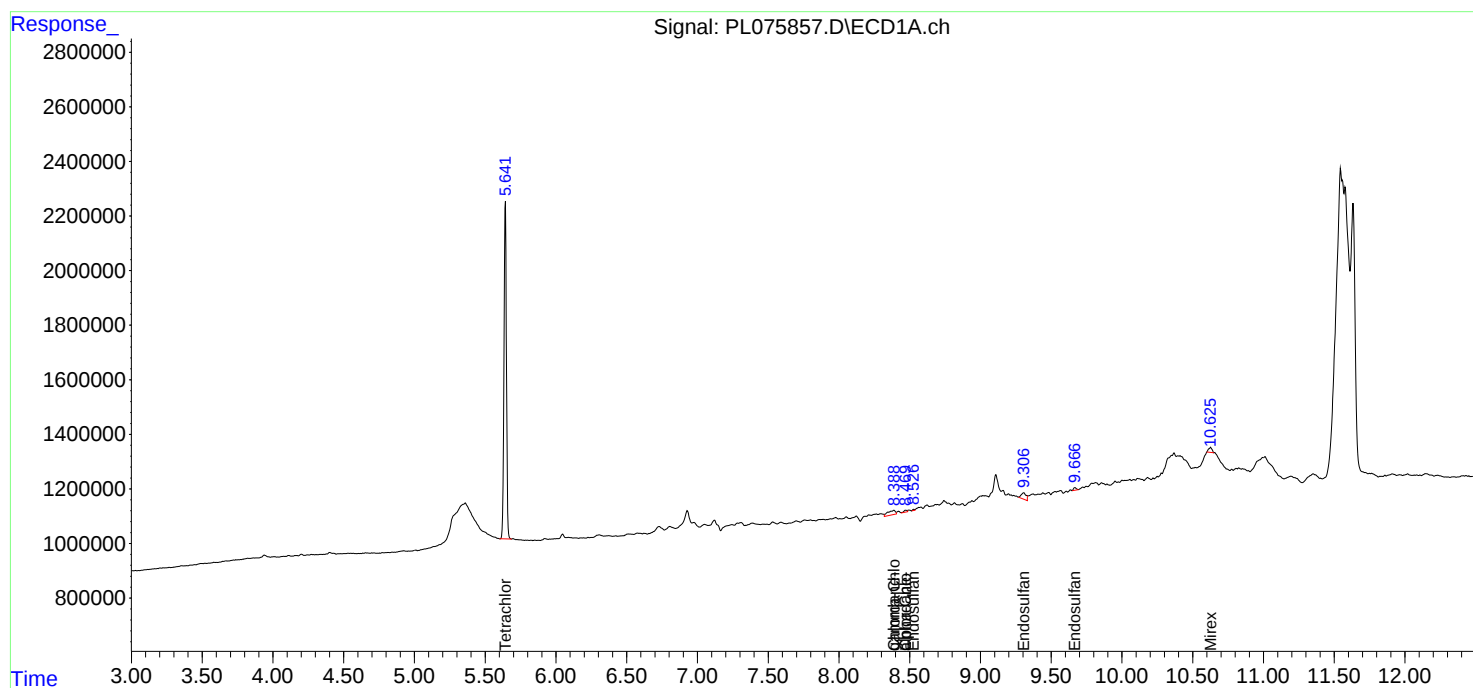


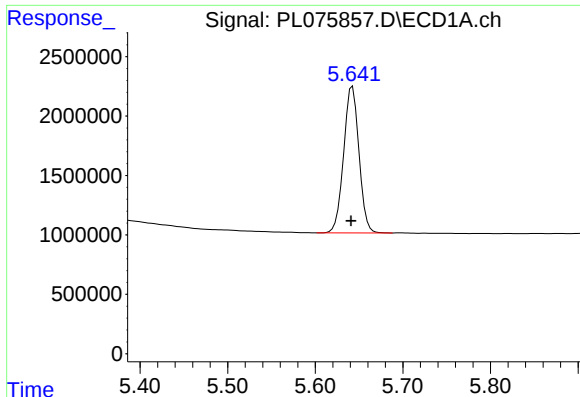

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 14982776
Conc: 22.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

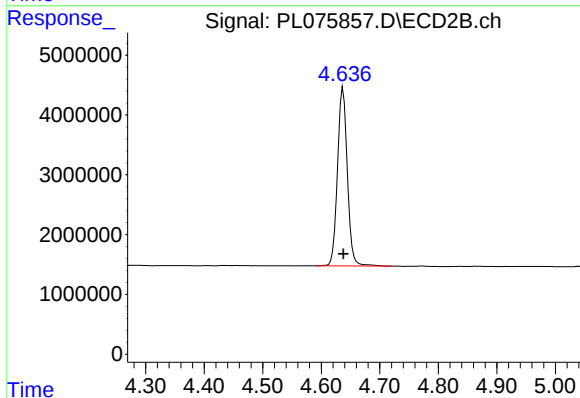


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 34789168
Conc: 20.73 ng/ml

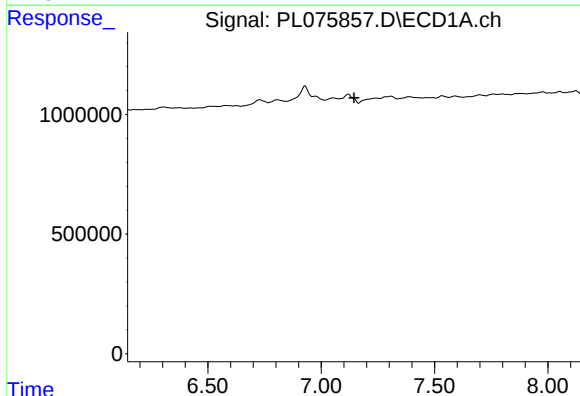


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

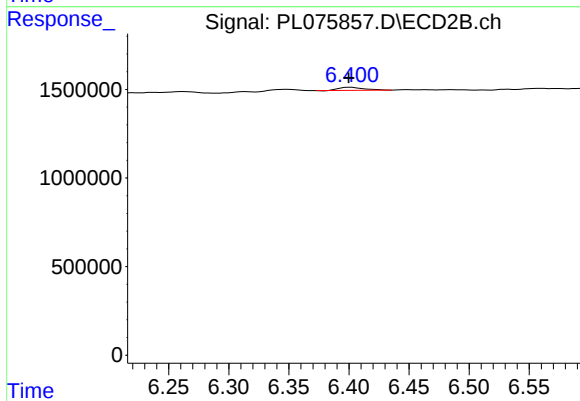

#7 delta-BHC


R.T.: 6.402 min
Delta R.T.: 0.002 min
Response: 259041
Conc: 0.12 ng/ml

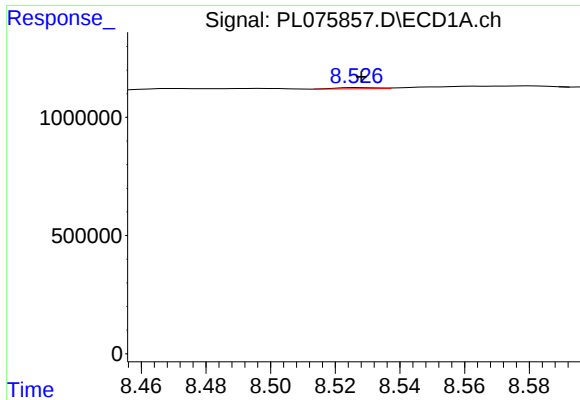

#9 Endosulfan I


R.T.: 8.527 min
Delta R.T.: 0.000 min
Response: 39991
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

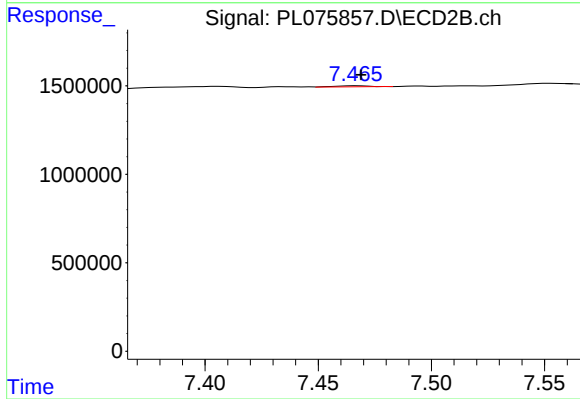


#9 Endosulfan I

R.T.: 7.467 min
Delta R.T.: -0.002 min
Response: 62581
Conc: 0.04 ng/ml

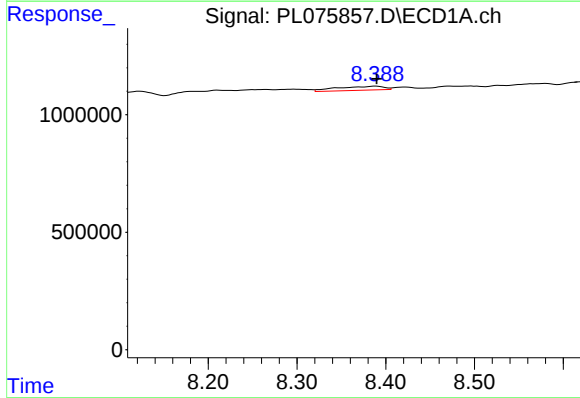


#10 gamma-Chlordane

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 610034
Conc: 0.79 ng/ml

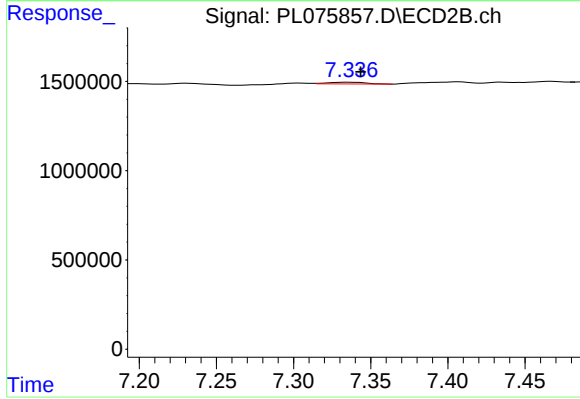

#10 gamma-Chlordane


R.T.: 7.336 min
Delta R.T.: -0.007 min
Response: 159534
Conc: 0.09 ng/ml

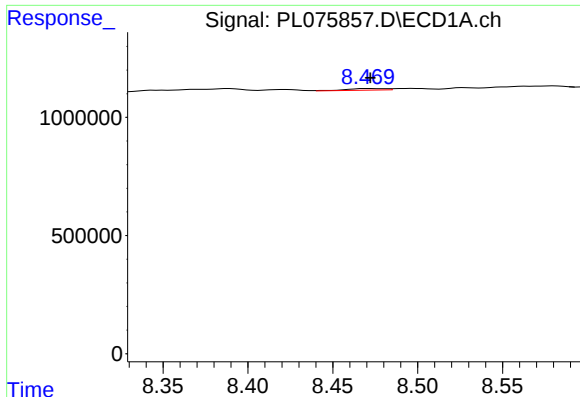

#11 alpha-Chlordane


R.T.: 8.471 min
Delta R.T.: -0.001 min
Response: 111408
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

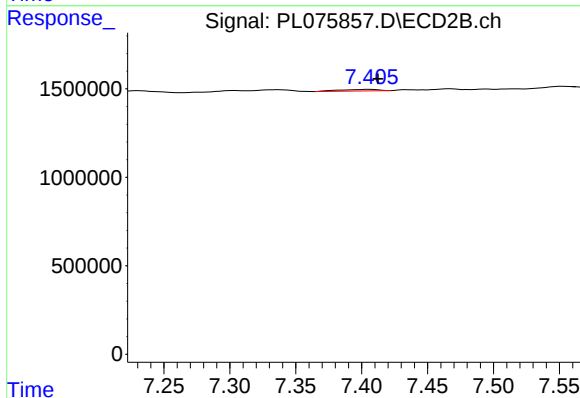


#11 alpha-Chlordane

R.T.: 7.407 min
Delta R.T.: -0.006 min
Response: 180157
Conc: 0.10 ng/ml

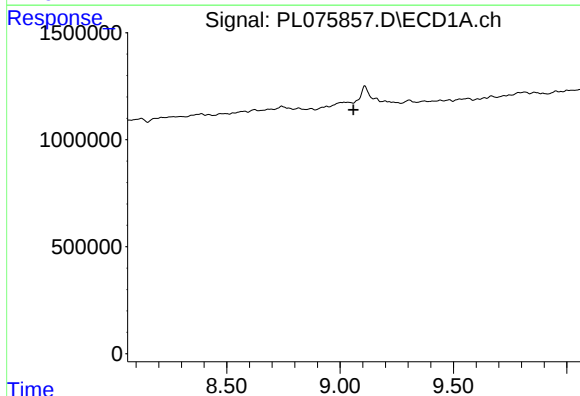


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

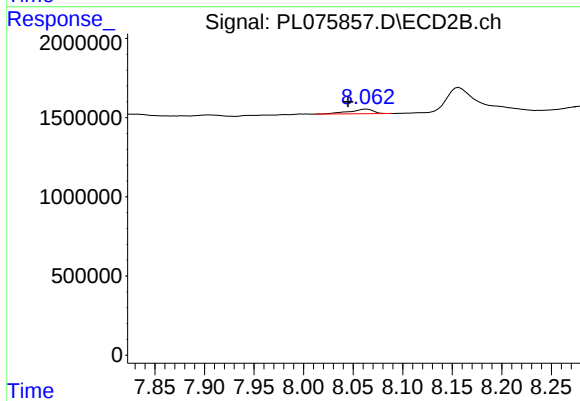

#14 Endrin


R.T.: 8.064 min
Delta R.T.: 0.019 min
Response: 486228
Conc: 0.36 ng/ml

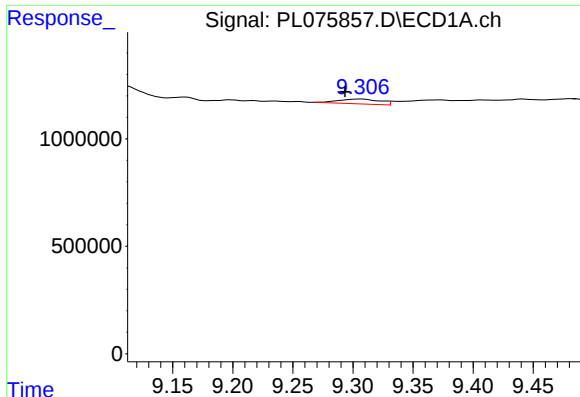

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.013 min
Response: 519499
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

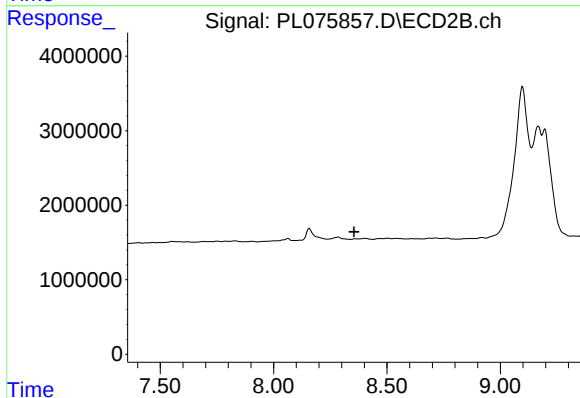


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

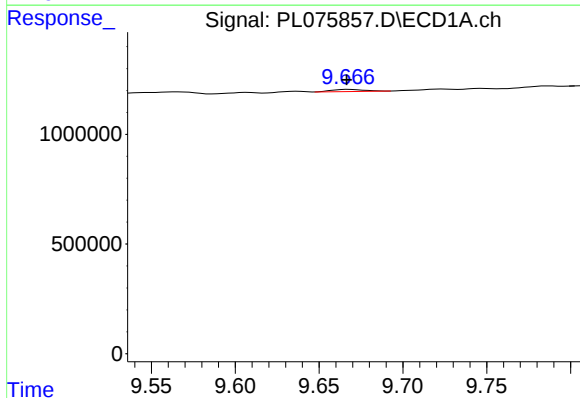


#19 Endosulfan Sulfate

R.T.: 9.667 min
Delta R.T.: 0.001 min
Response: 130419
Conc: 0.21 ng/ml

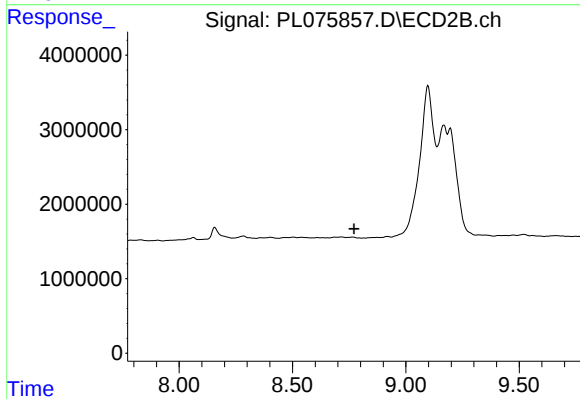

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.772 min
Response: 0
Conc: N.D.

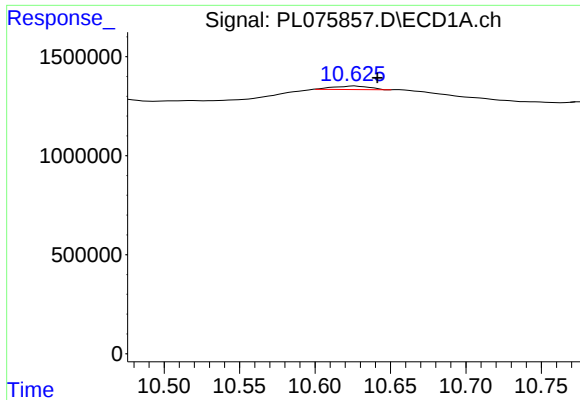

#22 Mirex


R.T.: 10.627 min
Delta R.T.: -0.015 min
Response: 297530
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

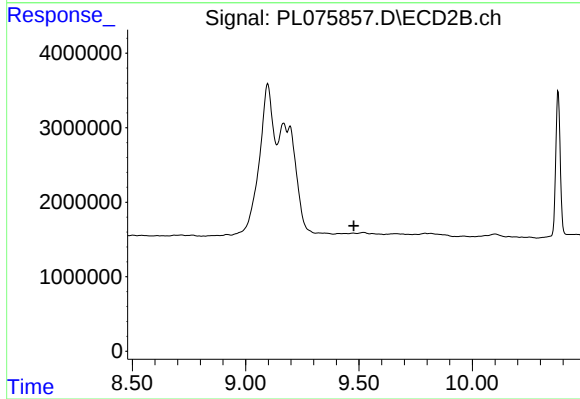


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.477 min
Response: 0
Conc: N.D.

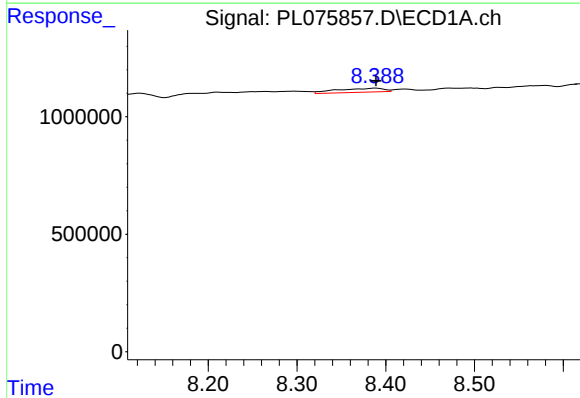


#25 Chlordane-3

R.T.: 8.389 min
Delta R.T.: 0.000 min
Response: 610034
Conc: 5.91 ng/ml

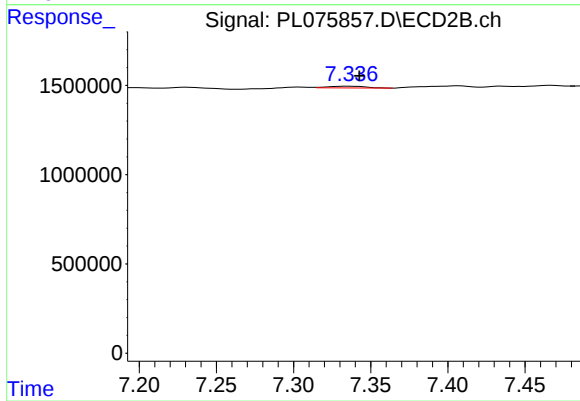

#25 Chlordane-3


R.T.: 7.336 min
Delta R.T.: -0.006 min
Response: 159534
Conc: 0.93 ng/ml

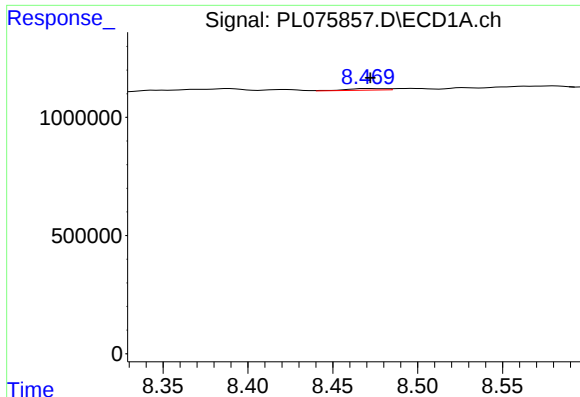

#26 Chlordane-4


R.T.: 8.471 min
Delta R.T.: -0.001 min
Response: 111408
Conc: 0.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

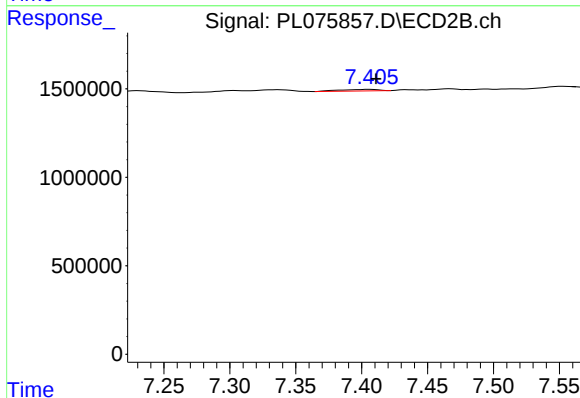


#26 Chlordane-4

R.T.: 7.407 min
Delta R.T.: -0.004 min
Response: 180157
Conc: 0.98 ng/ml

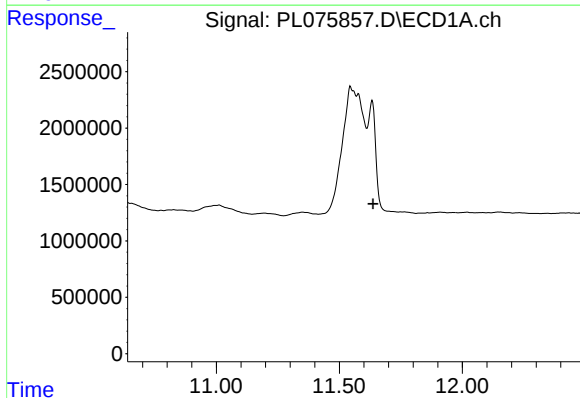

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.002 min
Response: -4717646
Conc: N.D.

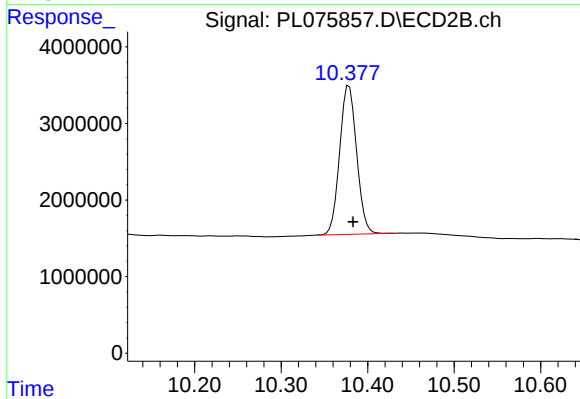

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.005 min
Response: 26398675
Conc: 18.74 ng/ml