

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 09:54
 Operator : AR\AJ
 Sample : PB145650BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:46:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.647	4.636	12622126	29822310	18.703	17.771
28)	SA Decachlor...	11.640	10.380	12089121	25038856	19.746	17.771
Target Compounds							
3)	MA gamma-BHC...	6.601f	0.000	505821	0	0.576	N.D. #
6)	B beta-BHC	6.870	0.000	729008	0	1.776	N.D. #
9)	A Endosulfan I	8.532	0.000	167382	0	0.239	N.D. #
10)	B gamma-Chl...	8.371f	0.000	1555674	0	2.003	N.D. #
11)	B alpha-Chl...	8.464	0.000	95227	0	0.125	N.D. #
14)	MA Endrin	0.000	8.064f	0	270925	N.D.	0.198 #
15)	B Endosulfa...	9.304	0.000	356890	0	0.574	N.D. #
21)	B Endrin ke...	10.186f	0.000	334889	0	0.476	N.D. #
25)	Chlordane-3	8.371f	0.000	1555674	0	15.067	N.D. #
26)	Chlordane-4	8.464	0.000	95227	0	0.752	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 09:54
Operator : AR\AJ
Sample : PB145650BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:46:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

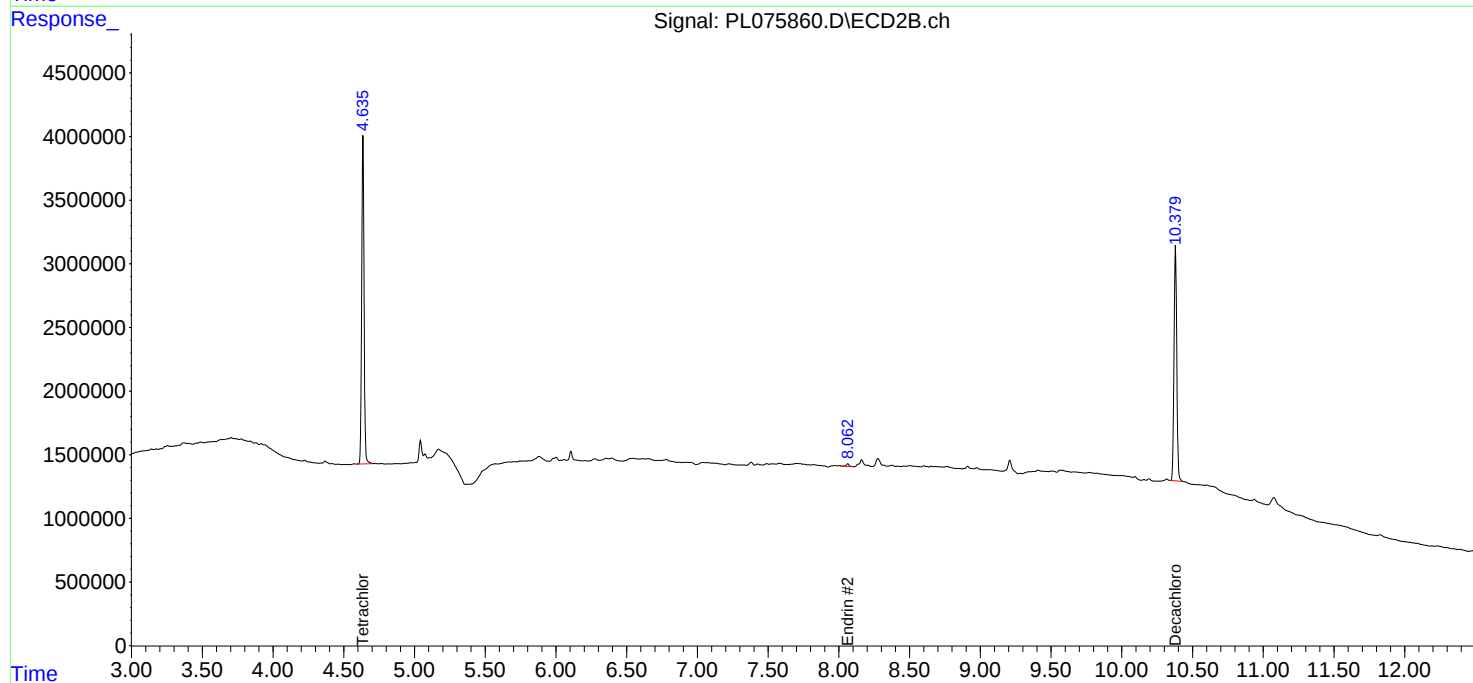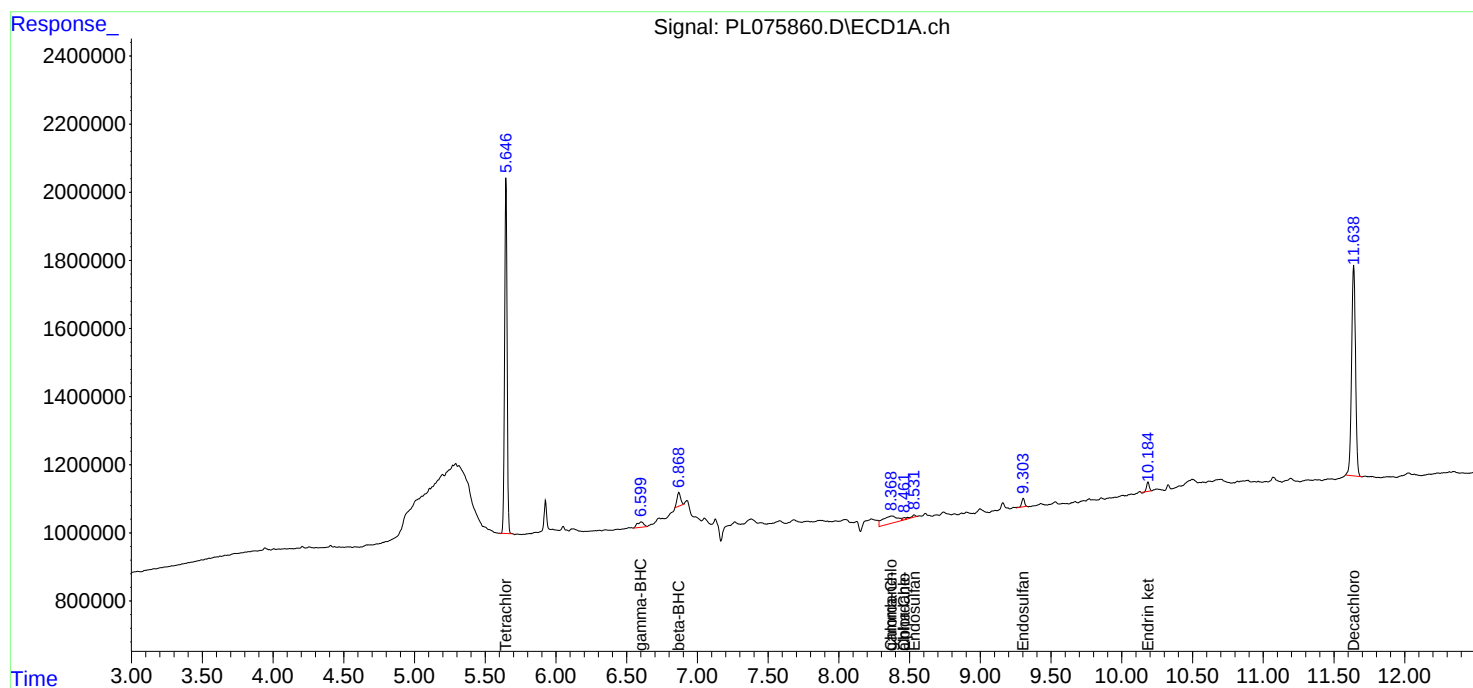


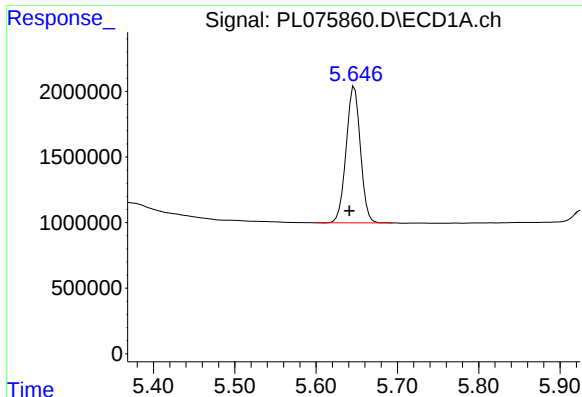

#1 Tetrachloro-m-xylene


R.T.: 5.647 min
Delta R.T.: 0.006 min
Response: 12622126
Conc: 18.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

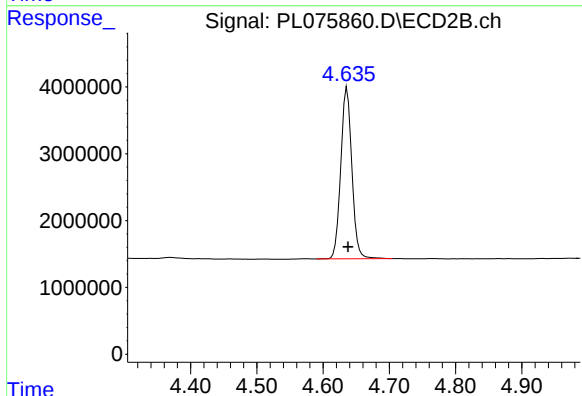


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 29822310
Conc: 17.77 ng/ml

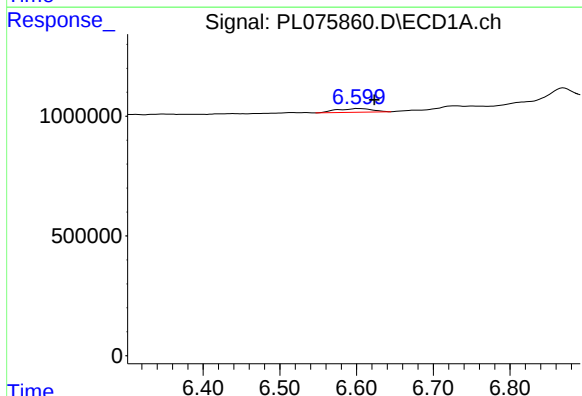


#3 gamma-BHC (Lindane)

R.T.: 6.601 min
Delta R.T.: -0.022 min
Response: 505821
Conc: 0.58 ng/ml

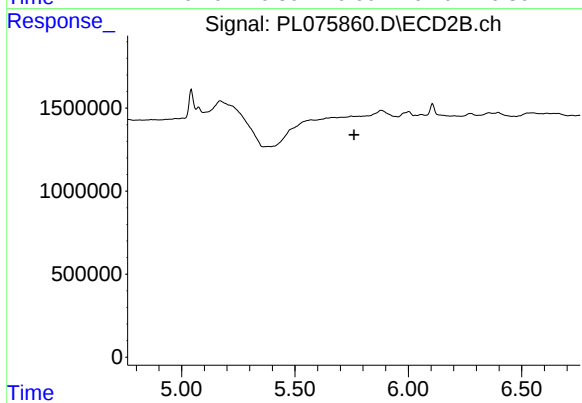

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 5.761 min
Response: 0
Conc: N.D.

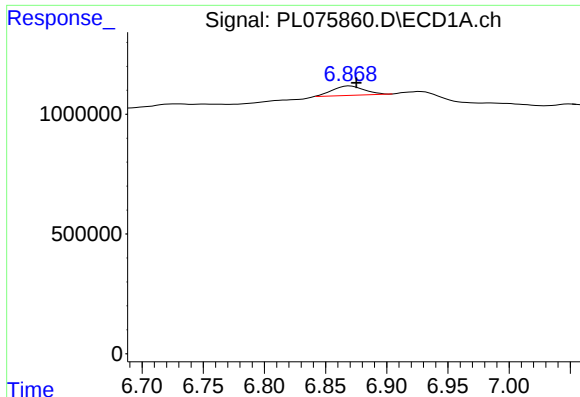

#6 beta-BHC

R.T.: 6.870 min
Delta R.T.: -0.005 min
Response: 729008
Conc: 1.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

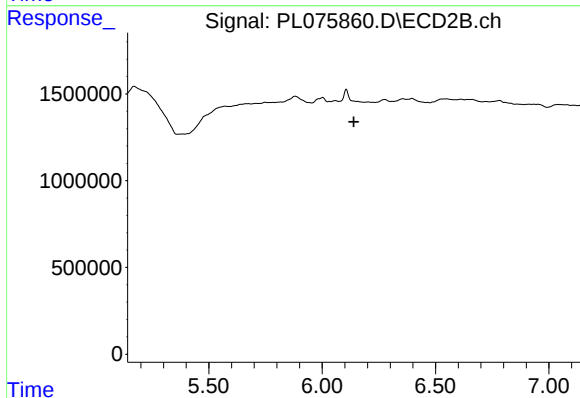


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.


#9 Endosulfan I

R.T.: 8.532 min
Delta R.T.: 0.004 min
Response: 167382
Conc: 0.24 ng/ml

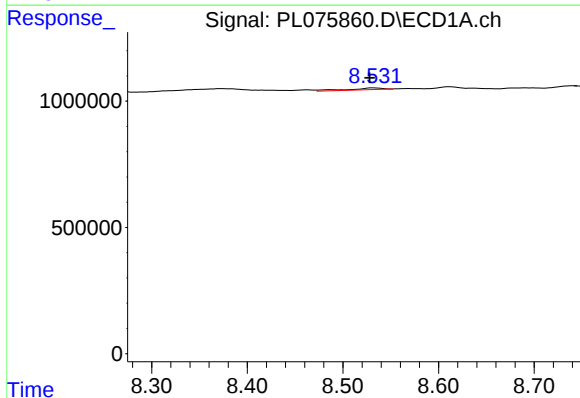

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

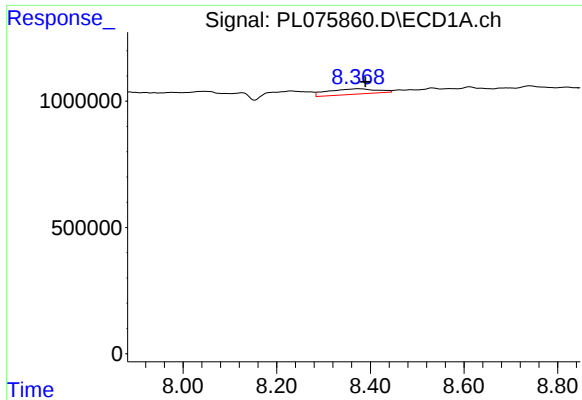

#10 gamma-Chlordane


R.T.: 8.371 min
Delta R.T.: -0.019 min
Response: 1555674
Conc: 2.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

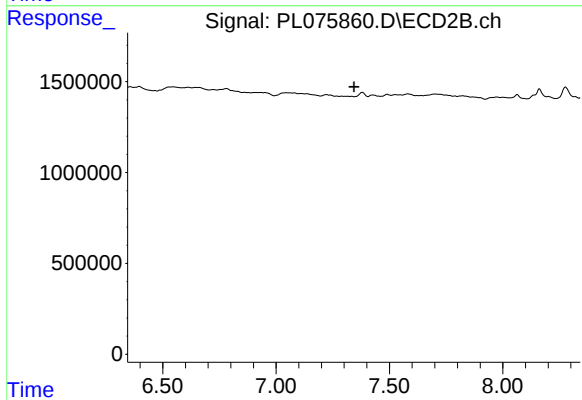


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

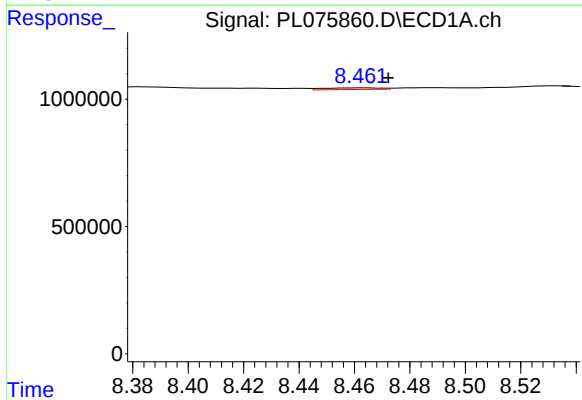


#11 alpha-Chlordane

R.T.: 8.464 min
Delta R.T.: -0.008 min
Response: 95227
Conc: 0.12 ng/ml

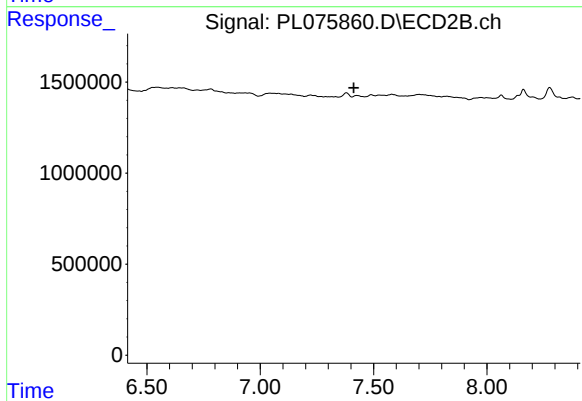

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

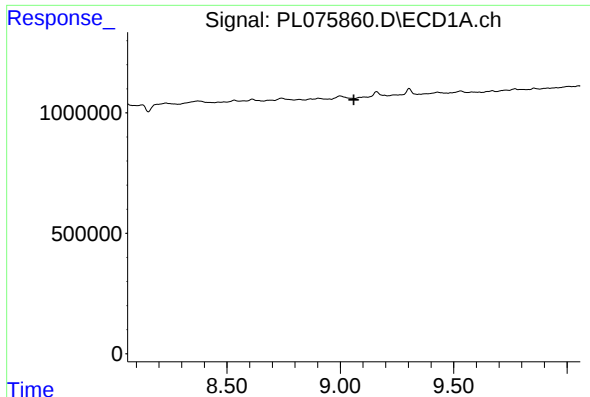

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

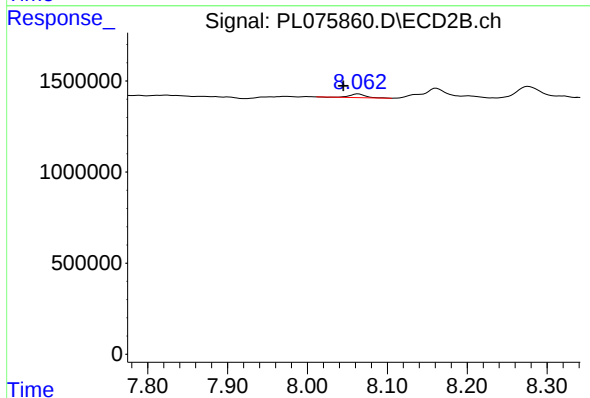


#14 Endrin

R.T.: 8.064 min
Delta R.T.: 0.019 min
Response: 270925
Conc: 0.20 ng/ml

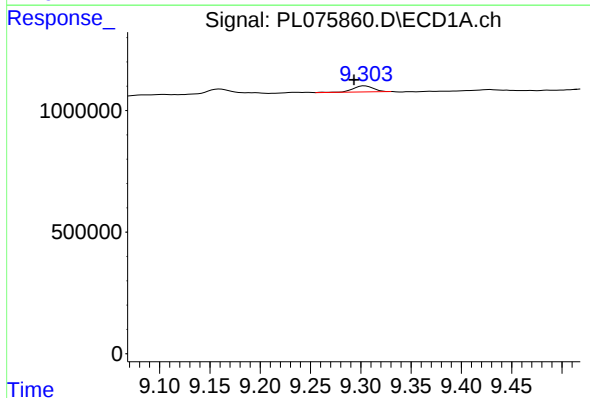


#15 Endosulfan II

R.T.: 9.304 min
Delta R.T.: 0.011 min
Response: 356890
Conc: 0.57 ng/ml

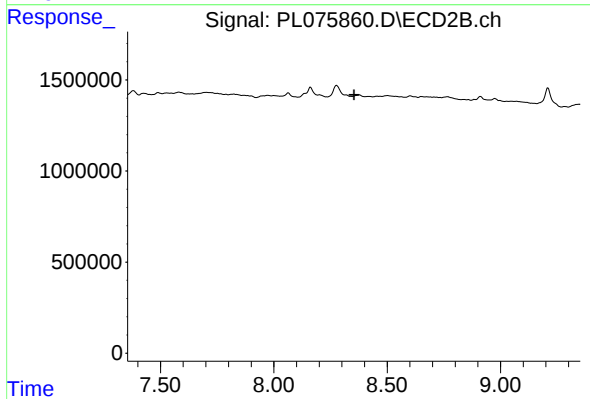

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

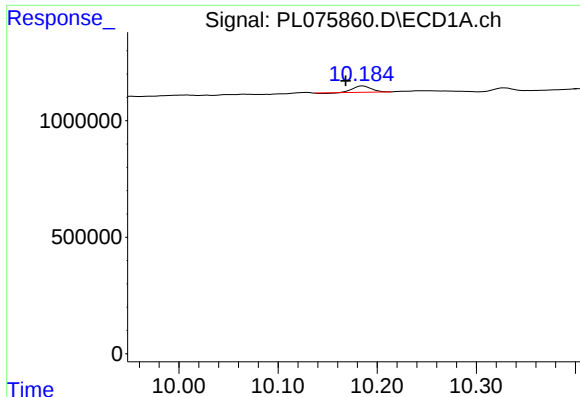

#21 Endrin ketone


R.T.: 10.186 min
Delta R.T.: 0.017 min
Response: 334889
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

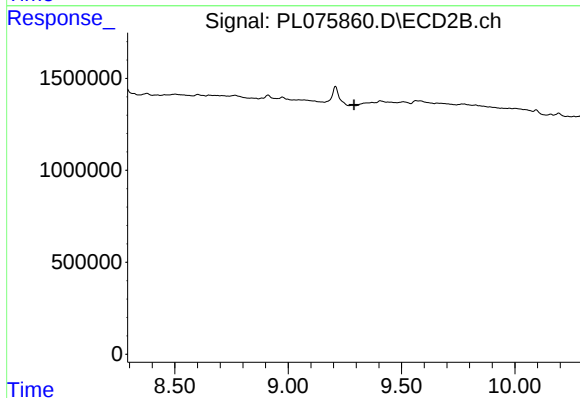


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

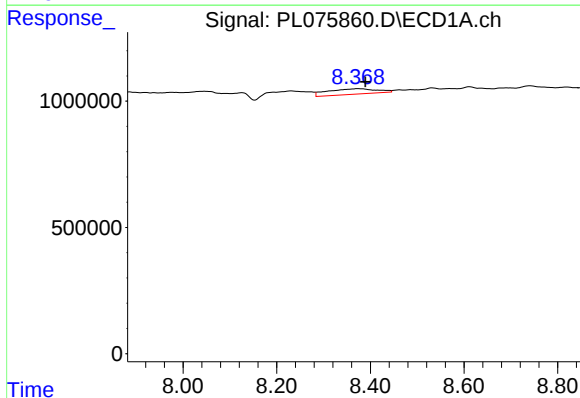


#25 Chlordane-3

R.T.: 8.371 min
Delta R.T.: -0.018 min
Response: 1555674
Conc: 15.07 ng/ml

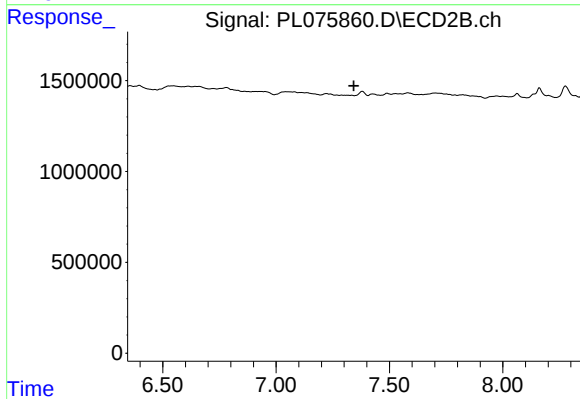

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

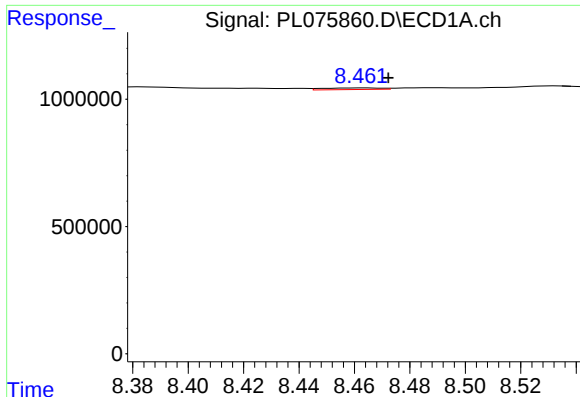

#26 Chlordane-4


R.T.: 8.464 min
Delta R.T.: -0.008 min
Response: 95227
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

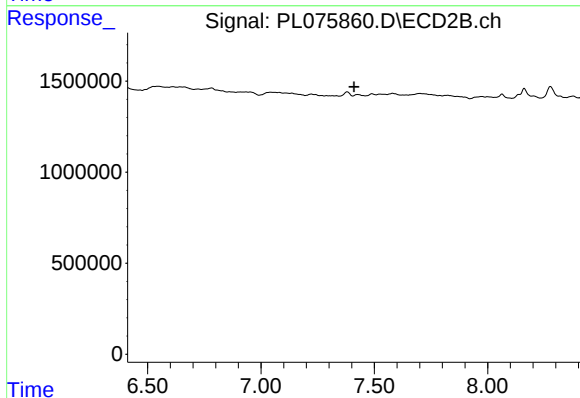


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

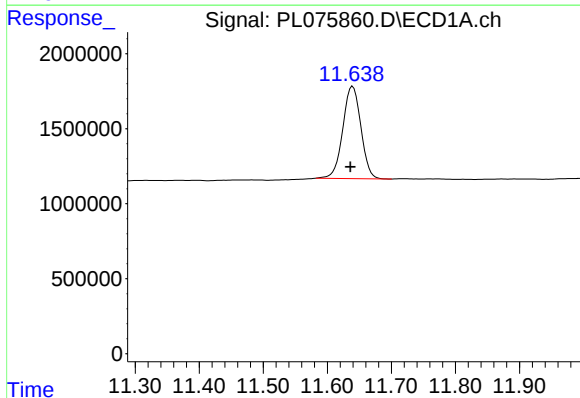

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.003 min
Response: 12089121
Conc: 19.75 ng/ml

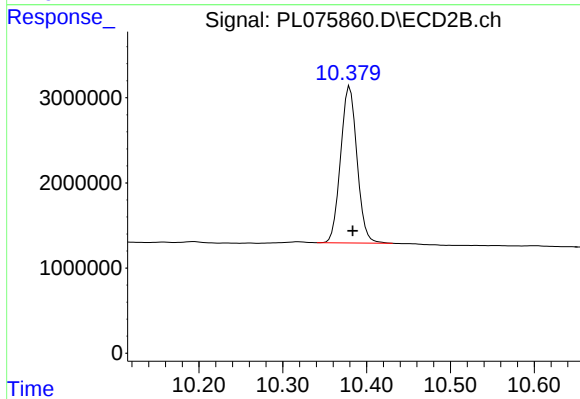

#28 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.003 min
Response: 25038856
Conc: 17.77 ng/ml