

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 10:34
 Operator : AR\AJ
 Sample : N3373-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DS-7D

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2022
 Supervised By :Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:46:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.645	4.636	9685648	23865411	14.352m	14.221
28) SA Decachlor...	11.640	10.375	13734949	31684488	22.435m	22.488
Target Compounds						
13) MA Dieldrin	8.813	7.758	168.8E6	904.4E6	233.703m	534.342m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075862.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 10:34
Operator : AR\AJ
Sample : N3373-12
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DS-7D


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:46:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

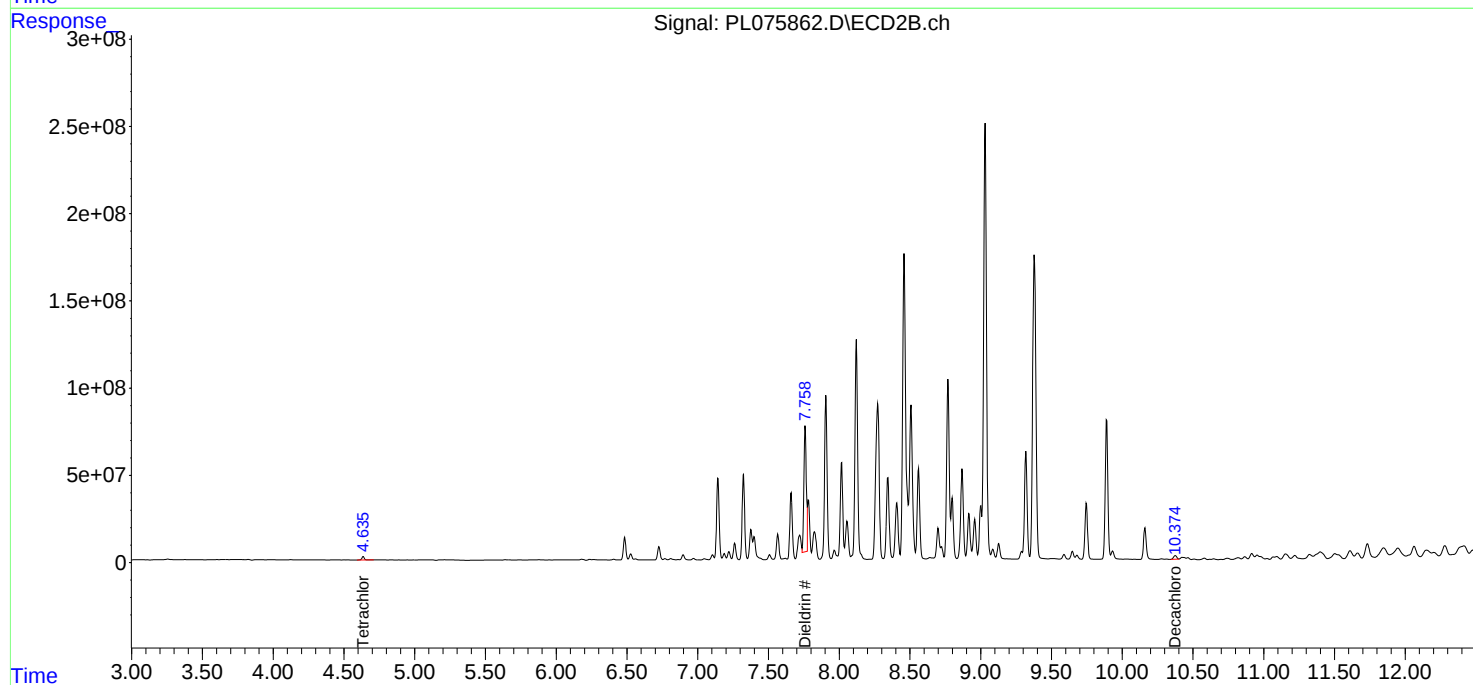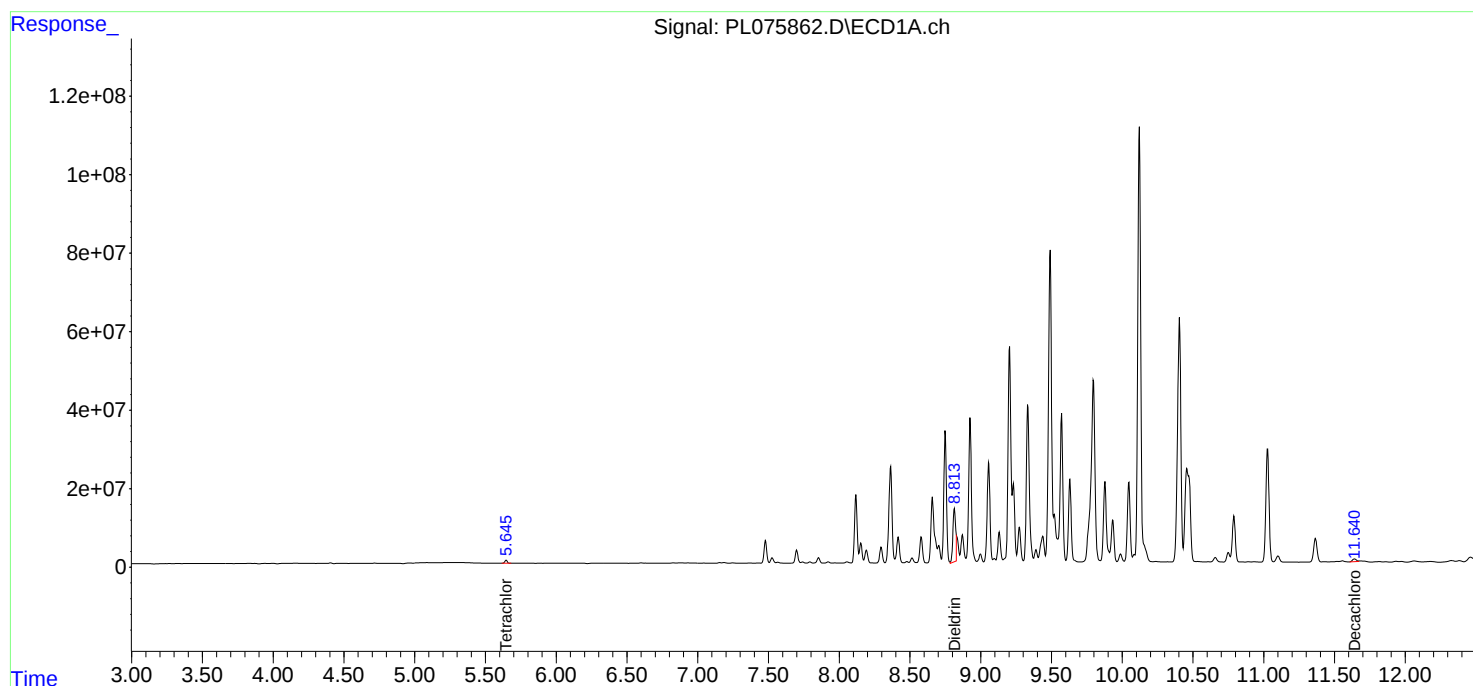

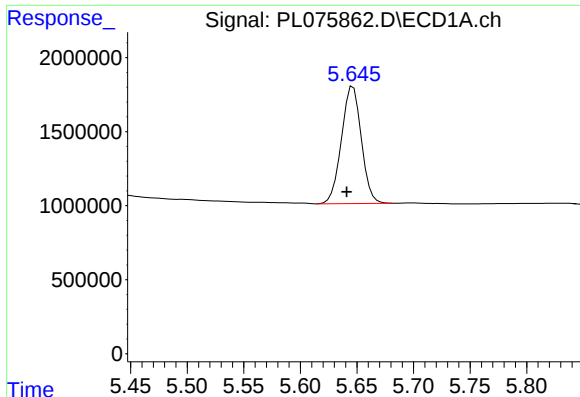


#1 Tetrachloro-m-xylene

R.T.: 5.645 min
Delta R.T.: 0.004 min
Response: 9685648
Conc: 14.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
DS-7D


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

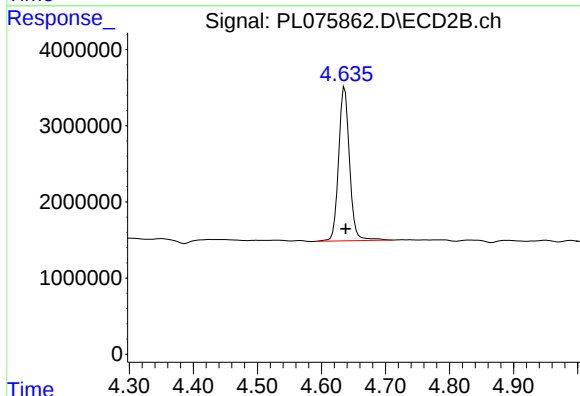


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.001 min
Response: 23865411
Conc: 14.22 ng/ml

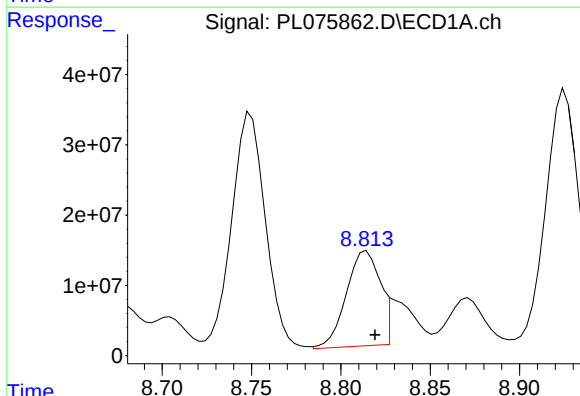


#13 Dieldrin

R.T.: 8.813 min
Delta R.T.: -0.006 min
Response: 168834541
Conc: 233.70 ng/ml m

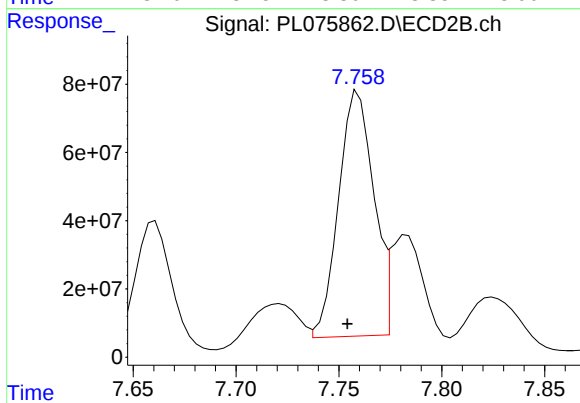

#13 Dieldrin

R.T.: 7.758 min
Delta R.T.: 0.004 min
Response: 904427176
Conc: 534.34 ng/ml m

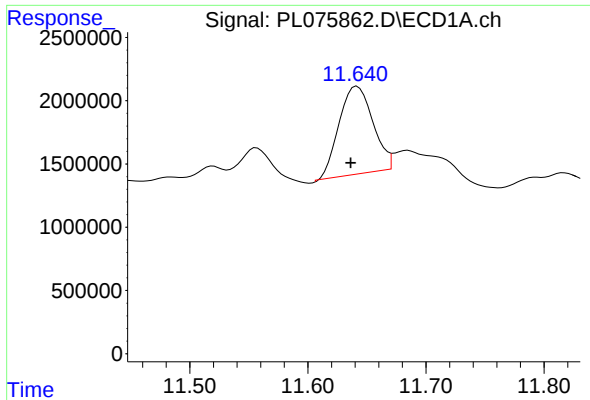


#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.004 min
Response: 13734949
Conc: 22.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
DS-7D

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

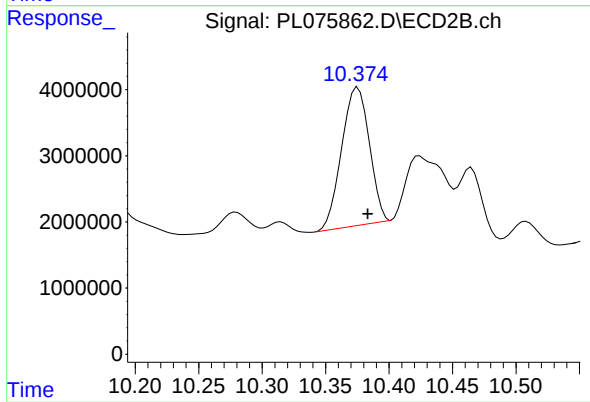

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: -0.008 min
Response: 31684488
Conc: 22.49 ng/ml