

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 14:15
 Operator : AR\AJ
 Sample : N3390-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-2-061722

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:48:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.637	6293913	14452480	9.326m	8.612
28)	SA Decachlor...	11.640	10.380	34446262	65939367	56.264	46.800
Target Compounds							
11)	B alpha-Chl...	8.478	7.405	4161971	9818607	5.458	5.377
12)	B 4,4'-DDE	8.660	7.621	4347420	6017457	6.569	3.764 #
13)	MA Dieldrin	8.815	7.757	769515	12578015	1.065	7.431m#
16)	A 4,4'-DDD	9.205	8.203	5627496	1824502	10.285	1.387m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 14:15
Operator : AR\AJ
Sample : N3390-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PT-2-061722


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2022
Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:48:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

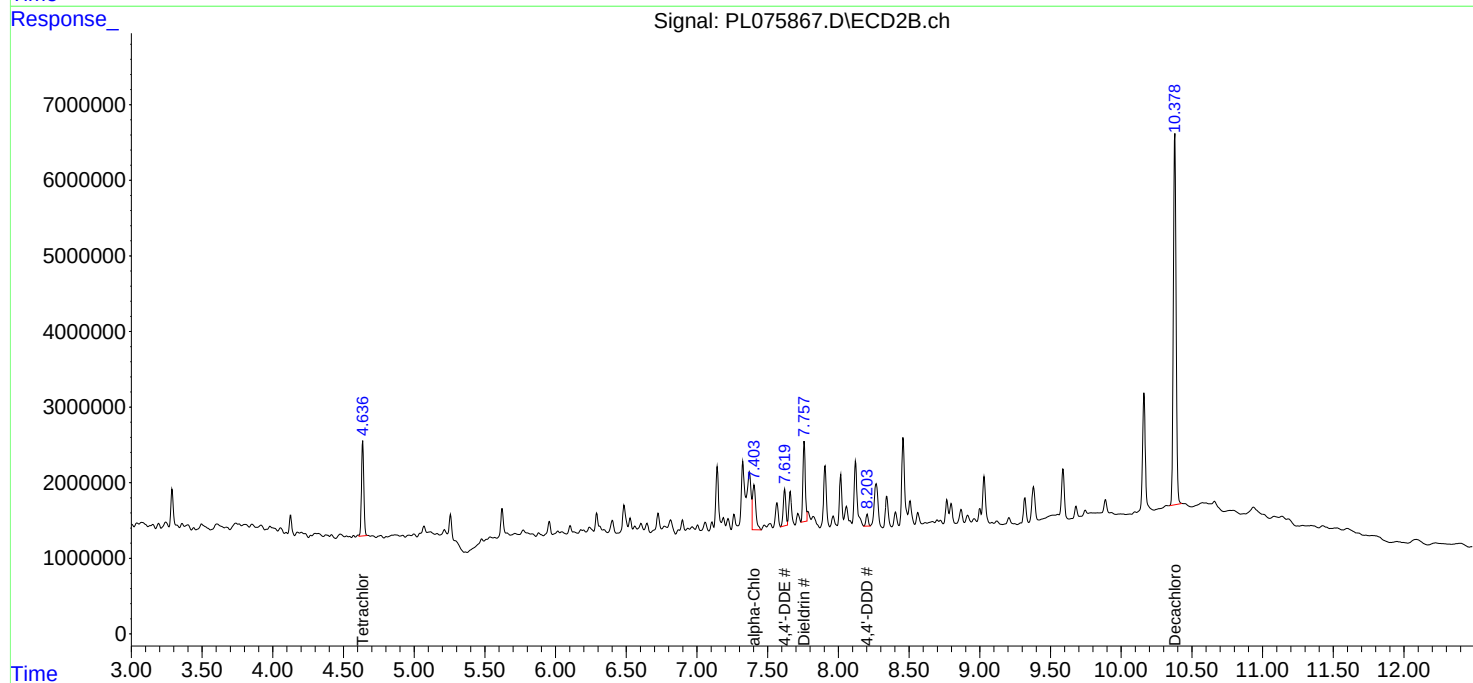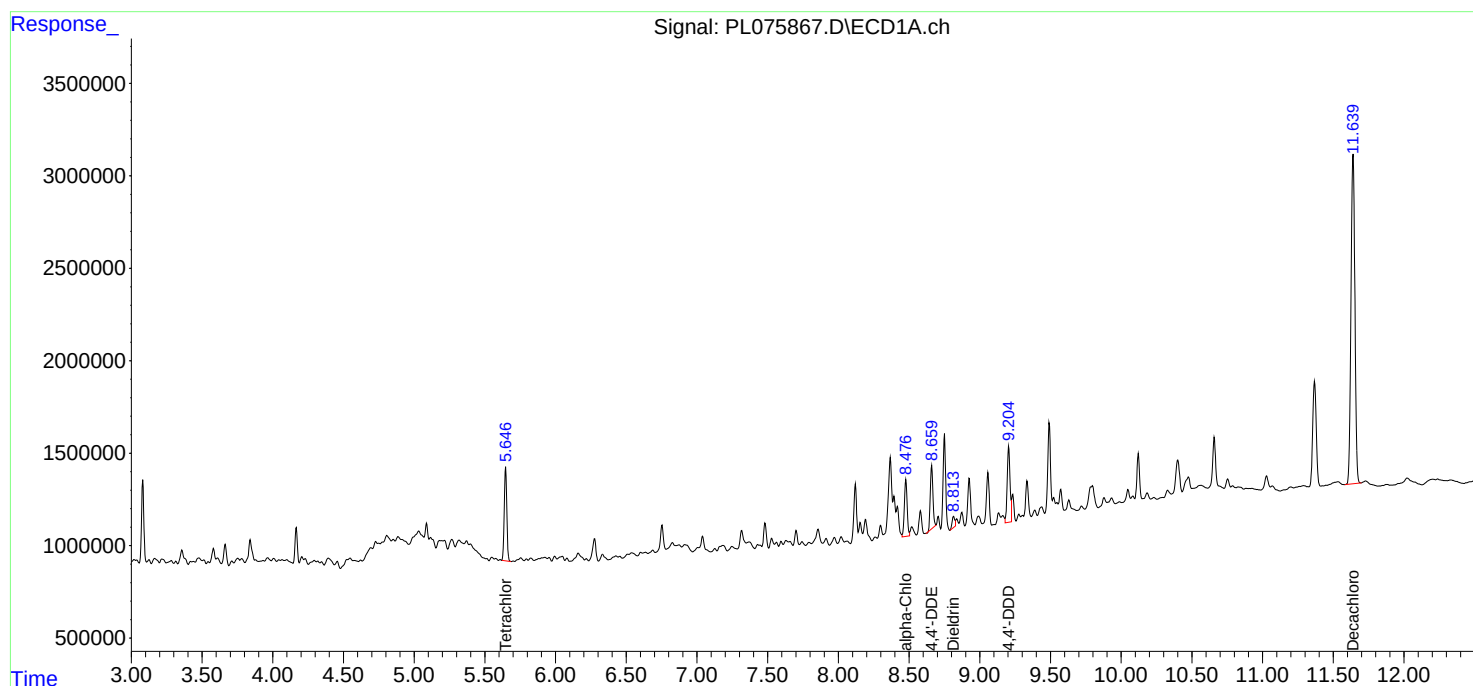

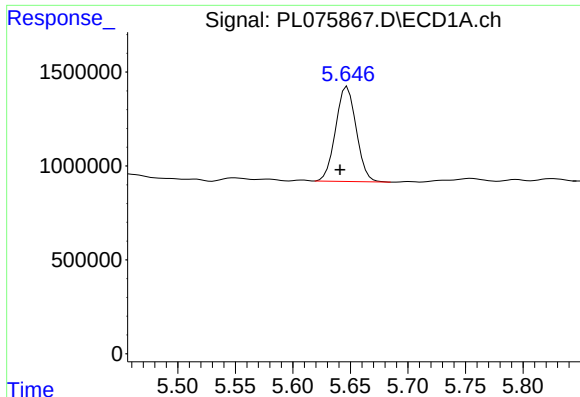


#1 Tetrachloro-m-xylene

R.T.: 5.646 min
Delta R.T.: 0.005 min
Response: 6293913
Conc: 9.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

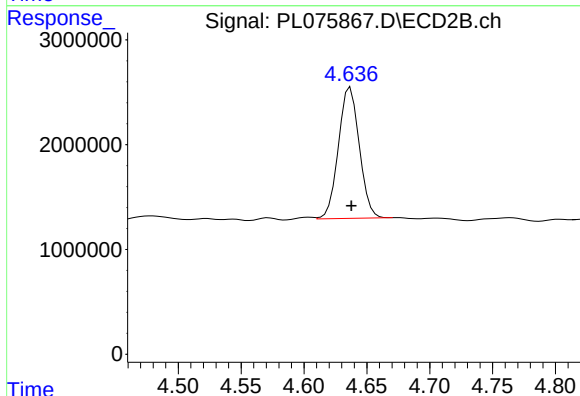


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 14452480
Conc: 8.61 ng/ml

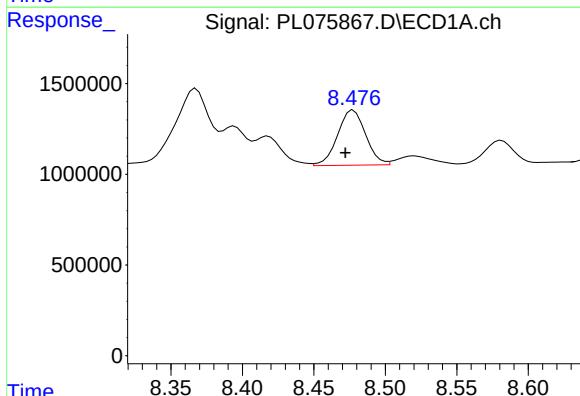


#11 alpha-Chlordane

R.T.: 8.478 min
Delta R.T.: 0.005 min
Response: 4161971
Conc: 5.46 ng/ml

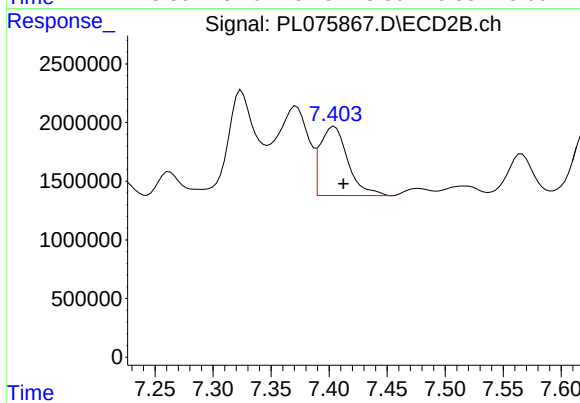

#11 alpha-Chlordane

R.T.: 7.405 min
Delta R.T.: -0.008 min
Response: 9818607
Conc: 5.38 ng/ml

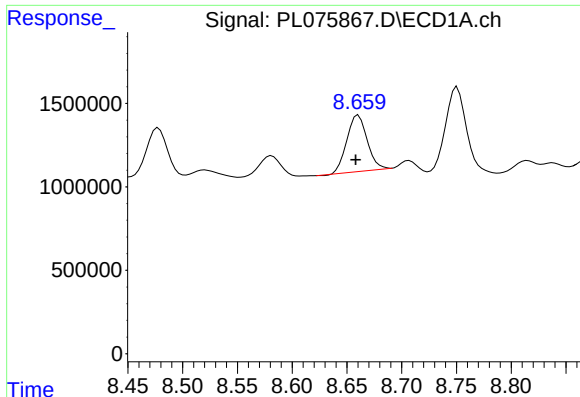


#12 4,4'-DDE

R.T.: 8.660 min
Delta R.T.: 0.002 min
Response: 4347420
Conc: 6.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

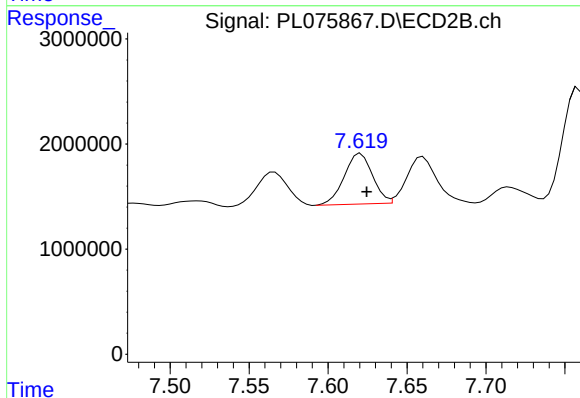


#12 4,4'-DDE

R.T.: 7.621 min
Delta R.T.: -0.004 min
Response: 6017457
Conc: 3.76 ng/ml

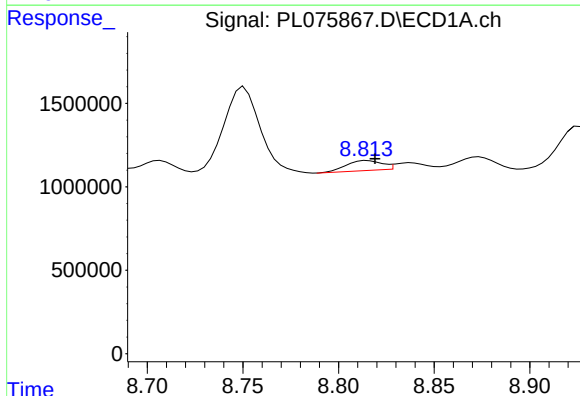


#13 Dieldrin

R.T.: 8.815 min
Delta R.T.: -0.004 min
Response: 769515
Conc: 1.07 ng/ml

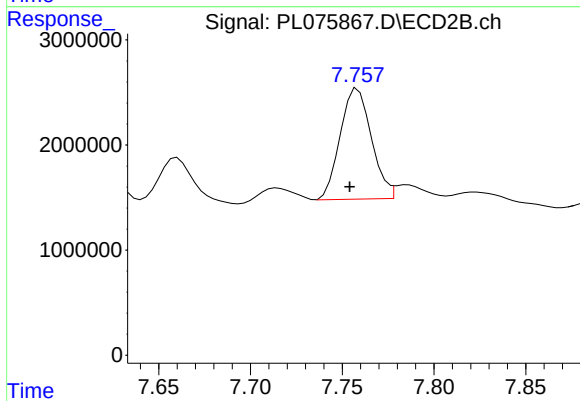

#13 Dieldrin

R.T.: 7.757 min
Delta R.T.: 0.003 min
Response: 12578015
Conc: 7.43 ng/ml m

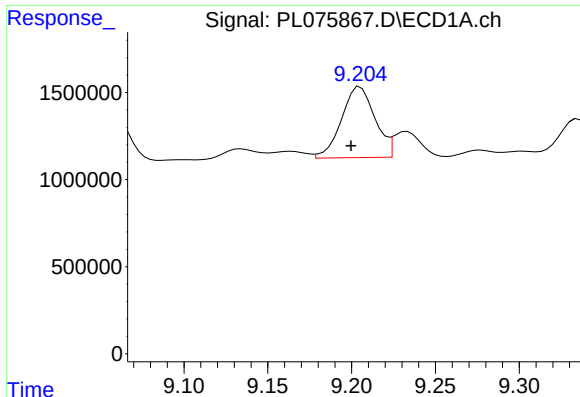


#16 4,4'-DDD

R.T.: 9.205 min
Delta R.T.: 0.005 min
Response: 5627496
Conc: 10.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-2-061722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

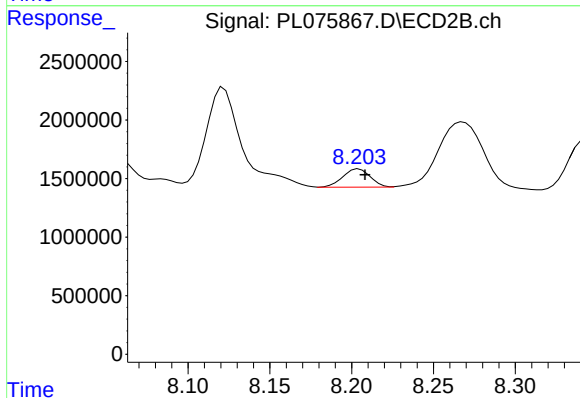


#16 4,4'-DDD

R.T.: 8.203 min
Delta R.T.: -0.005 min
Response: 1824502
Conc: 1.39 ng/ml m

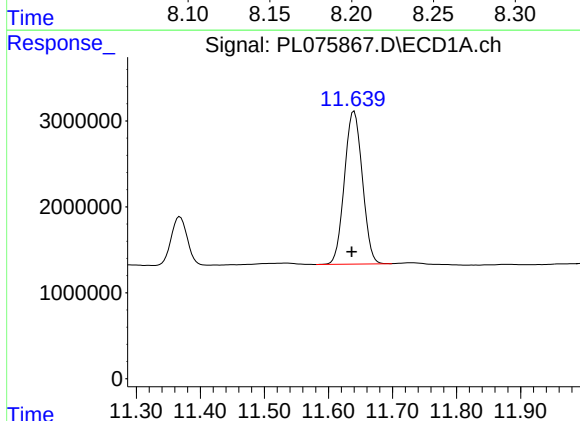

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.004 min
Response: 34446262
Conc: 56.26 ng/ml

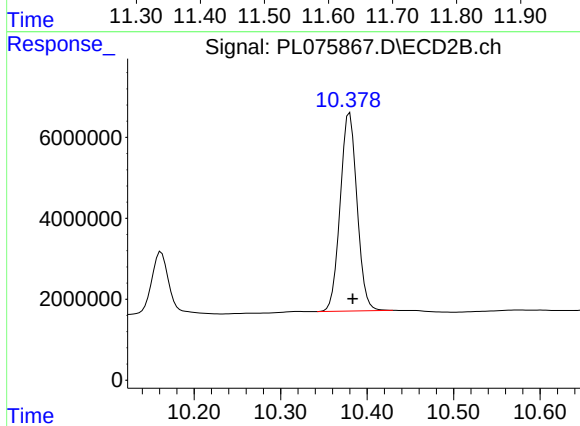

#28 Decachlorobiphenyl

R.T.: 10.380 min
Delta R.T.: -0.003 min
Response: 65939367
Conc: 46.80 ng/ml