

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
 Data File : PL075868.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 14:32
 Operator : AR\AJ
 Sample : N3397-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-2-061722

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/21/2022
 Supervised By :Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:49:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.640	4.635	1293117	2949955	1.916m	1.758m
28) SA Decachlor...	11.634	10.377	1890045	2724520	3.087m	1.934 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062022\
Data File : PL075868.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 14:32
Operator : AR\AJ
Sample : N3397-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-2-061722


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/21/2022
Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:49:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

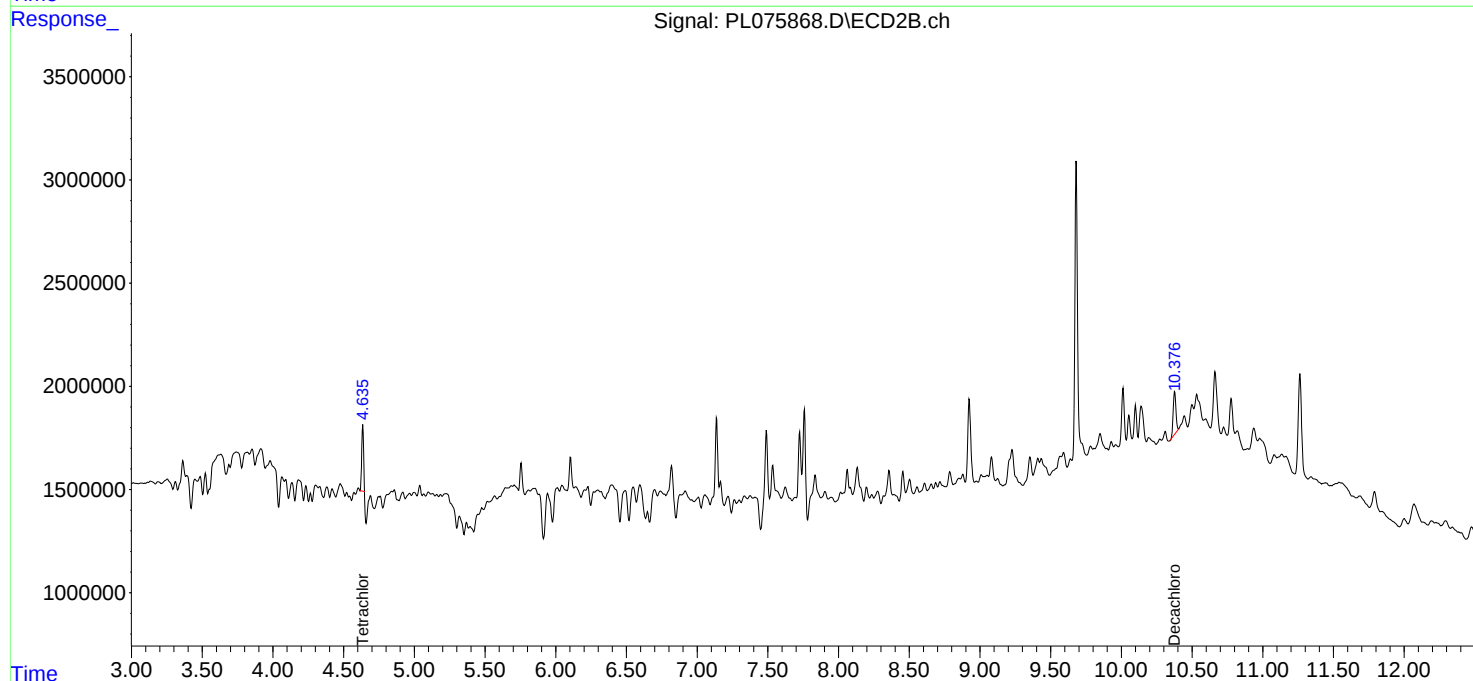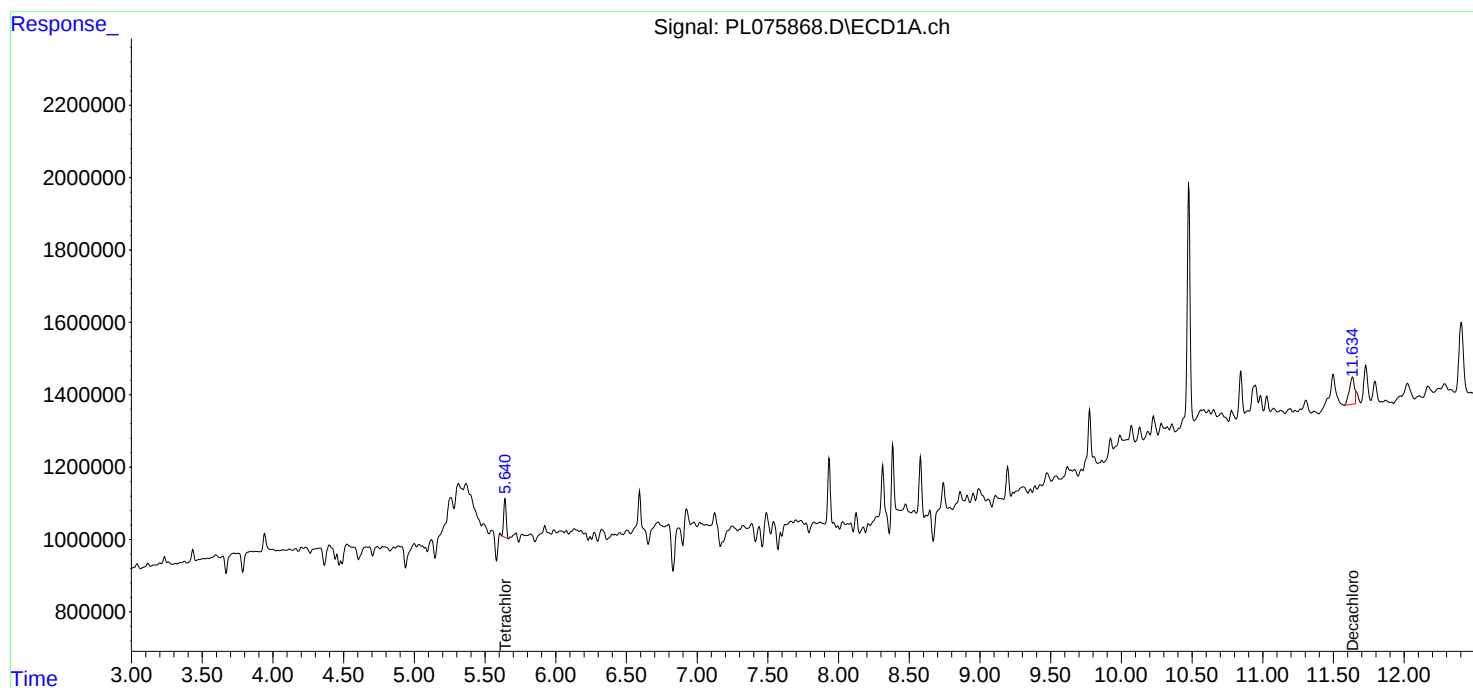

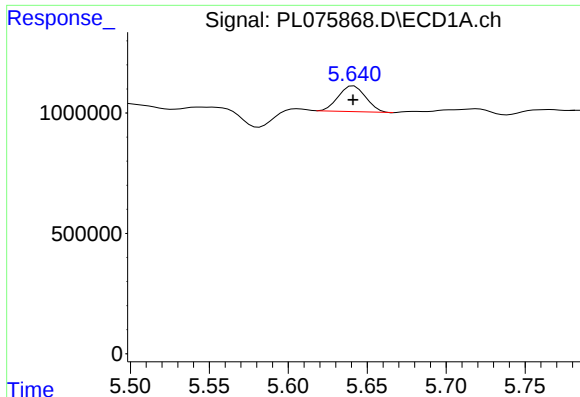


#1 Tetrachloro-m-xylene

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 1293117
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-2-061722


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/21/2022
Supervised By :Ankita Jodhani 06/22/2022

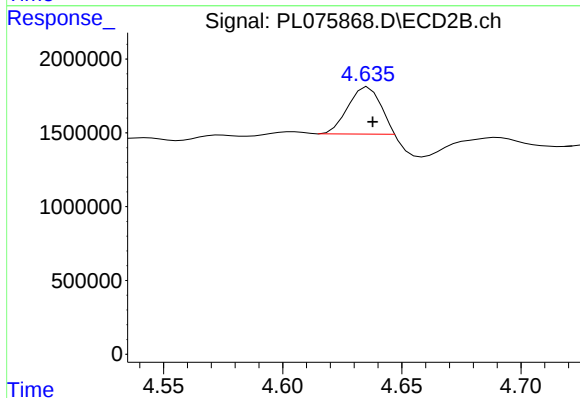


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 2949955
Conc: 1.76 ng/ml m

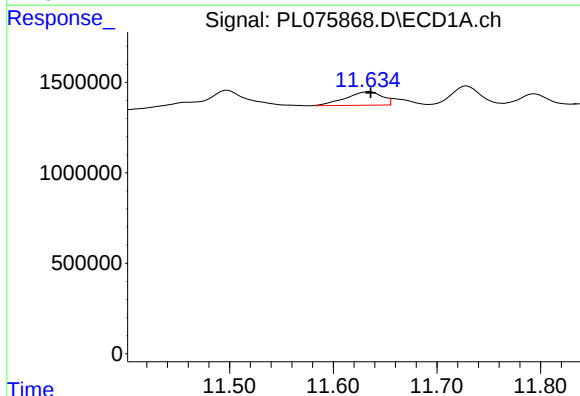

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.002 min
Response: 1890045
Conc: 3.09 ng/ml m

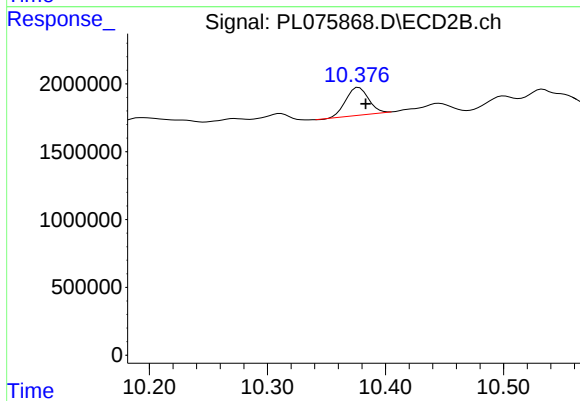

#28 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: -0.006 min
Response: 2724520
Conc: 1.93 ng/ml